

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070325\
 Data File : VX046877.D
 Acq On : 03 Jul 2025 11:25
 Operator : JC/MD
 Sample : Q2455-02 500X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Title : SW846 8260

Signal : TIC: VX046877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.233	183	188	199	rVB	23901	45670	1.49%	0.216%
2	5.397	696	707	723	rBV2	316106	999027	32.70%	4.721%
3	5.562	723	734	760	rVB	544718	1695112	55.48%	8.011%
4	5.964	788	800	810	rBV	345460	968719	31.71%	4.578%
5	6.769	922	932	954	rBV	866322	2237004	73.22%	10.571%
6	8.647	1234	1240	1247	rBV	1891257	3055359	100.00%	14.439%
7	8.720	1247	1252	1267	rVB	1845737	2965998	97.08%	14.016%
8	10.055	1465	1471	1487	rBV	1819492	2648491	86.68%	12.516%
9	10.195	1489	1494	1505	rVB	92198	135797	4.44%	0.642%
10	10.299	1505	1511	1524	rBV	509785	705874	23.10%	3.336%
11	10.640	1561	1567	1578	rBV	223629	303630	9.94%	1.435%
12	11.079	1633	1639	1654	rBV	1615466	2079000	68.04%	9.825%
13	11.378	1683	1688	1696	rBV	100908	182119	5.96%	0.861%
14	11.451	1696	1700	1712	rVB	50176	70870	2.32%	0.335%
15	11.610	1722	1726	1733	rVB	40116	55196	1.81%	0.261%
16	11.750	1744	1749	1761	rBV	167426	210664	6.89%	0.996%
17	12.018	1788	1793	1800	rBV	2233030	2696178	88.24%	12.741%
18	12.085	1800	1804	1811	rVB	39160	56383	1.85%	0.266%
19	12.244	1825	1830	1838	rBV3	30866	49993	1.64%	0.236%




Sum of corrected areas: 21161084

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070325\
Data File : VX046877.D
Acq On : 03 Jul 2025 11:25
Operator : JC/MD
Sample : Q2455-02 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

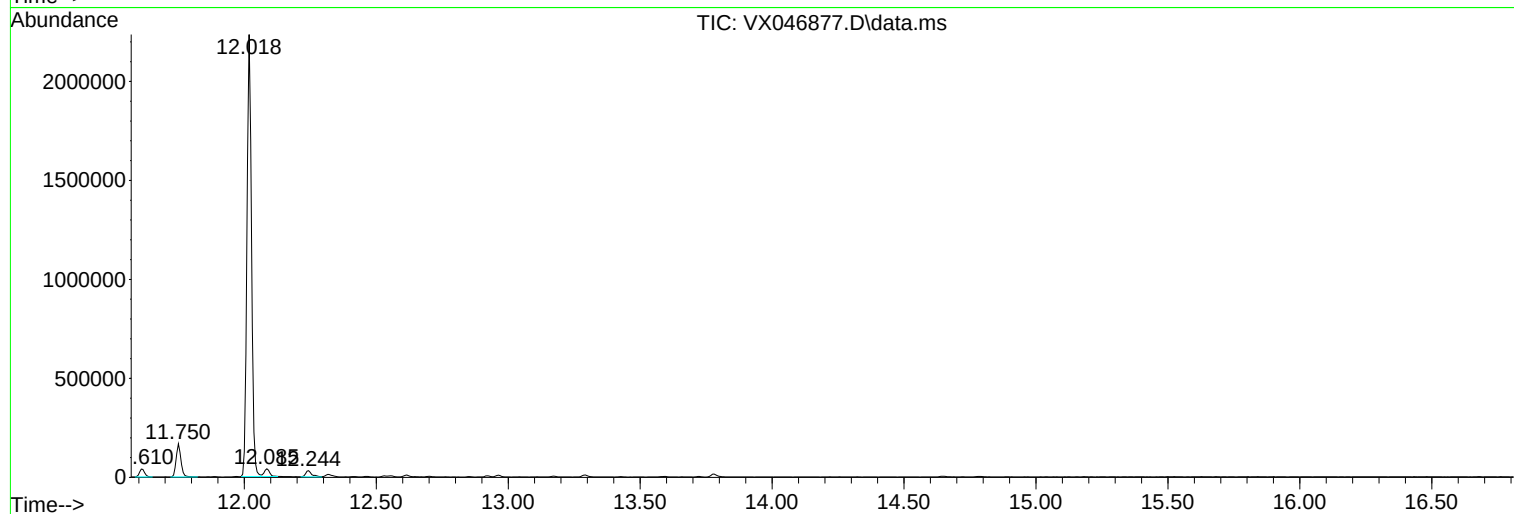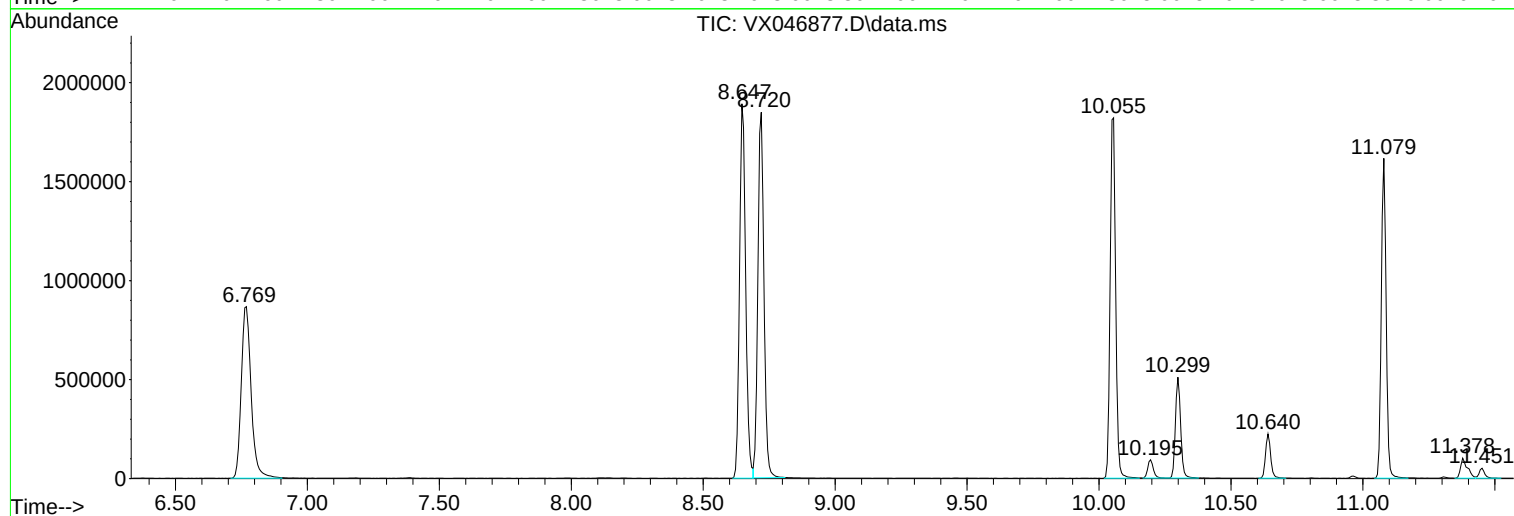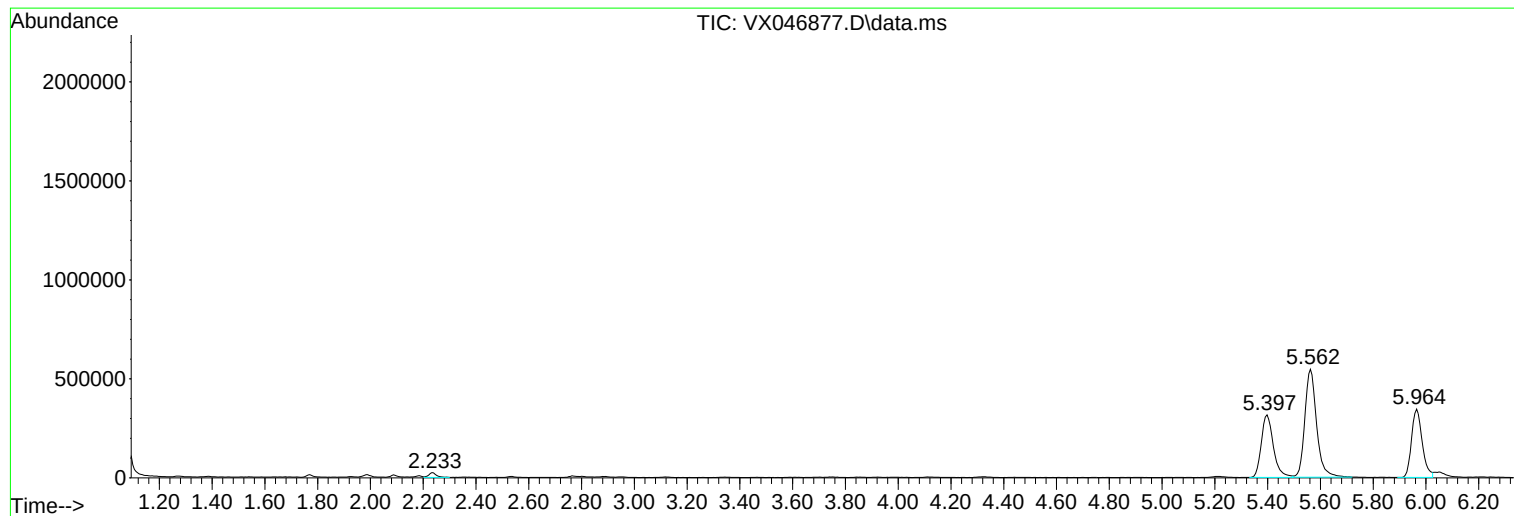

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070325\
Data File : VX046877.D
Acq On : 03 Jul 2025 11:25
Operator : JC/MD
Sample : Q2455-02 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070325\
Data File : VX046877.D
Acq On : 03 Jul 2025 11:25
Operator : JC/MD
Sample : Q2455-02 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc