

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
 Data File : VX042192.D
 Acq On : 04 Jul 2024 03:13
 Operator : JC/MD
 Sample : P3087-21ME
 Misc : 4.44g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 04 05:18:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 04 05:08:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	256219	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	230744	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	113237	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.373	65	56624	37.968	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.940%
7) Chloroethane-d5	1.648	69	17015	18.120	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	36.240%#
11) 1,1-Dichloroethene-d2	2.276	65	24651	37.768	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.540%
21) 2-Butanone-d5	4.489	46	84800	78.903	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	78.900%
24) Chloroform-d	5.056	84	113270	37.774	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.540%
26) 1,2-Dichloroethane-d4	5.952	65	73100	41.302	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.600%
32) Benzene-d6	5.964	84	253363	42.481	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.960%
36) 1,2-Dichloropropane-d6	7.305	67	76569	42.660	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.320%
41) Toluene-d8	8.647	98	228998	41.202	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.400%
43) trans-1,3-Dichloroprop...	8.951	79	27437	35.369	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.740%
47) 2-Hexanone-d5	9.390	63	65792	80.753	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.750%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	105033	39.582	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.160%
66) 1,2-Dichlorobenzene-d4	12.323	152	93990	42.734	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.460%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.715	43	9452	5.074	ug/L	99
61) 1,2,3-Trichloropropane	12.018	75	10658	5.300	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
Data File : VX042192.D
Acq On : 04 Jul 2024 03:13
Operator : JC/MD
Sample : P3087-21ME
Misc : 4.44g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 04 05:18:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 04 05:08:27 2024
Response via : Initial Calibration

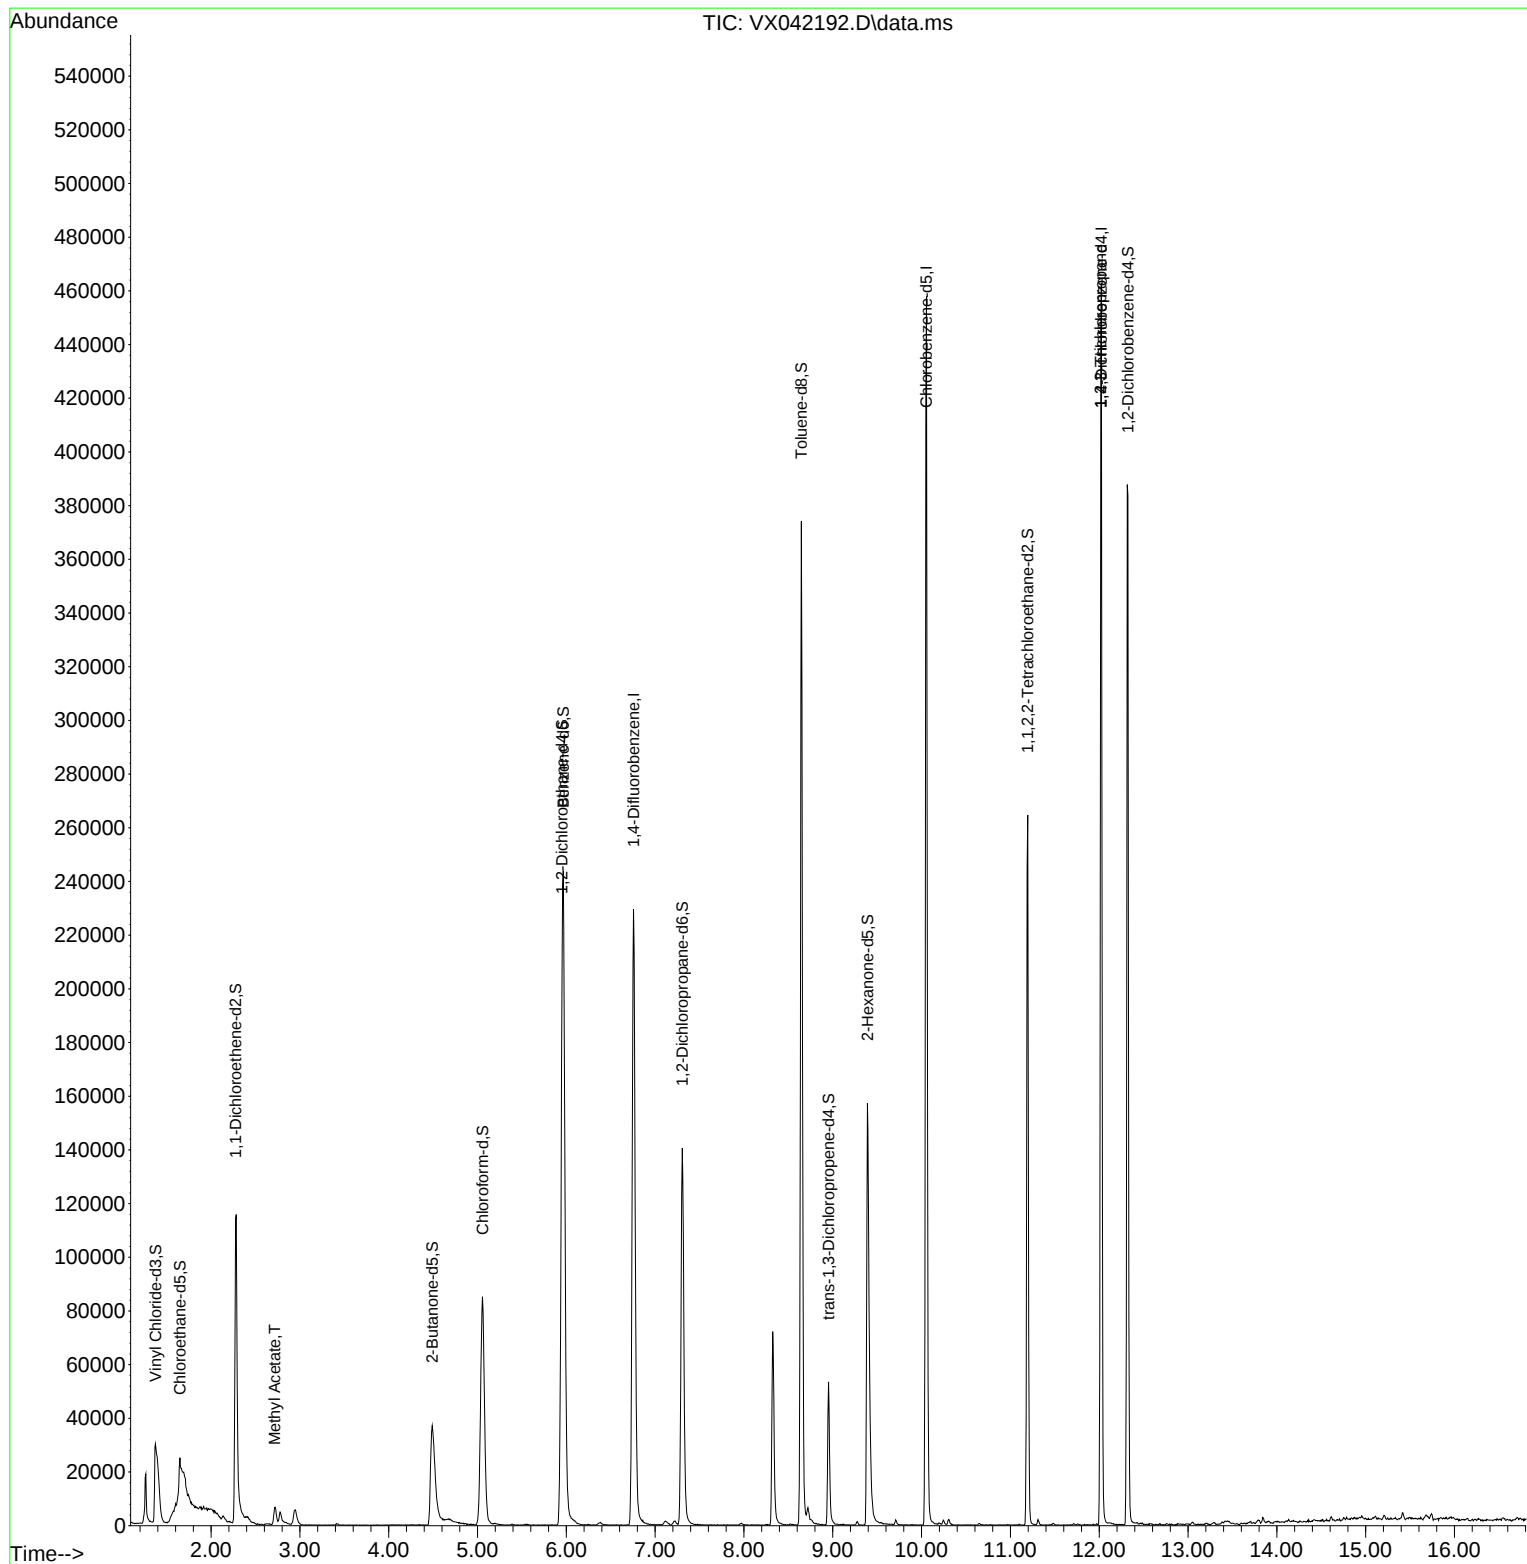

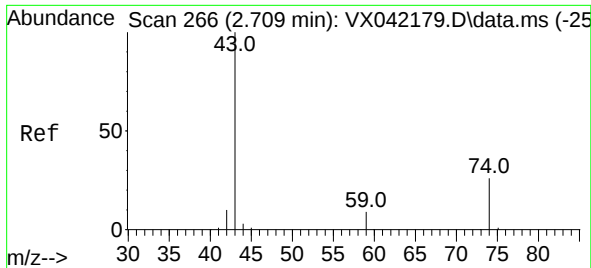

#15

Methyl Acetate

Concen: 5.074 ug/L

RT: 2.715 min Scan# 2

Delta R.T. 0.006 min

Lab File: VX042192.D

Acq: 04 Jul 2024 03:13

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 9452

Ion Ratio Lower Upper

43 100

74 24.8 20.1 30.1

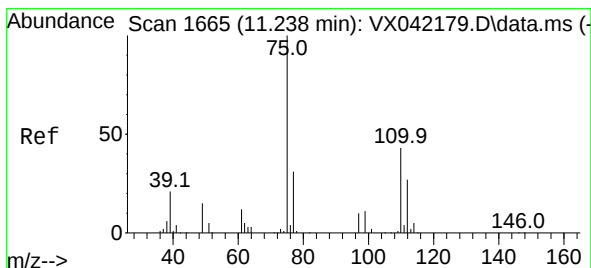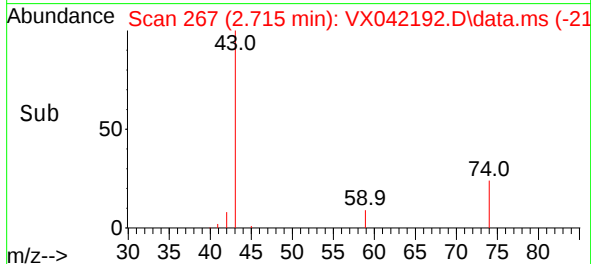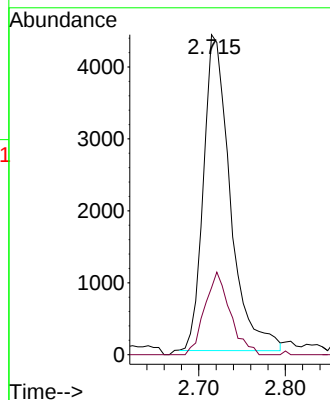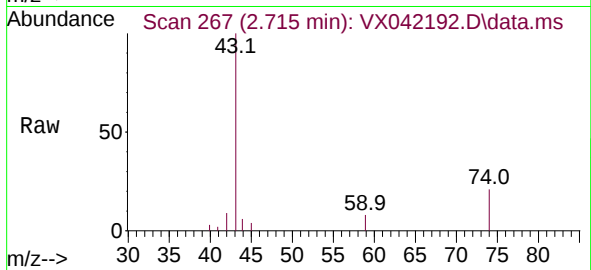

#61

1,2,3-Trichloropropane

Concen: 5.300 ug/L

RT: 12.018 min Scan# 1793

Delta R.T. 0.780 min

Lab File: VX042192.D

Acq: 04 Jul 2024 03:13

Tgt Ion: 75 Resp: 10658

Ion Ratio Lower Upper

75 100

77 31.5 25.8 38.8

110 3.0 35.4 53.0#

