




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
Data File : VX042183.D
Acq On : 03 Jul 2024 23:44
Operator : JC/MD
Sample : P3087-06ME
Misc : 5.10g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4CB1ME

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:16:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 04 05:08:27 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

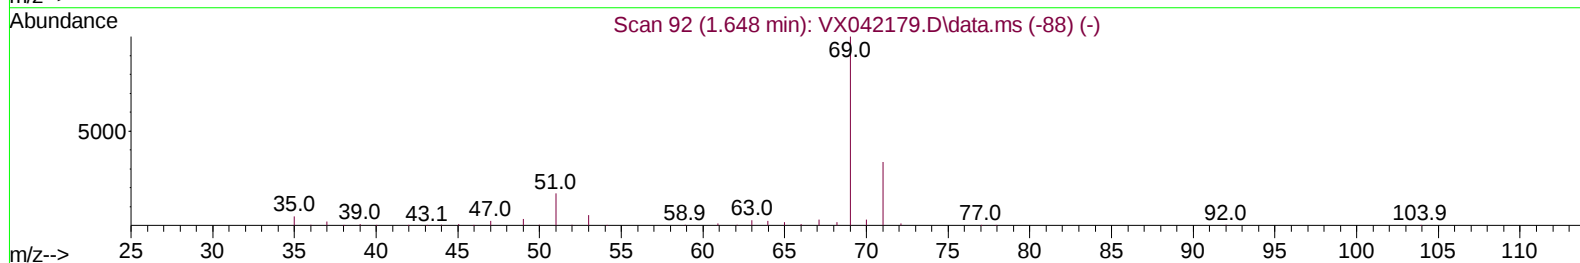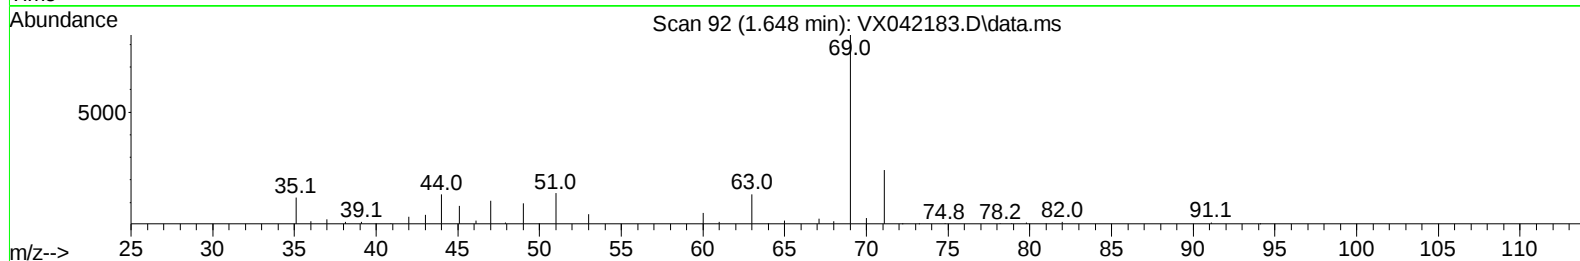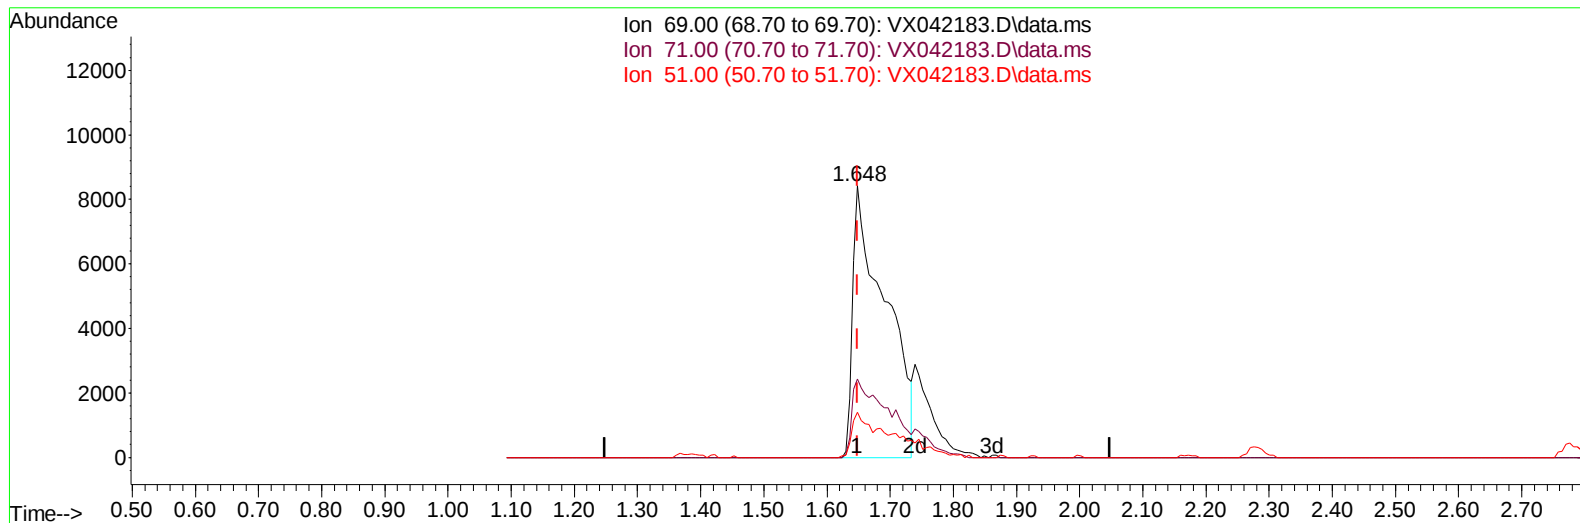

TIC: VX042183.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 31.56 ug/L

response 30202

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	13.54#
51.00	12.70	8.59#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
Data File : VX042183.D
Acq On : 03 Jul 2024 23:44
Operator : JC/MD
Sample : P3087-06ME
Misc : 5.10g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4CB1ME

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:16:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 04 05:08:27 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

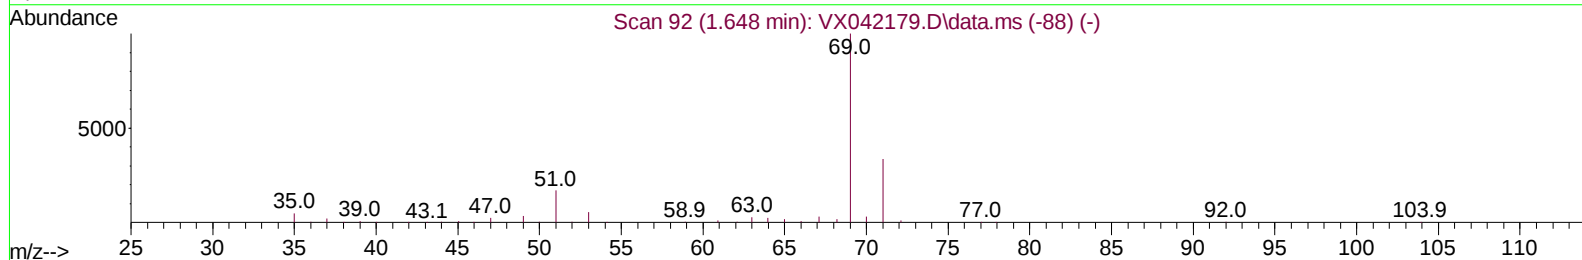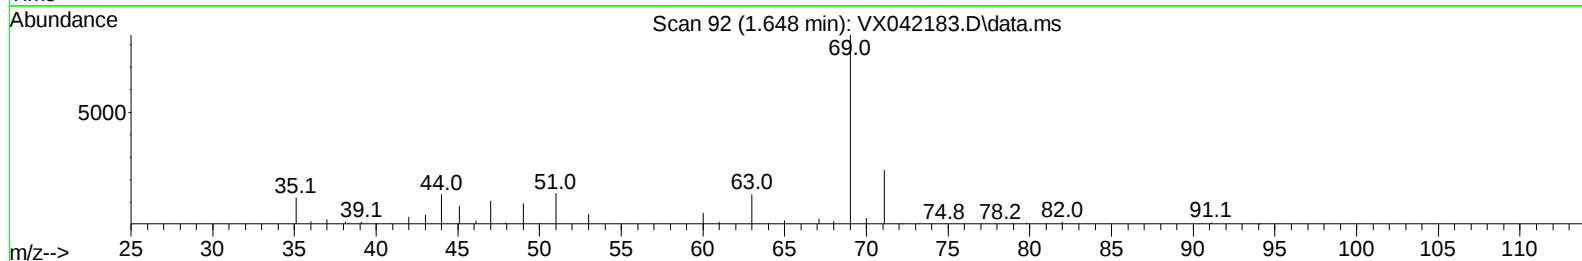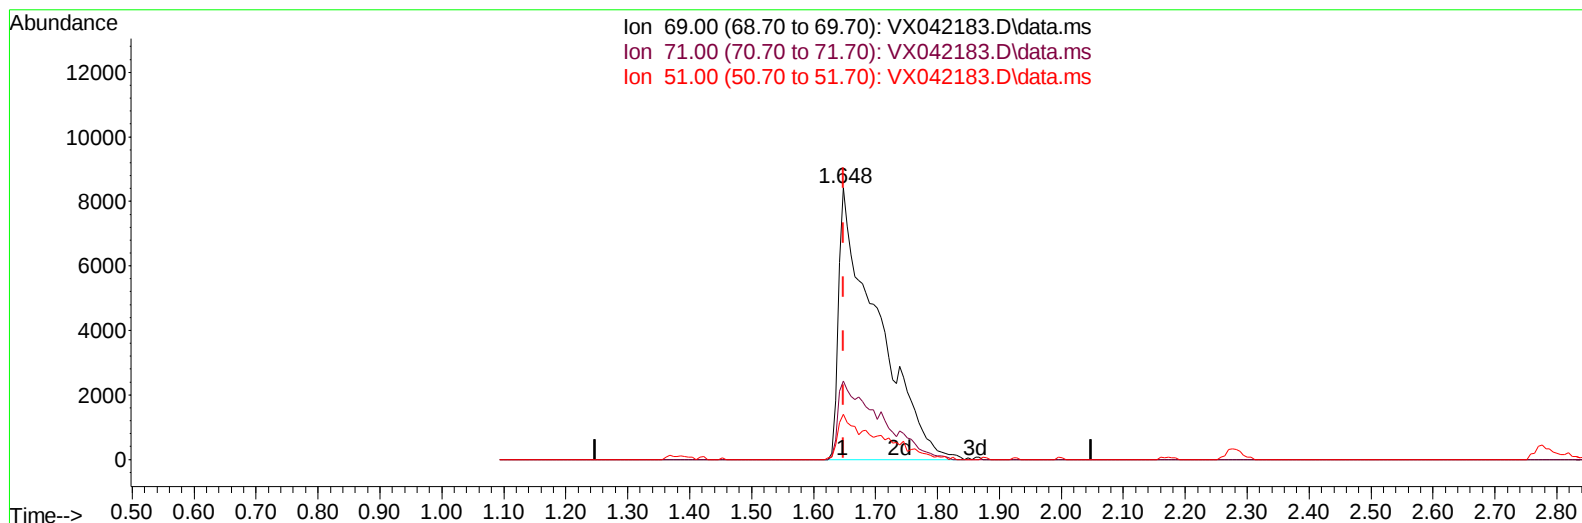

TIC: VX042183.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 37.57 ug/L m

response 35950

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	11.37#
51.00	12.70	7.22#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
 Data File : VX042183.D
 Acq On : 03 Jul 2024 23:44
 Operator : JC/MD
 Sample : P3087-06ME
 Misc : 5.10g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4CB1ME

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/05/2024
 Supervised By :Semsettin Yesilyurt 07/05/2024

Quant Time: Jul 04 05:16:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 04 05:08:27 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.757	114		261124	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117		231170	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152		113603	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.374	65		57126	37.585	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery =	75.180%		
7) Chloroethane-d5	1.648	69		35950m	37.566	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery =	75.140%		
11) 1,1-Dichloroethene-d2	2.276	65		25464	38.280	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125		Recovery =	76.560%		
21) 2-Butanone-d5	4.489	46		79934	72.979	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130		Recovery =	72.980%		
24) Chloroform-d	5.056	84		113531	37.150	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	74.300%		
26) 1,2-Dichloroethane-d4	5.952	65		72796	40.357	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	80.720%		
32) Benzene-d6	5.964	84		255121	42.696	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	85.400%		
36) 1,2-Dichloropropane-d6	7.306	67		75936	42.229	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery =	84.460%		
41) Toluene-d8	8.647	98		231118	41.506	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	83.020%		
43) trans-1,3-Dichloroprop...	8.952	79		28857	37.131	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery =	74.260%		
47) 2-Hexanone-d5	9.391	63		65590	80.357	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery =	80.360%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84		105294	39.607	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery =	79.220%		
66) 1,2-Dichlorobenzene-d4	12.323	152		95221	43.154	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	86.300%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
Data File : VX042183.D
Acq On : 03 Jul 2024 23:44
Operator : JC/MD
Sample : P3087-06ME
Misc : 5.10g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4CB1ME

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:16:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXL070324WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 04 05:08:27 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/05/2024
Supervised By :Semsettin Yesilyurt 07/05/2024

