

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
 Data File : VX042181.D
 Acq On : 03 Jul 2024 22:58
 Operator : JC/MD
 Sample : VX0704WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK681

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	7218	8021	0.87%	0.113%
2	1.368	43	46	61	rVB	95327	124190	13.43%	1.755%
3	1.648	88	92	101	rVB	68788	91833	9.93%	1.297%
4	2.294	192	198	210	rBV	197326	313527	33.91%	4.430%
5	2.502	227	232	237	rBV	1715	2733	0.30%	0.039%
6	2.666	256	259	263	rBV	257	421	0.05%	0.006%
7	2.788	273	279	290	rBV	13956	28964	3.13%	0.409%
8	2.947	297	305	314	rBV	4920	11054	1.20%	0.156%
9	3.087	323	328	329	rBV2	876	1178	0.13%	0.017%
10	3.184	340	344	346	rBV2	100	128	0.01%	0.002%
11	3.221	348	350	351	rVV	154	93	0.01%	0.001%
12	3.373	373	375	378	rBV2	110	129	0.01%	0.002%
13	3.440	382	386	389	rBV2	91	116	0.01%	0.002%
14	3.544	401	403	407	rBV	132	133	0.01%	0.002%
15	3.672	422	424	427	rBV2	89	92	0.01%	0.001%
16	3.727	431	433	436	rVV2	153	143	0.02%	0.002%
17	3.806	445	446	449	rVB	125	112	0.01%	0.002%
18	3.879	456	458	459	rBV	155	142	0.02%	0.002%
19	3.977	473	474	476	rBV	155	129	0.01%	0.002%
20	4.068	488	489	491	rBV2	143	124	0.01%	0.002%
21	4.263	519	521	522	rBV2	108	107	0.01%	0.002%
22	4.300	526	527	529	rBV	117	108	0.01%	0.002%
23	4.465	546	554	573	rBV	67669	200485	21.68%	2.833%
24	4.812	609	611	613	rVB	201	128	0.01%	0.002%
25	5.056	639	651	671	rBV	113119	353965	38.28%	5.001%
26	5.324	694	695	697	rBV	194	138	0.01%	0.002%
27	5.385	700	705	708	rBV3	318	576	0.06%	0.008%
28	5.544	728	731	732	rBV2	217	225	0.02%	0.003%
29	5.635	744	746	748	rBV2	97	108	0.01%	0.002%
30	5.666	748	751	753	rBV2	285	381	0.04%	0.005%
31	5.964	789	800	824	rBV2	317158	924659	100.00%	13.064%
32	6.373	865	867	868	rBV2	206	129	0.01%	0.002%
33	6.580	900	901	904	rBV	118	118	0.01%	0.002%
34	6.757	921	930	950	rBV	246988	600966	64.99%	8.491%
35	7.117	982	989	1001	rVB6	2559	7615	0.82%	0.108%
36	7.220	1001	1006	1012	rVB3	370	739	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
 Data File : VX042181.D
 Acq On : 03 Jul 2024 22:58
 Operator : JC/MD
 Sample : VX0704WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK681

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1042	rBV	181703	408325	44.16%	5.769%
38	7.476	1047	1048	1054	rVB3	474	691	0.07%	0.010%
39	7.574	1063	1064	1070	rVB	144	146	0.02%	0.002%
40	7.665	1077	1079	1080	rBV	138	92	0.01%	0.001%
41	7.744	1090	1092	1094	rVB	175	133	0.01%	0.002%
42	7.787	1096	1099	1101	rVB2	150	193	0.02%	0.003%
43	7.836	1103	1107	1111	rVV3	257	388	0.04%	0.005%
44	7.872	1111	1113	1117	rVB2	164	173	0.02%	0.002%
45	7.909	1117	1119	1121	rBV2	131	133	0.01%	0.002%
46	7.970	1126	1129	1133	rVV2	238	453	0.05%	0.006%
47	8.031	1136	1139	1141	rBV	201	179	0.02%	0.003%
48	8.263	1175	1177	1180	rBV2	136	187	0.02%	0.003%
49	8.324	1181	1187	1205	rVV	106852	183842	19.88%	2.597%
50	8.580	1226	1229	1231	rBV2	270	304	0.03%	0.004%
51	8.647	1234	1240	1252	rBV	484520	763518	82.57%	10.787%
52	8.952	1285	1290	1309	rBV	75788	120264	13.01%	1.699%
53	9.195	1328	1330	1332	rVB2	180	121	0.01%	0.002%
54	9.220	1332	1334	1338	rBV2	278	294	0.03%	0.004%
55	9.275	1338	1343	1349	rBV	1950	3082	0.33%	0.044%
56	9.342	1352	1354	1356	rBV	144	143	0.02%	0.002%
57	9.384	1356	1361	1381	rBV	290480	435894	47.14%	6.158%
58	9.811	1429	1431	1433	rVV	295	198	0.02%	0.003%
59	9.848	1435	1437	1439	rVB2	285	236	0.03%	0.003%
60	9.915	1446	1448	1450	rBV2	101	98	0.01%	0.001%
61	10.055	1465	1471	1483	rBV	500035	694788	75.14%	9.816%
62	10.201	1491	1495	1505	rVB	1963	2824	0.31%	0.040%
63	10.311	1508	1513	1521	rBV	1753	3079	0.33%	0.044%
64	10.421	1527	1531	1533	rBV2	122	199	0.02%	0.003%
65	10.439	1533	1534	1537	rVV	157	117	0.01%	0.002%
66	10.500	1542	1544	1548	rVV2	133	179	0.02%	0.003%
67	10.652	1564	1569	1570	rBV2	1371	1872	0.20%	0.026%
68	10.768	1587	1588	1591	rBV2	127	116	0.01%	0.002%
69	10.811	1591	1595	1599	rVB3	232	317	0.03%	0.004%
70	10.890	1606	1608	1610	rBV2	148	120	0.01%	0.002%
71	10.963	1617	1620	1628	rBV	1761	2146	0.23%	0.030%
72	11.098	1640	1642	1646	rVB3	230	261	0.03%	0.004%
73	11.189	1652	1657	1665	rBV	364750	469179	50.74%	6.629%
74	11.457	1697	1701	1706	rVB2	1169	1652	0.18%	0.023%
75	11.549	1714	1716	1717	rBV	94	95	0.01%	0.001%
76	11.707	1739	1742	1746	rBV3	281	361	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
 Data File : VX042181.D
 Acq On : 03 Jul 2024 22:58
 Operator : JC/MD
 Sample : VX0704WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK681

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.756	1746	1750	1755	rVB	1526	1972	0.21%	0.028%
78	11.921	1774	1777	1780	rBV	134	145	0.02%	0.002%
79	11.975	1782	1786	1788	rBV	3100	3659	0.40%	0.052%
80	12.018	1788	1793	1806	rVB	476879	632433	68.40%	8.935%
81	12.317	1837	1842	1857	rBV	506482	652914	70.61%	9.225%
82	12.530	1875	1877	1881	rBV3	201	269	0.03%	0.004%
83	12.567	1881	1883	1884	rBV	197	109	0.01%	0.002%
84	12.713	1906	1907	1909	rBV	145	133	0.01%	0.002%
85	12.737	1909	1911	1912	rVB	214	127	0.01%	0.002%
86	12.792	1919	1920	1923	rBV	151	120	0.01%	0.002%
87	13.036	1958	1960	1961	rBV2	155	125	0.01%	0.002%
88	13.115	1968	1973	1980	rBV3	1899	2743	0.30%	0.039%
89	13.268	1996	1998	1999	rBV	142	95	0.01%	0.001%
90	13.591	2046	2051	2060	rBV3	2591	3712	0.40%	0.052%
91	13.676	2063	2065	2066	rBV	232	136	0.01%	0.002%
92	13.749	2076	2077	2078	rBV	243	153	0.02%	0.002%
93	13.780	2078	2082	2090	rVV2	2729	4311	0.47%	0.061%
94	13.853	2093	2094	2096	rVV	269	154	0.02%	0.002%
95	13.896	2100	2101	2103	rVB	183	103	0.01%	0.001%
96	13.963	2108	2112	2118	rBV3	2205	3204	0.35%	0.045%
97	14.164	2143	2145	2146	rBV	166	96	0.01%	0.001%
98	14.457	2192	2193	2194	rBV	223	133	0.01%	0.002%
99	14.755	2240	2242	2245	rVB2	493	451	0.05%	0.006%
100	15.487	2360	2362	2366	rBV	635	592	0.06%	0.008%

Sum of corrected areas: 7077990




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
Data File : VX042181.D
Acq On : 03 Jul 2024 22:58
Operator : JC/MD
Sample : VX0704WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK681

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

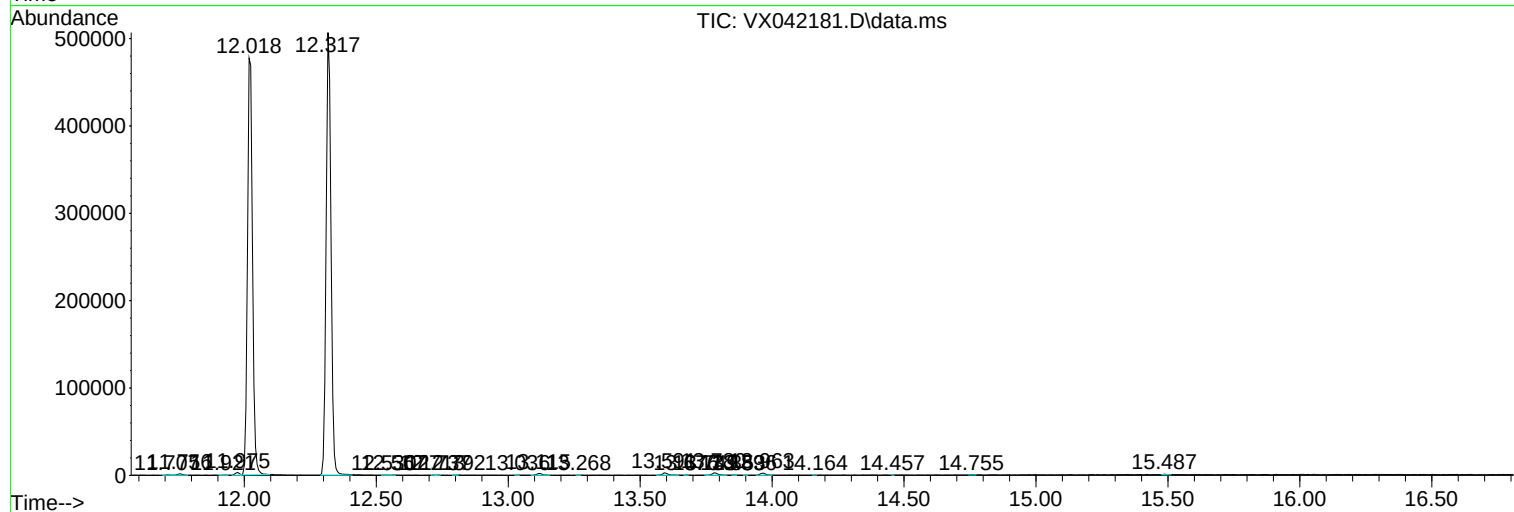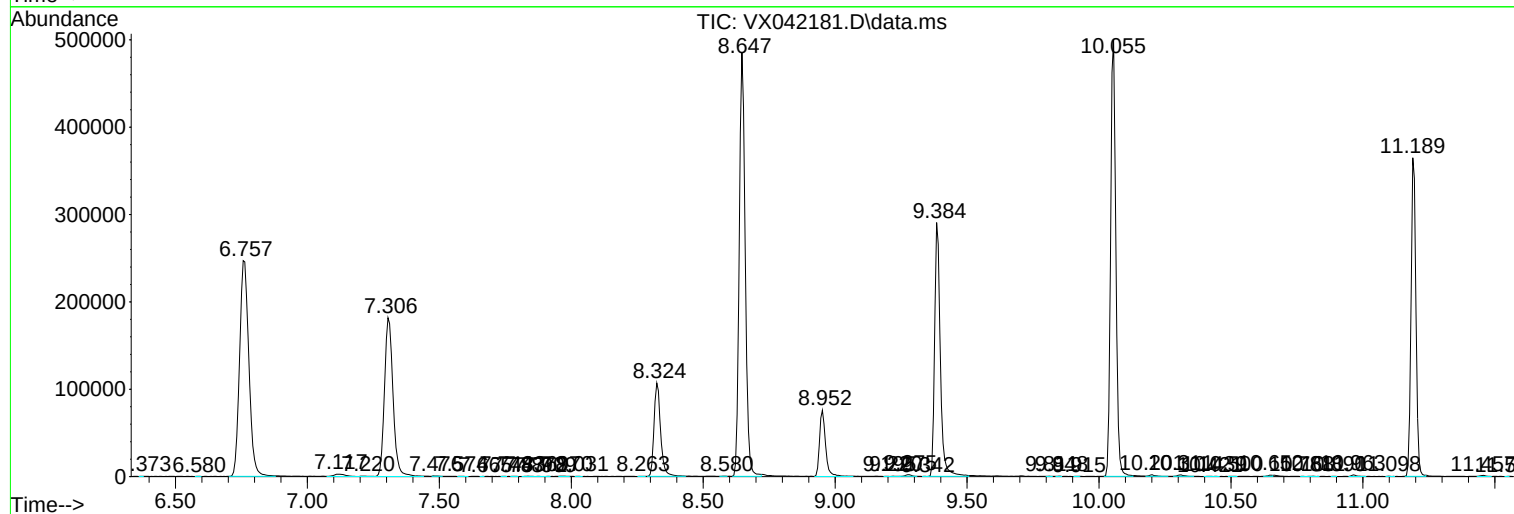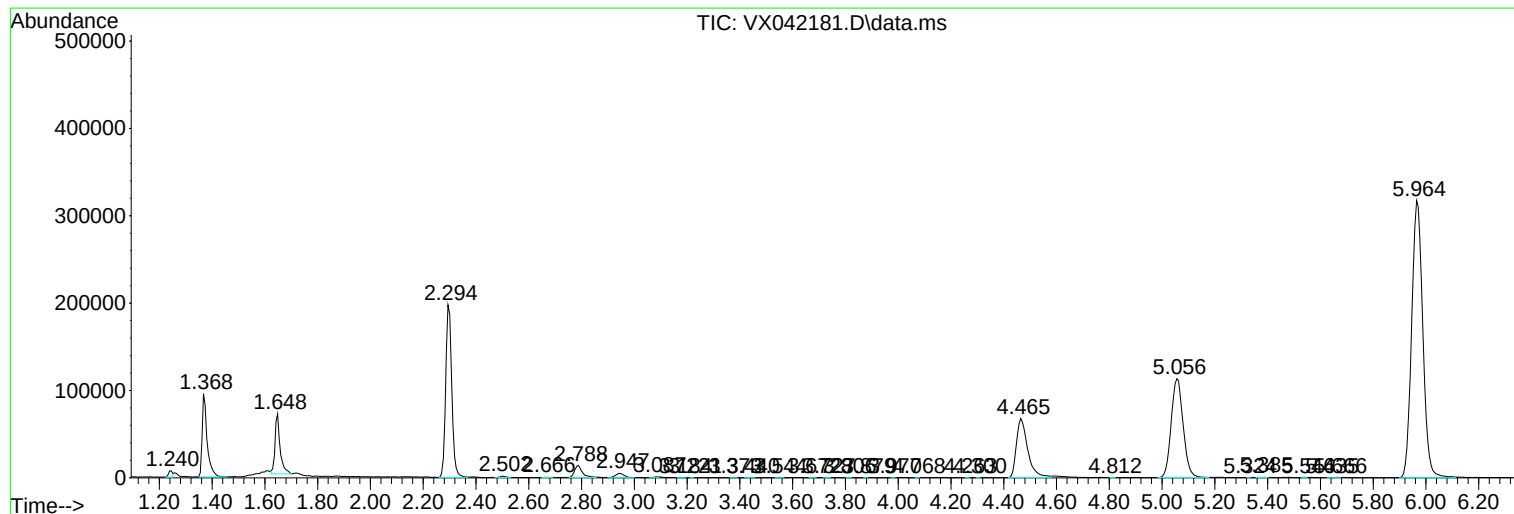

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
Data File : VX042181.D
Acq On : 03 Jul 2024 22:58
Operator : JC/MD
Sample : VX0704WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK681

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070424\
Data File : VX042181.D
Acq On : 03 Jul 2024 22:58
Operator : JC/MD
Sample : VX0704WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK681

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc