


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX070518\
Data File : VX003164.D
Acq On : 05 Jul 2018 09:32
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Title : SW846 8260
Last Update : Mon Jun 25 14:38:05 2018

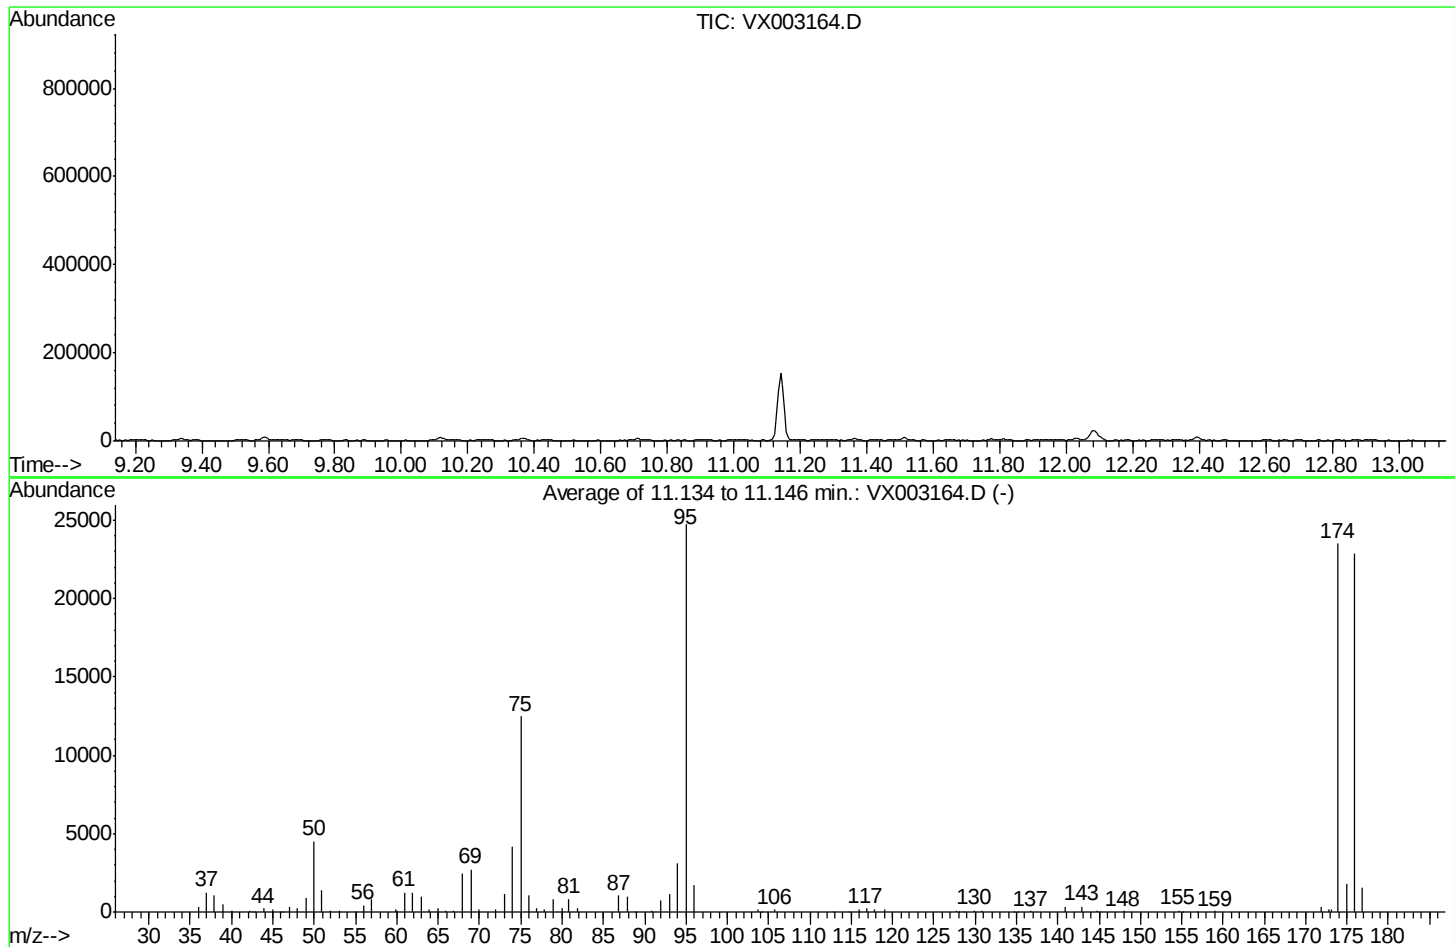

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	4507	PASS
75	95	30	60	50.5	12485	PASS
95	95	100	100	100.0	24730	PASS
96	95	5	9	6.9	1707	PASS
173	174	0.00	2	0.9	201	PASS
174	95	50	100	95.0	23485	PASS
175	174	5	9	7.8	1830	PASS
176	174	95	101	97.4	22885	PASS
177	176	5	9	6.8	1555	PASS