
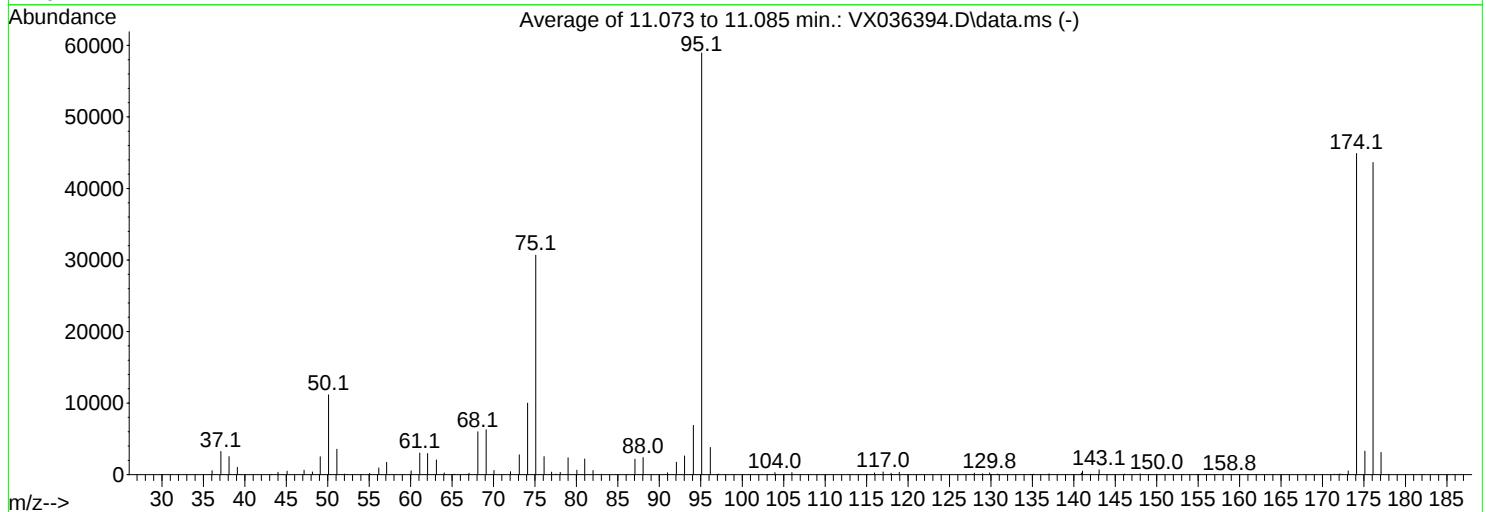


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070523\
Data File : VX036394.D
Acq On : 05 Jul 2023 11:22
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Title : SW846 8260
Last Update : Fri Jun 23 15:03:28 2023

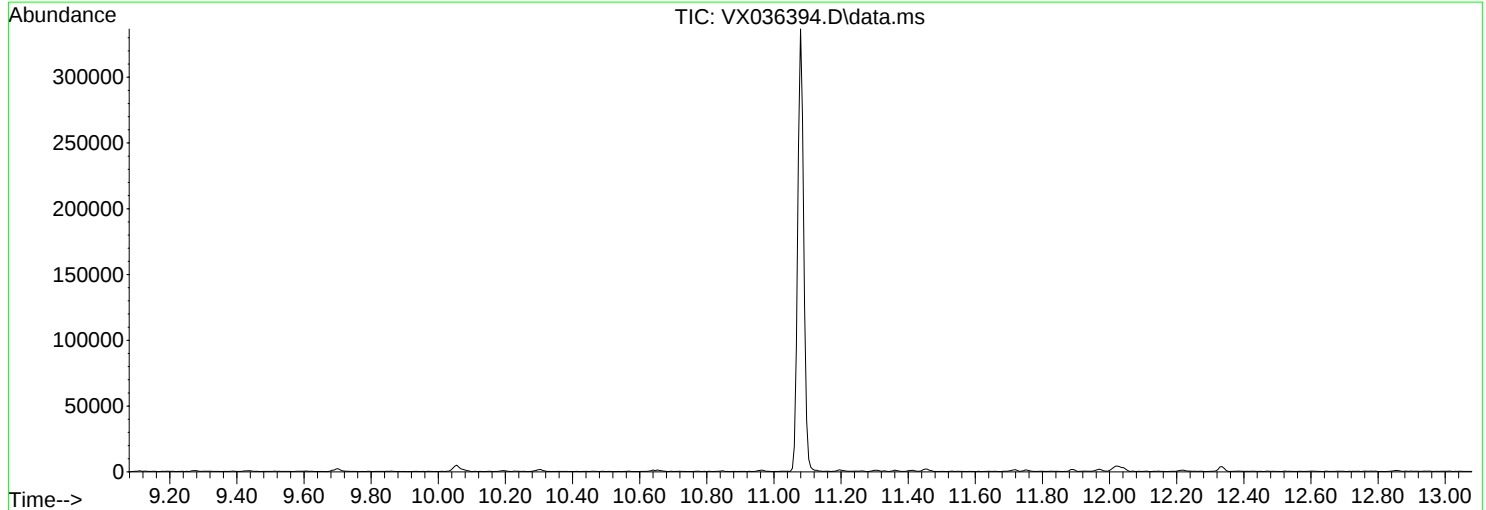

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	11153	PASS
75	95	30	60	52.0	30677	PASS
95	95	100	100	100.0	58960	PASS
96	95	5	9	6.4	3801	PASS
173	174	0.00	2	1.2	519	PASS
174	95	50	100	76.1	44880	PASS
175	174	5	9	7.3	3296	PASS
176	174	95	101	97.2	43645	PASS
177	176	5	9	7.1	3100	PASS