

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070618\
 Data File : VX003224.D
 Acq On : 06 Jul 2018 20:40
 Operator : JC/MD
 Sample : J3754-02DL 40X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S10-0139DL

Quant Time: Jul 09 09:27:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 25 14:38:05 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	285516	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	396400	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	366767	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	206892	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	179091	45.38	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.76%	
35) Dibromofluoromethane	5.51	113	151203	48.17	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.34%	
50) Toluene-d8	8.72	98	550875	48.06	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.12%	
62) 4-Bromofluorobenzene	11.14	95	193169	43.69	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.38%	
Target Compounds						
40) Benzene	6.15	78	497801	39.413	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070618\
Data File : VX003224.D
Acq On : 06 Jul 2018 20:40
Operator : JC/MD
Sample : J3754-02DL 40X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S10-0139DL

Quant Time: Jul 09 09:27:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 25 14:38:05 2018
Response via : Initial Calibration

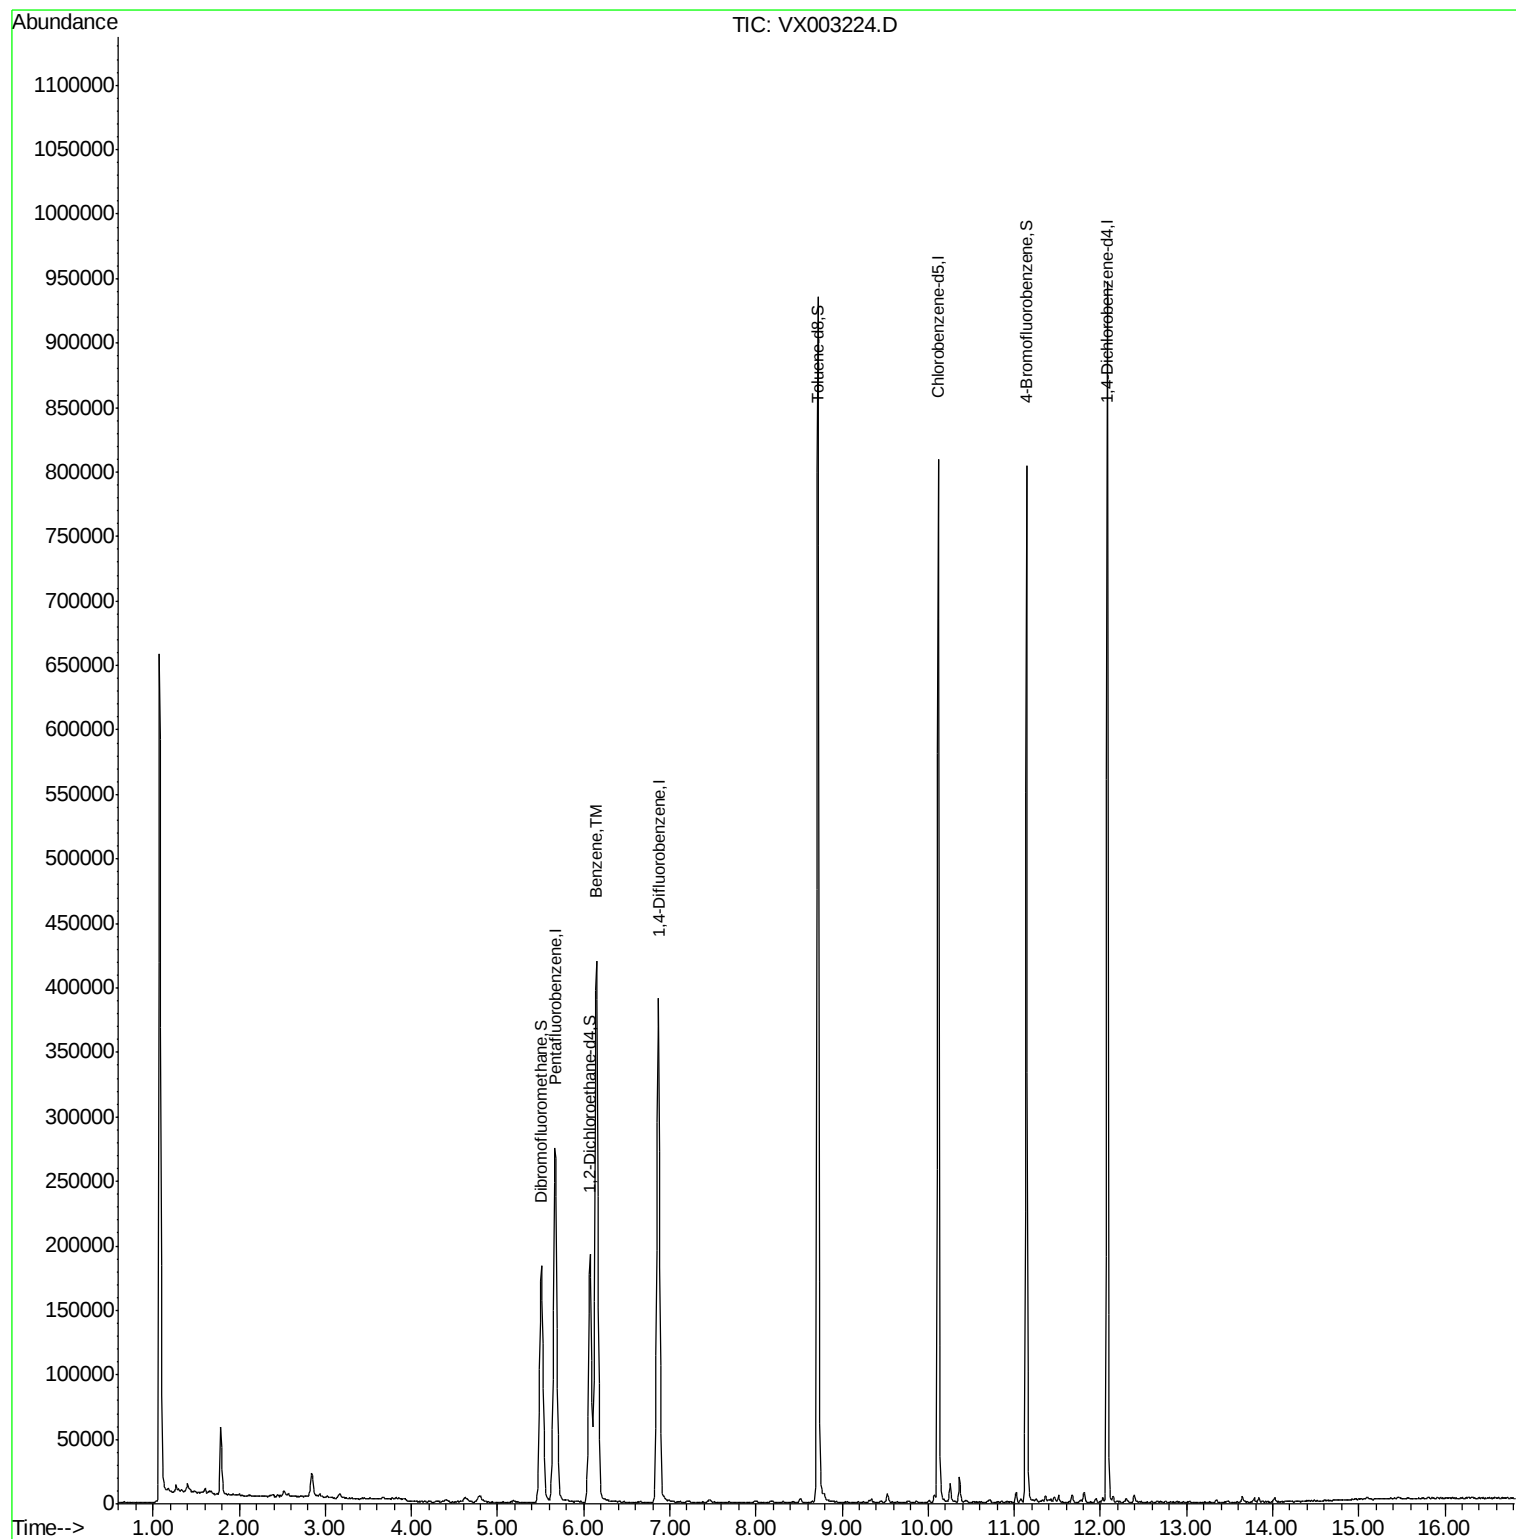

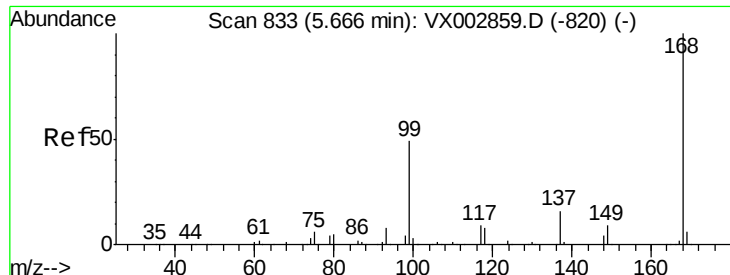

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.00 min

Lab File: VX003224.D

Acq: 06 Jul 2018 20:40

Instrument :

MSVOA_X

ClientSampled :


S10-0139DL

Tot Ion:168 Resp: 285516

Ion Ratio Lower Upper

168 100

99 49.0 39.3 58.9

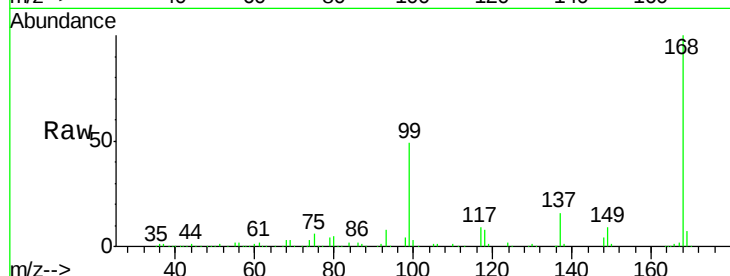

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

120000

100000

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

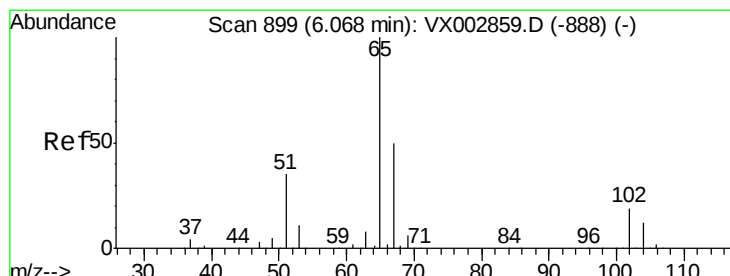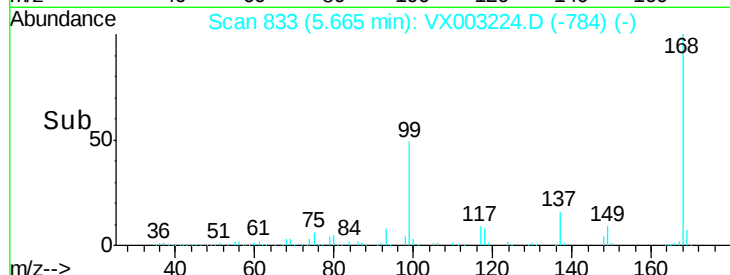

#33

1,2-Dichloroethane-d4

Concen: 45.381 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.01 min

Lab File: VX003224.D


Acq: 06 Jul 2018 20:40

Tgt Ion: 65 Resp: 179091

Ion Ratio Lower Upper

65 100

67 52.7 0.0 102.6

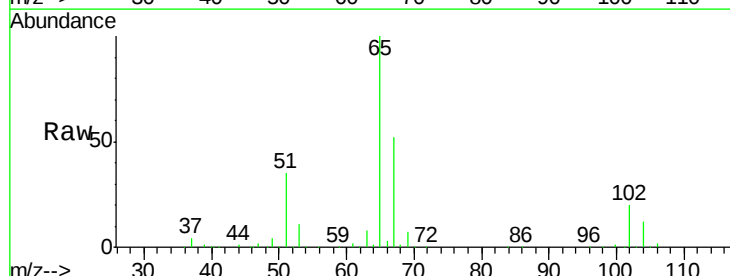

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

80000


60000


40000

20000

0

Time--> 6.00 6.10 6.20

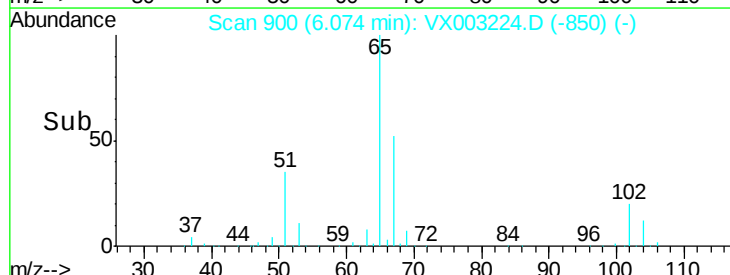

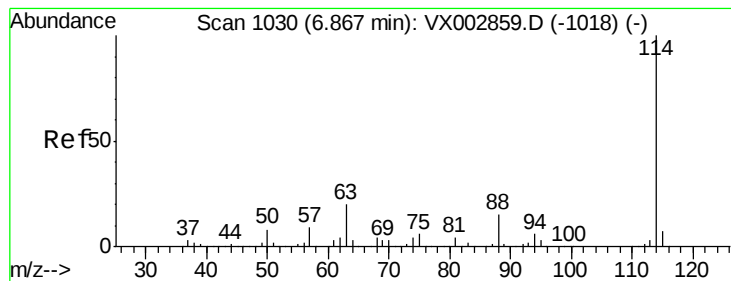

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX003224.D

Acq: 06 Jul 2018 20:40

Instrument :

MSVOA_X

ClientSampleId :

S10-0139DL


Tot Ion:114 Resp: 396400

Ion Ratio Lower Upper

114 100

63 19.7 0.0 41.4




88 15.1 0.0 30.0

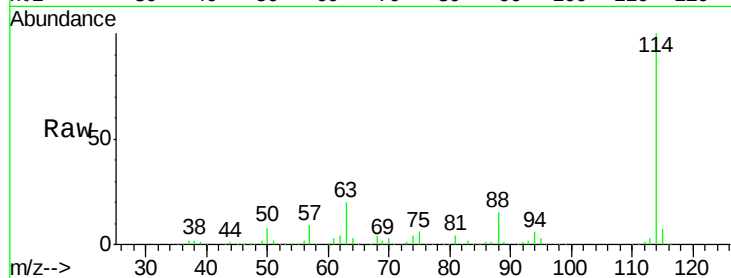

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

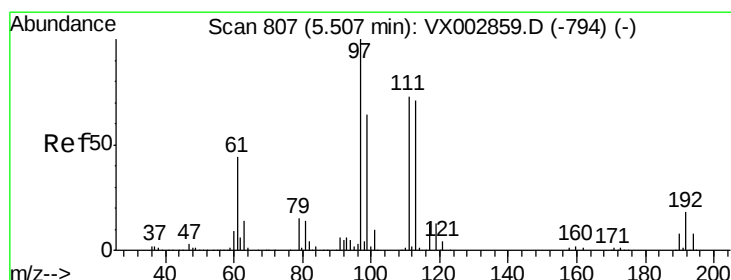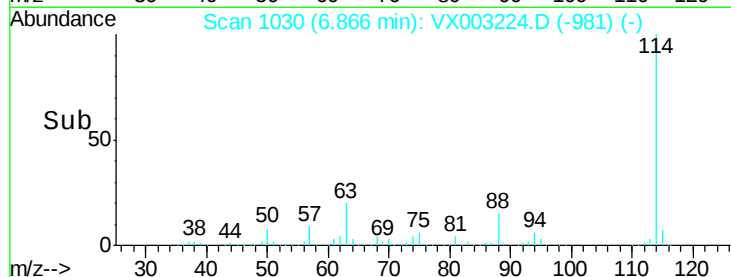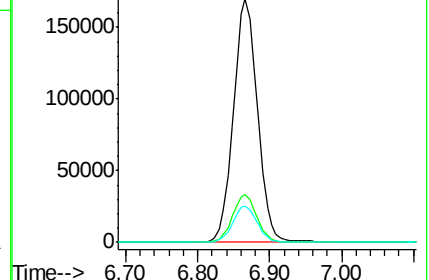

#35

Dibromofluoromethane

Concen: 48.167 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.00 min

Lab File: VX003224.D

Acq: 06 Jul 2018 20:40


Tgt Ion:113 Resp: 151203

Ion Ratio Lower Upper

113 100

111 104.4 81.4 122.0



192 25.4 19.1 28.7

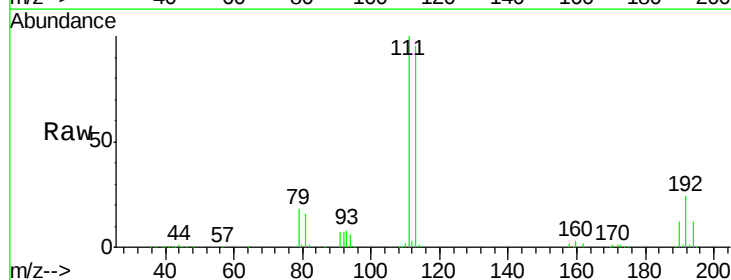


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

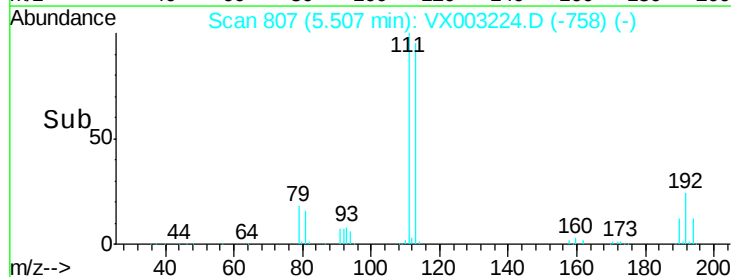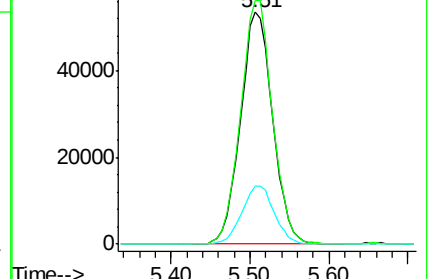

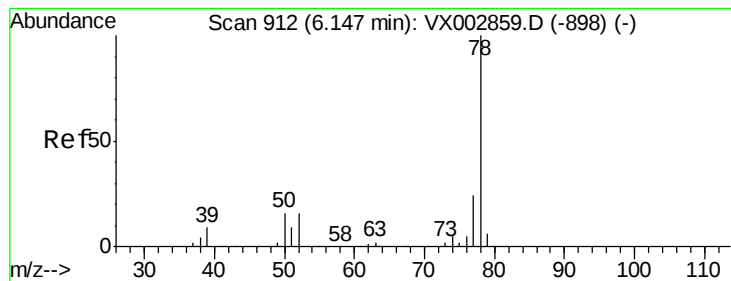

#40

Benzene

Concen: 39.413 ug/l

RT: 6.15 min Scan# 912

Delta R.T. -0.00 min

Lab File: VX003224.D

Acq: 06 Jul 2018 20:40

Instrument :

MSVOA_X

ClientSampled :


S10-0139DL

Tot Ion: 78 Resp: 497801

Ion Ratio Lower Upper

78 100

77 23.4 19.1 28.7

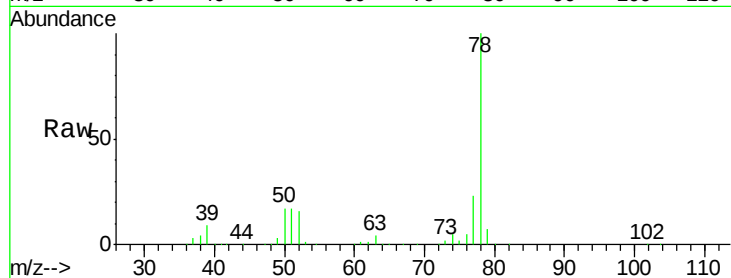

Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

6.15

200000



150000

100000

50000

0

Time-->

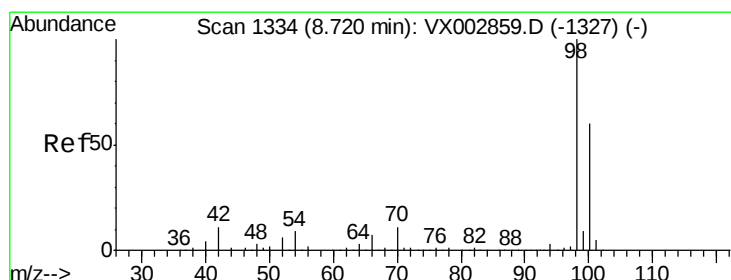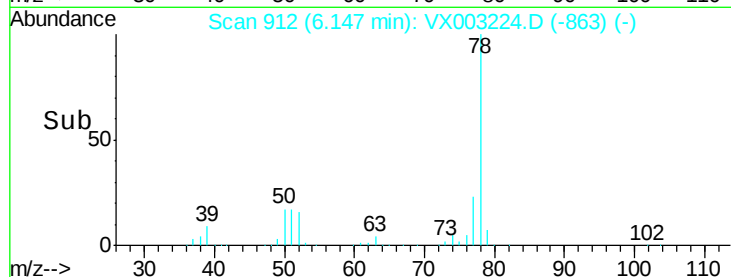

#50

Toluene-d8

Concen: 48.056 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX003224.D


Acq: 06 Jul 2018 20:40

Tgt Ion: 98 Resp: 550875

Ion Ratio Lower Upper

98 100

100 64.2 50.9 76.3

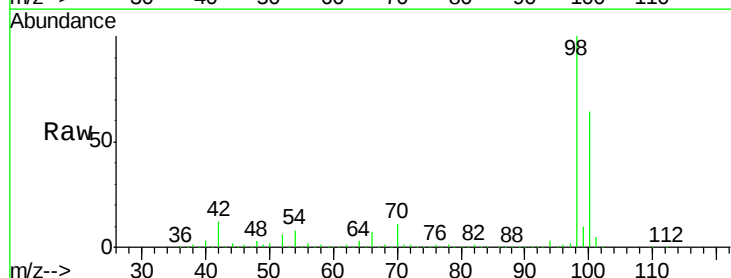

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

8.72

400000


300000


200000

100000

0

Time-->

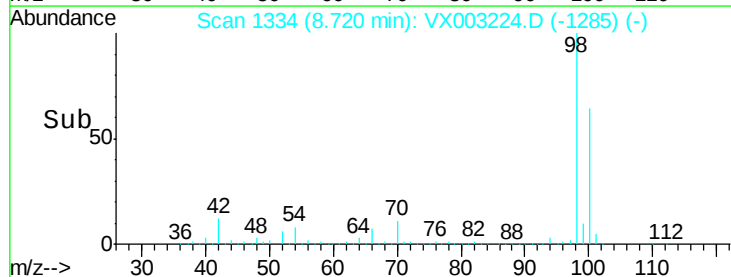

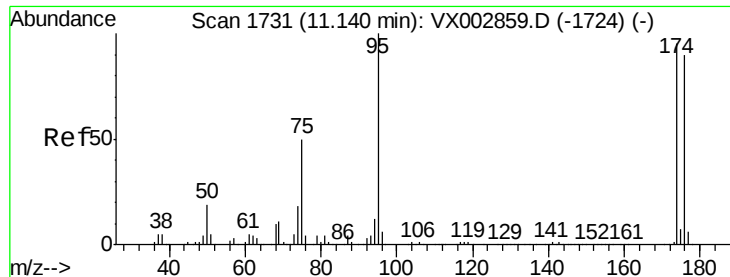

#62

4-Bromofluorobenzene

Concen: 43.694 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX003224.D

Acq: 06 Jul 2018 20:40

Instrument :

MSVOA_X

ClientSampleId :

S10-0139DL


Tot Ion: 95 Resp: 193169

Ion Ratio Lower Upper

95 100

174 99.0 0.0 187.4




176 95.8 0.0 181.0

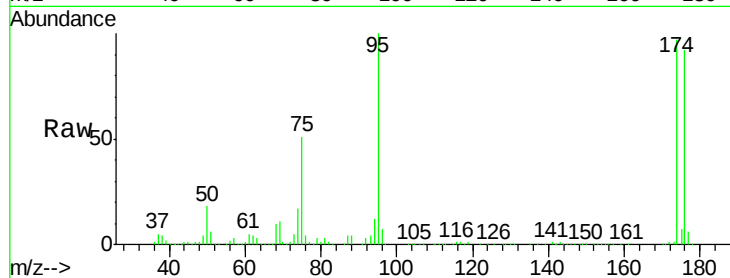

Abundance Ion 94.90 (94.60 to 95.60): VX002859.D (-1724) (-)

Ion 173.80 (173.50 to 174.50): VX002859.D (-1724) (-)

Ion 175.80 (175.50 to 176.50): VX002859.D (-1724) (-)

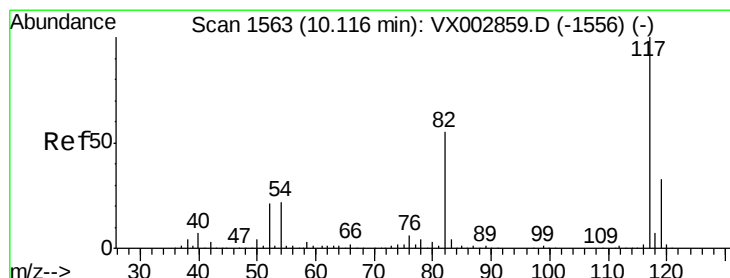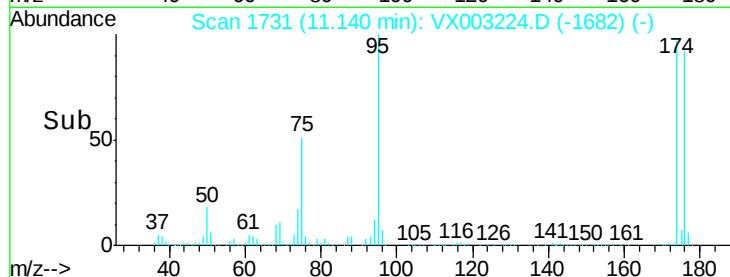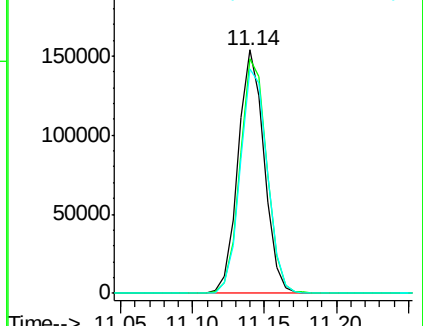

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1563

Delta R.T. -0.00 min

Lab File: VX003224.D

Acq: 06 Jul 2018 20:40


Tgt Ion: 117 Resp: 366767

Ion Ratio Lower Upper

117 100

82 52.2 45.0 67.4



119 32.2 25.8 38.6

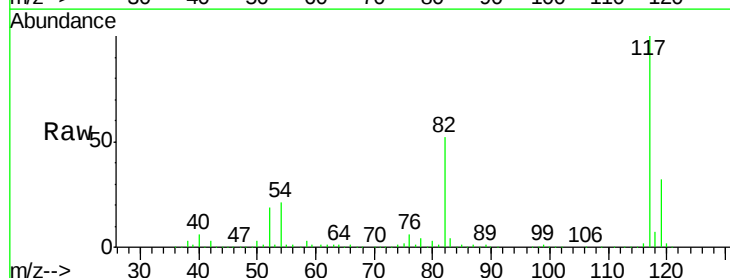


Abundance Ion 116.90 (116.60 to 117.60): VX002859.D (-1556) (-)

Ion 82.00 (81.70 to 82.70): VX002859.D (-1556) (-)

Ion 118.90 (118.60 to 119.60): VX002859.D (-1556) (-)

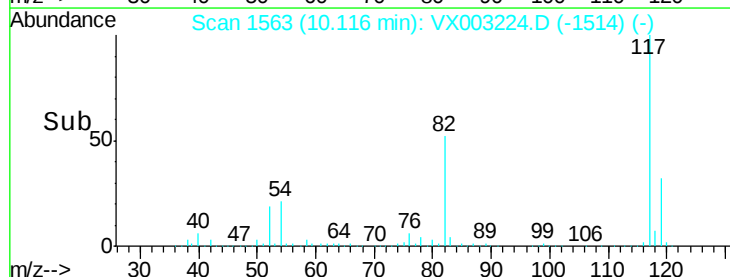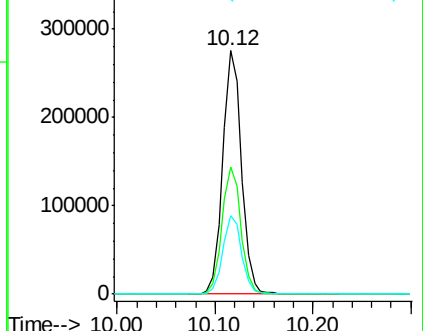


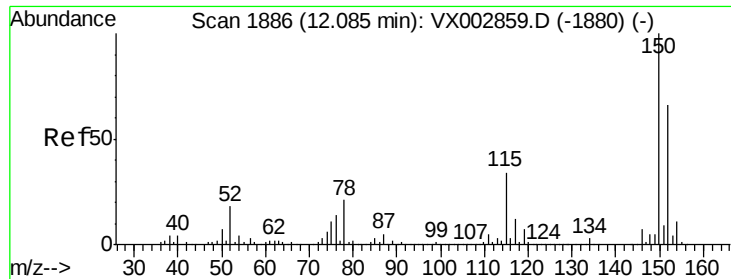

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1885
 Delta R.T. -0.01 min
 Lab File: VX003224.D
 Acq: 06 Jul 2018 20:40

Instrument :
 MSVOA_X
 ClientSampleId :
 S10-0139DL

Tot Ion	Ratio	Lower	Upper
152	100		
115	53.2	40.1	120.2
150	155.7	0.0	347.2

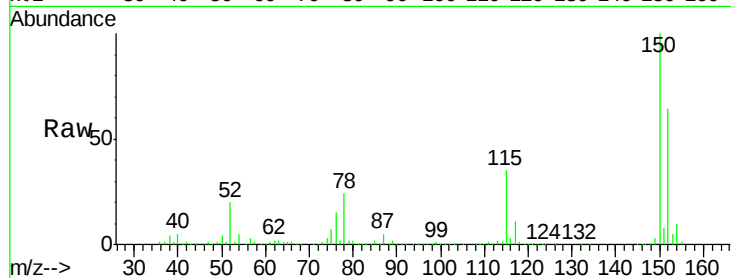

Abundance Ion 151.90 (151.60 to 152.60): V
 Ion 114.90 (114.60 to 115.60): V
 Ion 149.90 (149.60 to 150.60): V

