


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070618\  
Data File : VX003219.D  
Acq On : 06 Jul 2018 16:47  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X062518W.M  
Title : SW846 8260  
Last Update : Mon Jun 25 14:38:05 2018

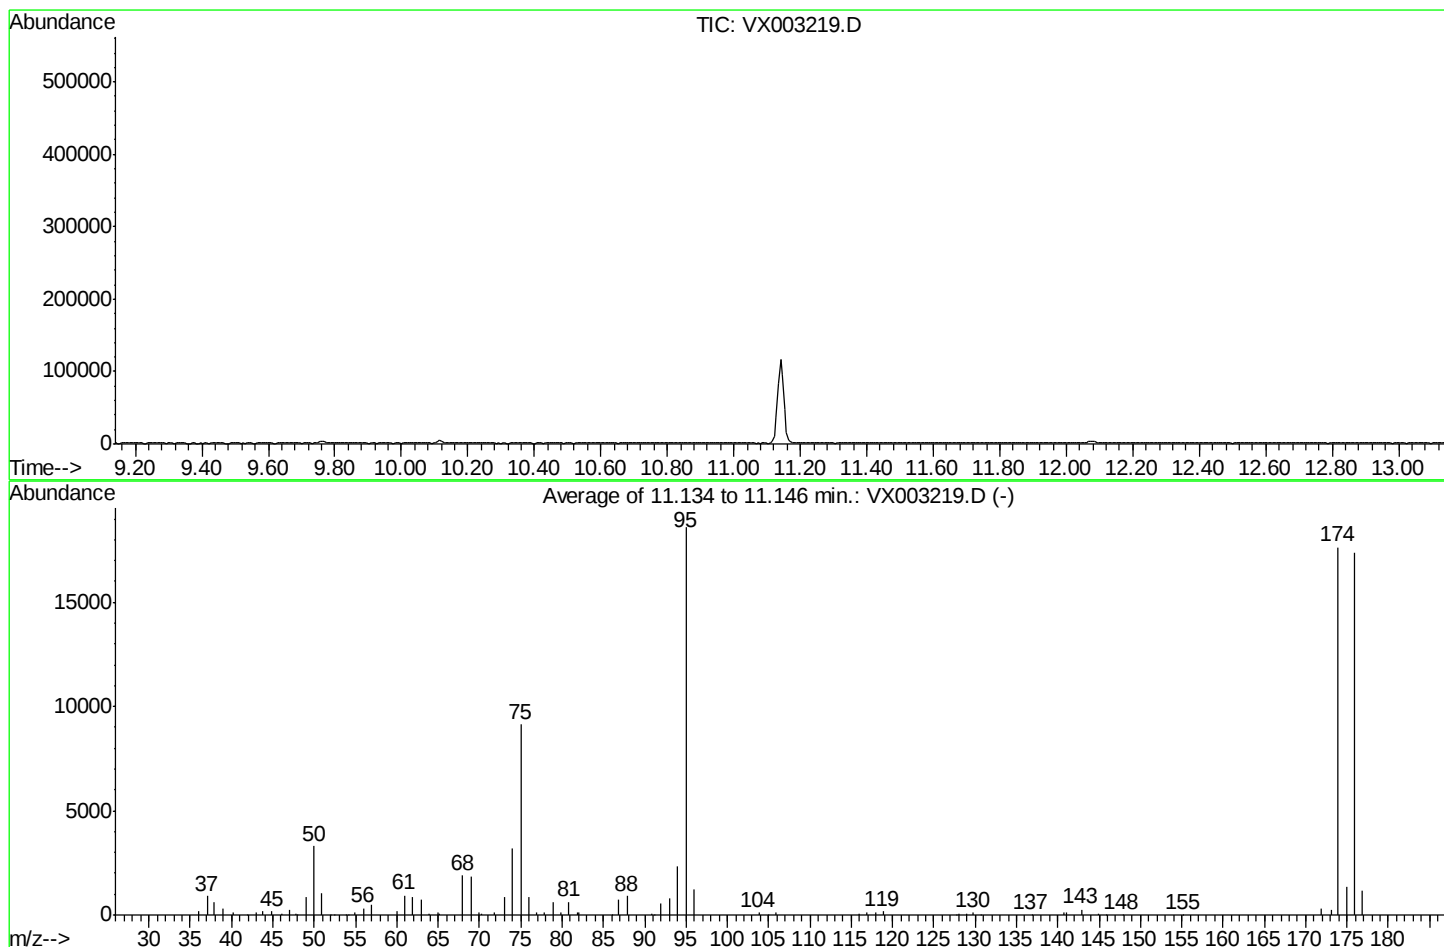

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.8      | 3301    | PASS             |
| 75          | 95           | 30           | 60           | 49.1      | 9132    | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 18592   | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 1201    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.5       | 260     | PASS             |
| 174         | 95           | 50           | 100          | 94.8      | 17630   | PASS             |
| 175         | 174          | 5            | 9            | 7.7       | 1359    | PASS             |
| 176         | 174          | 95           | 101          | 98.7      | 17393   | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 1169    | PASS             |