

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070621\
 Data File : VX023140.D
 Acq On : 06 Jul 2021 12:57
 Operator : JC/MD
 Sample : M2907-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-01-1.5-6.5-063021

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M

Title : SW846 8260

Signal : TIC: VX023140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.142	167	173	181	rBV2	17362	28973	1.15%	0.273%
2	2.331	197	204	210	rBV2	28355	53048	2.11%	0.500%
3	4.501	548	560	572	rBV	148002	410053	16.34%	3.862%
4	5.397	692	707	722	rBV2	170429	492305	19.62%	4.637%
5	5.562	722	734	750	rVB	306915	856774	34.15%	8.069%
6	5.970	790	801	813	rBV	188206	503757	20.08%	4.744%
7	6.769	919	932	948	rBV	465772	1085947	43.29%	10.228%
8	7.135	982	992	1008	rBV	1155772	2508779	100.00%	23.628%
9	8.653	1234	1241	1252	rBV	949915	1446354	57.65%	13.622%
10	9.275	1338	1343	1351	rBV2	16163	25273	1.01%	0.238%
11	10.055	1464	1471	1486	rBV	885578	1232613	49.13%	11.609%
12	11.085	1633	1640	1651	rBV	747209	931185	37.12%	8.770%
13	12.024	1789	1794	1806	rBV	838084	1042668	41.56%	9.820%




Sum of corrected areas: 10617729

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070621\
Data File : VX023140.D
Acq On : 06 Jul 2021 12:57
Operator : JC/MD
Sample : M2907-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01-1.5-6.5-063021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

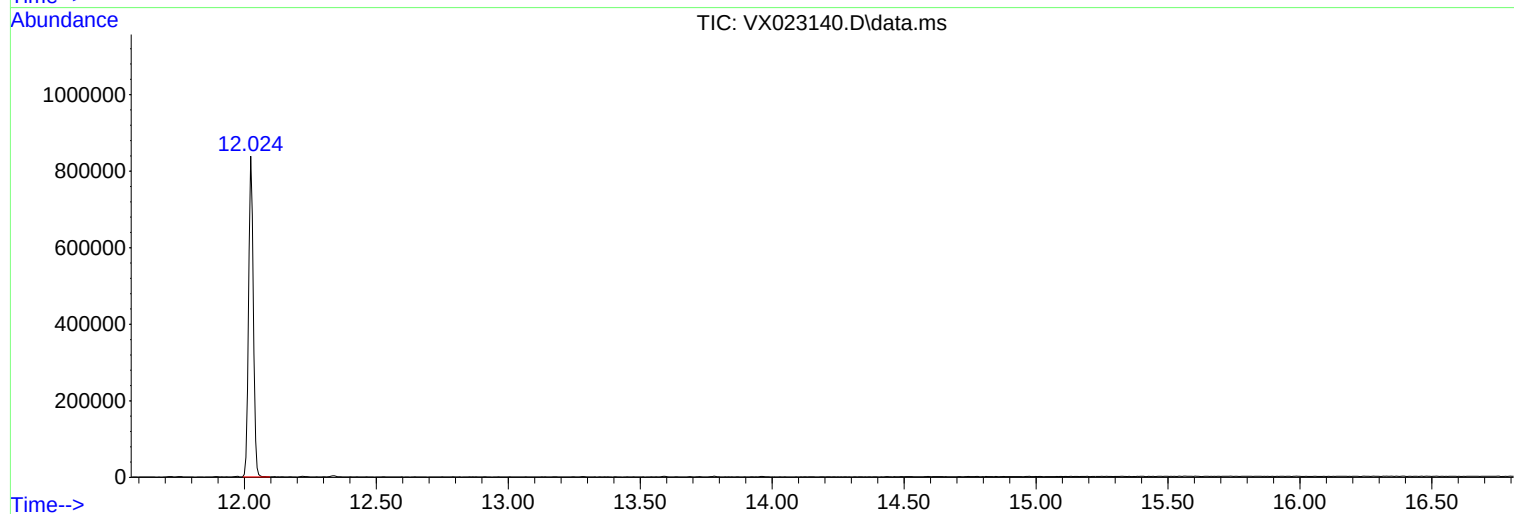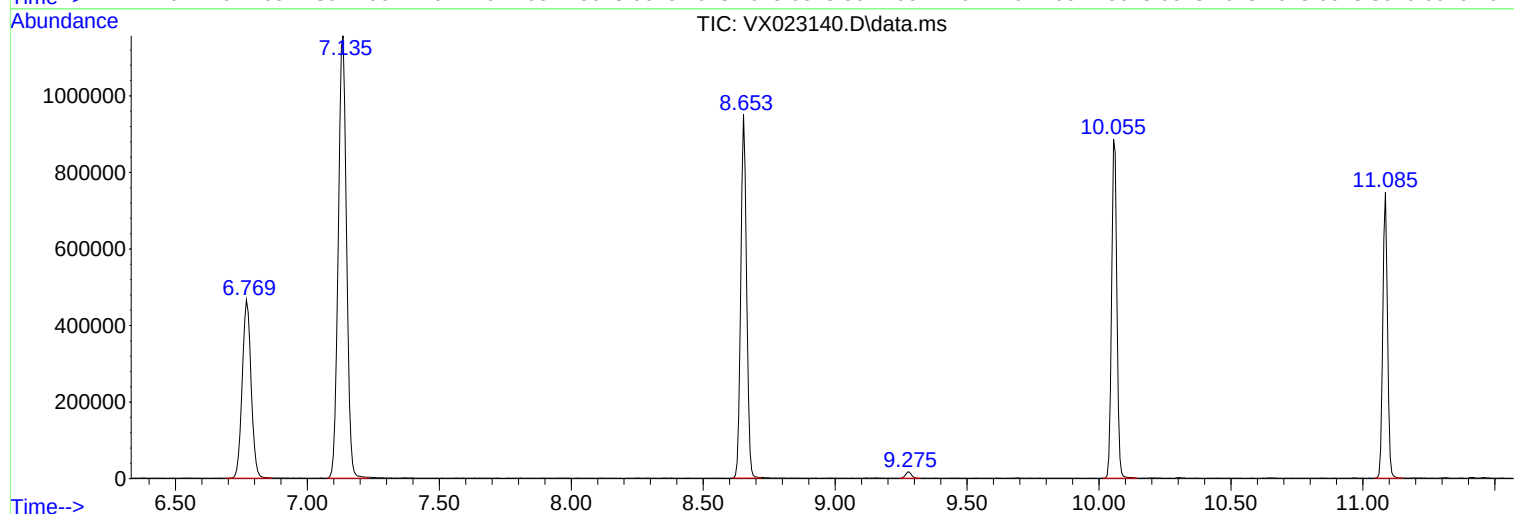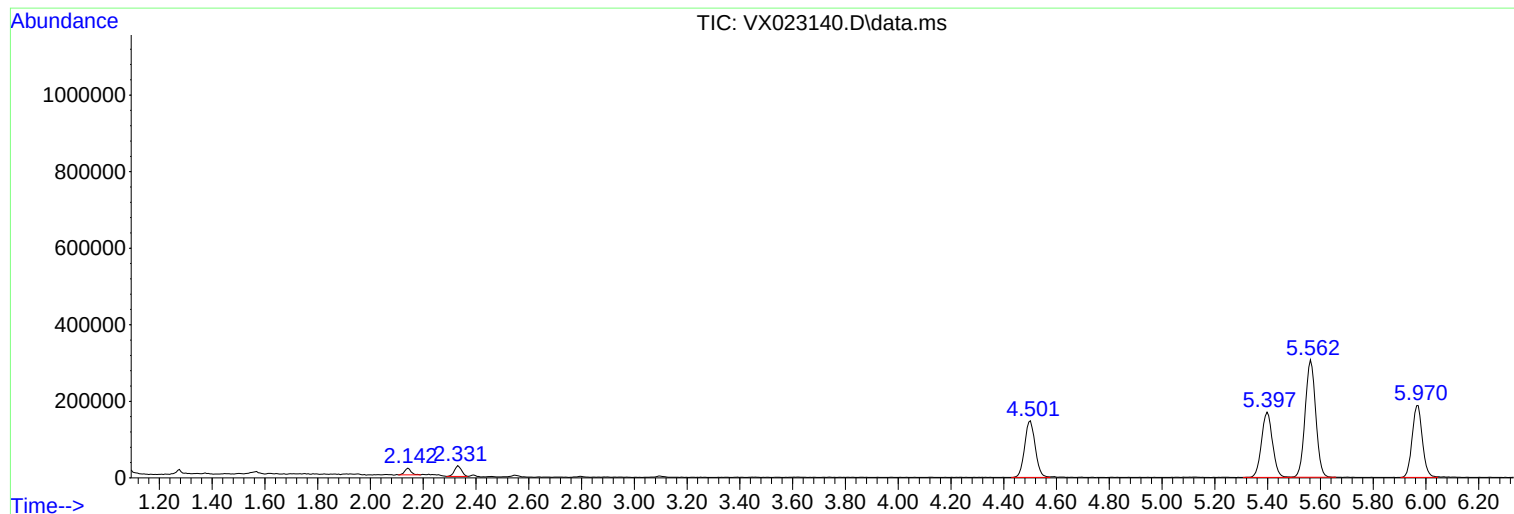

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070621\
Data File : VX023140.D
Acq On : 06 Jul 2021 12:57
Operator : JC/MD
Sample : M2907-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01-1.5-6.5-063021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070621\
Data File : VX023140.D
Acq On : 06 Jul 2021 12:57
Operator : JC/MD
Sample : M2907-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01-1.5-6.5-063021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
