

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070622\
 Data File : VX029936.D
 Acq On : 06 Jul 2022 12:10
 Operator : JC/MD
 Sample : N3591-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OW-01B-64-69-070522

Quant Time: Jul 07 02:33:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 05:54:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	195374	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	335305	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	284588	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	114268	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	106081	42.894	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	85.780%		
35) Dibromofluoromethane	5.391	113	93983	44.850	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.700%		
50) Toluene-d8	8.653	98	375691	47.791	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	95.580%		
62) 4-Bromofluorobenzene	11.085	95	123036	44.277	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	88.560%		
Target Compounds						Qvalue
3) Chloromethane	1.288	50	658	0.300	ug/l #	88
5) Bromomethane	1.611	94	408	0.339	ug/l #	53
6) Chloroethane	1.691	64	294	1.216	ug/l #	41
9) 1,1,2-Trichlorotrifluo...	2.331	101	768	0.392	ug/l	95
10) Methyl Iodide	2.453	142	916	2.202	ug/l	97
12) 1,1-Dichloroethene	2.325	96	451	0.224	ug/l #	76
13) Acrolein	2.239	56	102	Below Cal		97
15) Acrylonitrile	3.075	53	483	0.320	ug/l #	79
16) Acetone	2.386	43	3421	2.827	ug/l	98
17) Carbon Disulfide	2.514	76	1681	0.336	ug/l	96
19) Methyl tert-butyl Ether	3.105	73	1363	0.201	ug/l #	77
20) Methylene Chloride	2.800	84	1020	0.399	ug/l #	67
25) 2-Butanone	4.574	43	429	0.204	ug/l #	88
27) cis-1,2-Dichloroethene	4.501	96	860	0.330	ug/l	98
30) Chloroform	5.105	83	1067	0.275	ug/l #	66
31) Cyclohexane	5.556	56	4004	1.161	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	14297	5.130	ug/l #	48
38) Carbon Tetrachloride	5.556	117	18193	7.533	ug/l #	18
44) Trichloroethene	7.129	130	9097	3.748	ug/l	94
49) 1,4-Dioxane	7.927	88	21	0.326	ug/l #	25
51) 4-Methyl-2-Pentanone	8.573	43	1325	0.350	ug/l #	75
60) Dibromochloromethane	9.275	129	1988	0.950	ug/l #	14
64) Tetrachloroethene	9.281	164	1995	1.162	ug/l	93
76) 1,2,3-Trichloropropane	11.085	75	56885	20.796	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	56885	66.042	ug/l #	13
89) n-Butylbenzene	12.341	91	1341	0.209	ug/l	83
93) 1,2,4-Trichlorobenzene	13.597	180	646	0.284	ug/l	91
94) Hexachlorobutadiene	13.731	225	340	0.404	ug/l	90
95) Naphthalene	13.780	128	2070	0.224	ug/l #	90
96) 1,2,3-Trichlorobenzene	13.969	180	636	0.273	ug/l	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070622\
Data File : VX029936.D
Acq On : 06 Jul 2022 12:10
Operator : JC/MD
Sample : N3591-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522

Quant Time: Jul 07 02:33:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 05:54:51 2022
Response via : Initial Calibration




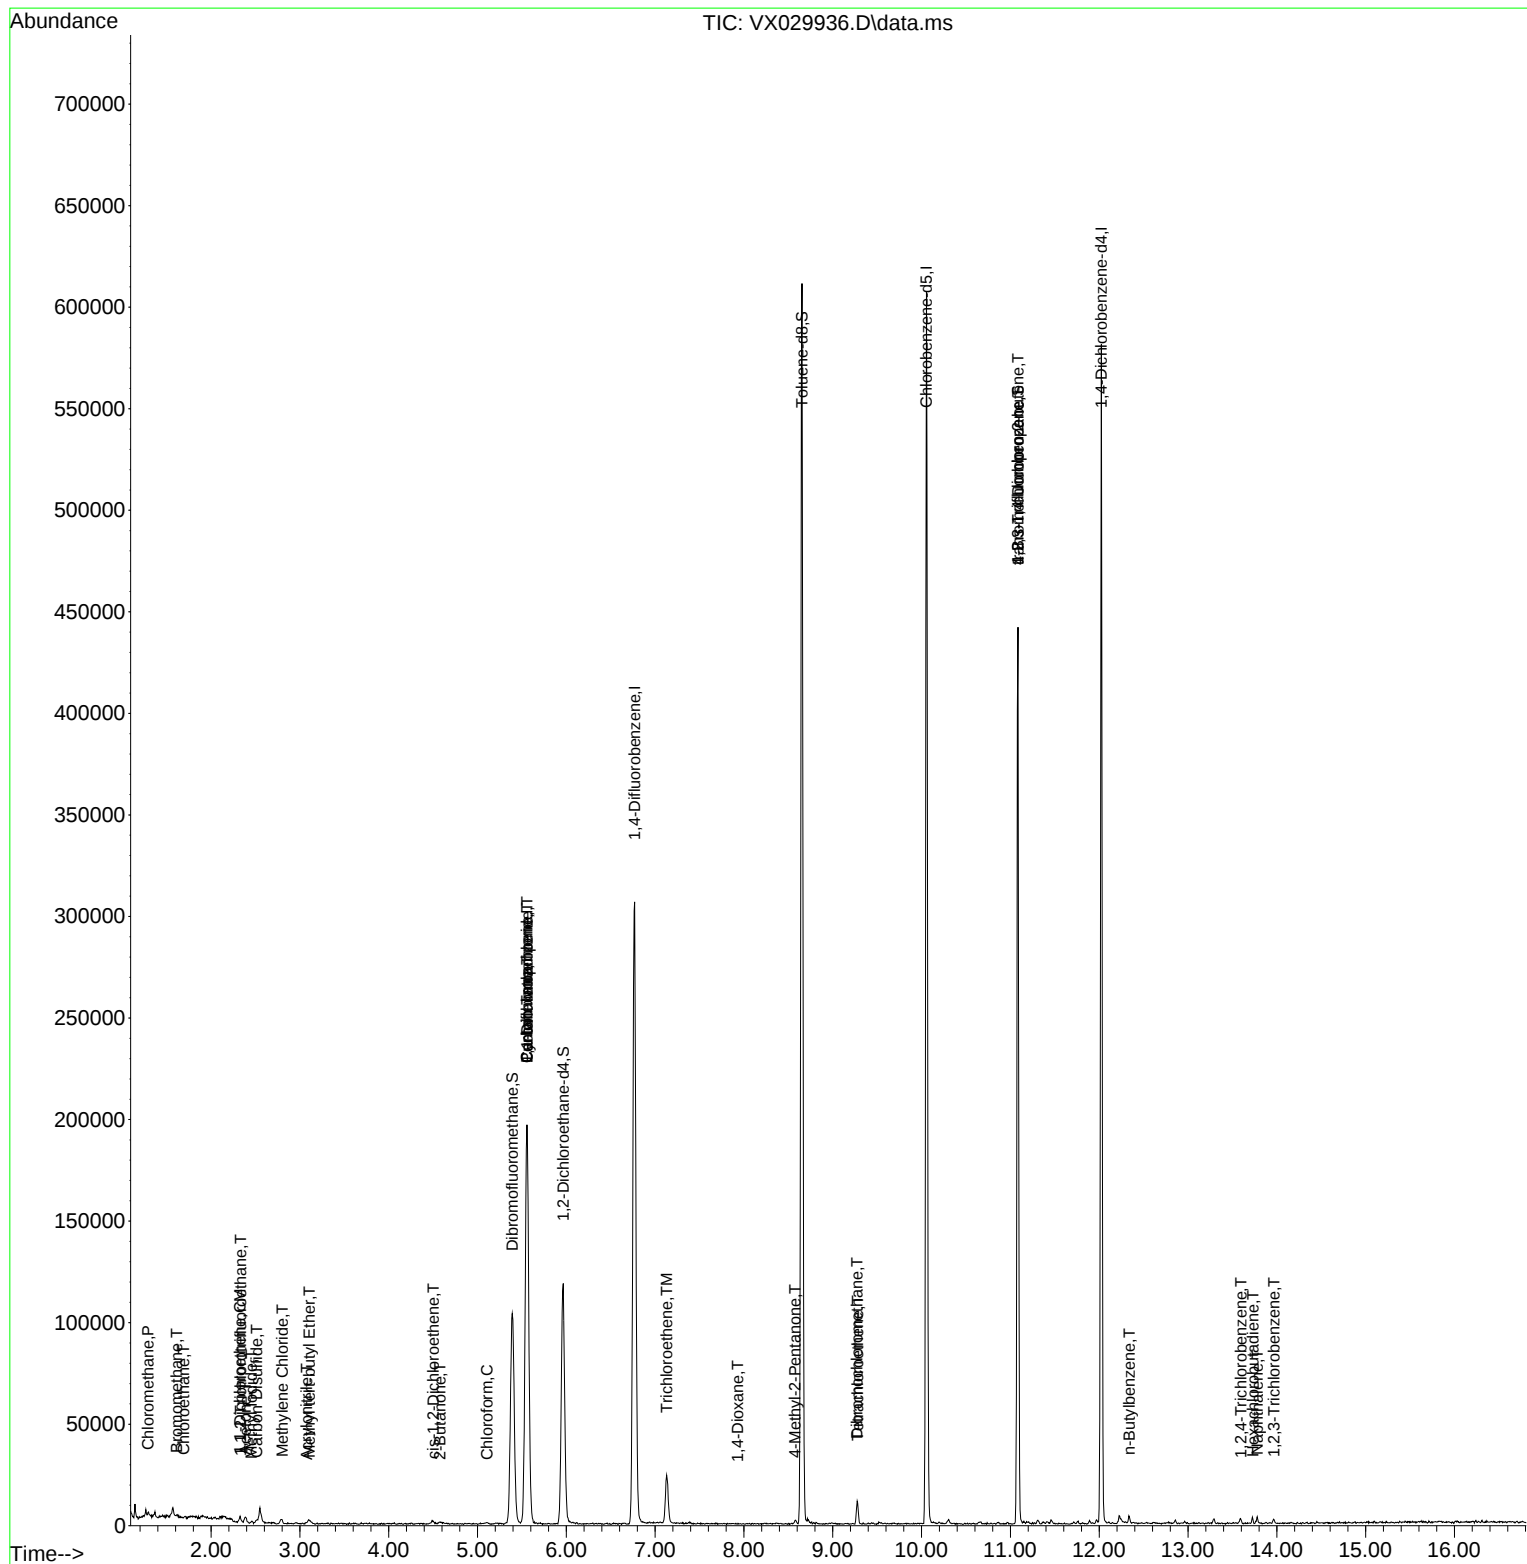




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion:168 Resp: 195374
Ion Ratio Lower Upper
168 100
99 56.4 44.0 66.0

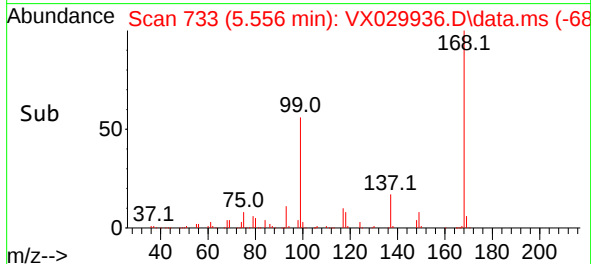

#3
Chloromethane
Concen: 0.300 ug/l
RT: 1.288 min Scan# 33
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 50 Resp: 658
Ion Ratio Lower Upper
50 100
52 39.7 26.3 39.5




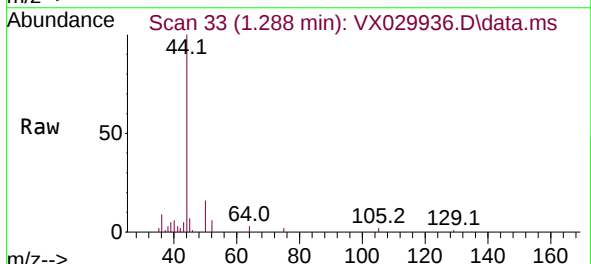


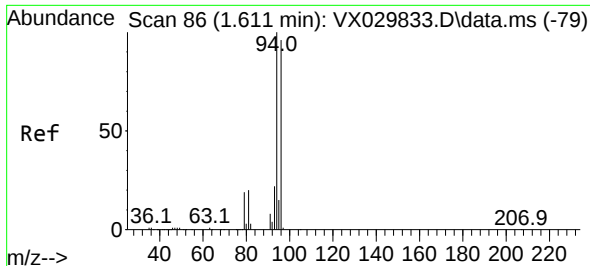

#5
Bromomethane
Concen: 0.339 ug/l
RT: 1.611 min Scan# 86
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion: 94 Resp: 408
Ion Ratio Lower Upper
94 100
96 141.7 76.9 115.3#

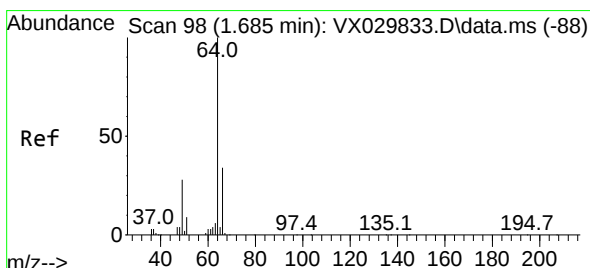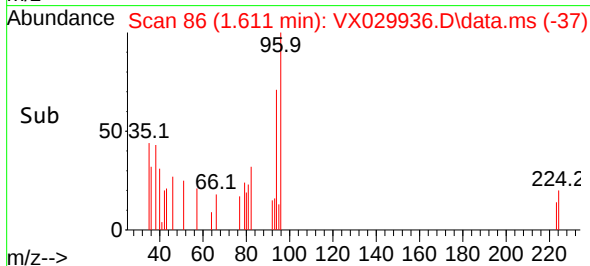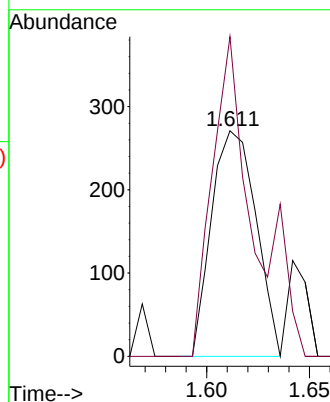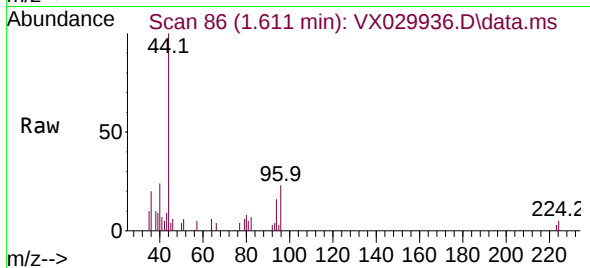

#6
Chloroethane
Concen: 1.216 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 64 Resp: 294
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#


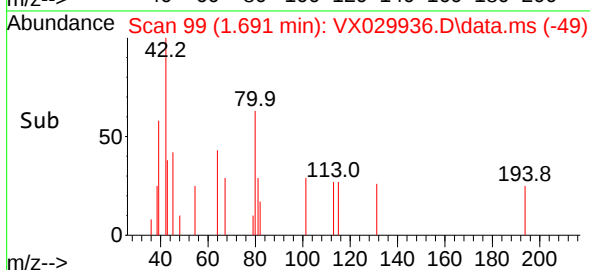

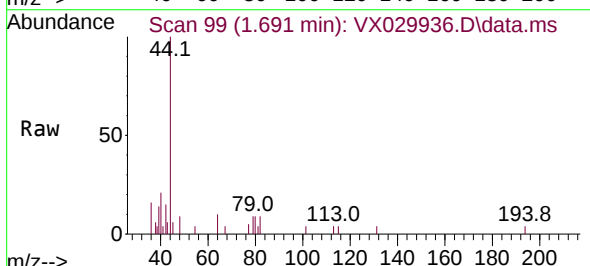


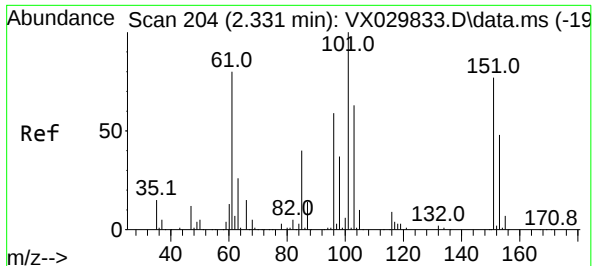

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.392 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion:	101	Resp:	768
Ion	Ratio	Lower	Upper
101	100		
85	44.1	34.0	51.0
151	79.3	59.4	89.0

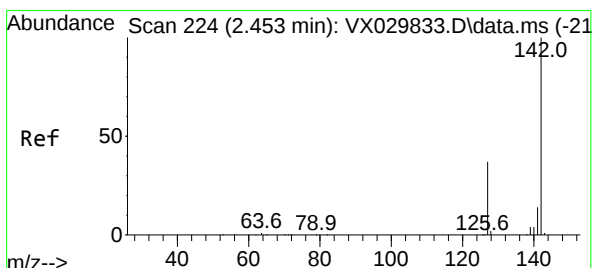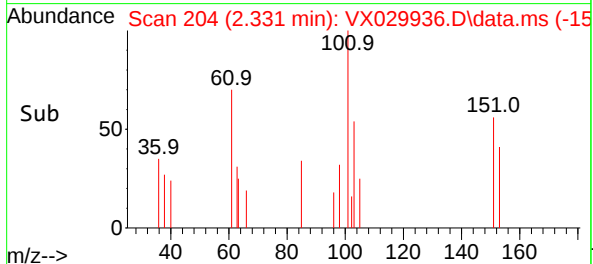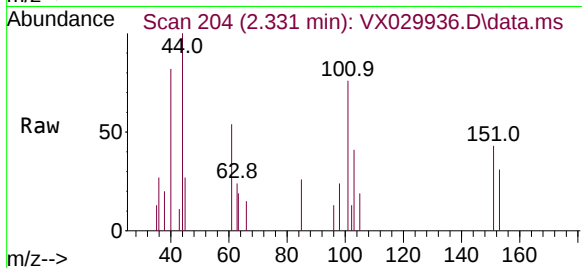

#10
Methyl Iodide
Concen: 2.202 ug/l
RT: 2.453 min Scan# 224
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion:	142	Resp:	916
Ion	Ratio	Lower	Upper
142	100		
127	39.4	30.2	45.2
141	13.1	11.3	16.9

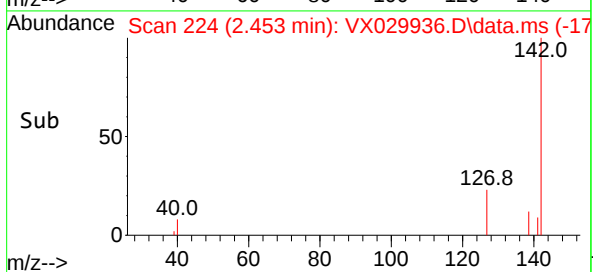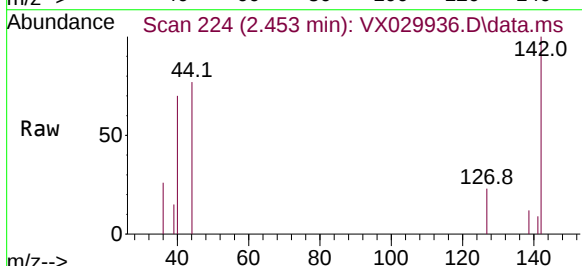

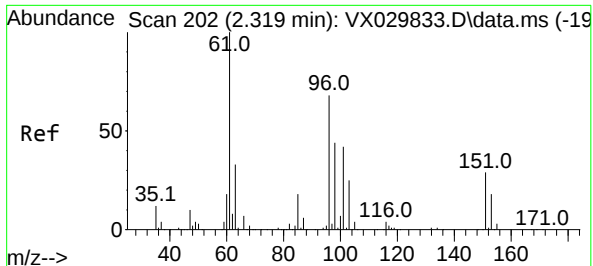

#12

1,1-Dichloroethene

Concen: 0.224 ug/l

RT: 2.325 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX029936.D

Acq: 06 Jul 2022 12:10

Instrument :

MSVOA_X

ClientSampleId :

OW-01B-64-69-070522





Tgt Ion: 96 Resp: 451

Ion Ratio Lower Upper

96 100

61 110.7 117.4 176.0#

98 53.6 52.2 78.4

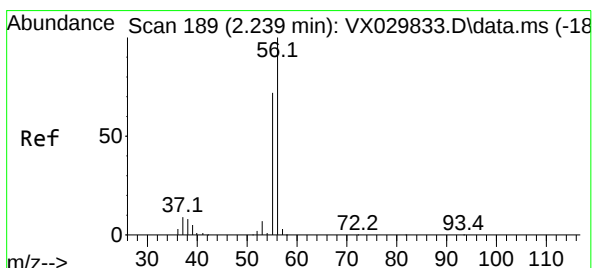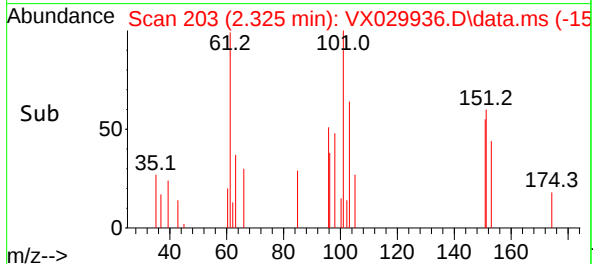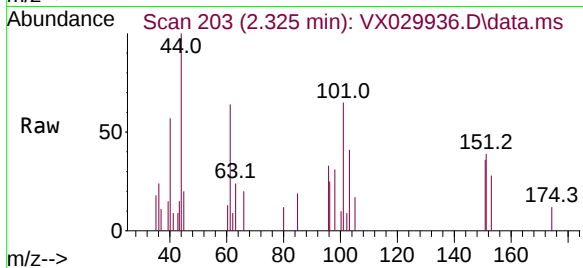

#13

Acrolein

Concen: Below Cal

RT: 2.239 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX029936.D




Acq: 06 Jul 2022 12:10


Tgt Ion: 56 Resp: 102

Ion Ratio Lower Upper

56 100

55 68.6 56.6 84.8


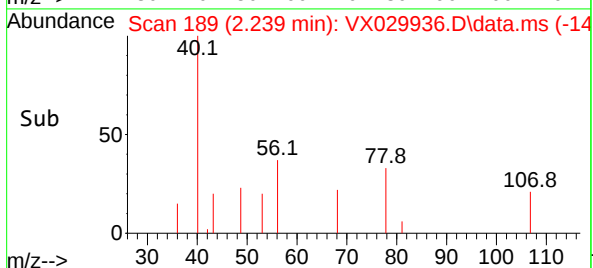

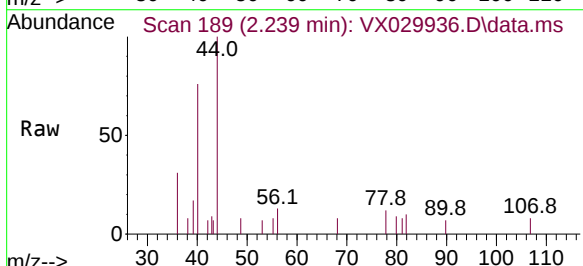




#15
Acrylonitrile
Concen: 0.320 ug/l
RT: 3.075 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion: 53 Resp: 483
Ion Ratio Lower Upper
53 100
52 96.5 65.4 98.0
51 16.8 27.7 41.5#

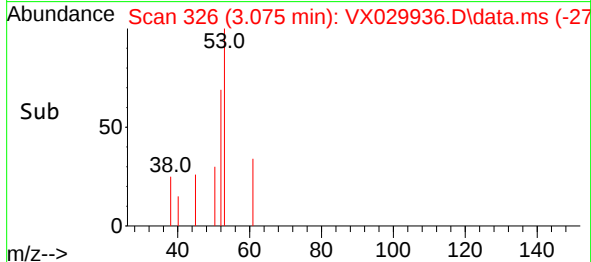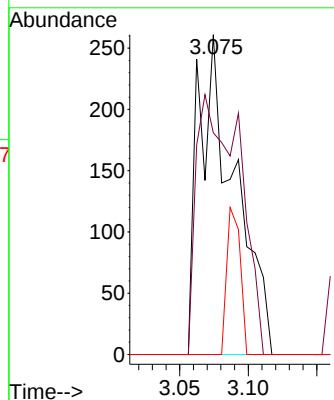

#16
Acetone
Concen: 2.827 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 43 Resp: 3421
Ion Ratio Lower Upper
43 100
58 33.2 27.7 41.5

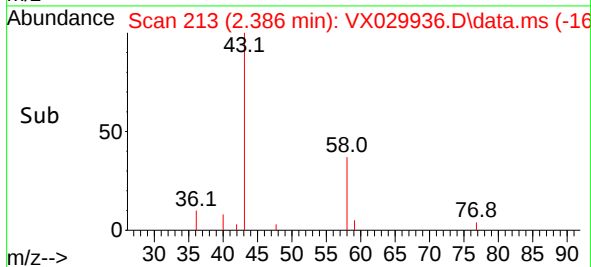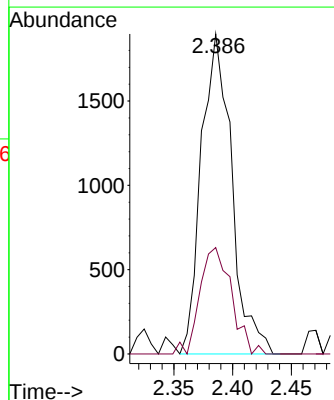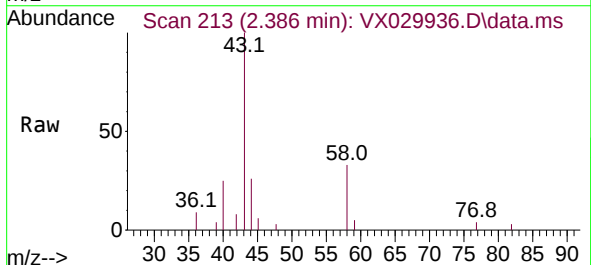



#17

Carbon Disulfide

Concen: 0.336 ug/l

RT: 2.514 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX029936.D


Acq: 06 Jul 2022 12:10

Instrument :

MSVOA_X

ClientSampleId :

OW-01B-64-69-070522






Tgt Ion: 76 Resp: 1681

Ion Ratio Lower Upper

76 100

78 11.3 7.8 11.6



#19

Methyl tert-butyl Ether

Concen: 0.201 ug/l

RT: 3.105 min Scan# 331

Delta R.T. -0.012 min

Lab File: VX029936.D




Acq: 06 Jul 2022 12:10


Tgt Ion: 73 Resp: 1363

Ion Ratio Lower Upper

73 100

57 12.6 19.0 28.6#


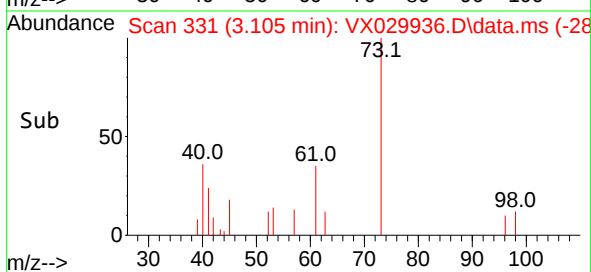






#20
Methylene Chloride
Concen: 0.399 ug/l
RT: 2.800 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion: 84	Resp: 1020
Ion Ratio	Lower Upper
84	100
49	58.3 93.8 140.6#
51	27.3 29.4 44.0#
86	67.5 51.0 76.4

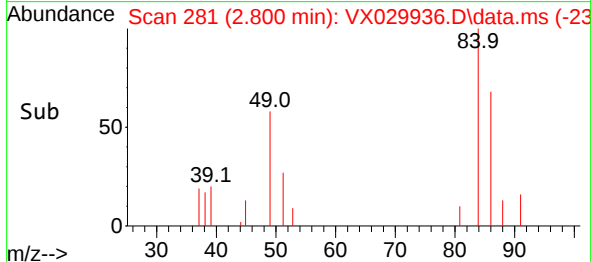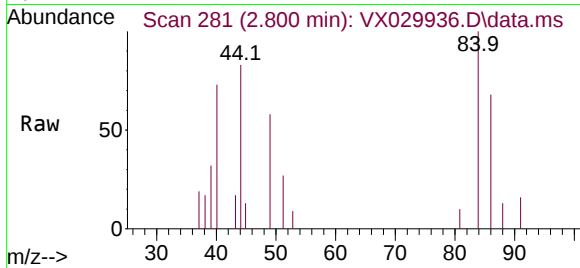

#25
2-Butanone
Concen: 0.204 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 43	Resp: 429
Ion Ratio	Lower Upper
43	100
72	20.7 21.7 32.5#

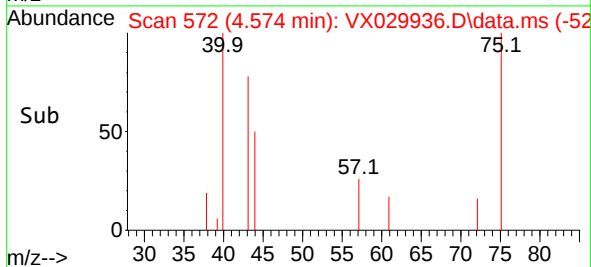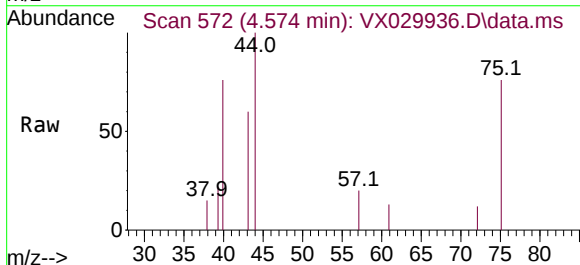



#27

cis-1,2-Dichloroethene

Concen: 0.330 ug/l

RT: 4.501 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX029936.D

Acq: 06 Jul 2022 12:10

Instrument :

MSVOA_X

ClientSampleId :

OW-01B-64-69-070522





Tgt Ion: 96 Resp: 860

Ion Ratio Lower Upper

96 100

61 136.5 0.0 270.0

98 67.7 0.0 127.8

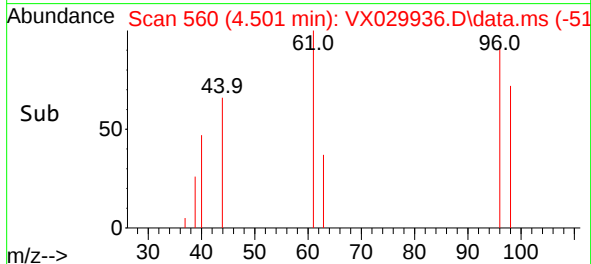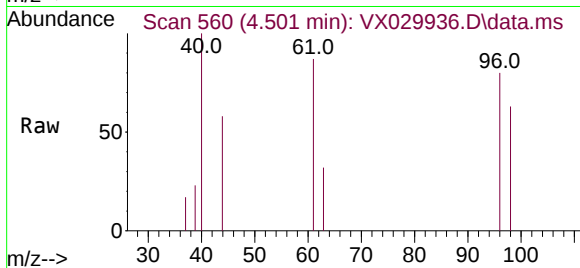

#30

Chloroform

Concen: 0.275 ug/l

RT: 5.105 min Scan# 659

Delta R.T. -0.000 min

Lab File: VX029936.D




Acq: 06 Jul 2022 12:10


Tgt Ion: 83 Resp: 1067

Ion Ratio Lower Upper

83 100


85 37.9 51.5 77.3#

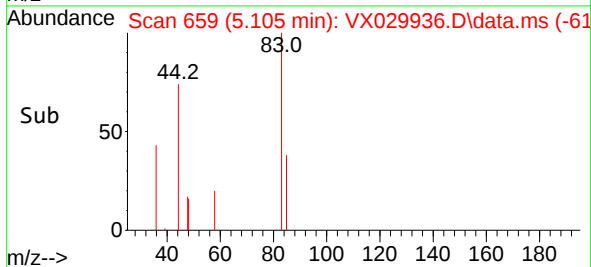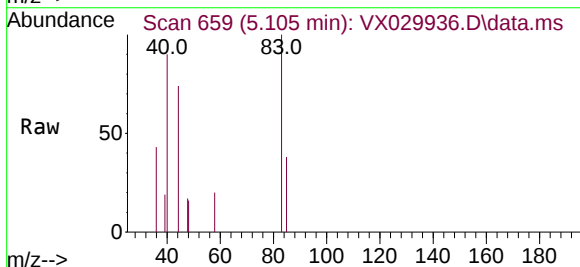






#31
Cyclohexane
Concen: 1.161 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.085 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522







Tgt Ion: 56 Resp: 4004
Ion Ratio Lower Upper
56 100
69 179.3 25.4 38.0#
84 185.2 68.9 103.3#

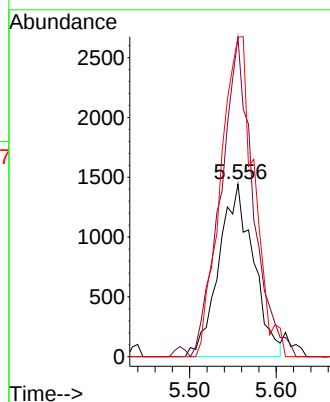

#33
1,2-Dichloroethane-d4
Concen: 42.894 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 65 Resp: 106081
Ion Ratio Lower Upper
65 100
67 54.4 0.0 109.6



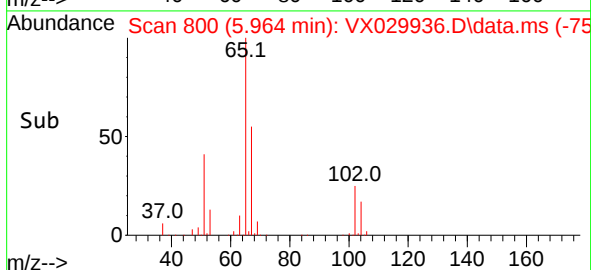
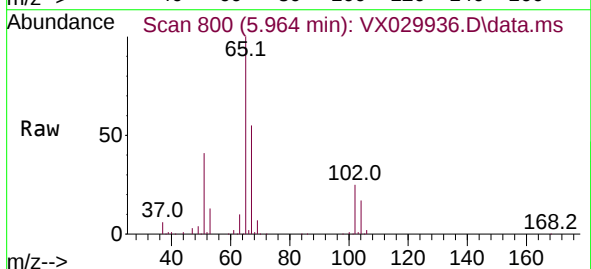


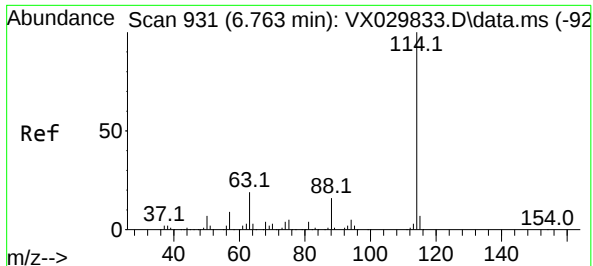

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion:114 Resp: 335305
Ion Ratio Lower Upper
114 100
63 17.8 0.0 38.4
88 14.8 0.0 31.8

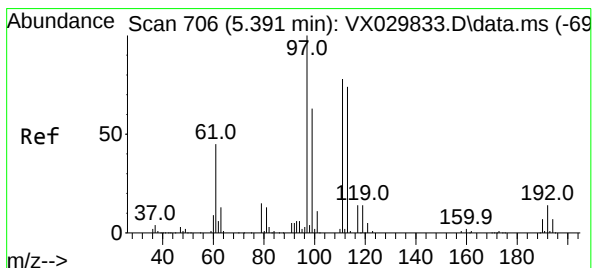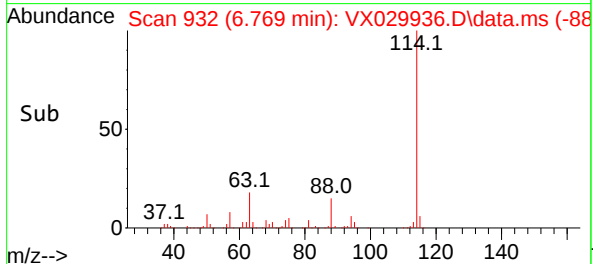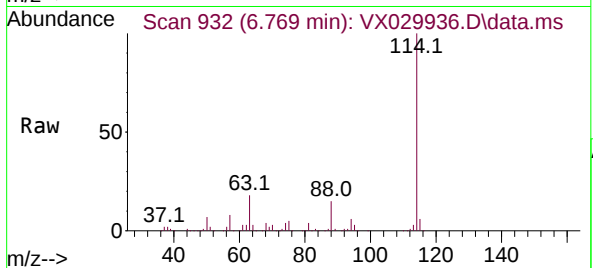

#35
Dibromofluoromethane
Concen: 44.850 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion:113 Resp: 93983
Ion Ratio Lower Upper
113 100
111 105.4 83.2 124.8
192 19.5 14.8 22.2

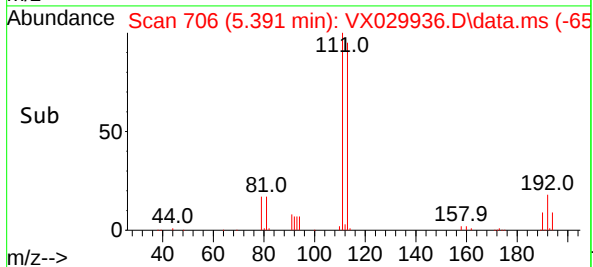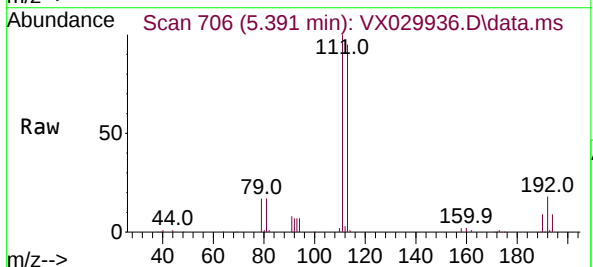



#36

1,1-Dichloropropene

Concen: 5.130 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.140 min

Lab File: VX029936.D


Acq: 06 Jul 2022 12:10

Instrument :

MSVOA_X

ClientSampleId :

OW-01B-64-69-070522






Tgt Ion: 75 Resp: 14297

Ion Ratio Lower Upper

75 100

110 9.0 19.3 57.9#

77 0.3 24.4 36.6#

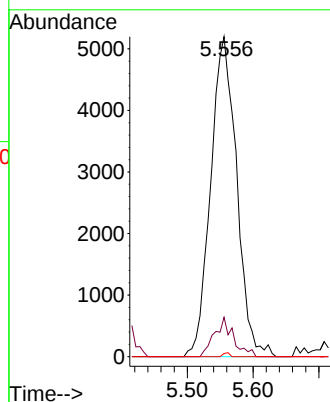

#38

Carbon Tetrachloride

Concen: 7.533 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX029936.D

Acq: 06 Jul 2022 12:10




Tgt Ion: 117 Resp: 18193


Ion Ratio Lower Upper

117 100

119 5.5 74.1 111.1#

121 0.0 25.8 38.8#


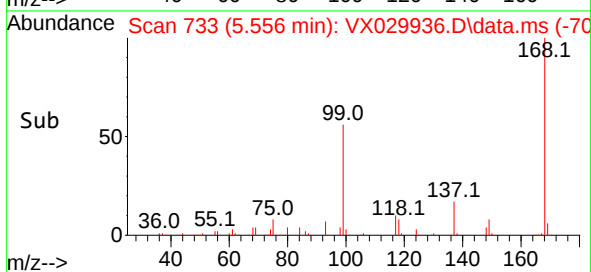
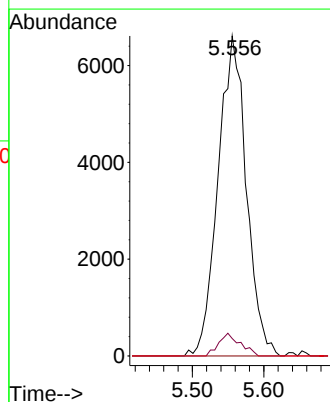





#44
Trichloroethene
Concen: 3.748 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion:130 Resp: 9097
Ion Ratio Lower Upper
130 100
95 102.9 0.0 194.8

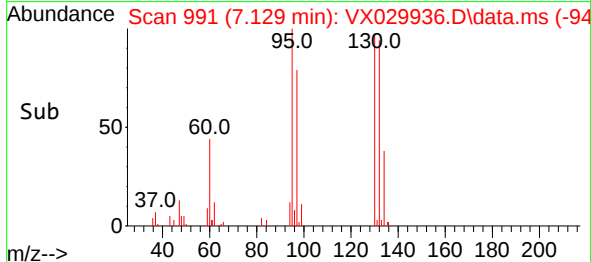

#49
1,4-Dioxane
Concen: 0.326 ug/l
RT: 7.927 min Scan# 1122
Delta R.T. 0.244 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 88 Resp: 21
Ion Ratio Lower Upper
88 100
43 0.0 23.8 35.8#
58 0.0 53.8 80.6#


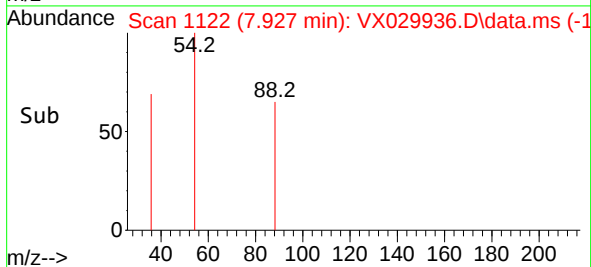

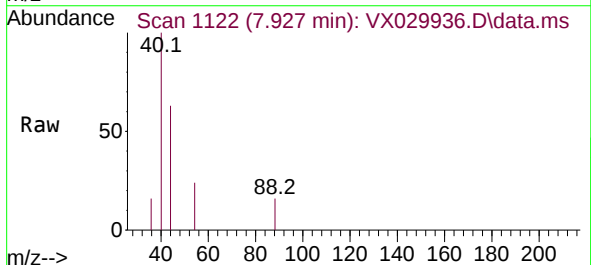




#50
Toluene-d8
Concen: 47.791 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion: 98 Resp: 375691
Ion Ratio Lower Upper
98 100
100 66.4 52.3 78.5

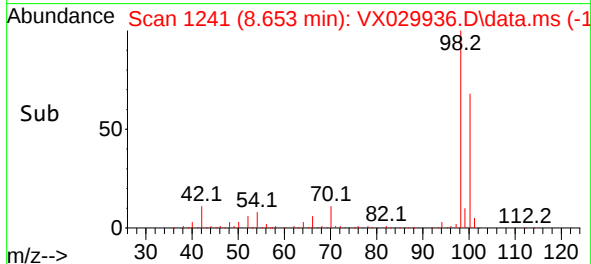

#51
4-Methyl-2-Pentanone
Concen: 0.350 ug/l
RT: 8.573 min Scan# 1228
Delta R.T. -0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 43 Resp: 1325
Ion Ratio Lower Upper
43 100
58 23.8 31.4 47.2#


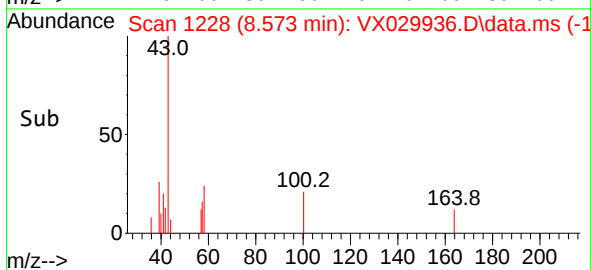

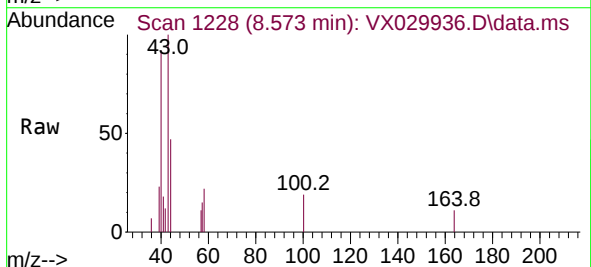


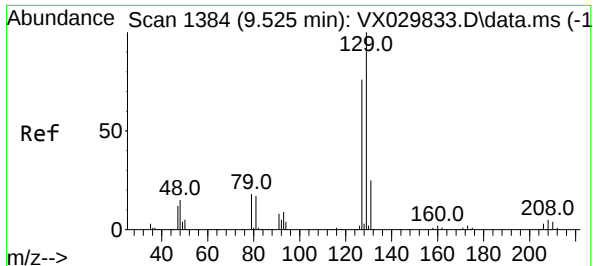

#60
Dibromochloromethane
Concen: 0.950 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.250 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion:129 Resp: 1988
Ion Ratio Lower Upper
129 100
127 2.4 38.5 115.5#

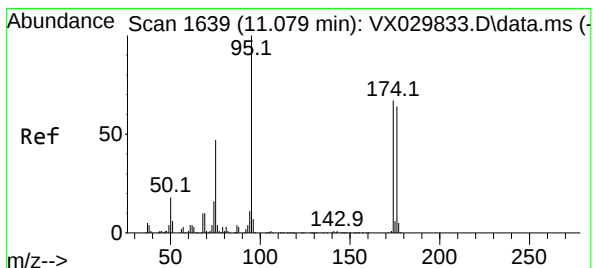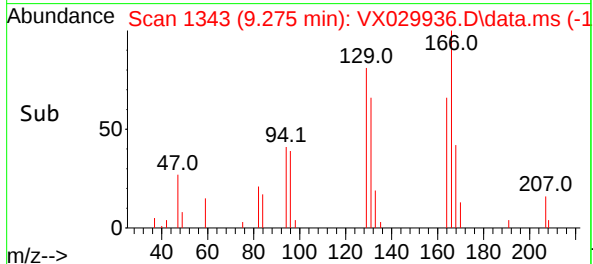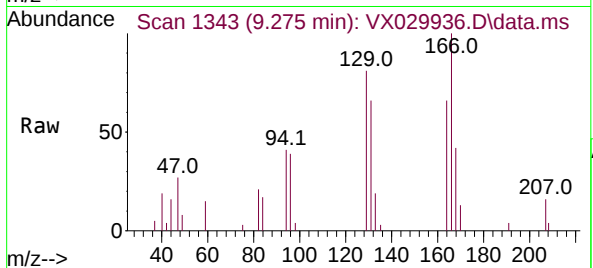

#62
4-Bromofluorobenzene
Concen: 44.277 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 95 Resp: 123036
Ion Ratio Lower Upper
95 100
174 75.9 0.0 149.0
176 72.7 0.0 146.0


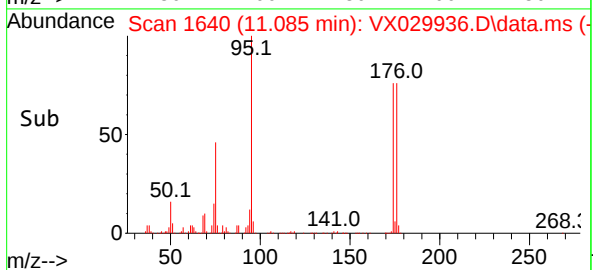

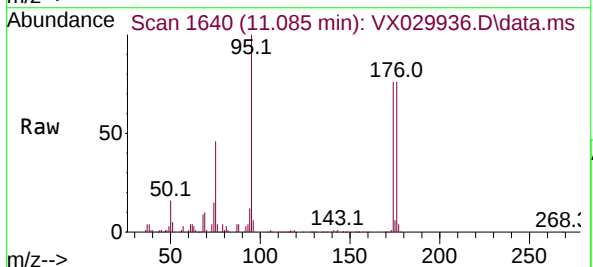




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion:117 Resp: 284588
Ion Ratio Lower Upper
117 100
82 52.8 42.7 64.1
119 30.8 25.4 38.2

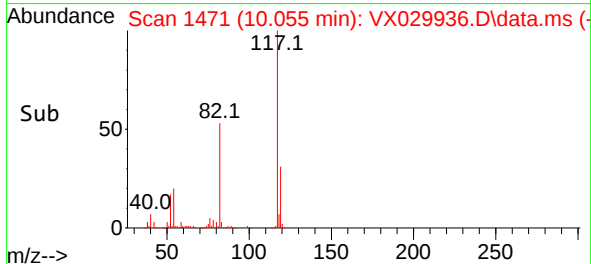

#64
Tetrachloroethene
Concen: 1.162 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. 0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion:164 Resp: 1995
Ion Ratio Lower Upper
164 100
166 121.9 98.2 147.4
129 86.6 80.8 121.2
131 101.5 75.5 113.3

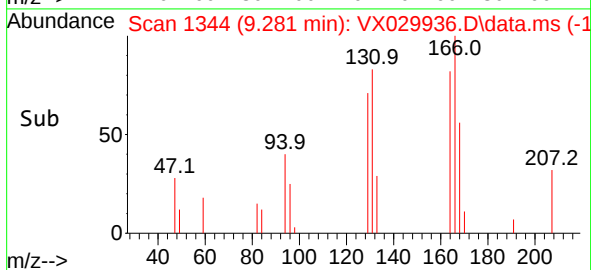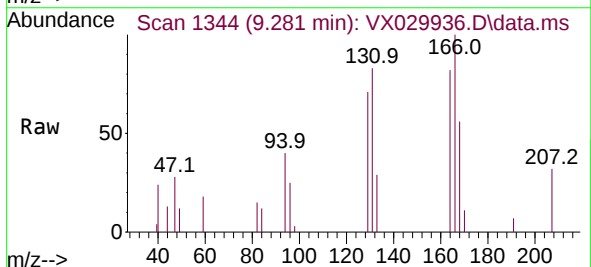



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX029936.D

Acq: 06 Jul 2022 12:10

Instrument :

MSVOA_X

ClientSampleId :

OW-01B-64-69-070522





Tgt Ion:152 Resp: 114268

Ion Ratio Lower Upper

152 100

115 61.3 40.5 121.5

150 160.5 0.0 347.0

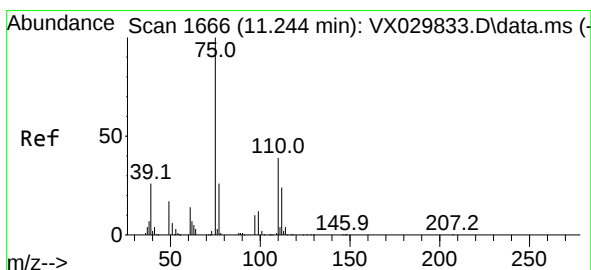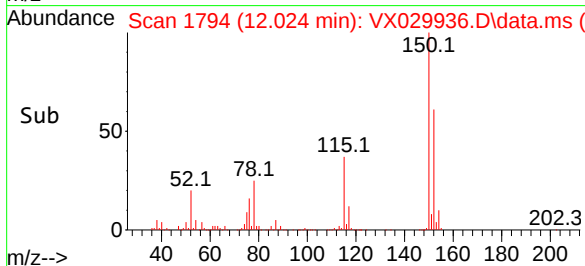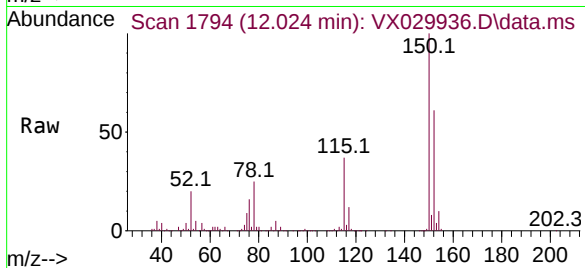

#76

1,2,3-Trichloropropane

Concen: 20.796 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.159 min

Lab File: VX029936.D




Acq: 06 Jul 2022 12:10


Tgt Ion: 75 Resp: 56885

Ion Ratio Lower Upper

75 100

77 1.3 19.8 59.3#


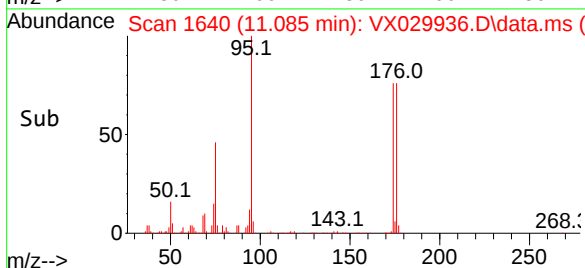

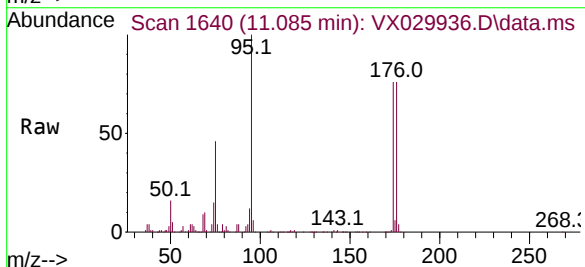




#81
trans-1,4-Dichloro-2-butene
Concen: 66.042 ug/l
RT: 11.085 min Scan# 11085
Delta R.T. 0.067 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10




Instrument :
MSVOA_X
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion: 75 Resp: 56885
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.1 34.8 52.2#

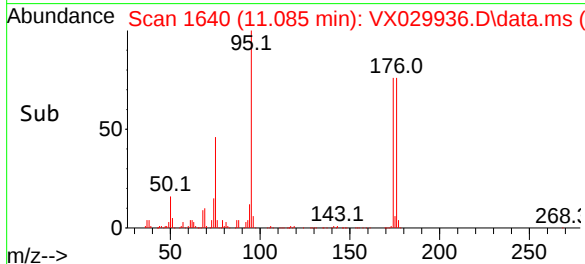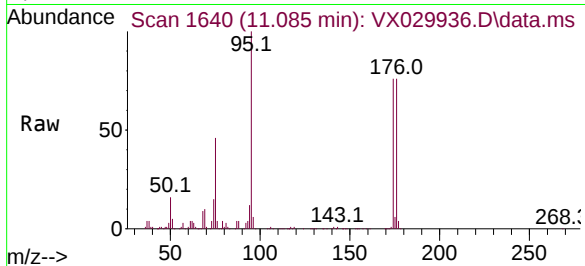

#89
n-Butylbenzene
Concen: 0.209 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VX029936.D
Acq: 06 Jul 2022 12:10

Tgt Ion: 91 Resp: 1341
Ion Ratio Lower Upper
91 100
92 40.6 26.2 78.5
134 16.3 12.6 37.8

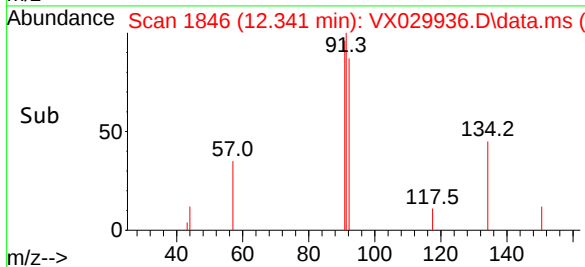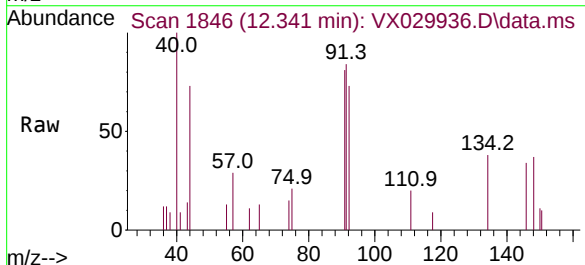



#93

1,2,4-Trichlorobenzene

Concen: 0.284 ug/l

RT: 13.597 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX029936.D

Acq: 06 Jul 2022 12:10

Instrument :

MSVOA_X

ClientSampleId :

OW-01B-64-69-070522





Tgt Ion:180 Resp: 646

Ion Ratio Lower Upper

180 100

182 89.3 48.2 144.6

145 40.4 15.9 47.6

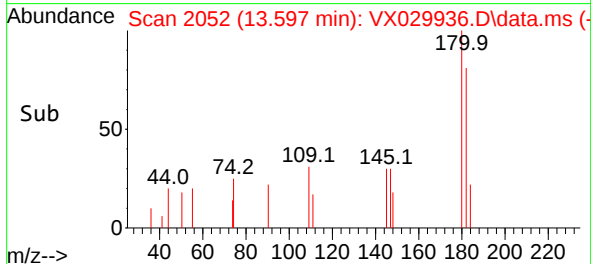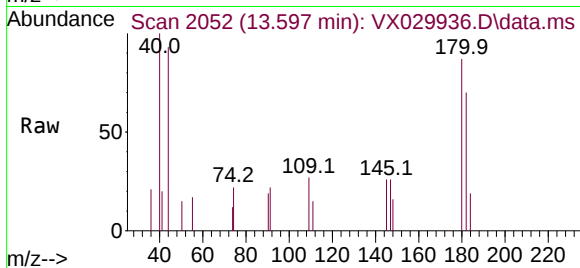

#94

Hexachlorobutadiene

Concen: 0.404 ug/l

RT: 13.731 min Scan# 2074

Delta R.T. 0.006 min

Lab File: VX029936.D

Acq: 06 Jul 2022 12:10




Tgt Ion:225 Resp: 340


Ion Ratio Lower Upper

225 100

223 72.6 30.6 91.6

227 67.9 31.9 95.9

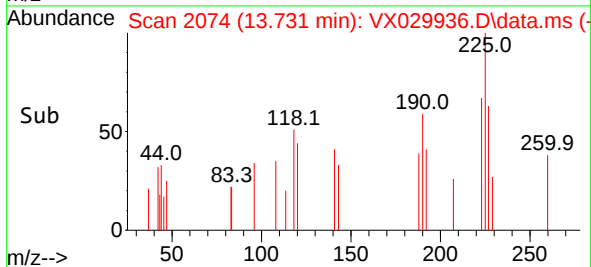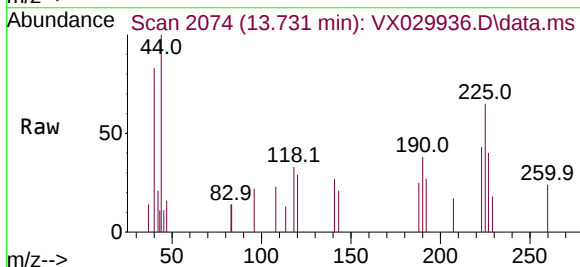



#95

Naphthalene

Concen: 0.224 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. -0.000 min

Lab File: VX029936.D

Acq: 06 Jul 2022 12:10

Instrument :

MSVOA_X

ClientSampleId :

OW-01B-64-69-070522





Tgt Ion:128 Resp: 2070

Ion Ratio Lower Upper

128 100

127 10.0 10.2 15.2#

129 15.9 8.6 13.0#

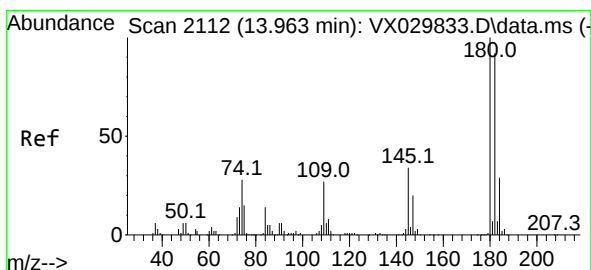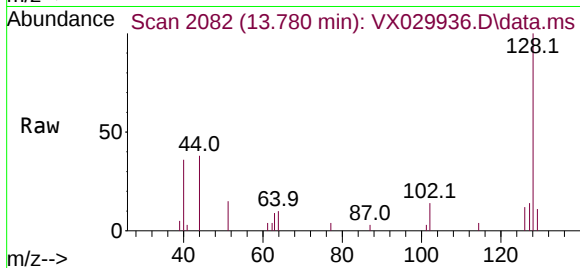

#96

1,2,3-Trichlorobenzene

Concen: 0.273 ug/l

RT: 13.969 min Scan# 2113

Delta R.T. 0.006 min

Lab File: VX029936.D

Acq: 06 Jul 2022 12:10

Tgt Ion:180 Resp: 636

Ion Ratio Lower Upper

180 100

182 94.8 47.0 141.0

145 23.9 17.0 50.9

