
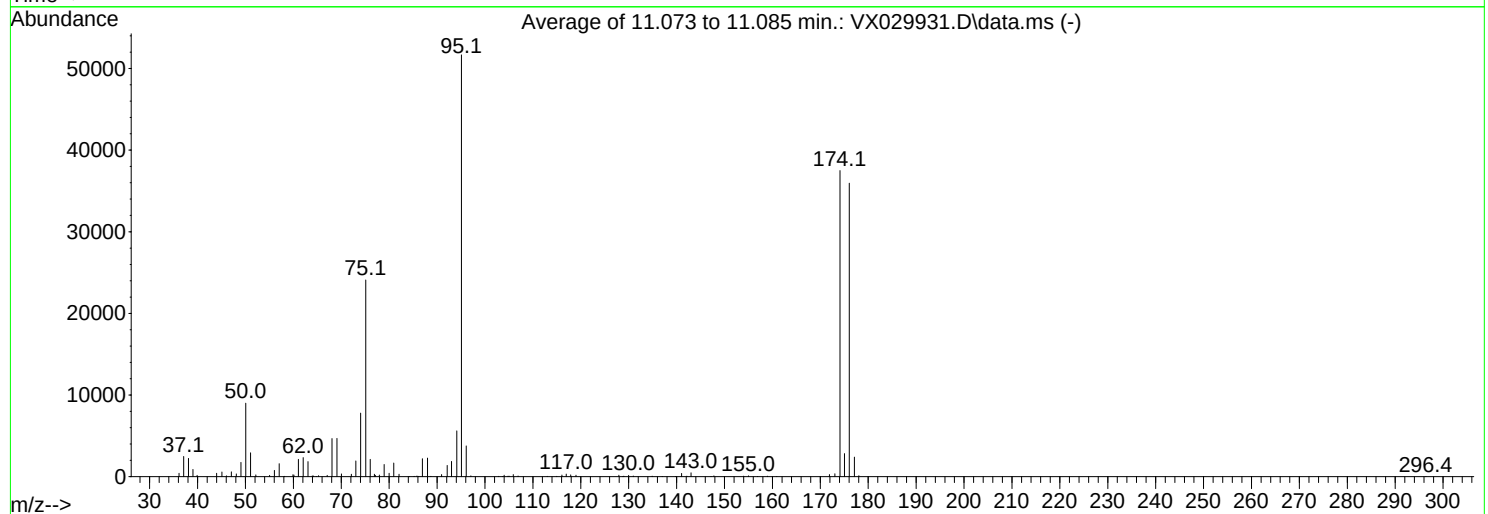


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070622\
Data File : VX029931.D
Acq On : 06 Jul 2022 08:34
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 05:54:51 2022

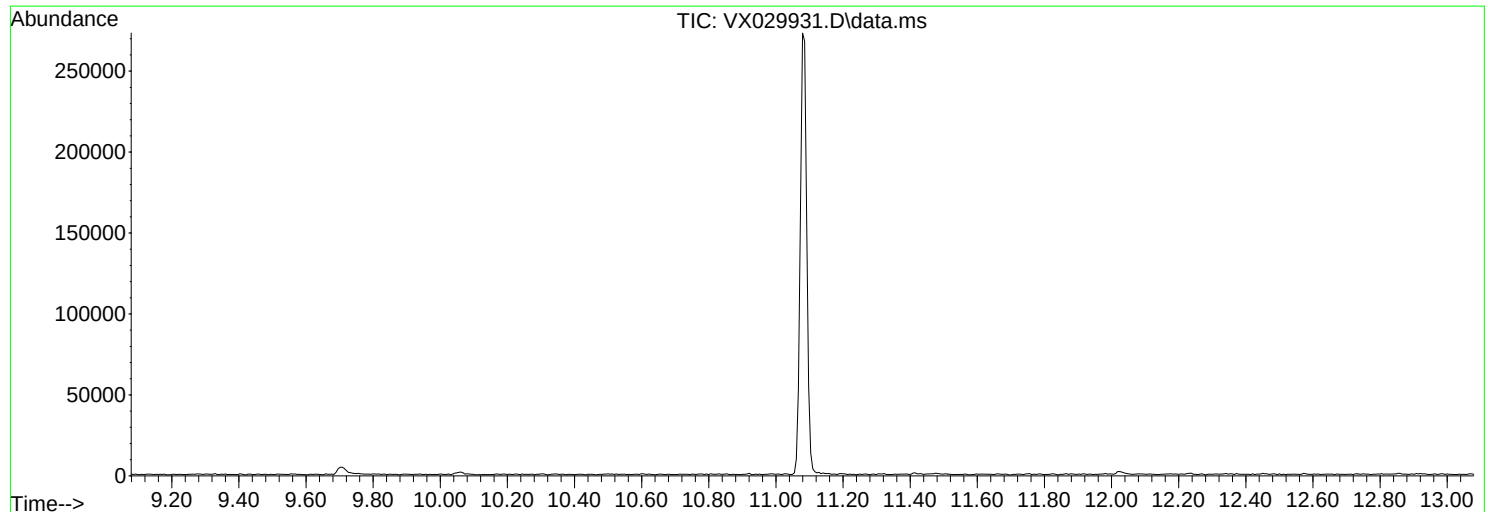

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	9003	PASS
75	95	30	60	46.6	24091	PASS
95	95	100	100	100.0	51672	PASS
96	95	5	9	7.3	3763	PASS
173	174	0.00	2	0.9	352	PASS
174	95	50	100	72.6	37501	PASS
175	174	5	9	7.5	2826	PASS
176	174	95	101	95.9	35952	PASS
177	176	5	9	6.6	2389	PASS