

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070623\
Data File : VX036427.D
Acq On : 06 Jul 2023 11:55
Operator : JC/MD
Sample : 03500-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-060923

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M

Title : SW846 8260

Signal : TIC: VX036427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.648	84	92	93	rBV5	5191	10431	1.19%	0.223%
2	2.392	207	214	223	rBV	6757	13983	1.60%	0.299%
3	5.385	694	705	721	rBV2	99826	290357	33.16%	6.208%
4	5.550	721	732	749	rVB	177408	496015	56.65%	10.605%
5	5.958	788	799	812	rBV	112443	295856	33.79%	6.326%
6	6.763	920	931	946	rBV	272688	643546	73.50%	13.760%
7	8.647	1233	1240	1248	rBV	559811	875604	100.00%	18.721%
8	10.055	1465	1471	1478	rBV	577186	771692	88.13%	16.499%
9	11.079	1634	1639	1649	rBV	459728	578528	66.07%	12.369%
10	12.024	1788	1794	1804	rBV	547609	701072	80.07%	14.990%




Sum of corrected areas: 4677084

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070623\
Data File : VX036427.D
Acq On : 06 Jul 2023 11:55
Operator : JC/MD
Sample : 03500-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-060923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

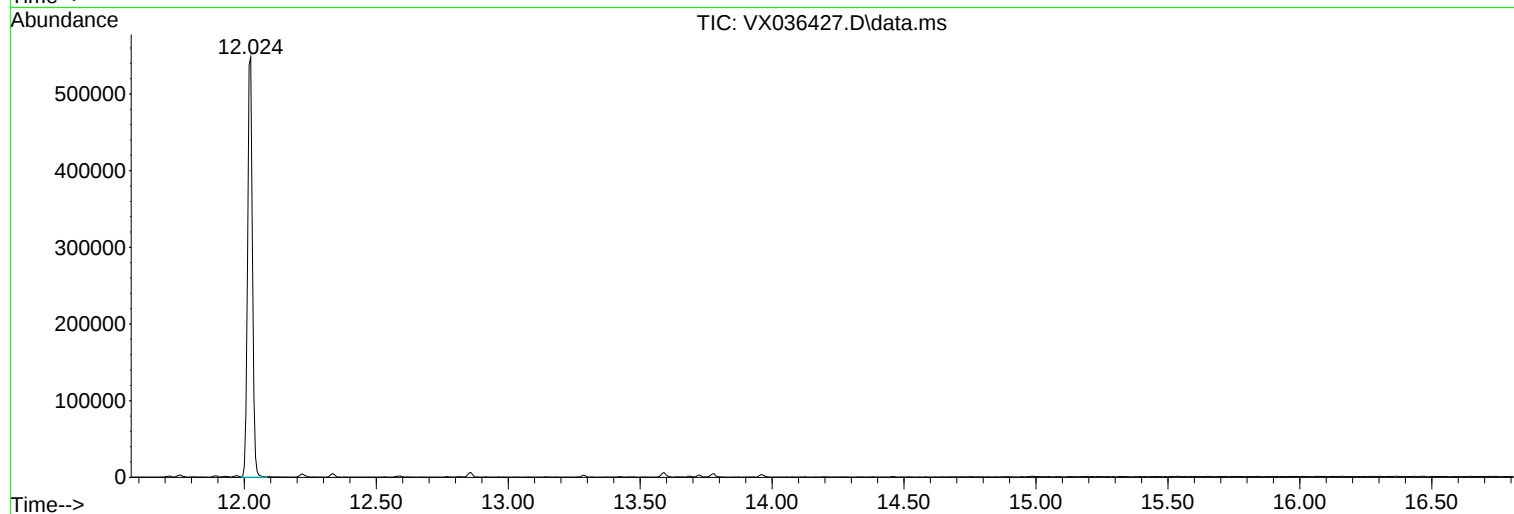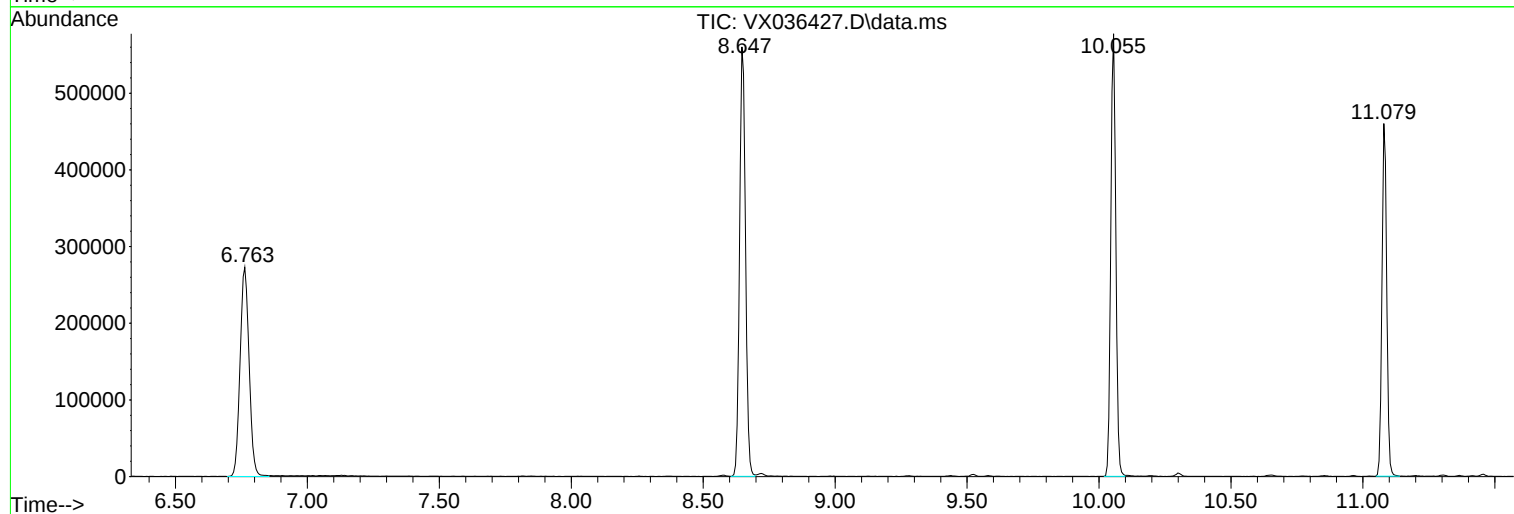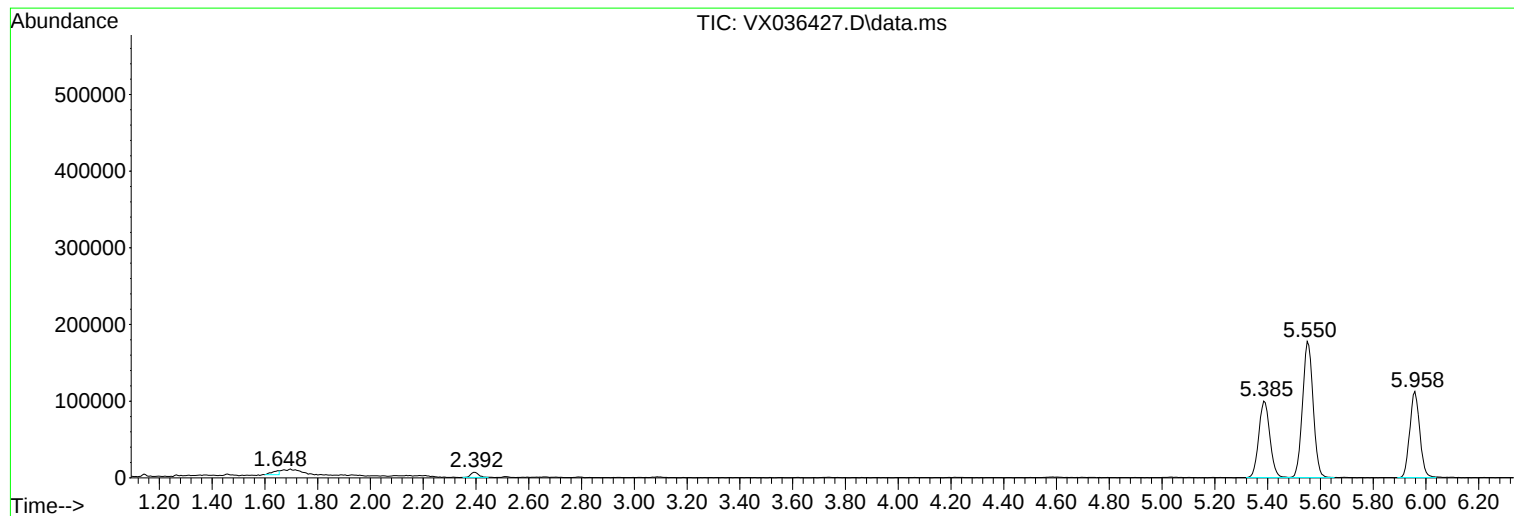

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070623\
Data File : VX036427.D
Acq On : 06 Jul 2023 11:55
Operator : JC/MD
Sample : 03500-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-060923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070623\
Data File : VX036427.D
Acq On : 06 Jul 2023 11:55
Operator : JC/MD
Sample : 03500-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-060923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------