

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
 Data File : VX042220.D
 Acq On : 05 Jul 2024 18:49
 Operator : JC/MD
 Sample : P3100-20ME
 Misc : 5.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 06 05:40:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 06 05:37:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	219830	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	197689	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	96468	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.416	65	43724	34.172	ug/L	0.05
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.340%
7) Chloroethane-d5	1.654	69	2277	2.826	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	5.660%#
11) 1,1-Dichloroethene-d2	2.264	65	19433	34.702	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.400%
21) 2-Butanone-d5	4.501	46	64666	70.129	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	70.130%
24) Chloroform-d	5.056	84	94301	36.654	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.300%
26) 1,2-Dichloroethane-d4	5.958	65	63719	41.961	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.920%
32) Benzene-d6	5.964	84	210555	41.206	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.420%
36) 1,2-Dichloropropane-d6	7.305	67	66871	43.486	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.980%
41) Toluene-d8	8.647	98	189003	39.692	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.380%#
43) trans-1,3-Dichloroprop...	8.951	79	23408	35.221	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.440%
47) 2-Hexanone-d5	9.397	63	63352	90.760	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.760%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	93317	41.047	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.100%
66) 1,2-Dichlorobenzene-d4	12.323	152	79877	42.630	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.260%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.721	43	80107	50.121	ug/L	99
16) Methylene chloride	2.770	84	2474	1.510	ug/L	90
48) 2-Hexanone	9.397	43	6762	4.256	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042220.D
Acq On : 05 Jul 2024 18:49
Operator : JC/MD
Sample : P3100-20ME
Misc : 5.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 06 05:40:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 06 05:37:46 2024
Response via : Initial Calibration




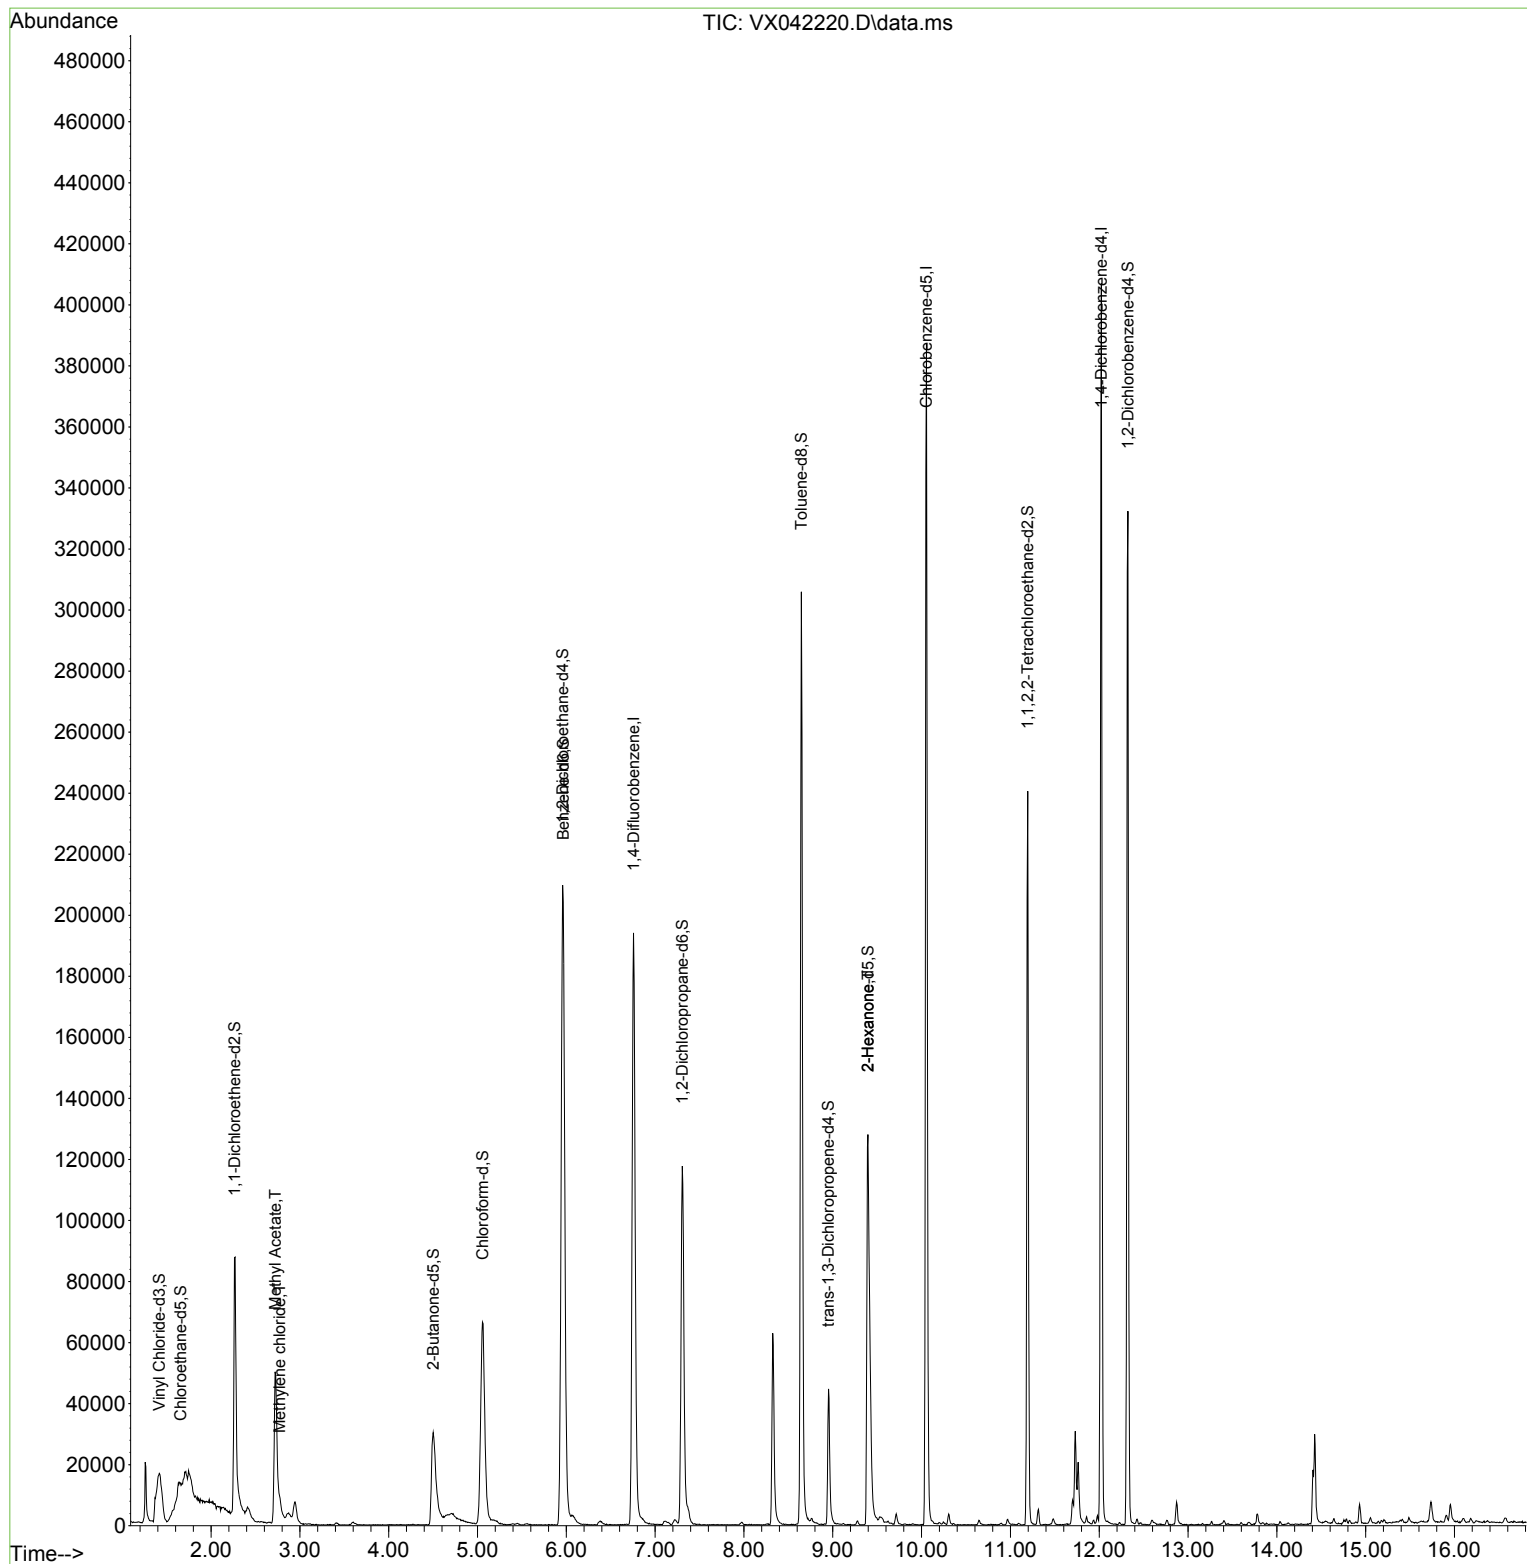


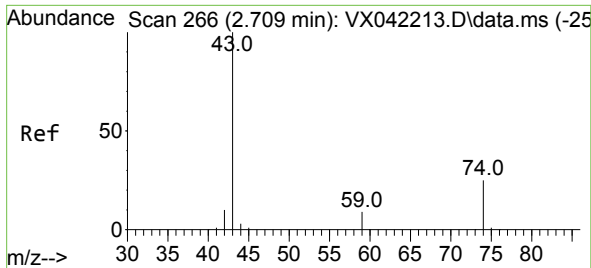

#15
Methyl Acetate
Concen: 50.121 ug/L
RT: 2.721 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX042220.D
Acq: 05 Jul 2024 18:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 80107
Ion Ratio Lower Upper
43 100
74 25.4 20.1 30.1

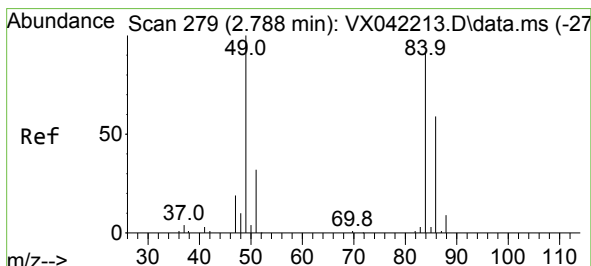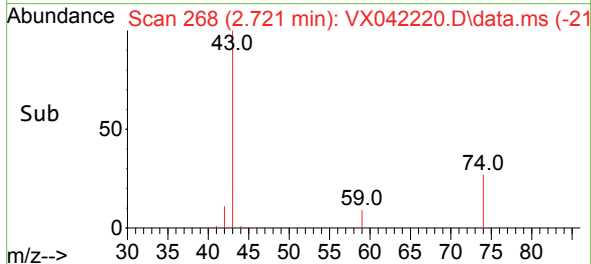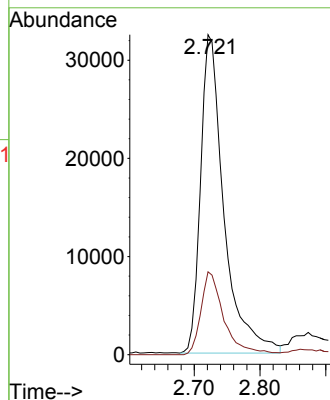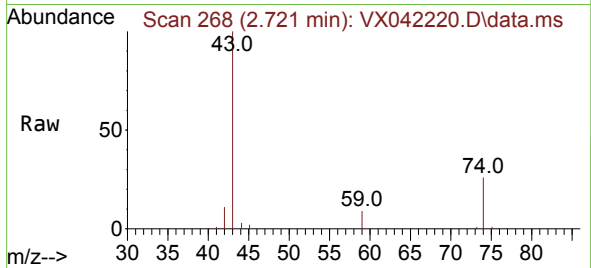

#16
Methylene chloride
Concen: 1.510 ug/L
RT: 2.770 min Scan# 276
Delta R.T. -0.018 min
Lab File: VX042220.D
Acq: 05 Jul 2024 18:49


Tgt Ion: 84 Resp: 2474
Ion Ratio Lower Upper
84 100
86 60.3 45.7 84.9
49 96.2 76.4 141.8

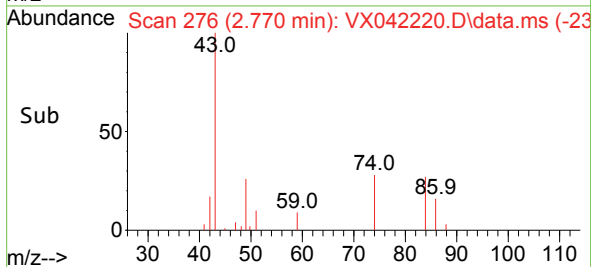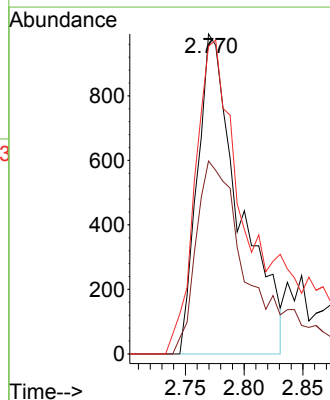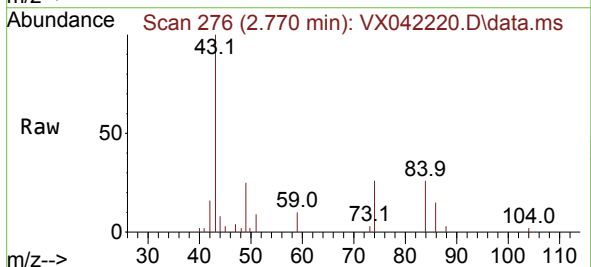

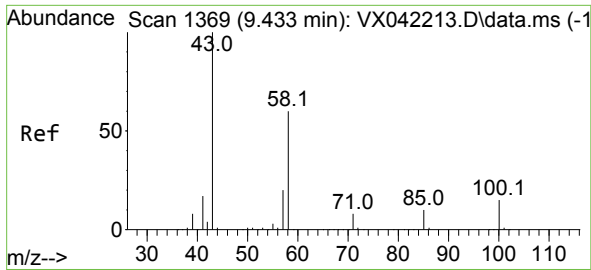

#48
 2-Hexanone
 Concen: 4.256 ug/L
 RT: 9.397 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VX042220.D
 Acq: 05 Jul 2024 18:49

Instrument :
 MSVOA_X
 ClientSampleId :

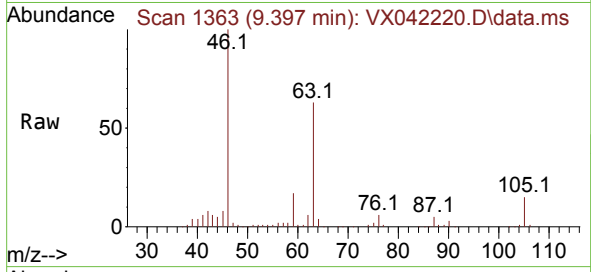

Tgt Ion: 43 Resp: 6762

Ion	Ratio	Lower	Upper
43	100		
58	30.2	46.4	69.6#
57	28.9	16.3	24.5#
100	0.0	12.1	18.1#

