




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042218.D
Acq On : 05 Jul 2024 18:03
Operator : JC/MD
Sample : P3100-17ME
Misc : 4.21g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D08ME

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
Supervised By :Semsettin Yesilyurt 07/08/2024

Quant Time: Jul 06 05:39:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 06 05:37:46 2024
Response via : Initial Calibration

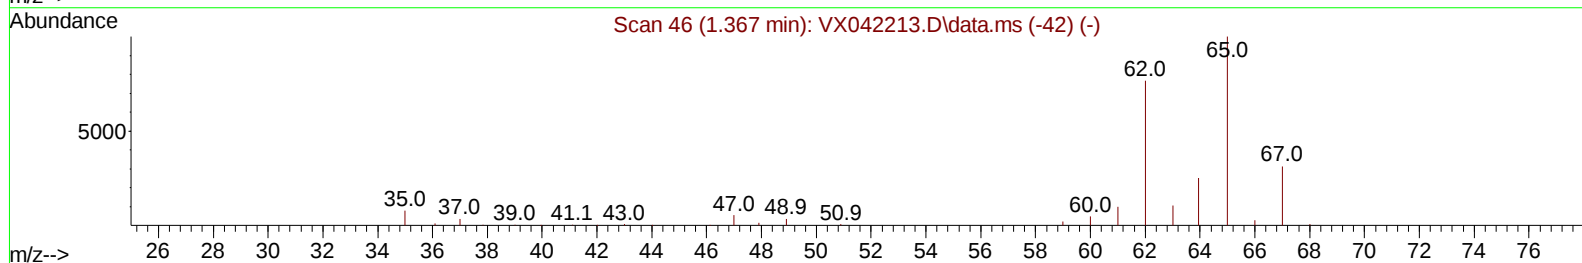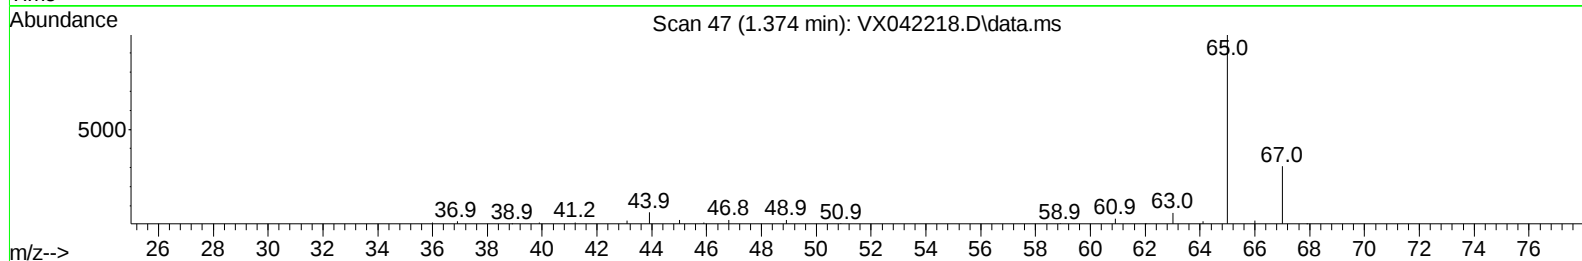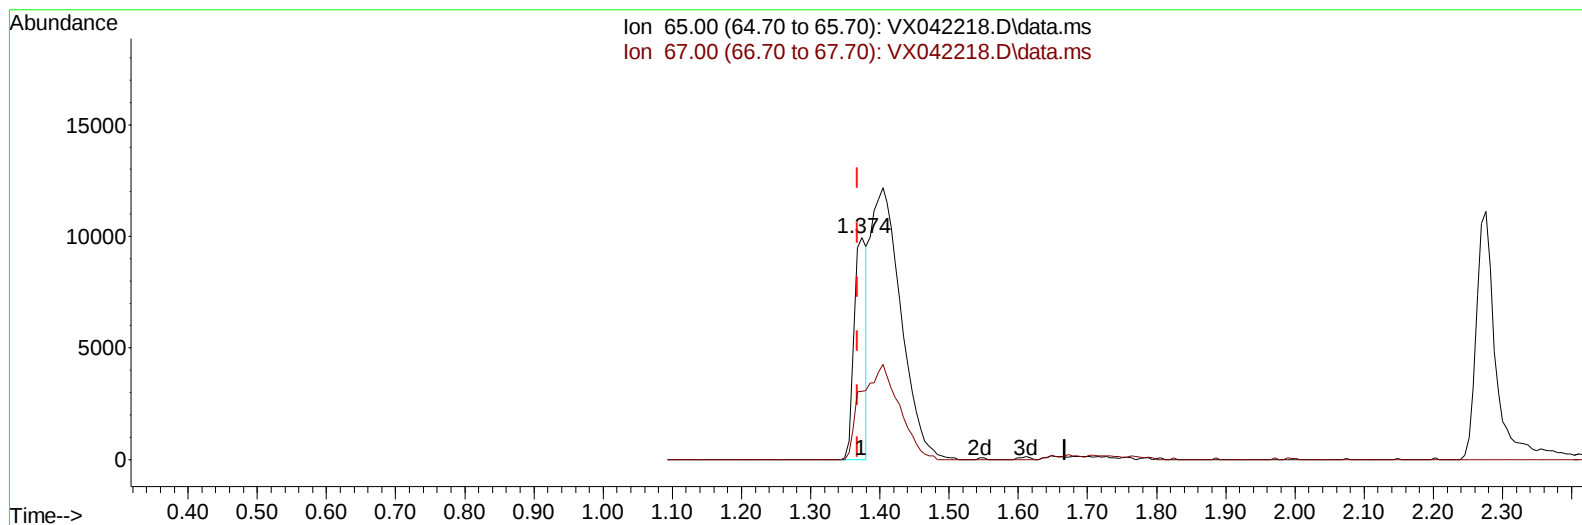

TIC: VX042218.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.374min (+ 0.006) 8.88 ug/L

response 12660

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.70	76.26#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042218.D
Acq On : 05 Jul 2024 18:03
Operator : JC/MD
Sample : P3100-17ME
Misc : 4.21g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D08ME

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
Supervised By :Semsettin Yesilyurt 07/08/2024

Quant Time: Jul 06 05:39:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 06 05:37:46 2024
Response via : Initial Calibration

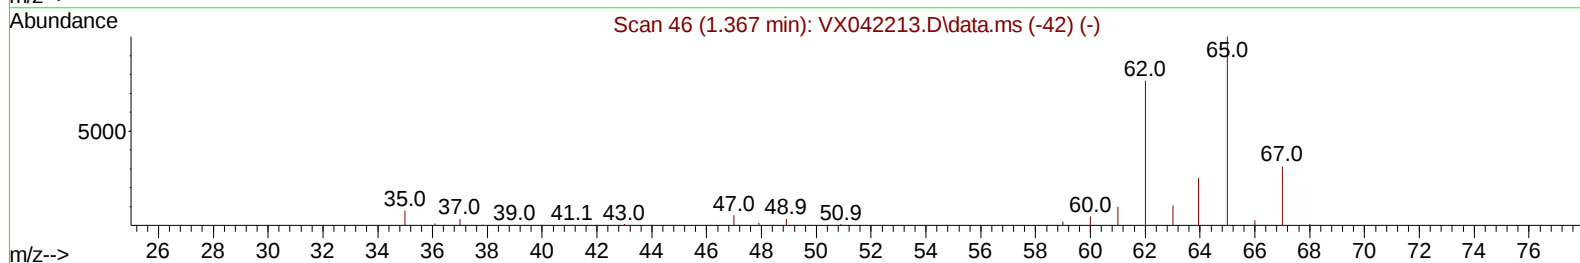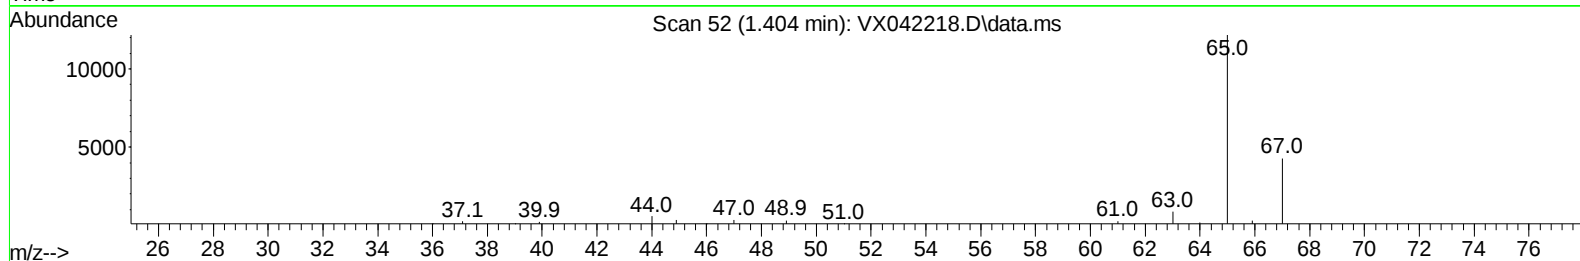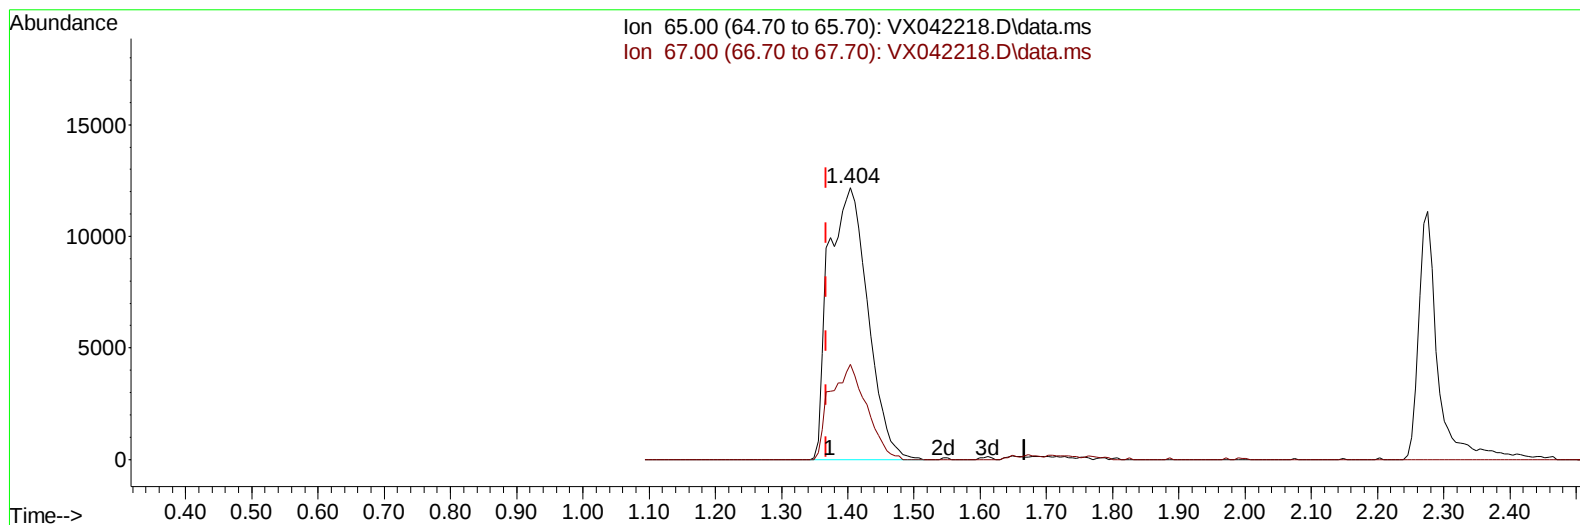

TIC: VX042218.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.404min (+ 0.037) 34.94 ug/L m

response 49815

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.70	19.38#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042218.D
Acq On : 05 Jul 2024 18:03
Operator : JC/MD
Sample : P3100-17ME
Misc : 4.21g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D08ME

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
Supervised By :Semsettin Yesilyurt 07/08/2024

Quant Time: Jul 06 05:39:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 06 05:37:46 2024
Response via : Initial Calibration

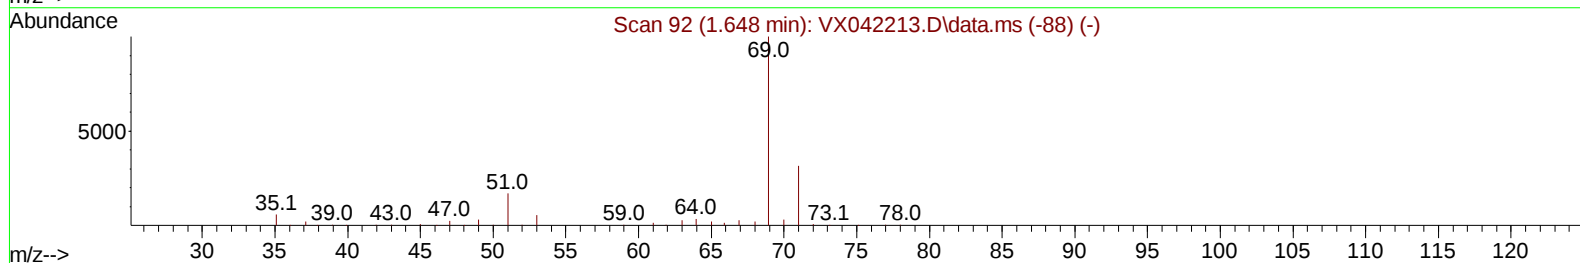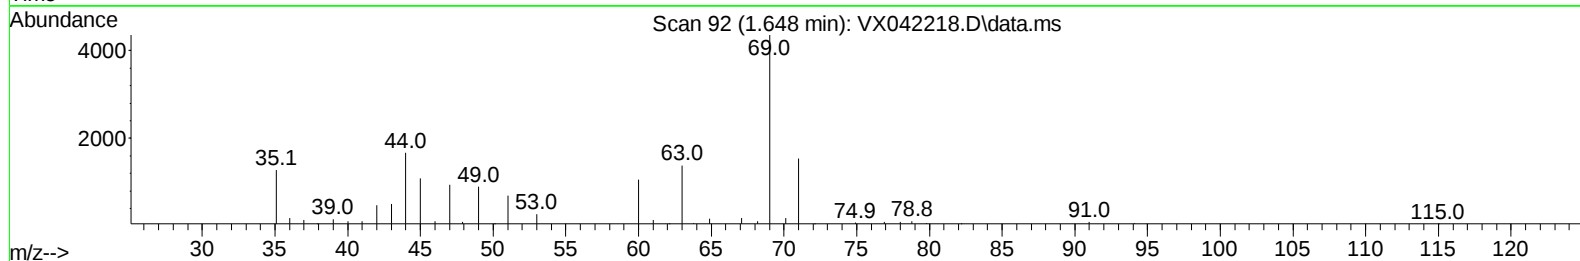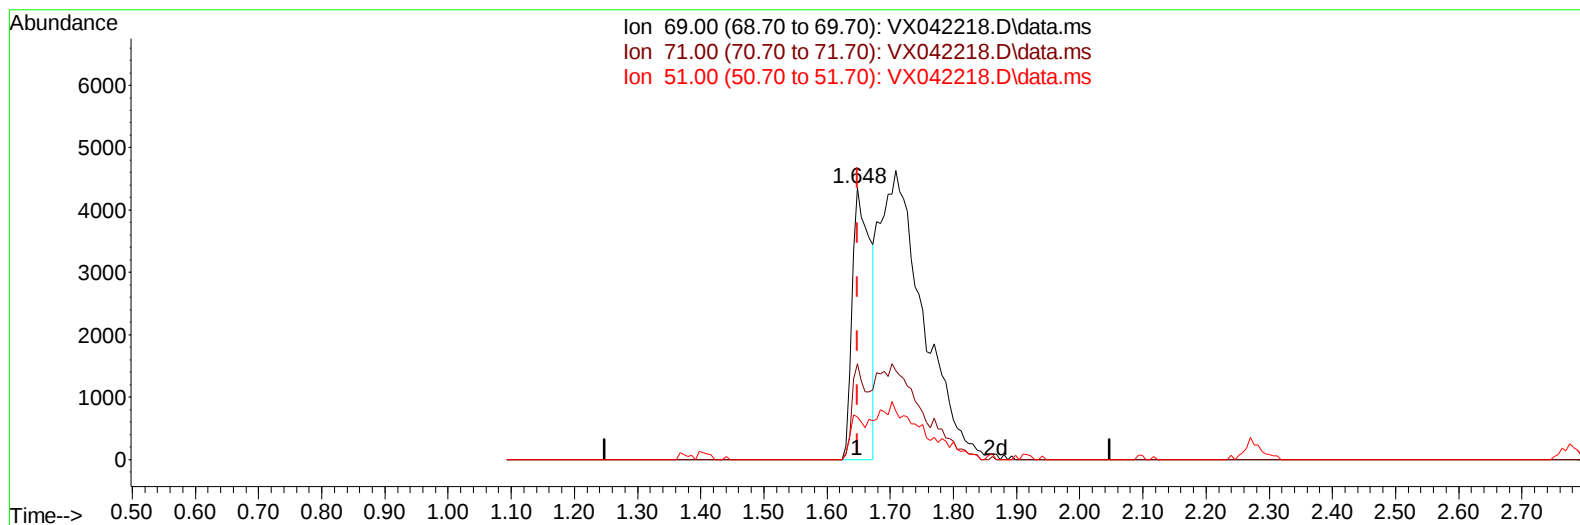

TIC: VX042218.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 9.76 ug/L

response 8758

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	27.91
51.00	12.70	12.46
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042218.D
Acq On : 05 Jul 2024 18:03
Operator : JC/MD
Sample : P3100-17ME
Misc : 4.21g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D08ME

Manual IntegrationsAPPROVED

Quant Time: Jul 06 05:39:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 06 05:37:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/08/2024
Supervised By :Semsettin Yesilyurt 07/08/2024

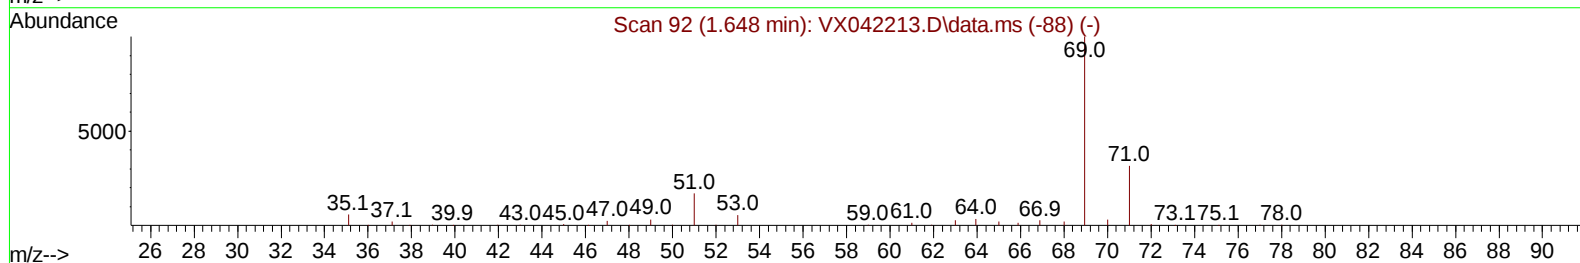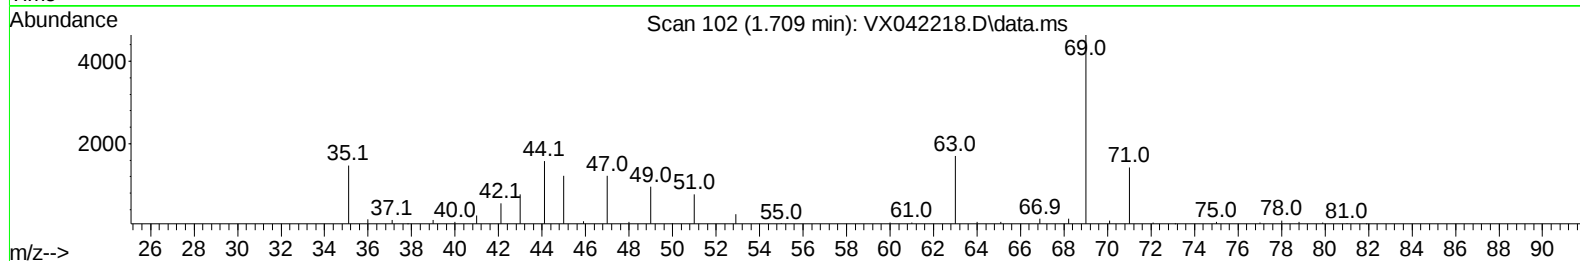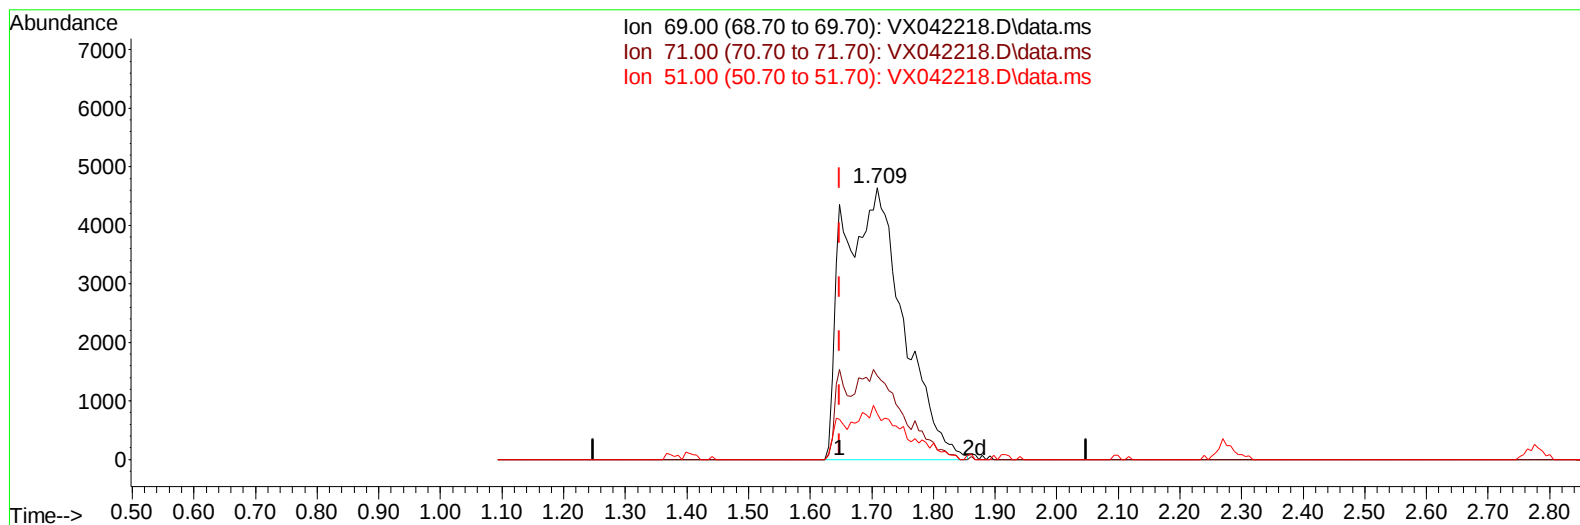

TIC: VX042218.D\data.ms

(7) Chloroethane-d5 (S)

1.709min (+ 0.061) 34.76 ug/L m

response 31205

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	7.83#
51.00	12.70	3.50#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
 Data File : VX042218.D
 Acq On : 05 Jul 2024 18:03
 Operator : JC/MD
 Sample : P3100-17ME
 Misc : 4.21g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4D08ME

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
 Supervised By :Semsettin Yesilyurt 07/08/2024

Quant Time: Jul 06 05:39:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 06 05:37:46 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.757	114		244921	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117		221774	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152		108557	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.404	65		49815m	34.943	ug/L	0.04
Spiked Amount 50.000	Range 60	- 135		Recovery =	69.880%		
7) Chloroethane-d5	1.709	69		31205m	34.765	ug/L	0.06
Spiked Amount 50.000	Range 70	- 130		Recovery =	69.520%#		
11) 1,1-Dichloroethene-d2	2.276	65		21050	33.738	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125		Recovery =	67.480%		
21) 2-Butanone-d5	4.495	46		89783	87.394	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130		Recovery =	87.390%		
24) Chloroform-d	5.056	84		108120	37.720	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	75.440%		
26) 1,2-Dichloroethane-d4	5.952	65		72017	42.567	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	85.140%		
32) Benzene-d6	5.964	84		236002	41.170	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	82.340%		
36) 1,2-Dichloropropane-d6	7.305	67		73733	42.741	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery =	85.480%		
41) Toluene-d8	8.647	98		210196	39.348	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	78.700%#		
43) trans-1,3-Dichloroprop...	8.951	79		26265	35.228	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery =	70.460%		
47) 2-Hexanone-d5	9.390	63		71179	90.899	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery =	90.900%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84		105610	41.409	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery =	82.820%		
66) 1,2-Dichlorobenzene-d4	12.323	152		89323	42.363	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	84.720%		
Target Compounds							
15) Methyl Acetate	2.721	43		42681	23.969	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042218.D
Acq On : 05 Jul 2024 18:03
Operator : JC/MD
Sample : P3100-17ME
Misc : 4.21g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D08ME

Manual IntegrationsAPPROVED

Quant Time: Jul 06 05:39:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 06 05:37:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/08/2024
Supervised By :Semsettin Yesilyurt 07/08/2024

