

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
 Data File : VX042215.D
 Acq On : 05 Jul 2024 16:52
 Operator : JC/MD
 Sample : P3087-13ME
 Misc : 4.61g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4BP1ME

Quant Time: Jul 06 05:39:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 06 05:37:46 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
 Supervised By :Semsettin Yesilyurt 07/08/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	252006	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	220112	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	103404	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	46645m	31.800	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	63.600%		
7) Chloroethane-d5	1.648	69	29926m	32.403	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	64.800%#		
11) 1,1-Dichloroethene-d2	2.276	65	19946	31.070	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.140%		
21) 2-Butanone-d5	4.489	46	77115	72.952	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	72.950%		
24) Chloroform-d	5.056	84	102551	34.771	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	69.540%#		
26) 1,2-Dichloroethane-d4	5.958	65	66414	38.151	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	76.300%		
32) Benzene-d6	5.964	84	222245	39.063	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.120%		
36) 1,2-Dichloropropane-d6	7.312	67	69894	40.822	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	81.640%		
41) Toluene-d8	8.647	98	201002	37.911	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	75.820%#		
43) trans-1,3-Dichloroprop...	8.952	79	25736	34.779	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.560%		
47) 2-Hexanone-d5	9.390	63	62863	80.885	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	80.890%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	97336	38.453	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	76.900%		
66) 1,2-Dichlorobenzene-d4	12.323	152	82852	41.252	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.500%		
Target Compounds						Qvalue
15) Methyl Acetate	2.721	43	10716	5.849	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042215.D
Acq On : 05 Jul 2024 16:52
Operator : JC/MD
Sample : P3087-13ME
Misc : 4.61g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
A4BP1ME

Quant Time: Jul 06 05:39:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 06 05:37:46 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
Supervised By :Semsettin Yesilyurt 07/08/2024

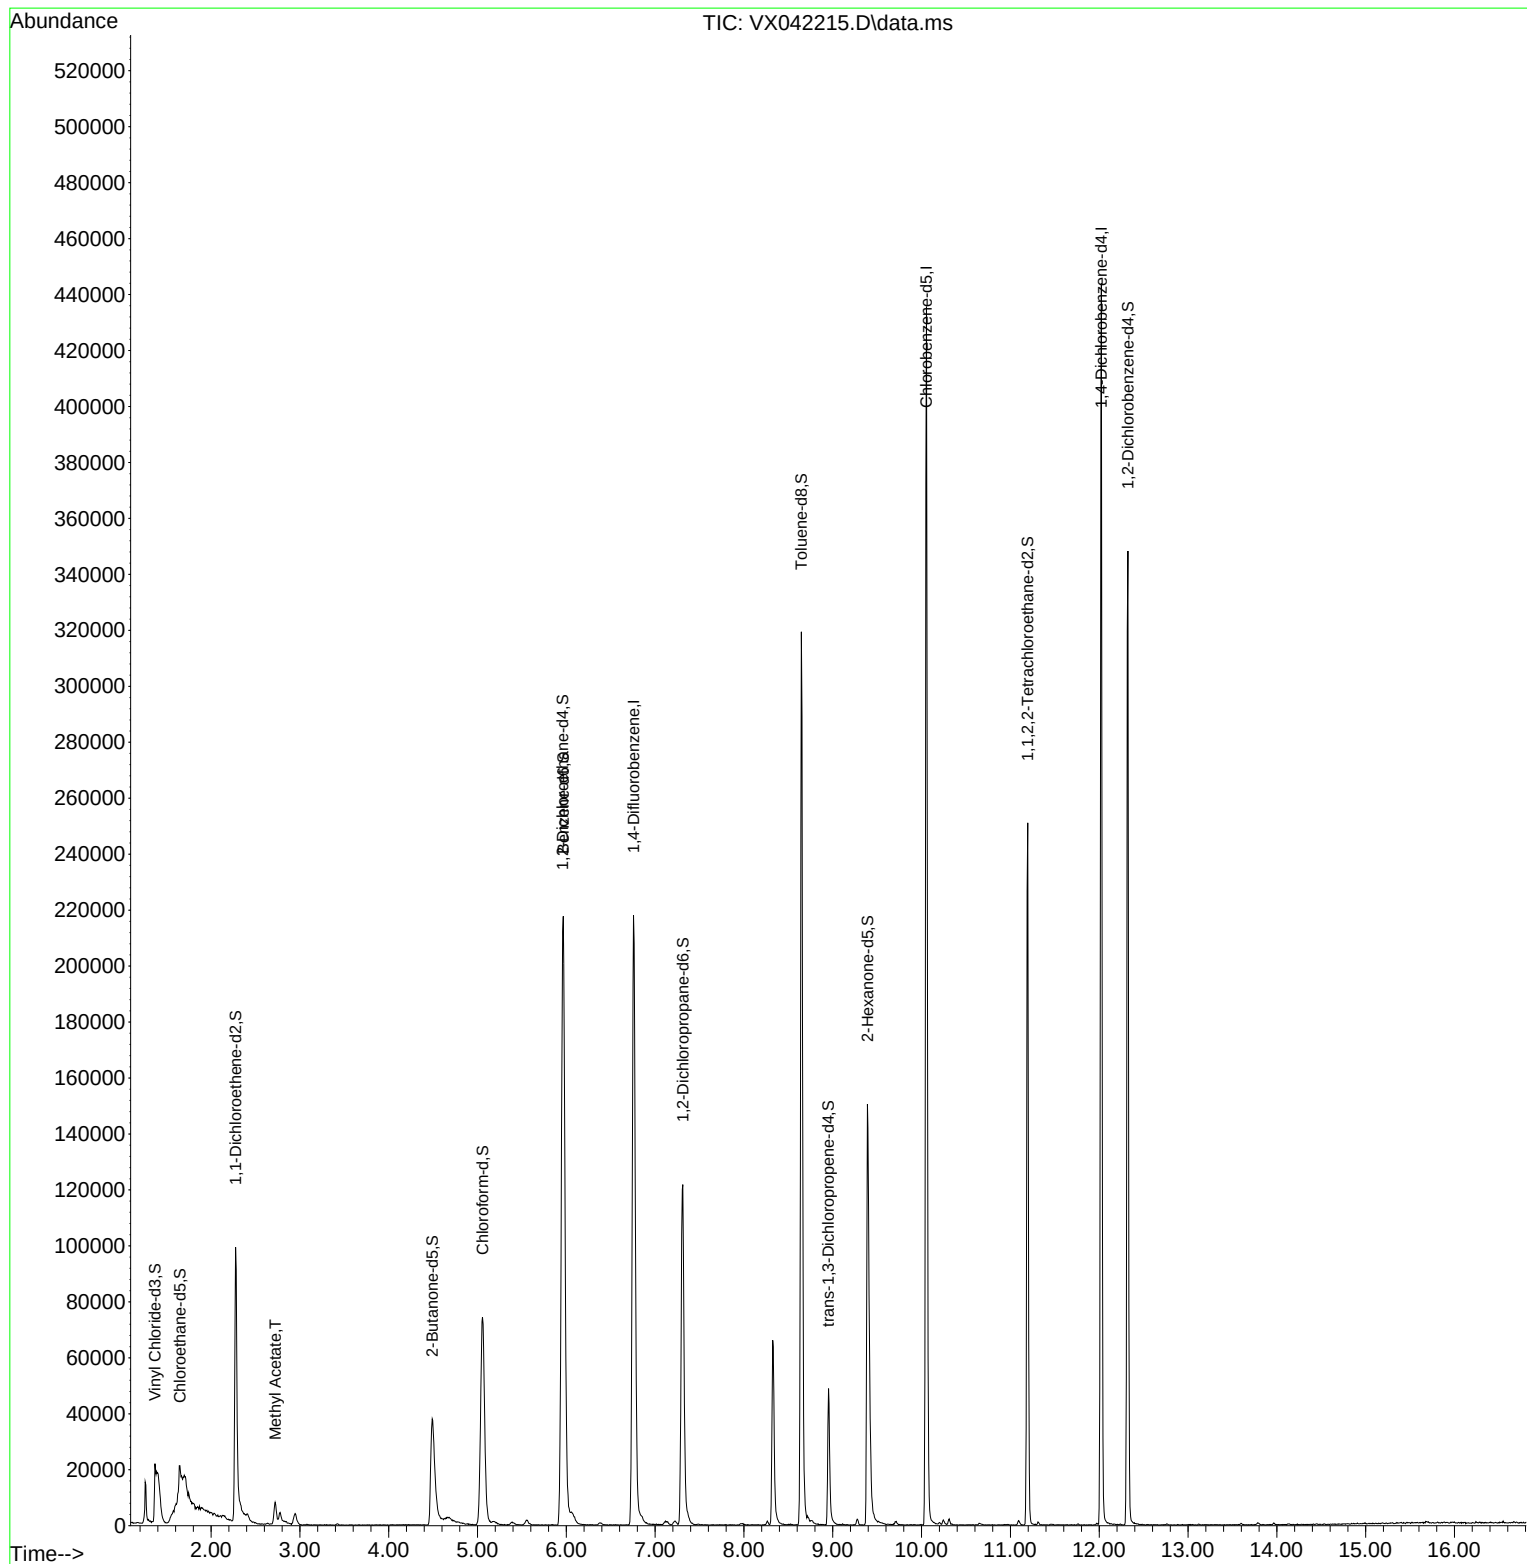

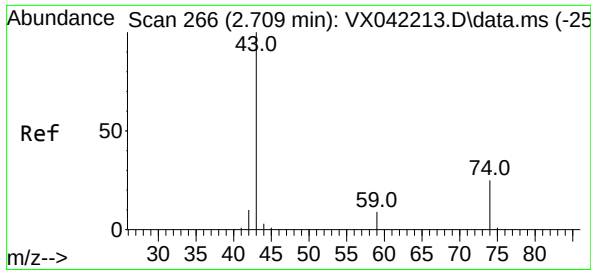

#15
Methyl Acetate
Concen: 5.849 ug/L
RT: 2.721 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX042215.D
Acq: 05 Jul 2024 16:52

Instrument :
MSVOA_X
ClientSampleId :
A4BP1ME

Tgt Ion: 43 Resp: 10710
Ion Ratio Lower Upper
43 100
74 27.5 20.1 30.1

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
Supervised By :Semsettin Yesilyurt 07/08/2024

