

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
 Data File : VX042221.D
 Acq On : 05 Jul 2024 19:13
 Operator : JC/MD
 Sample : P3100-21ME
 Misc : 4.86g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4D38ME

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
 Supervised By :Semsettin Yesilyurt 07/08/2024

Quant Time: Jul 06 05:40:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 06 05:37:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	193454	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	171046	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	81759	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.398	65	33217	29.499	ug/L	0.03
Spiked Amount 50.000	Range 60 - 135		Recovery =	59.000%#		
7) Chloroethane-d5	1.715	69	19872m	28.029	ug/L	0.07
Spiked Amount 50.000	Range 70 - 130		Recovery =	56.060%#		
11) 1,1-Dichloroethene-d2	2.270	65	13633	27.664	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.320%#		
21) 2-Butanone-d5	4.501	46	48433	59.686	ug/L	0.03
Spiked Amount 100.000	Range 40 - 130		Recovery =	59.690%		
24) Chloroform-d	5.056	84	70879	31.306	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	62.620%#		
26) 1,2-Dichloroethane-d4	5.952	65	47786	35.759	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	71.520%		
32) Benzene-d6	5.964	84	155643	35.204	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	70.400%		
36) 1,2-Dichloropropane-d6	7.306	67	47499	35.700	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	71.400%		
41) Toluene-d8	8.647	98	139863	33.947	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	67.900%#		
43) trans-1,3-Dichloroprop...	8.952	79	17000	29.563	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	59.120%#		
47) 2-Hexanone-d5	9.397	63	41076	68.013	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery =	68.010%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	65952	33.529	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	67.060%		
66) 1,2-Dichlorobenzene-d4	12.323	152	57463	36.185	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	72.380%#		
Target Compounds						Qvalue
15) Methyl Acetate	2.721	43	20368	14.481	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042221.D
Acq On : 05 Jul 2024 19:13
Operator : JC/MD
Sample : P3100-21ME
Misc : 4.86g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 27 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
A4D38ME

Quant Time: Jul 06 05:40:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 06 05:37:46 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Mahesh Dadoda 07/08/2024
Supervised By : Semsettin Yesilyurt 07/08/2024

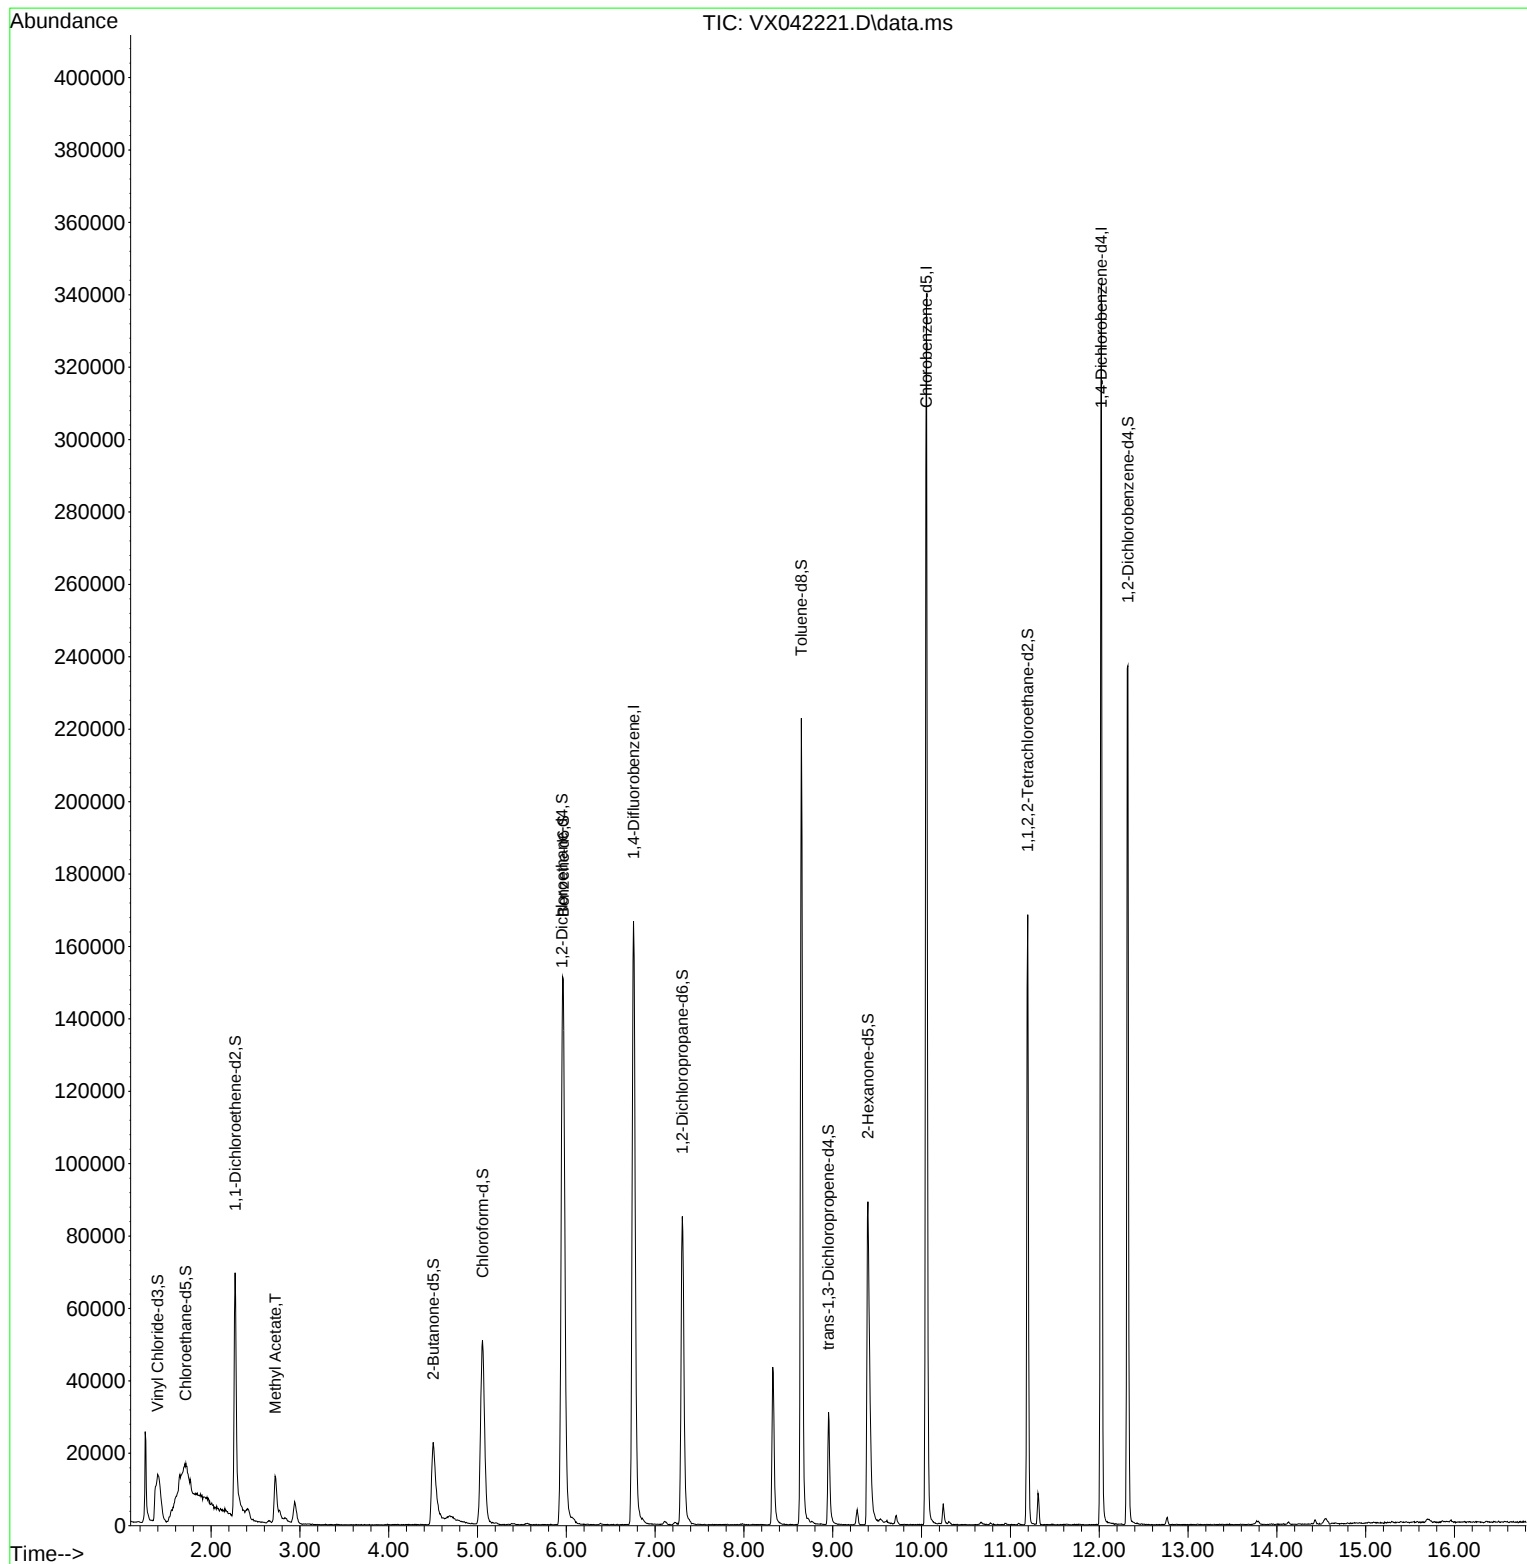

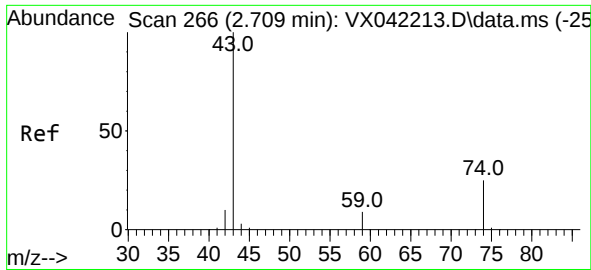

#15
Methyl Acetate
Concen: 14.481 ug/L
RT: 2.721 min Scan# 20368
Delta R.T. 0.012 min
Lab File: VX042221.D
Acq: 05 Jul 2024 19:13

Instrument :
MSVOA_X
ClientSampleId :
A4D38ME

Tgt Ion: 43 Resp: 20368
Ion Ratio Lower Upper
43 100
74 24.8 20.1 30.1

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/08/2024
Supervised By :Semsettin Yesilyurt 07/08/2024

