
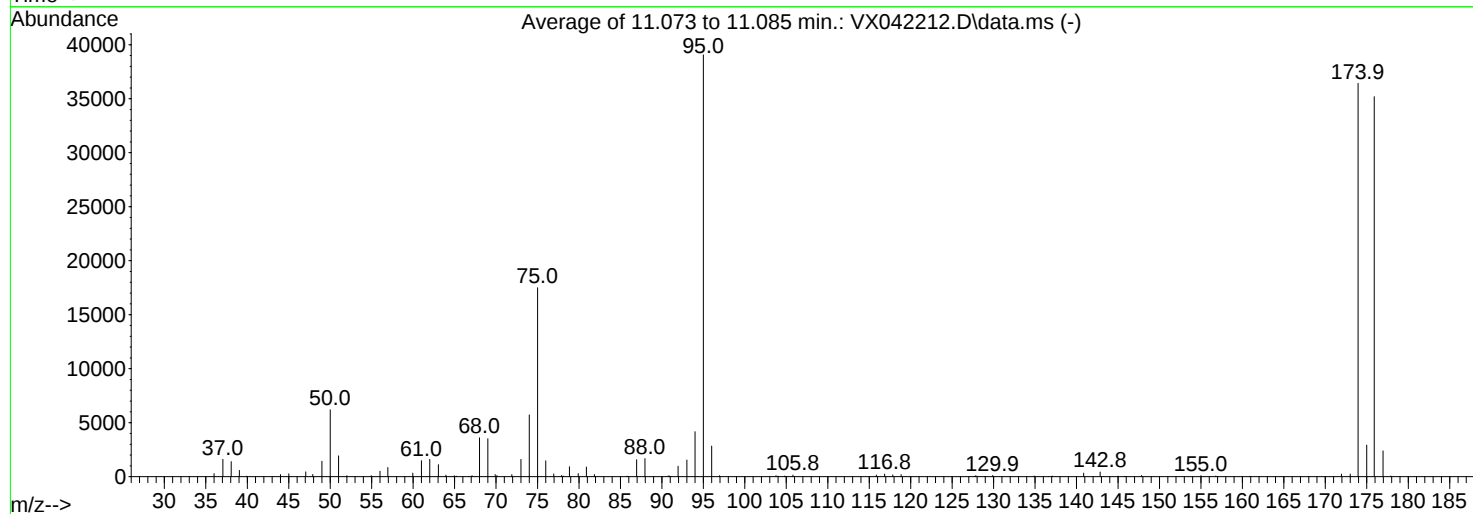


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070624\
Data File : VX042212.D
Acq On : 05 Jul 2024 15:19
Operator : JC/MD
Sample : BFB678
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB678

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM070324WMA.M
Title : VOC Analysis
Last Update : Sat Jul 06 05:37:46 2024

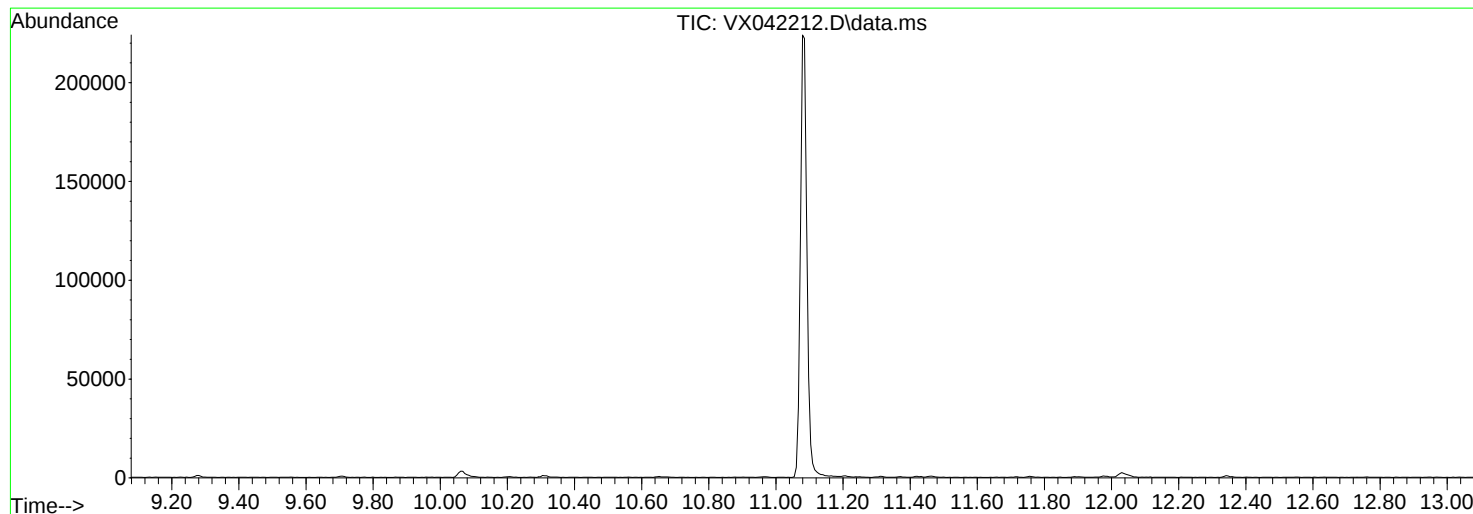

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.9	6196	PASS
75	95	30	80	44.8	17505	PASS
95	95	100	100	100.0	39064	PASS
96	95	5	9	7.3	2837	PASS
173	174	0.00	2	0.7	239	PASS
174	95	50	120	93.2	36421	PASS
175	174	5	9	8.0	2920	PASS
176	174	95	101	96.6	35200	PASS
177	176	5	9	6.8	2390	PASS

m/z	Abundance
39.90	155.0
44.10	106.0

Instrument :
MSVOA_X
ClientSampleId :
BFB678

m/z	Abundance
36.00	229.0
37.00	1302.0
38.00	1098.0
39.00	421.0
39.90	180.0
44.10	281.0
45.00	213.0
47.10	337.0
47.80	155.0
49.00	1121.0
50.00	4791.0
51.00	1348.0
52.00	101.0
55.10	71.0
56.00	429.0
57.00	570.0
59.90	240.0
61.00	1118.0
62.00	1286.0
63.10	745.0
64.00	126.0
64.90	101.0
67.10	91.0
68.00	2817.0
69.00	2665.0
69.90	290.0
71.80	112.0
73.00	1179.0
74.00	4159.0
75.00	13130.0
76.00	1037.0
77.00	185.0
77.90	164.0
78.90	680.0
79.90	224.0
80.90	677.0
81.80	169.0
86.90	940.0
88.00	1177.0
90.70	77.0
91.10	76.0
91.90	650.0
93.00	1121.0
94.00	2924.0
95.00	26552.0
96.00	2202.0
96.90	86.0
103.70	114.0
105.80	99.0
115.80	83.0
116.80	189.0
117.80	146.0
118.80	110.0
127.70	52.0
129.90	72.0
140.90	208.0
142.80	254.0
147.90	67.0
171.90	151.0
173.00	202.0
173.90	19816.0
175.00	1731.0
175.90	19424.0
176.90	1447.0

Instrument :
MSVOA_X
ClientSampleId :
BFB678

m/z	Abundance
36.00	341.0
37.00	1784.0
38.10	1625.0
39.10	668.0
40.00	220.0
44.00	377.0
45.00	337.0
47.00	551.0
47.90	251.0
49.00	1736.0
50.00	7424.0
51.00	2317.0
51.90	105.0
54.90	140.0
56.00	581.0
57.00	1073.0
60.00	367.0
61.00	1849.0
62.00	1858.0
63.00	1499.0
64.00	166.0
65.20	159.0
67.10	110.0
68.00	4310.0
69.00	3923.0
70.10	319.0
71.90	217.0
73.00	1935.0
74.00	6939.0
75.00	20392.0
76.00	1717.0
76.90	281.0
78.10	183.0
78.90	1159.0
79.90	342.0
80.90	1113.0
81.80	205.0
85.80	51.0
87.00	1929.0
87.90	1988.0
90.80	139.0
92.00	1135.0
93.00	1876.0
94.00	5088.0
95.00	46464.0
96.00	3121.0
96.90	100.0
103.80	177.0
104.80	87.0
105.70	169.0
115.80	222.0
116.90	307.0
117.90	212.0
118.90	281.0
127.90	119.0
129.90	146.0
134.90	80.0
137.00	89.0
140.90	434.0
142.90	583.0
145.00	57.0
145.80	88.0
147.90	102.0
155.00	146.0
156.80	113.0
172.00	282.0
173.00	516.0
173.90	42256.0
175.00	3453.0
175.90	40824.0
177.00	2761.0
177.90	140.0

Instrument :
MSVOA_X
ClientSampleId :
BFB678

m/z	Abundance
36.00	291.0
37.10	1706.0
38.00	1481.0
39.00	627.0
39.90	186.0
43.90	229.0
45.00	237.0
47.00	469.0
48.00	217.0
49.00	1434.0
50.00	6372.0
51.00	2120.0
52.10	56.0
54.90	67.0
56.00	491.0
56.90	878.0
60.00	366.0
61.00	1482.0
62.00	1642.0
63.00	1091.0
63.90	159.0
65.00	190.0
66.70	82.0
67.10	67.0
68.00	3701.0
69.00	3968.0
69.90	293.0
72.00	234.0
73.00	1671.0
74.00	6058.0
75.00	18992.0
76.00	1632.0
77.00	301.0
77.90	167.0
78.80	909.0
79.90	289.0
80.90	868.0
81.90	214.0
85.80	89.0
87.00	1842.0
87.90	1840.0
90.90	165.0
91.90	1121.0
93.00	1635.0
94.00	4480.0
95.00	44176.0
96.00	3188.0
97.00	72.0
104.00	153.0
104.80	79.0
105.90	169.0
115.90	129.0
116.80	215.0
117.90	122.0
118.90	201.0
127.80	207.0
128.90	61.0
129.90	131.0
134.90	115.0
136.60	54.0
137.10	76.0
140.80	339.0
142.90	441.0
145.00	95.0
146.00	68.0
147.80	138.0
155.00	118.0
156.80	57.0
160.90	80.0
171.90	274.0
174.00	47192.0
175.00	3575.0
175.90	45352.0
176.90	2963.0
177.90	55.0

Instrument :
MSVOA_X
ClientSampleId :
BFB678