

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070720\
 Data File : VX017196.D
 Acq On : 07 Jul 2020 12:27
 Operator : JC/SP
 Sample : L3159-24
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PDB-BLANK-20200629

Quant Time: Jul 08 05:24:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 29 17:10:38 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	265674	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	439570	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	444561	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	227249	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	170373	52.02	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.04%	
35) Dibromofluoromethane	5.47	113	144910	52.11	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.22%	
50) Toluene-d8	8.70	98	529875	51.53	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.06%	
62) 4-Bromofluorobenzene	11.12	95	210802	52.45	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.90%	
Target Compounds						
16) Acetone	2.42	43	10464	8.540	ug/l	98
27) cis-1,2-Dichloroethene	4.56	96	21287	6.441	ug/l	90
44) Trichloroethene	7.19	130	14288	3.957	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070720\
Data File : VX017196.D
Acq On : 07 Jul 2020 12:27
Operator : JC/SP
Sample : L3159-24
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PDB-BLANK-20200629

Quant Time: Jul 08 05:24:05 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 29 17:10:38 2020
Response via : Initial Calibration

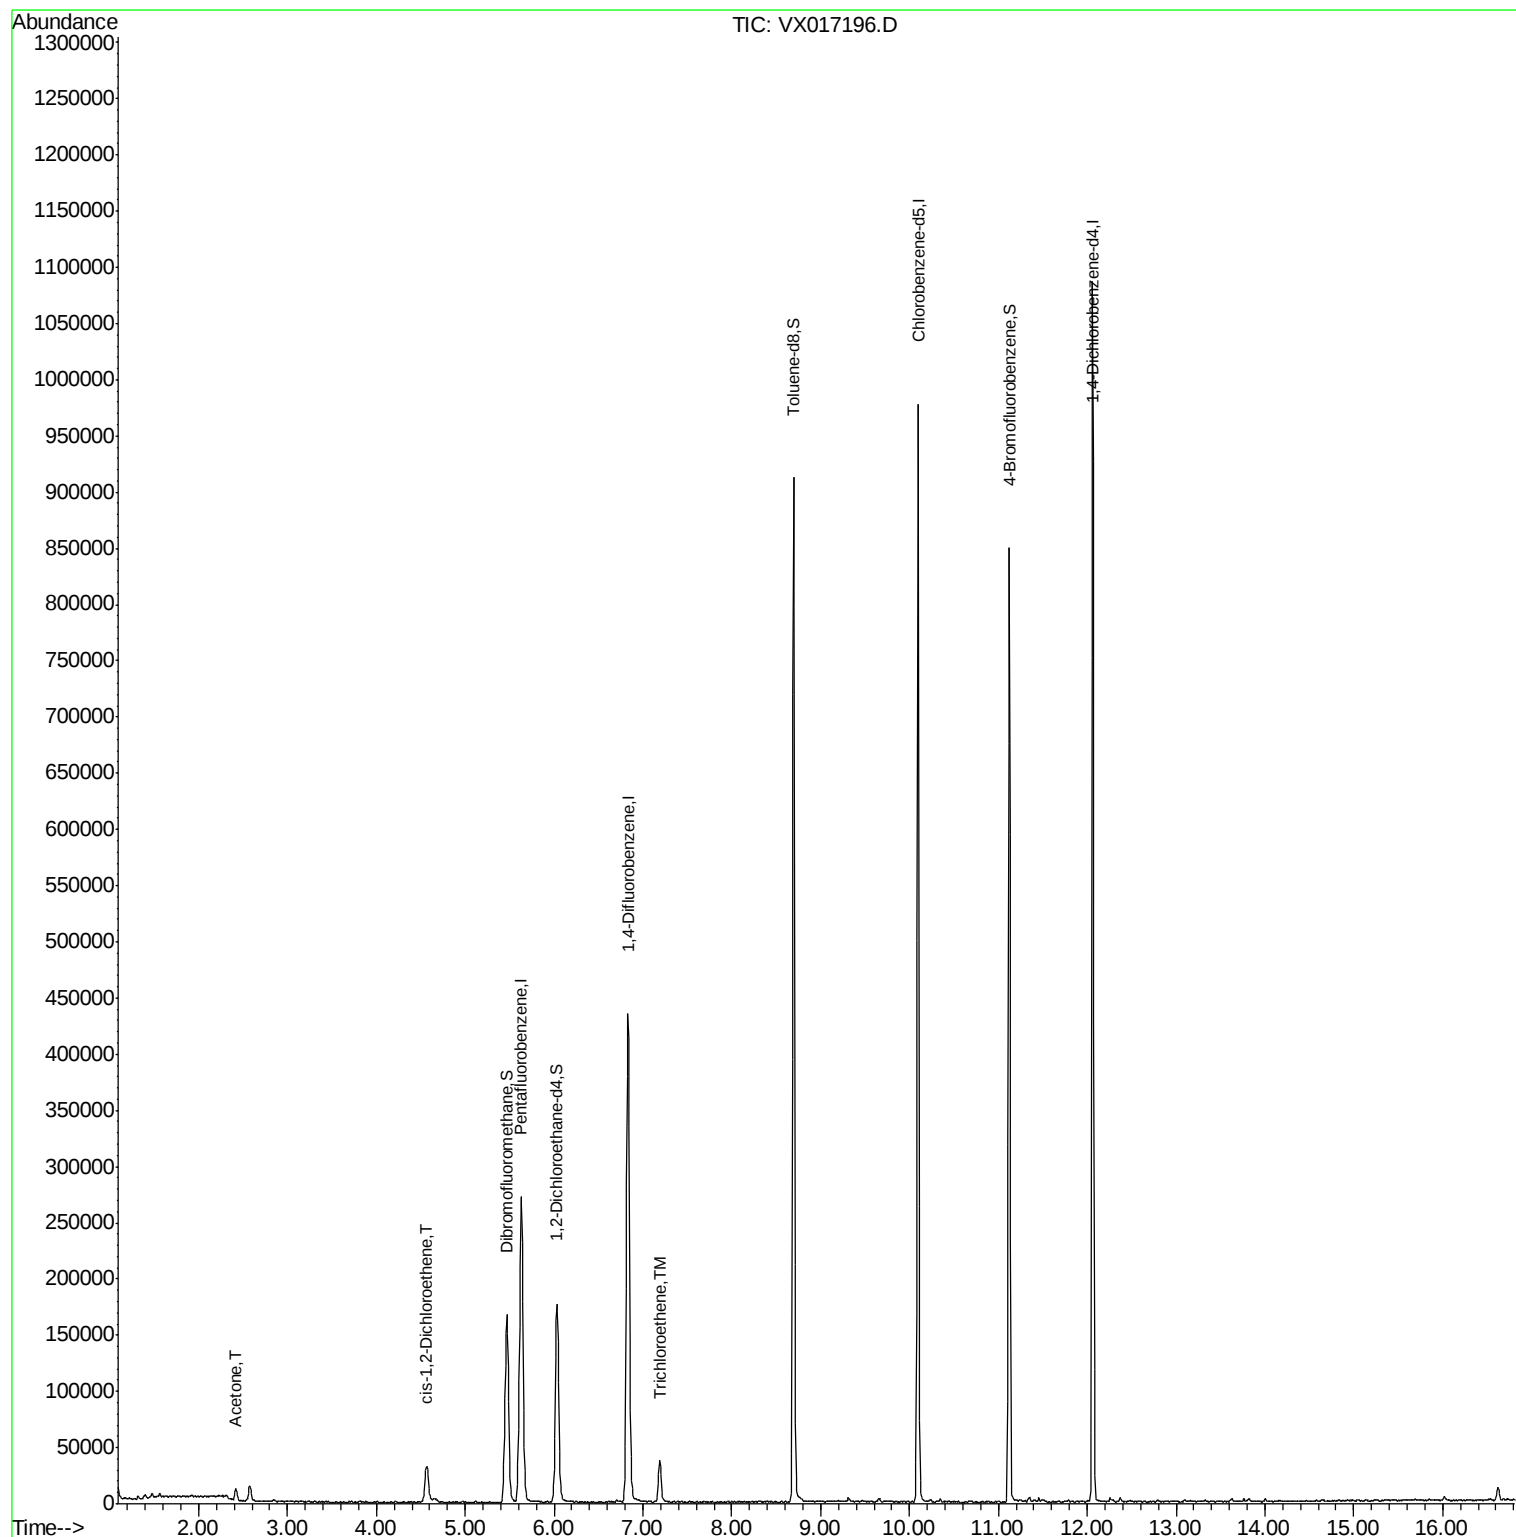



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017196.D

Acq: 07 Jul 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :


PDB-BLANK-20200629

Tot Ion:168 Resp: 265674

Ion Ratio Lower Upper

168 100

99 53.6 42.6 64.0

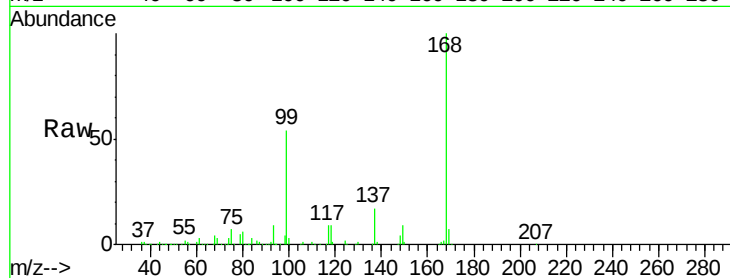

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

100000

80000



60000

40000

20000

0

Time-->

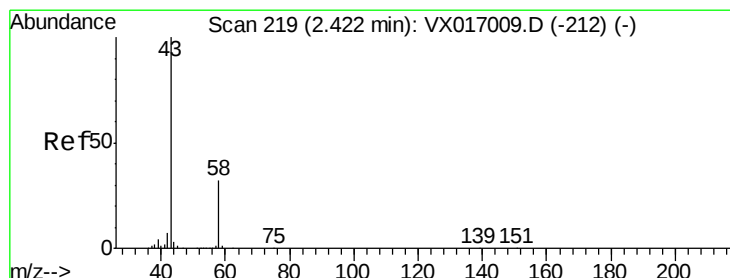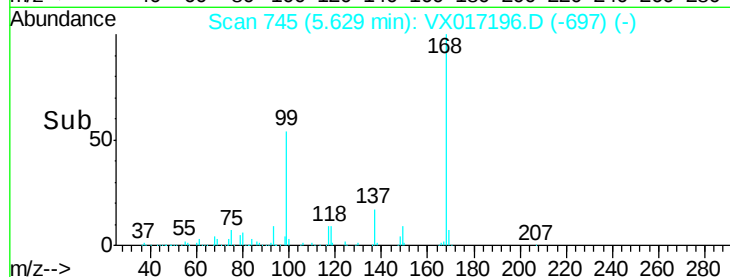

#16

Acetone

Concen: 8.540 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX017196.D


Acq: 07 Jul 2020 12:27

Tgt Ion: 43 Resp: 10464

Ion Ratio Lower Upper

43 100

58 31.1 25.7 38.5

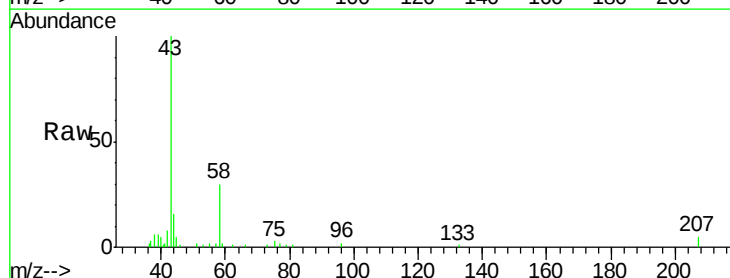

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.42


6000


4000

2000

0

Time-->

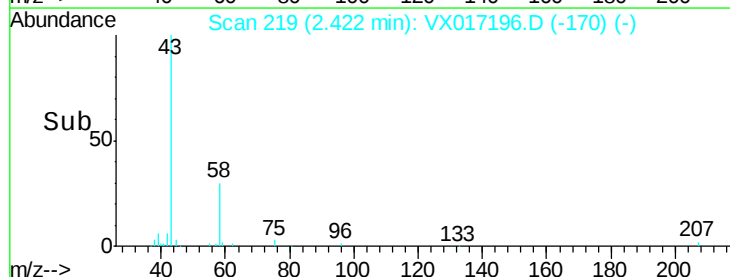




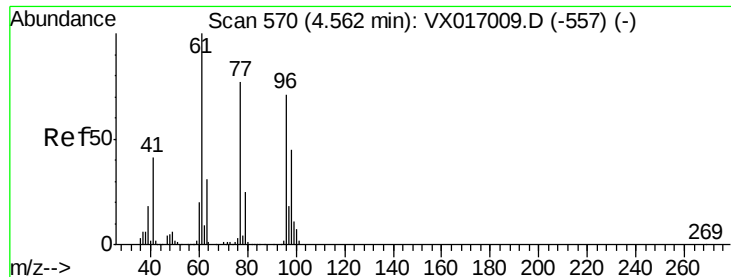


#27

cis-1,2-Dichloroethene
Concen: 6.441 ug/l
RT: 4.56 min Scan# 570
Delta R.T. -0.00 min
Lab File: VX017196.D
Acq: 07 Jul 2020 12:27

Instrument :
MSVOA_X
ClientSampleId :
PDB-BLANK-20200629




Tot Ion	96	Resp	21287
Ion	Ratio	Lower	Upper
96	100		
61	125.2	0.0	282.8
98	64.8	0.0	127.6

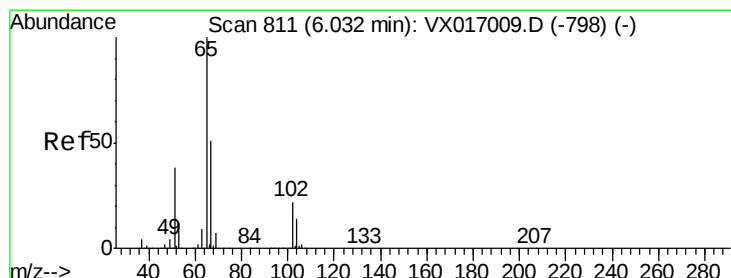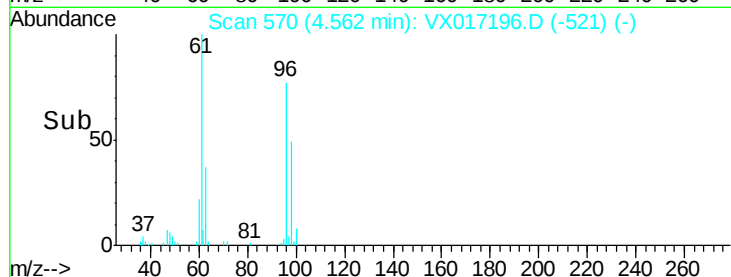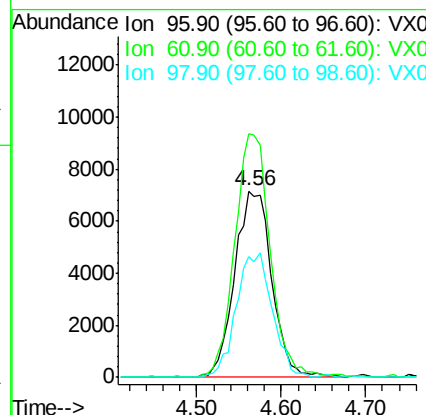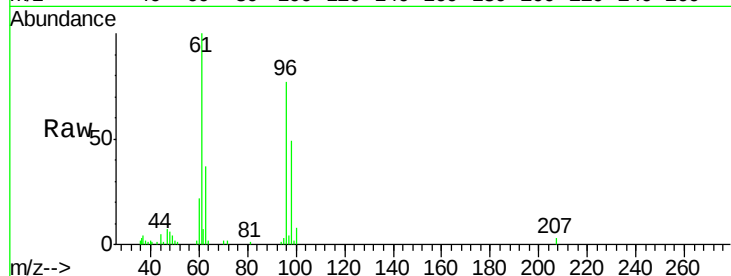


#33

1,2-Dichloroethane-d4
Concen: 52.019 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX017196.D
Acq: 07 Jul 2020 12:27

Tgt Ion	65	Resp	170373
Ion	Ratio	Lower	Upper
65	100		
67	51.3	0.0	103.8

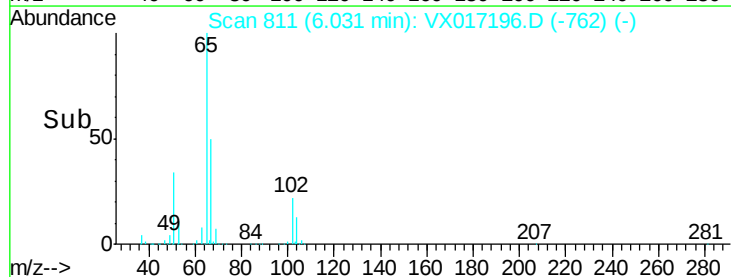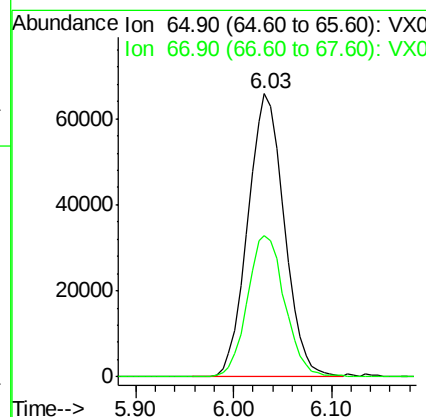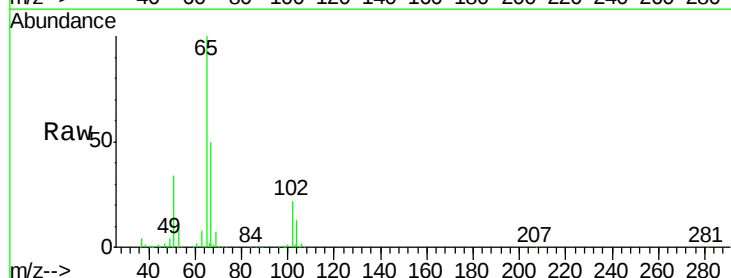

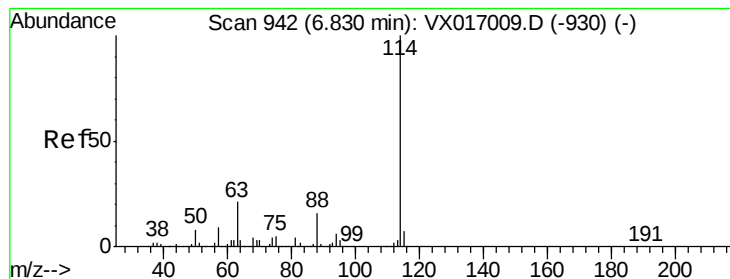

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017196.D

Acq: 07 Jul 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :

PDB-BLANK-20200629


Tot Ion:114 Resp: 439570

Ion Ratio Lower Upper

114 100

63 19.8 0.0 41.4

88 14.8 0.0 32.4

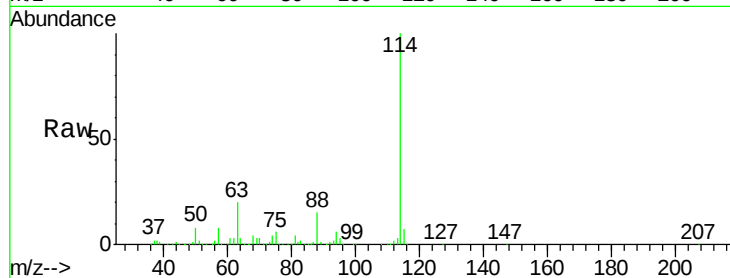

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

250000

200000

150000


100000

50000


0

6.83

6.70 6.80 6.90 7.00

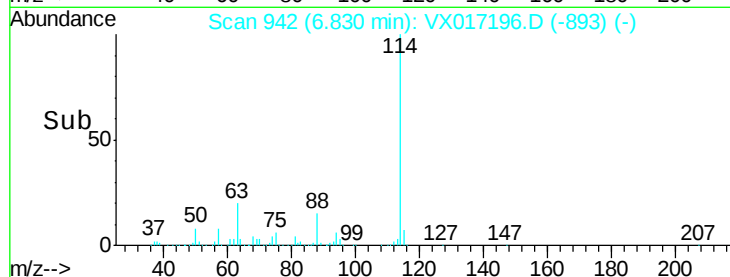

Time-->

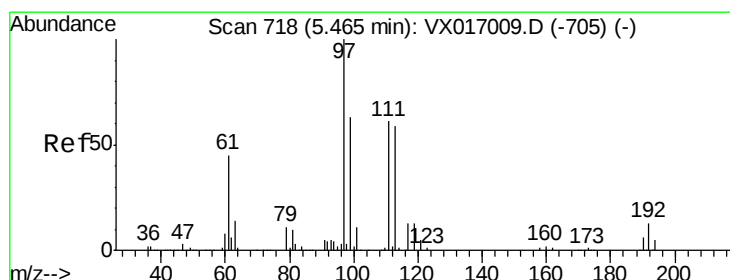

#35

Dibromofluoromethane

Concen: 52.115 ug/l

RT: 5.47 min Scan# 719

Delta R.T. 0.01 min

Lab File: VX017196.D

Acq: 07 Jul 2020 12:27


Tgt Ion:113 Resp: 144910

Ion Ratio Lower Upper

113 100

111 102.1 81.9 122.9

192 21.7 16.7 25.1

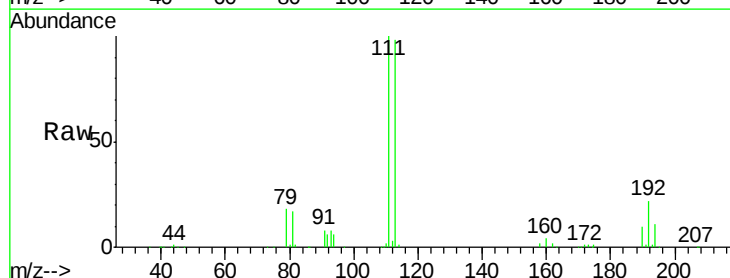

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

60000


40000

20000


0

5.47

5.30 5.40 5.50 5.60

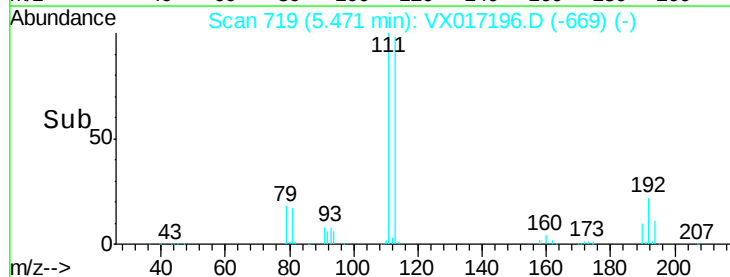

Time-->

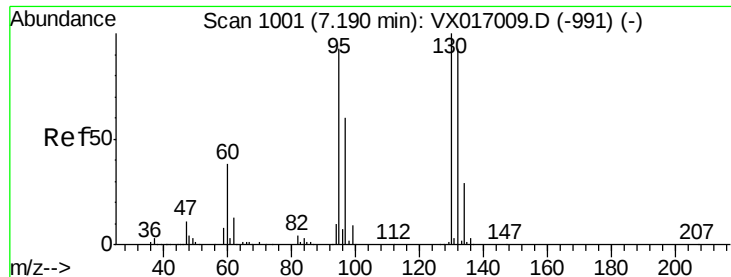

#44

Trichloroethene

Concen: 3.957 ug/l

RT: 7.19 min Scan# 1001

Delta R.T. 0.00 min

Lab File: VX017196.D

Acq: 07 Jul 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :


PDB-BLANK-20200629

Tot Ion:130 Resp: 14288

Ion Ratio Lower Upper




130 100

95 94.2 0.0 185.0

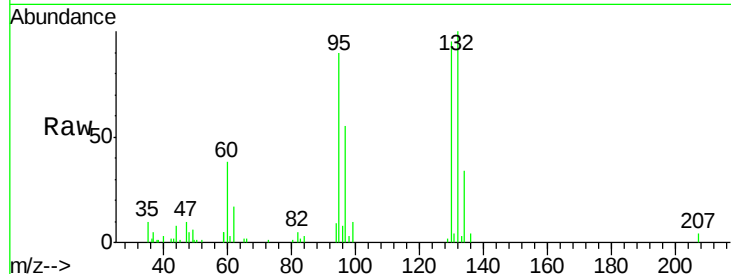

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

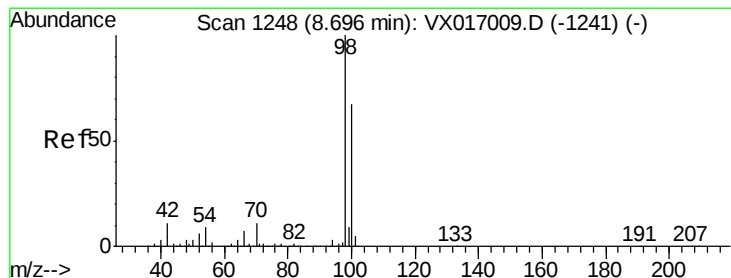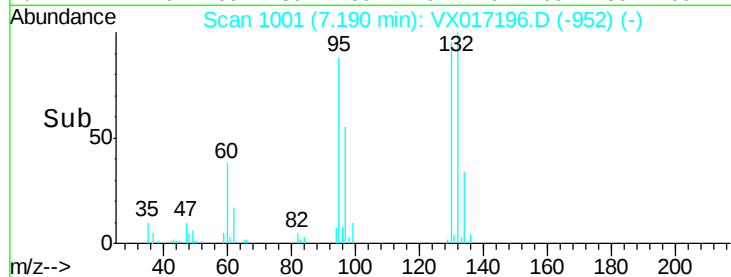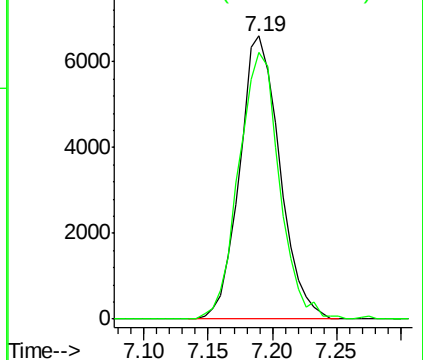

#50

Toluene-d8

Concen: 51.534 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017196.D


Acq: 07 Jul 2020 12:27

Tgt Ion: 98 Resp: 529875

Ion Ratio Lower Upper



98 100


100 66.6 53.8 80.6

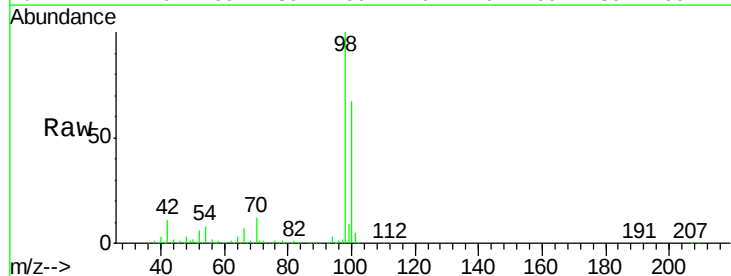

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

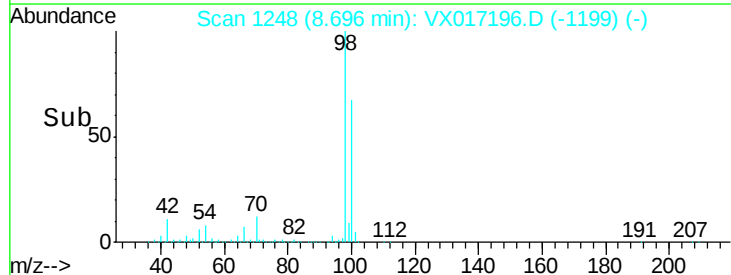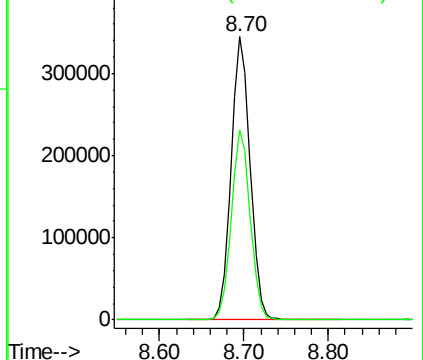

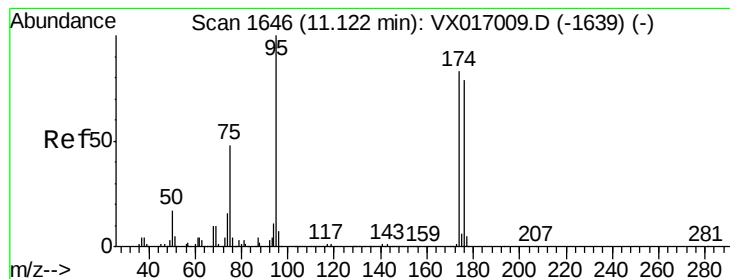

#62

4-Bromofluorobenzene

Concen: 52.446 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX017196.D

Acq: 07 Jul 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :

PDB-BLANK-20200629


Tot Ion: 95 Resp: 210802

Ion Ratio Lower Upper

95 100

174 87.5 0.0 164.0




176 81.7 0.0 157.6

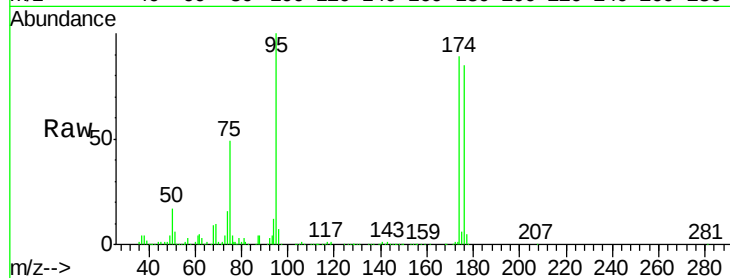

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): VX0

Ion 175.80 (175.50 to 176.50): VX0

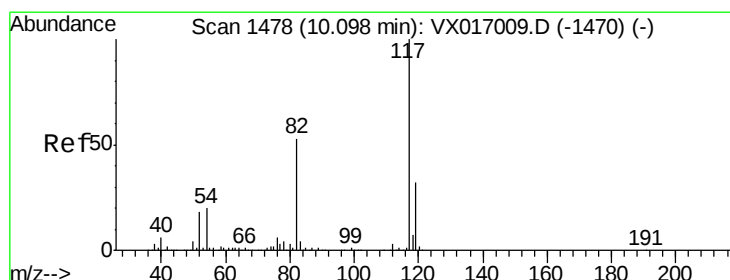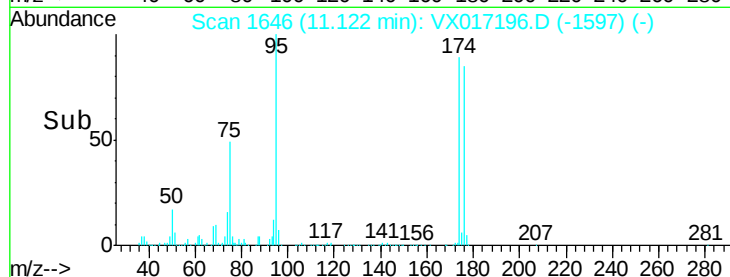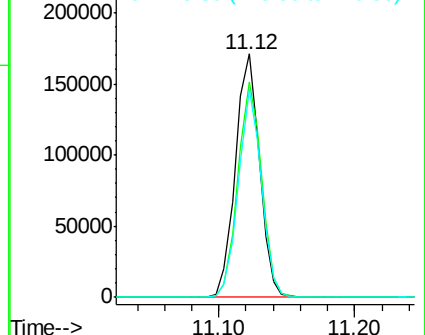

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX017196.D

Acq: 07 Jul 2020 12:27


Tgt Ion: 117 Resp: 444561

Ion Ratio Lower Upper

117 100

82 55.2 42.6 63.8



119 32.7 25.4 38.2

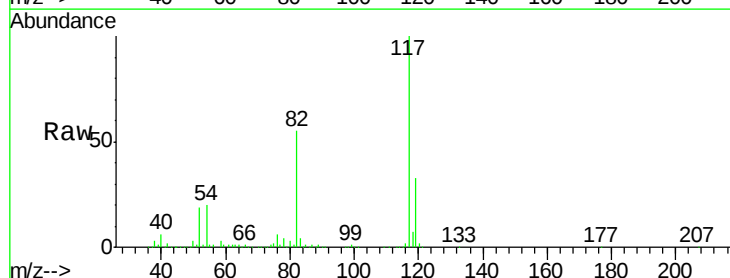


Abundance Ion 116.90 (116.60 to 117.60): VX0

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): VX0

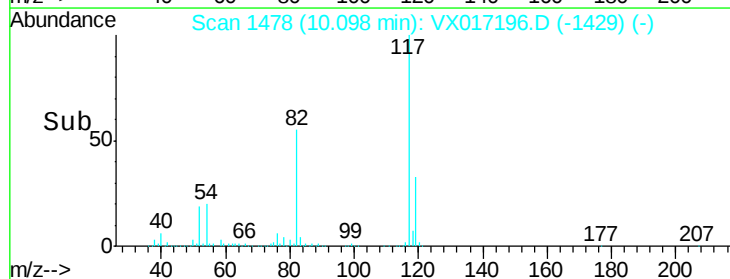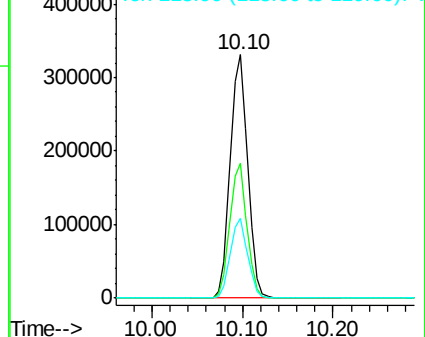

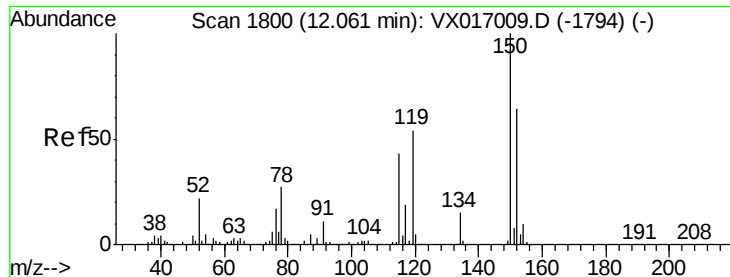

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX017196.D

Acq: 07 Jul 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :

PDB-BLANK-20200629


Tot Ion:152 Resp: 227249

Ion Ratio Lower Upper

152 100

115 57.4 40.9 122.7

150 154.6 0.0 351.6

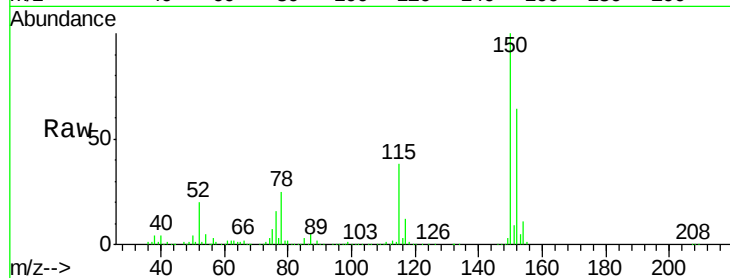

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

