

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070721\
 Data File : VX023176.D
 Acq On : 07 Jul 2021 16:39
 Operator : JC/MD
 Sample : M2953-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 08 03:21:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 02 14:29:42 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	218776	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	361930	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	328854	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	138550	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.971	65	155412	52.855	ug/l	0.00
Spiked Amount	50.000	Range 78 - 117	Recovery	= 105.700%		
35) Dibromofluoromethane	5.397	113	118182	50.566	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 101.140%		
50) Toluene-d8	8.653	98	435439	49.946	ug/l	0.00
Spiked Amount	50.000	Range 92 - 112	Recovery	= 99.900%		
62) 4-Bromofluorobenzene	11.085	95	158844	47.194	ug/l	0.00
Spiked Amount	50.000	Range 83 - 123	Recovery	= 94.380%		
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.148	85	6065	3.060	ug/l	99
3) Chloromethane	1.301	50	428	0.218	ug/l	94
4) Vinyl Chloride	1.374	62	7285	3.506	ug/l	99
5) Bromomethane	1.612	94	214	Below Cal		87
6) Chloroethane	1.691	64	274	0.202	ug/l #	1
9) 1,1,2-Trichlorotrifluo...	2.331	101	21035	9.955	ug/l	98
11) Tert butyl alcohol	2.983	59	185	0.299	ug/l #	73
12) 1,1-Dichloroethene	2.325	96	139294	71.426	ug/l	98
13) Acrolein	2.227	56	123	0.299	ug/l #	1
16) Acetone	2.392	43	3484	2.995	ug/l #	76
20) Methylene Chloride	2.800	84	739	0.295	ug/l #	68
21) trans-1,2-Dichloroethene	3.099	96	30485	14.474	ug/l	93
24) 1,1-Dichloroethane	3.617	63	450354	111.563	ug/l	98
27) cis-1,2-Dichloroethene	4.501	96	1394844	546.759	ug/l	93
31) Cyclohexane	5.568	56	4977	1.414	ug/l #	27
36) 1,1-Dichloropropene	5.562	75	17297	5.361	ug/l #	50
38) Carbon Tetrachloride	5.562	117	23548	6.992	ug/l #	18
39) Methylcyclohexane	7.141	83	123631	32.761	ug/l #	1
40) Benzene	6.050	78	8047	0.859	ug/l	99
42) 1,2-Dichloroethane	6.099	62	63592	16.894	ug/l	96
44) Trichloroethene	7.141	130	9633895	3625.287	ug/l	100
49) 1,4-Dioxane	7.665	88	8833	136.619	ug/l	98
51) 4-Methyl-2-Pentanone	8.653	43	2152	0.593	ug/l #	1
55) 1,1,2-Trichloroethane	9.159	97	1149	0.451	ug/l	98
60) Dibromochloromethane	9.275	129	12316	7.175	ug/l #	11
64) Tetrachloroethene	9.281	164	12477	4.757	ug/l	92
76) 1,2,3-Trichloropropane	11.085	75	83485	29.943	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.085	75	83485	80.407	ug/l #	12
87) 1,3-Dichlorobenzene	12.043	146	11653	2.546	ug/l #	80
88) 1,4-Dichlorobenzene	12.043	146	11653	2.529	ug/l #	79
91) 1,2-Dichlorobenzene	12.341	146	4771	1.048	ug/l	92
95) Naphthalene	13.780	128	236	1.298	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070721\
Data File : VX023176.D
Acq On : 07 Jul 2021 16:39
Operator : JC/MD
Sample : M2953-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 08 03:21:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 02 14:29:42 2021
Response via : Initial Calibration




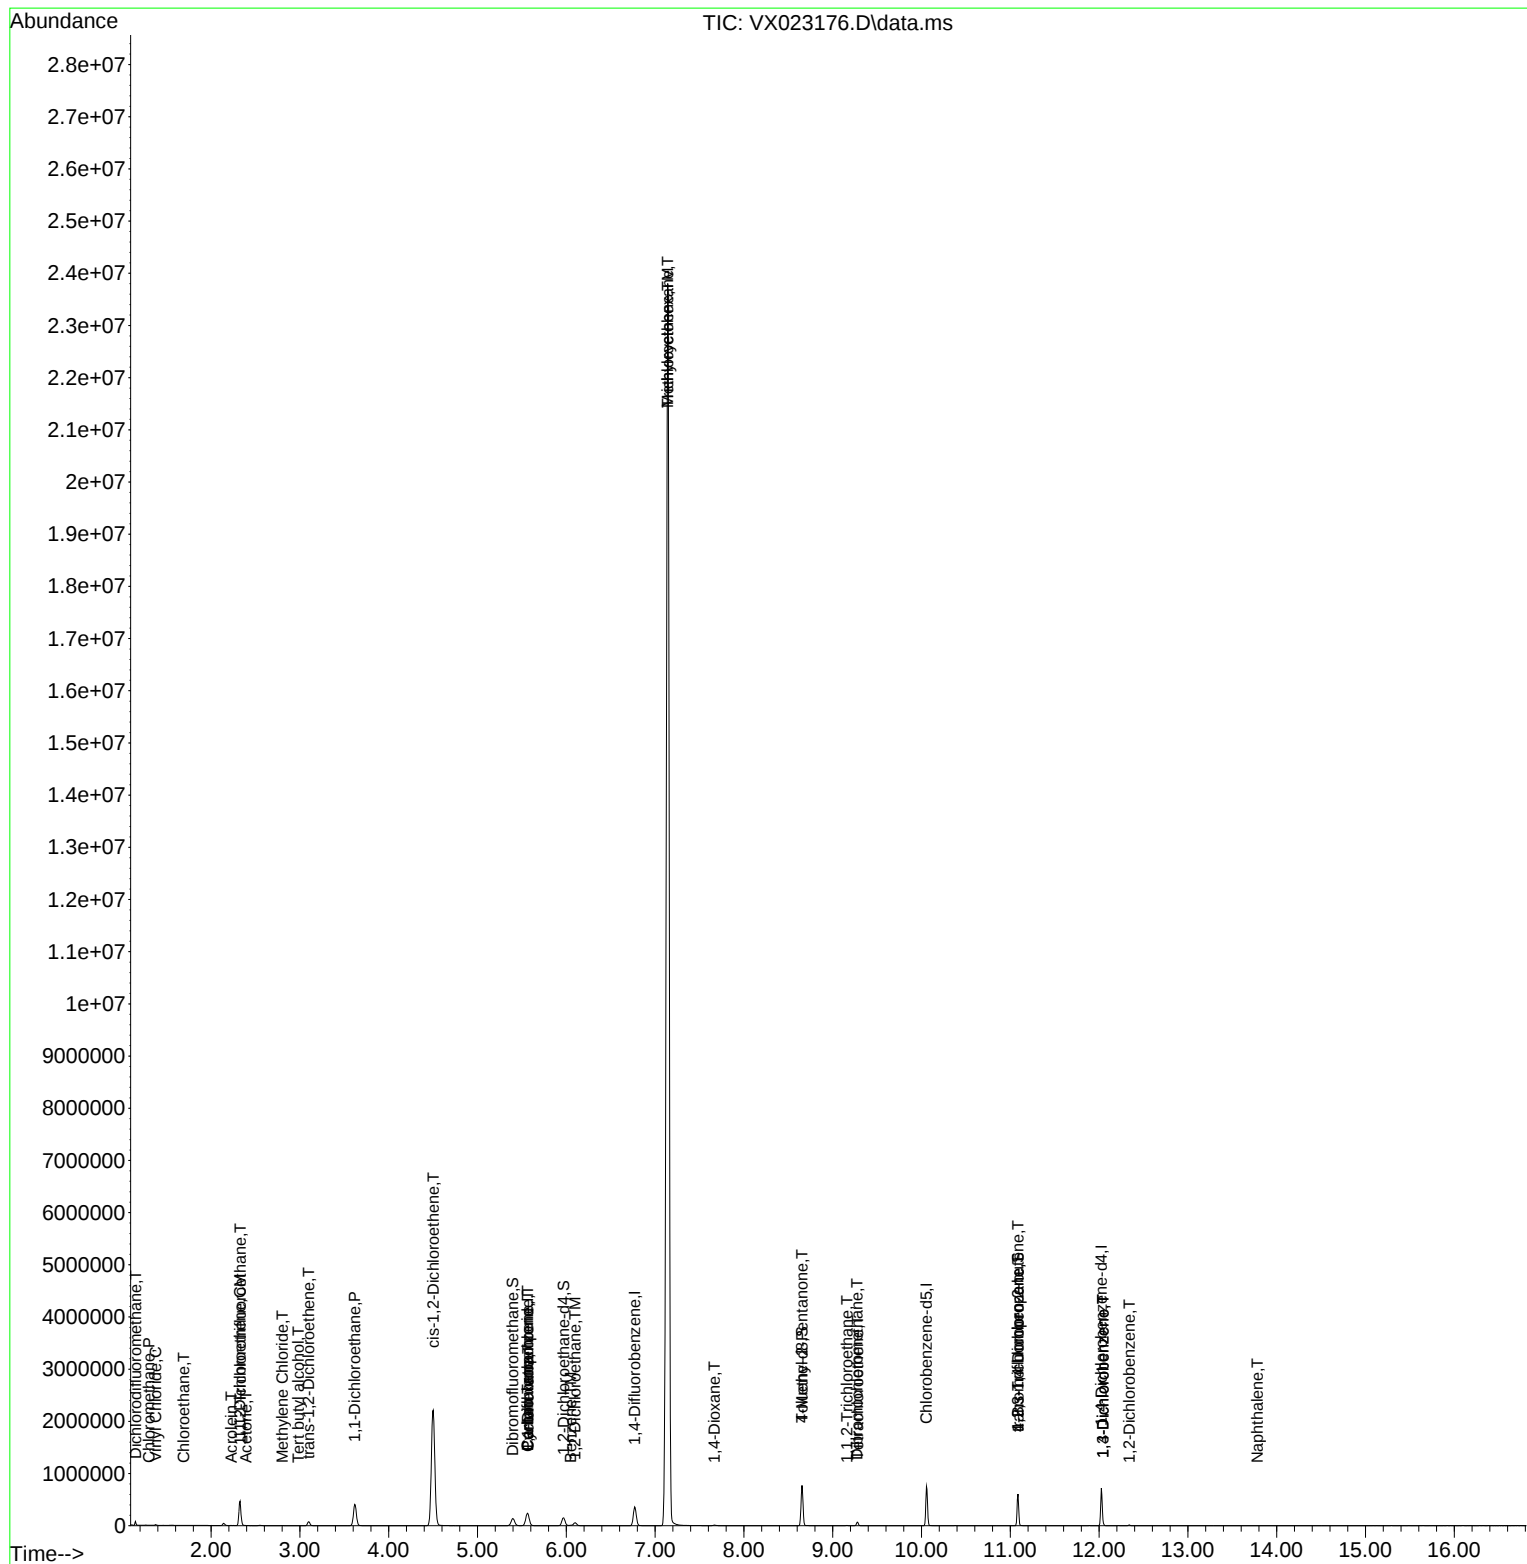




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 218776
Ion Ratio Lower Upper
168 100
99 61.6 45.8 68.6

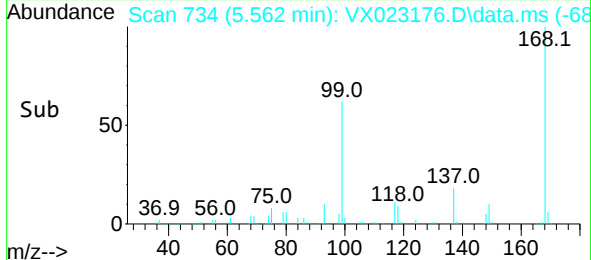

#2
Dichlorodifluoromethane
Concen: 3.060 ug/l
RT: 1.148 min Scan# 10
Delta R.T. -0.024 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 85 Resp: 6065
Ion Ratio Lower Upper
85 100
87 33.1 16.4 49.2


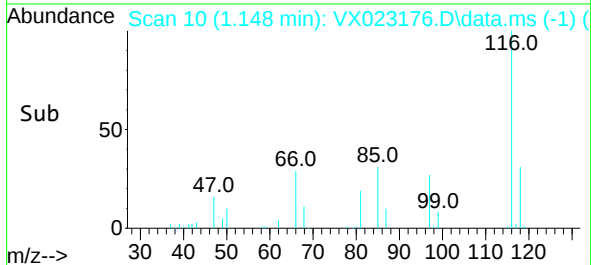

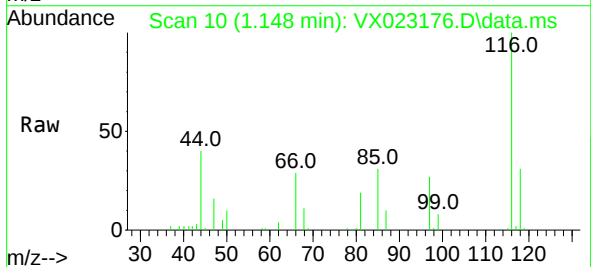


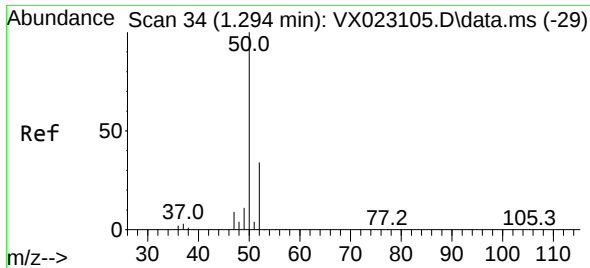

#3
Chloromethane
Concen: 0.218 ug/l
RT: 1.301 min Scan# 35
Delta R.T. 0.007 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 50 Resp: 428
Ion Ratio Lower Upper
50 100
52 36.6 26.4 39.6

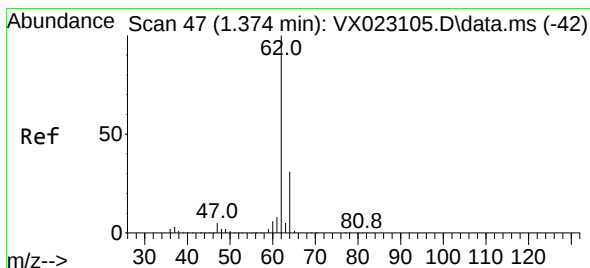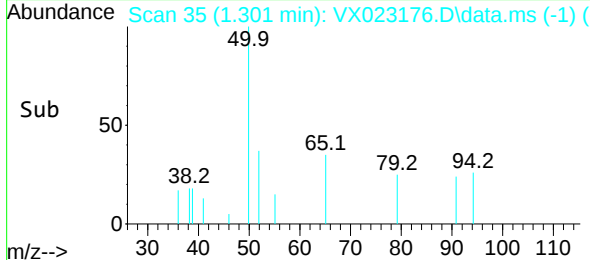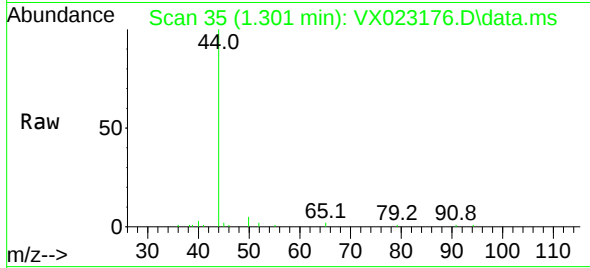

#4
Vinyl Chloride
Concen: 3.506 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 62 Resp: 7285
Ion Ratio Lower Upper
62 100
64 31.6 25.7 38.5


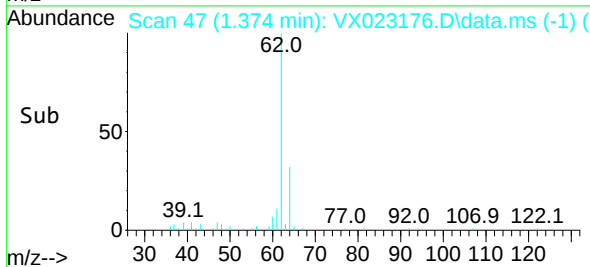

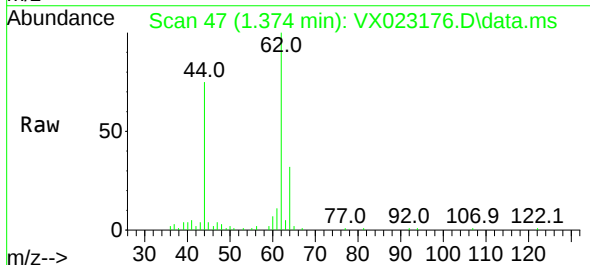


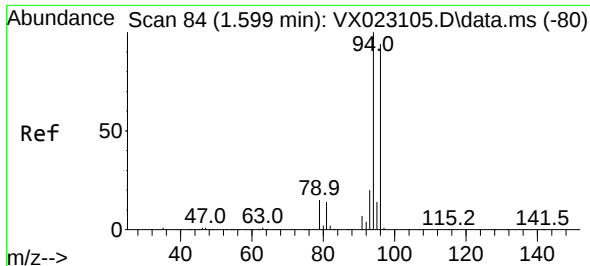

#5
Bromomethane
Concen: Below Cal
RT: 1.612 min Scan# 86
Delta R.T. 0.013 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 94 Resp: 214
Ion Ratio Lower Upper
94 100
96 108.2 76.4 114.6

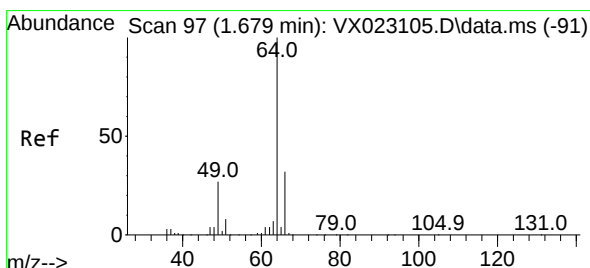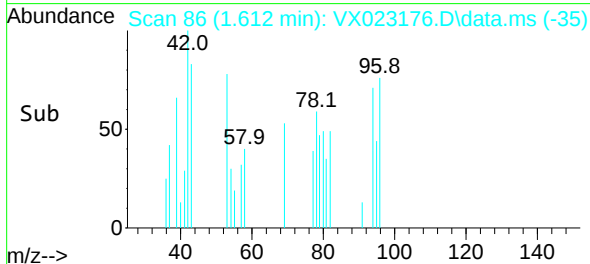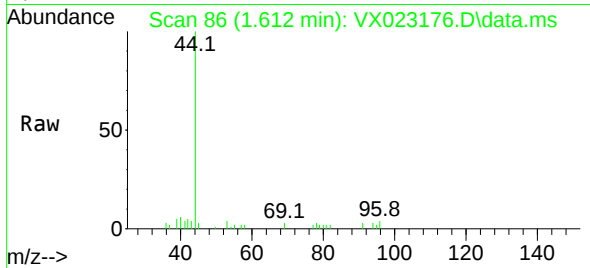

#6
Chloroethane
Concen: 0.202 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.012 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 64 Resp: 274
Ion Ratio Lower Upper
64 100
66 115.7 25.4 38.0#


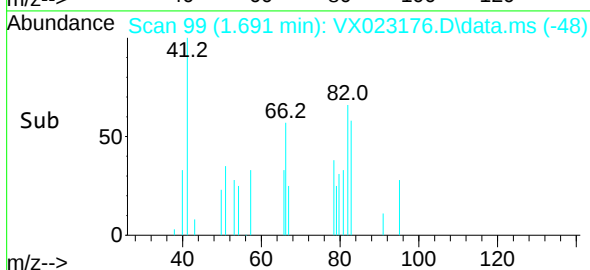

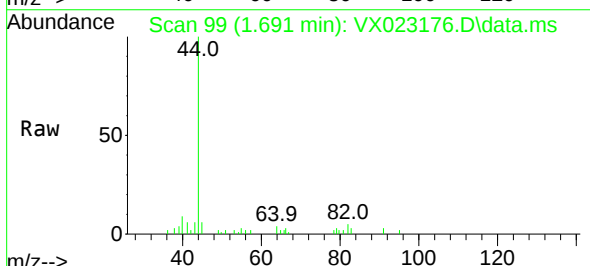




#9
1,1,2-Trichlorotrifluoroethane
Concen: 9.955 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:101 Resp: 21035
Ion Ratio Lower Upper
101 100
85 44.5 34.9 52.3
151 74.7 61.4 92.2

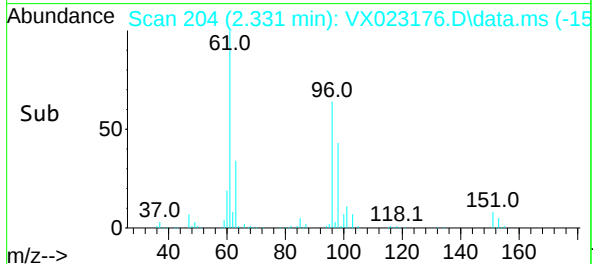

#11
Tert butyl alcohol
Concen: 0.299 ug/l
RT: 2.983 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 59 Resp: 185
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

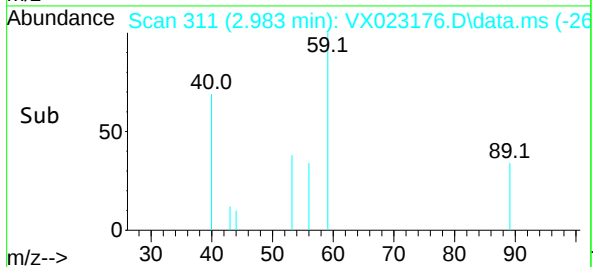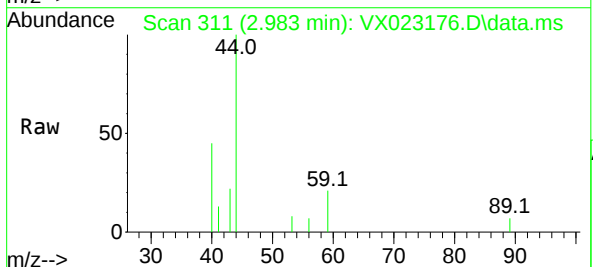



#12

1,1-Dichloroethene

Concen: 71.426 ug/l

RT: 2.325 min Scan# 203





Delta R.T. 0.006 min

Lab File: VX023176.D

Acq: 07 Jul 2021 16:39

Tgt Ion: 96 Resp: 139294

Ion	Ratio	Lower	Upper
96	100		
61	158.5	124.6	187.0
98	64.0	50.6	76.0

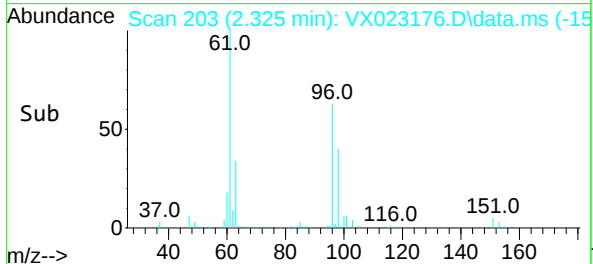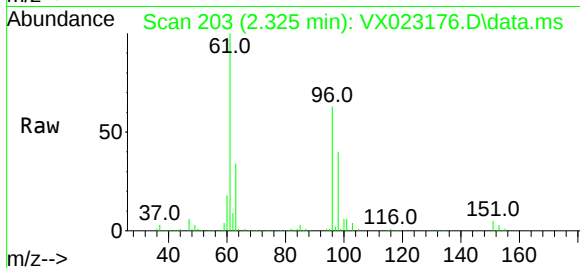

#13

Acrolein

Concen: 0.299 ug/l

RT: 2.227 min Scan# 187




Delta R.T. -0.018 min


Lab File: VX023176.D

Acq: 07 Jul 2021 16:39

Tgt Ion: 56 Resp: 123

Ion	Ratio	Lower	Upper
56	100		
55	248.0	56.4	84.6#


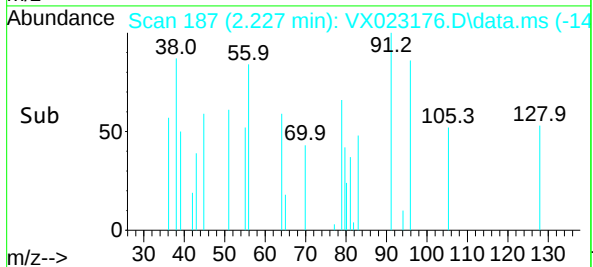

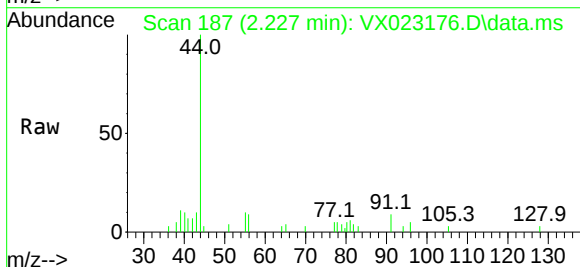




#16
Acetone
Concen: 2.995 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 3484
Ion Ratio Lower Upper
43 100
58 20.7 27.8 41.8#

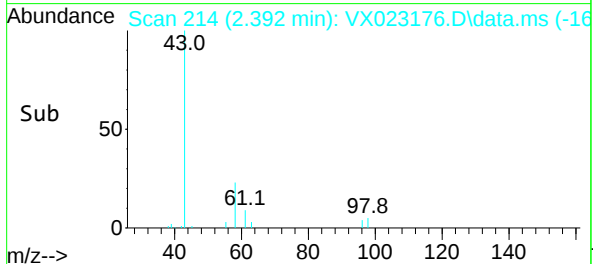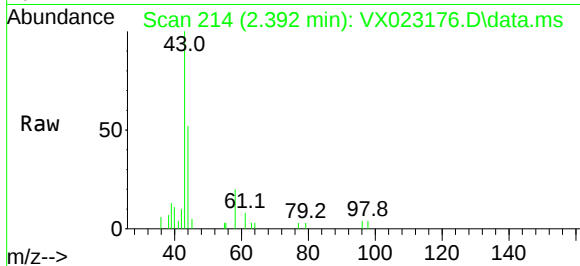

#20
Methylene Chloride
Concen: 0.295 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 84 Resp: 739
Ion Ratio Lower Upper
84 100
49 74.3 88.6 132.8#
51 27.2 27.0 40.6
86 32.8 50.3 75.5#


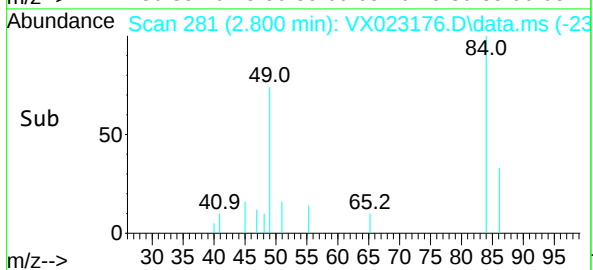

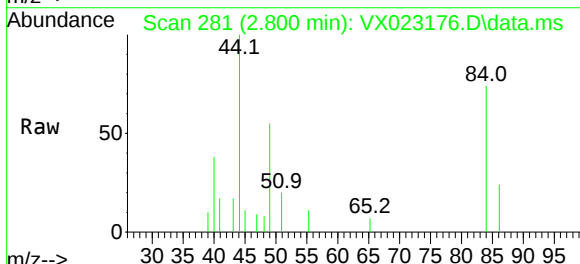




#21
trans-1,2-Dichloroethene
Concen: 14.474 ug/l
RT: 3.099 min Scan# 330
Delta R.T. 0.006 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 96 Resp: 30485
Ion Ratio Lower Upper
96 100
61 145.0 107.7 161.5
98 66.1 50.4 75.6

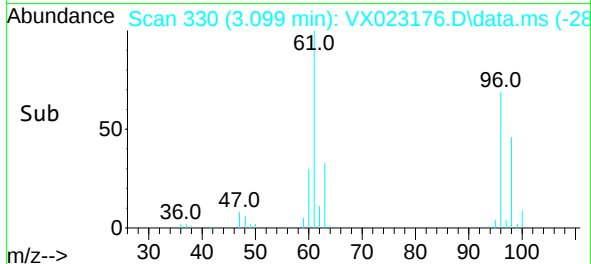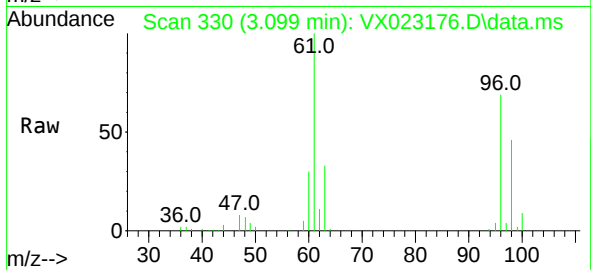

#24
1,1-Dichloroethane
Concen: 111.563 ug/l
RT: 3.617 min Scan# 415
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 63 Resp: 450354
Ion Ratio Lower Upper
63 100
98 6.6 3.8 11.2
100 4.3 2.5 7.5

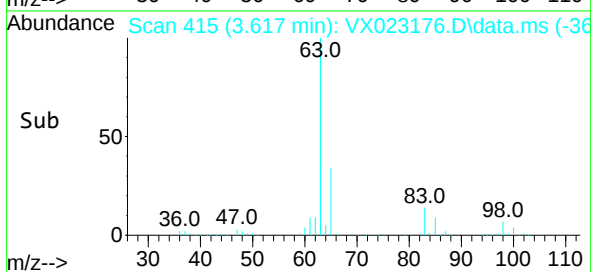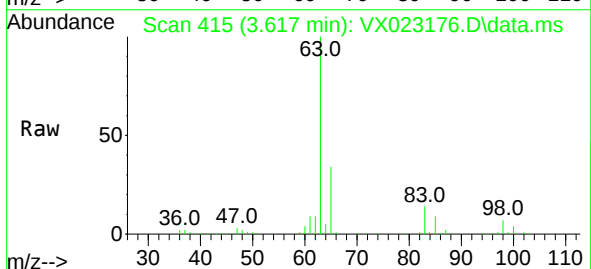

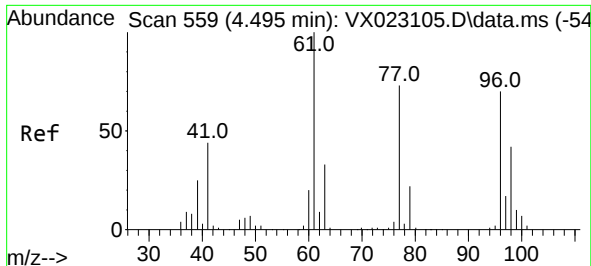

#27

cis-1,2-Dichloroethene

Concen: 546.759 ug/l

RT: 4.501 min Scan# 560

Delta R.T. 0.006 min





Lab File: VX023176.D

Acq: 07 Jul 2021 16:39

Tgt Ion: 96 Resp: 1394844

Ion	Ratio	Lower	Upper
96	100		
61	129.9	0.0	285.6
98	64.7	0.0	129.6

Instrument :
MSVOA_X
ClientSampleId :

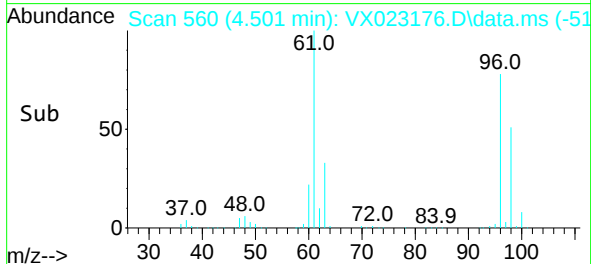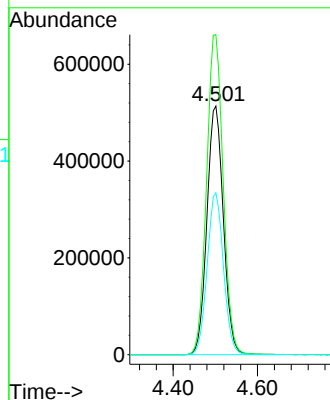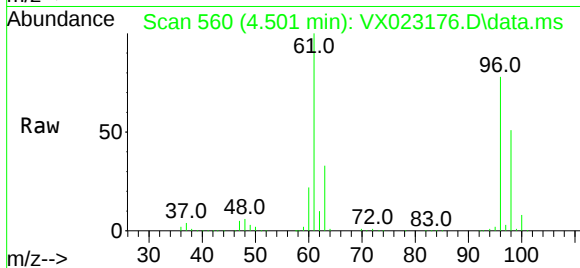

#31

Cyclohexane

Concen: 1.414 ug/l

RT: 5.568 min Scan# 735




Delta R.T. 0.091 min


Lab File: VX023176.D

Acq: 07 Jul 2021 16:39

Tgt Ion: 56 Resp: 4977

Ion	Ratio	Lower	Upper
56	100		
69	166.5	25.3	37.9#
84	101.2	71.4	107.0


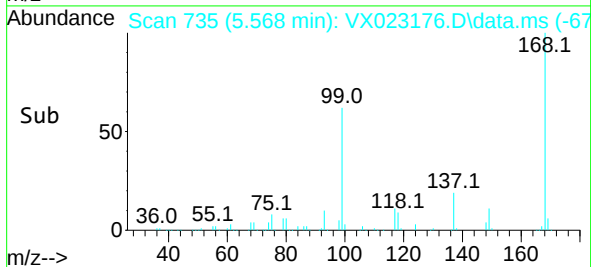
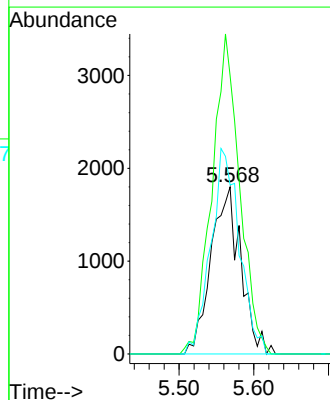
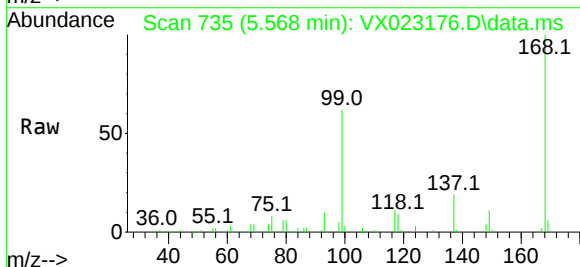




#33
 1,2-Dichloroethane-d4
 Concen: 52.855 ug/l
 RT: 5.971 min Scan# 801
 Delta R.T. 0.007 min
 Lab File: VX023176.D
 Acq: 07 Jul 2021 16:39




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 65 Resp: 155412
 Ion Ratio Lower Upper
 65 100
 67 50.0 0.0 105.4

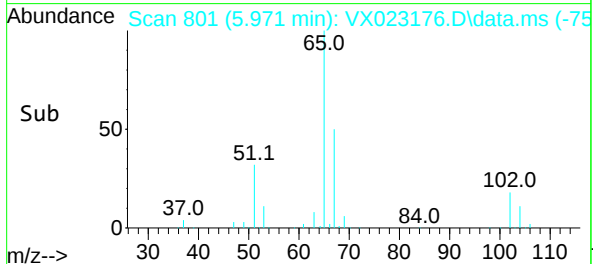

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.769 min Scan# 932
 Delta R.T. 0.000 min
 Lab File: VX023176.D
 Acq: 07 Jul 2021 16:39

Tgt Ion: 114 Resp: 361930
 Ion Ratio Lower Upper
 114 100
 63 21.2 0.0 40.8
 88 16.8 0.0 32.8


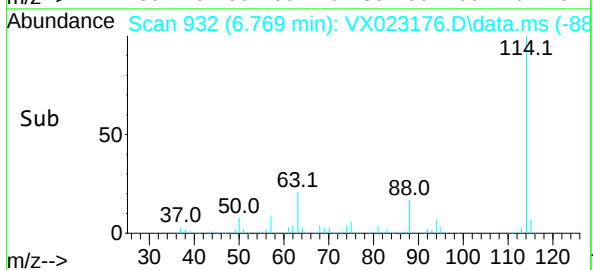

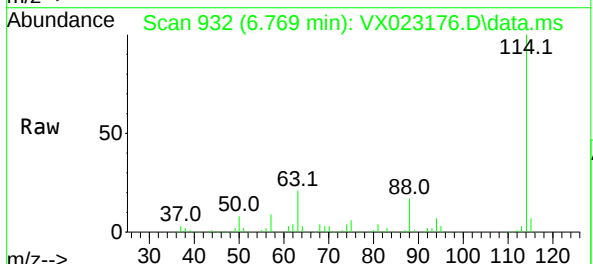




#35
Dibromofluoromethane
Concen: 50.566 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:113 Resp: 118182
Ion Ratio Lower Upper
113 100
111 101.9 81.9 122.9
192 19.1 16.7 25.1

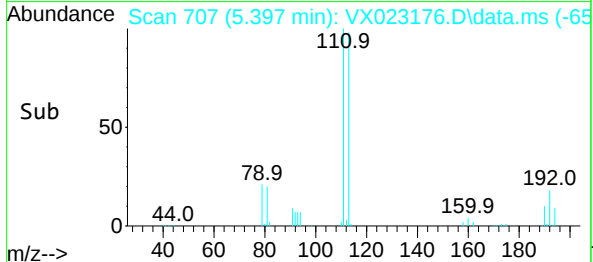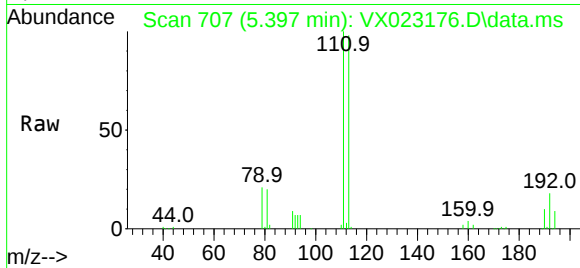

#36
1,1-Dichloropropene
Concen: 5.361 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39


Tgt Ion: 75 Resp: 17297
Ion Ratio Lower Upper
75 100
110 10.7 18.1 54.4#
77 0.0 25.3 37.9#

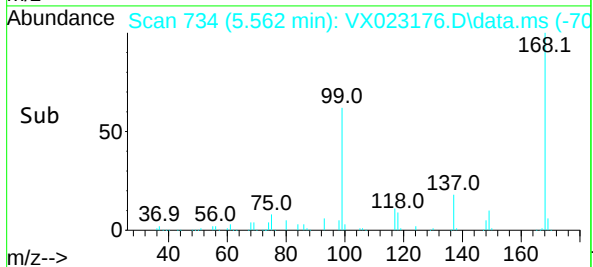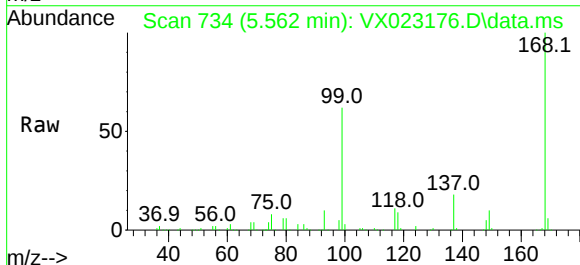






#38
Carbon Tetrachloride
Concen: 6.992 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.122 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39


Instrument :
MSVOA_X
ClientSampleId :

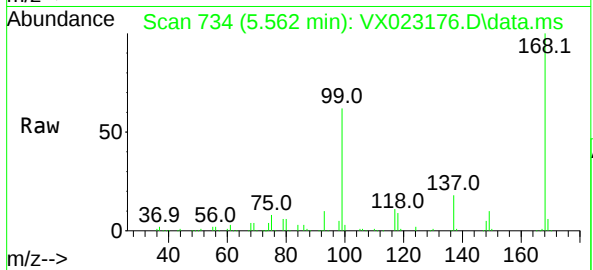



Tgt Ion:117 Resp: 23548
Ion Ratio Lower Upper
117 100
119 6.7 76.2 114.2#
121 0.0 24.8 37.2#

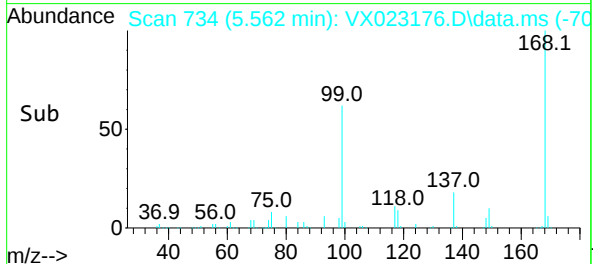


#39
Methylcyclohexane
Concen: 32.761 ug/l
RT: 7.141 min Scan# 993
Delta R.T. -0.244 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

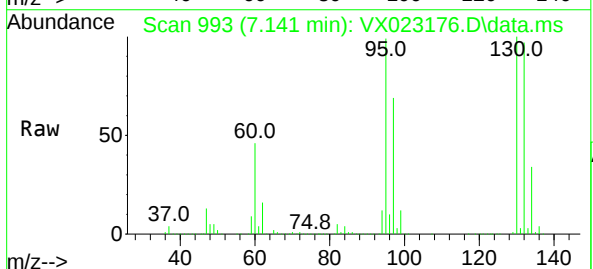

Tgt Ion: 83 Resp: 123631
Ion Ratio Lower Upper
83 100
55 0.2 58.9 88.3#
98 211.0 38.1 57.1#









#40
Benzene
Concen: 0.859 ug/l
RT: 6.050 min Scan# 814
Delta R.T. -0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 78 Resp: 8047
Ion Ratio Lower Upper
78 100
77 22.9 18.9 28.3

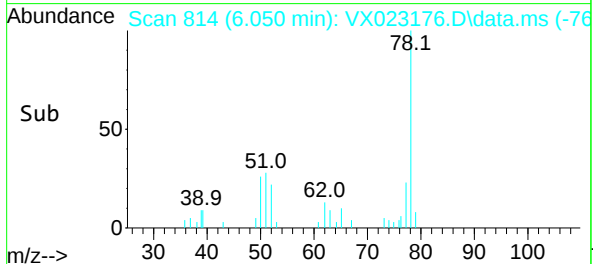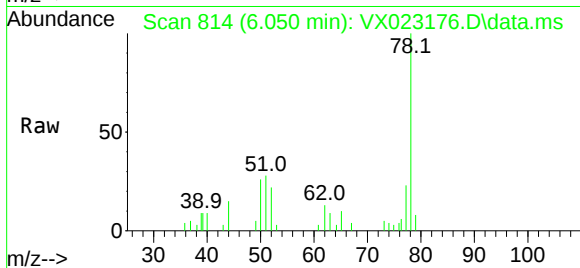

#42
1,2-Dichloroethane
Concen: 16.894 ug/l
RT: 6.099 min Scan# 822
Delta R.T. 0.001 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 62 Resp: 63592
Ion Ratio Lower Upper
62 100
98 8.6 0.0 20.2


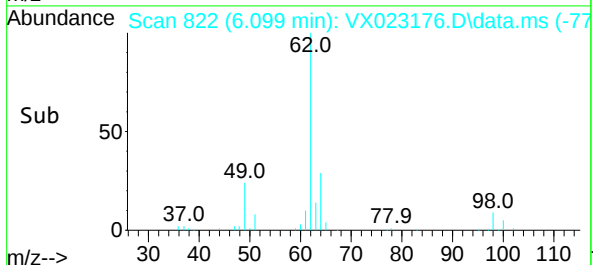

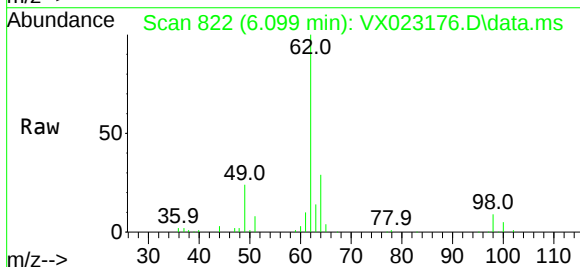




#44
Trichloroethene
Concen: 3625.287 ug/l
RT: 7.141 min Scan# 993
Delta R.T. 0.006 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:130 Resp: 9633895
Ion Ratio Lower Upper
130 100
95 99.5 0.0 198.0

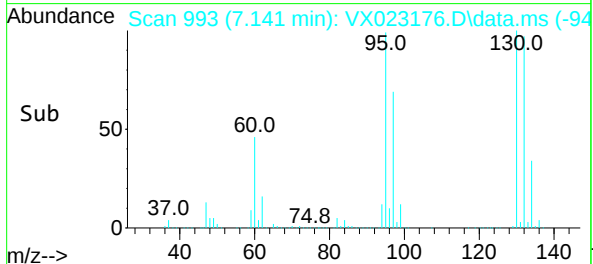

#49
1,4-Dioxane
Concen: 136.619 ug/l
RT: 7.665 min Scan# 1079
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 88 Resp: 8833
Ion Ratio Lower Upper
88 100
43 32.7 23.2 34.8
58 68.5 55.0 82.4


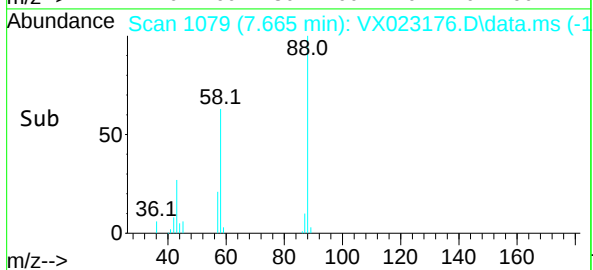

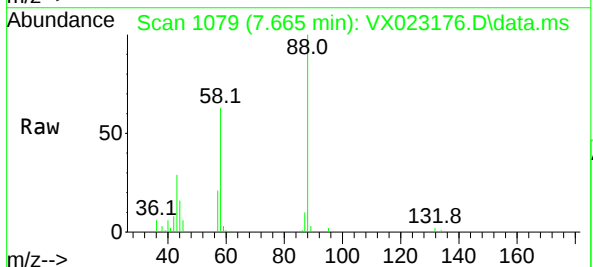




#50
Toluene-d8
Concen: 49.946 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 98 Resp: 435439
Ion Ratio Lower Upper
98 100
100 63.9 51.9 77.9

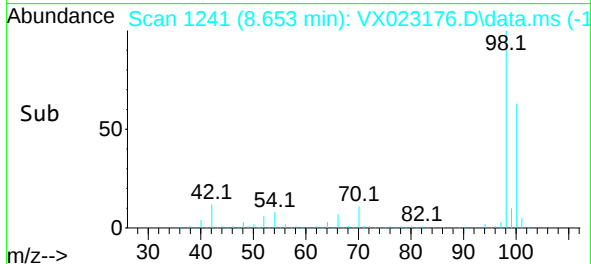

#51
4-Methyl-2-Pentanone
Concen: 0.593 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.073 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 43 Resp: 2152
Ion Ratio Lower Upper
43 100
58 161.5 35.4 53.0#

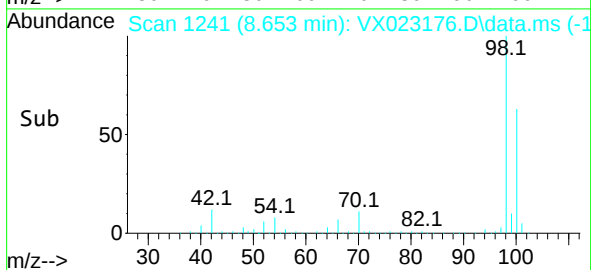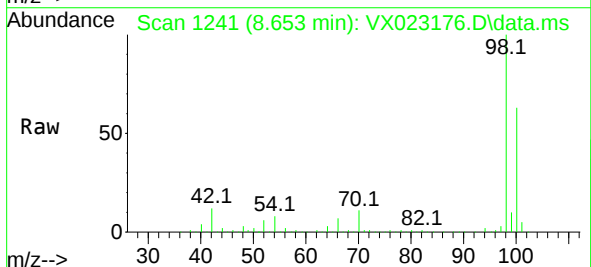



#55

1,1,2-Trichloroethane

Concen: 0.451 ug/l

RT: 9.159 min Scan# 1324

Delta R.T. -0.000 min

Lab File: VX023176.D

Acq: 07 Jul 2021 16:39

Tgt Ion: 97 Resp: 1149





Ion Ratio Lower Upper

97 100

83 86.9 69.3 103.9

85 55.9 44.3 66.5

99 59.0 50.3 75.5

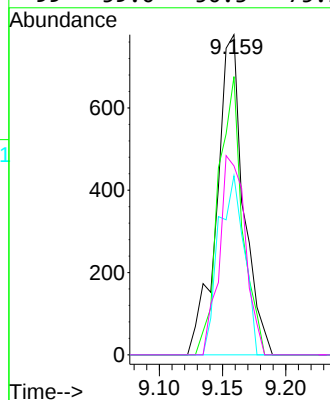

#60

Dibromochloromethane

Concen: 7.175 ug/l

RT: 9.275 min Scan# 1343

Delta R.T. -0.250 min

Lab File: VX023176.D




Acq: 07 Jul 2021 16:39

Tgt Ion: 129 Resp: 12316


Ion Ratio Lower Upper

129 100

127 0.0 38.4 115.2#

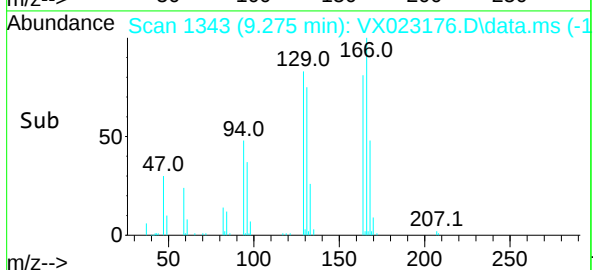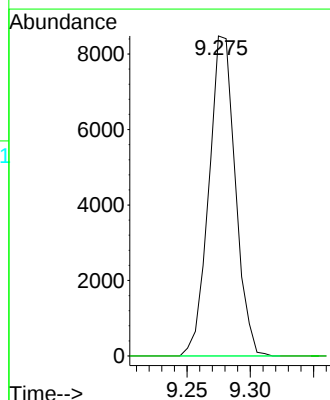





Instrument :
MSVOA_X
ClientSampled :

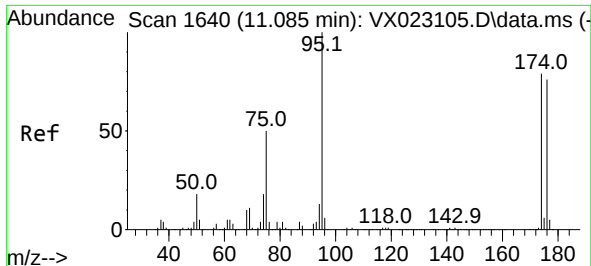

#62
4-Bromofluorobenzene
Concen: 47.194 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 95 Resp: 158844
Ion Ratio Lower Upper
95 100
174 76.4 0.0 154.6
176 73.6 0.0 155.8

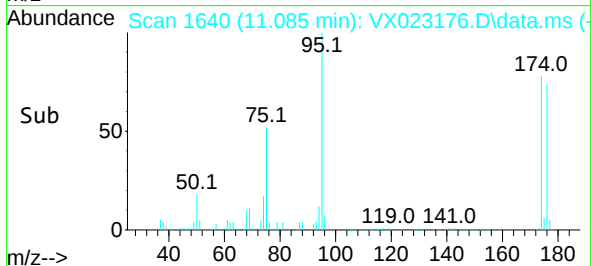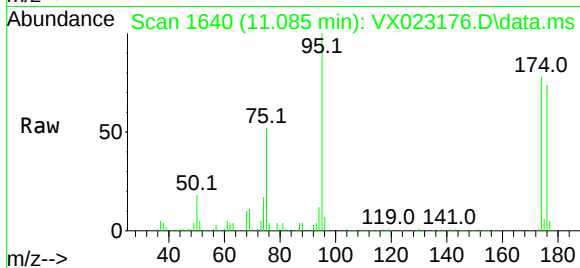

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39


Tgt Ion: 117 Resp: 328854
Ion Ratio Lower Upper
117 100
82 59.7 47.4 71.2
119 32.5 26.6 39.8

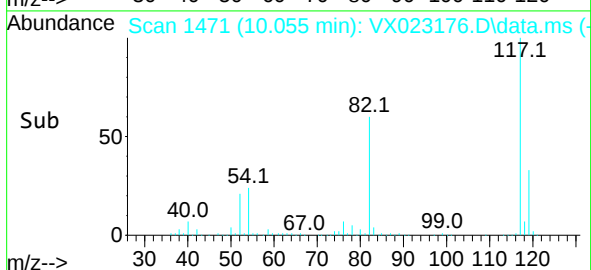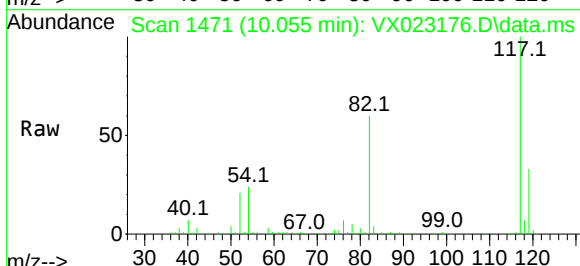



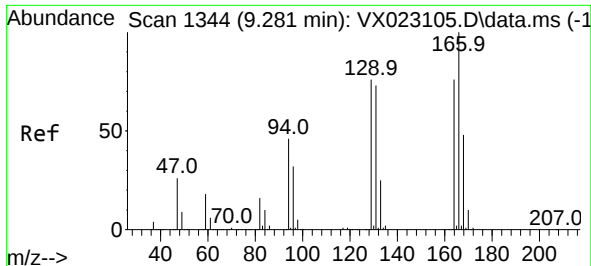


#64
Tetrachloroethene
Concen: 4.757 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:164	Resp:	12477
Ion	Ratio	Lower Upper
164	100	
166	120.7	103.4 155.2
129	98.9	70.8 106.2
131	95.7	72.5 108.7

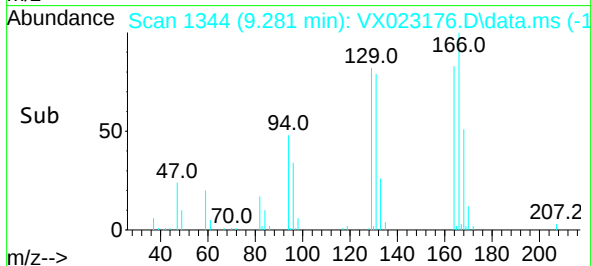


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

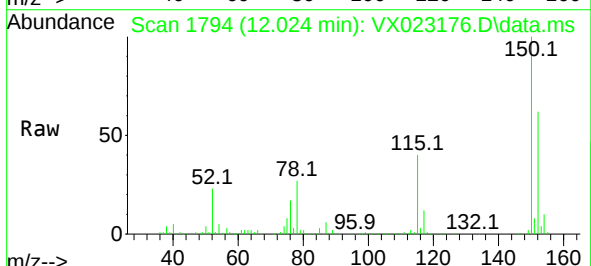

Tgt Ion:152	Resp:	138550
Ion	Ratio	Lower Upper
152	100	
115	61.9	41.1 123.3
150	157.7	0.0 349.0




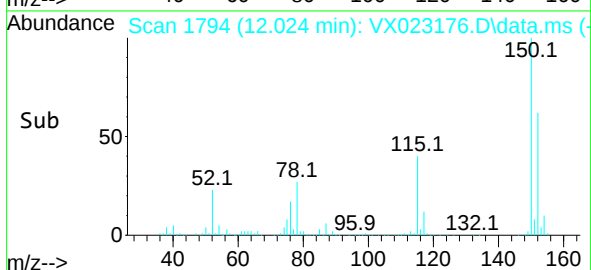


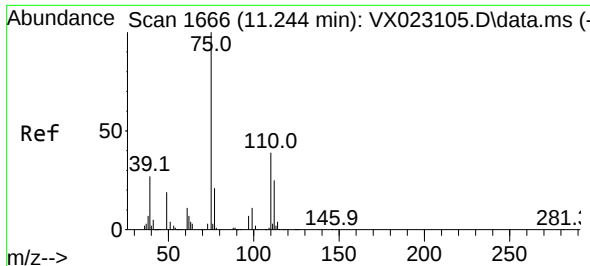

#76
1,2,3-Trichloropropane
Concen: 29.943 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 83485
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#

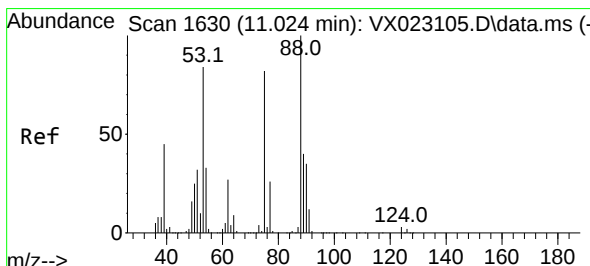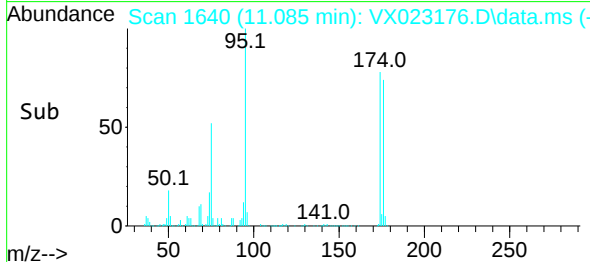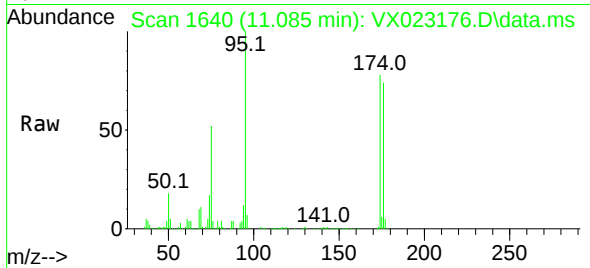

#81
trans-1,4-Dichloro-2-butene
Concen: 80.407 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion: 75 Resp: 83485
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#


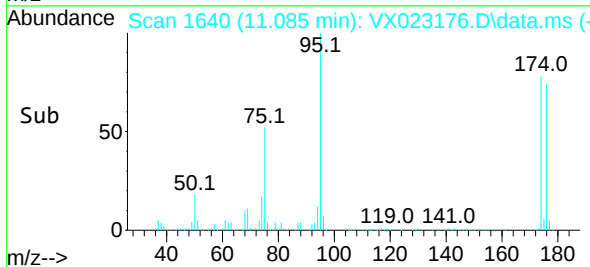

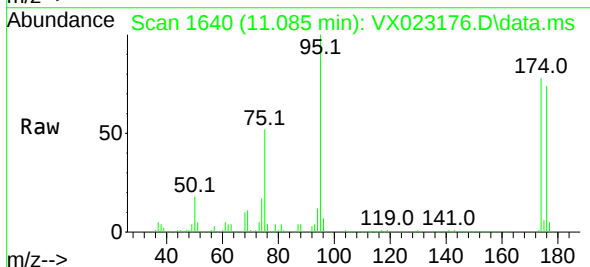


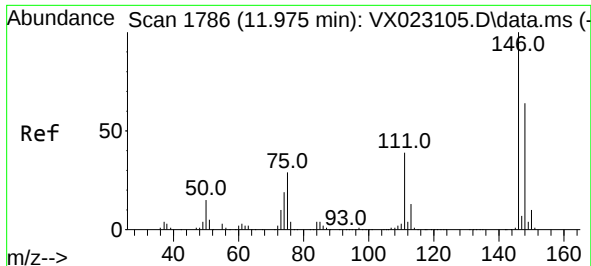

#87
1,3-Dichlorobenzene
Concen: 2.546 ug/l
RT: 12.043 min Scan# 1797
Delta R.T. 0.068 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:146 Resp: 11653
Ion Ratio Lower Upper
146 100
111 61.4 20.2 60.5#
148 72.4 31.9 95.7

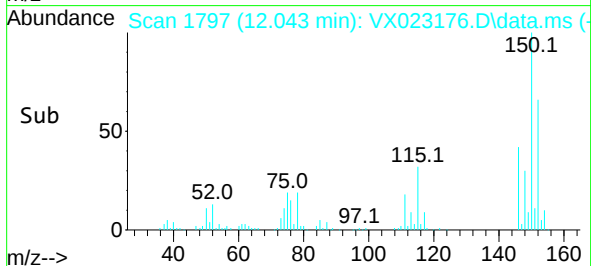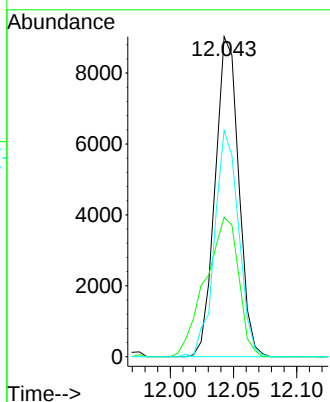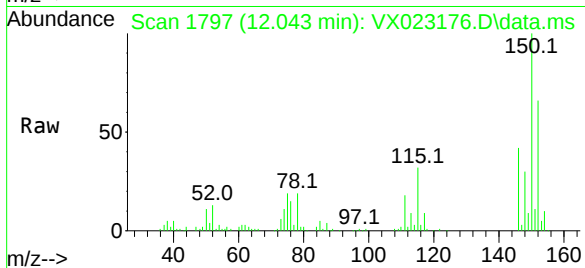

#88
1,4-Dichlorobenzene
Concen: 2.529 ug/l
RT: 12.043 min Scan# 1797
Delta R.T. 0.001 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion:146 Resp: 11653
Ion Ratio Lower Upper
146 100
111 61.4 19.6 58.8#
148 72.4 31.6 95.0


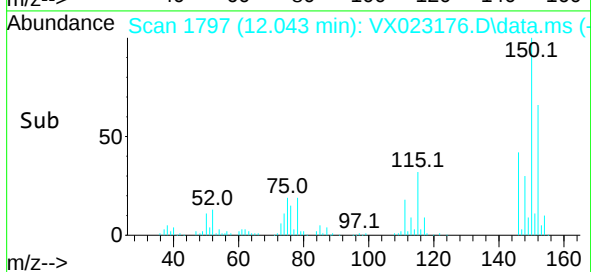
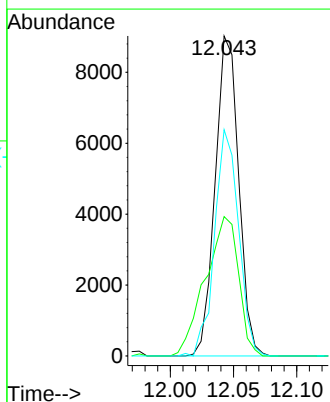
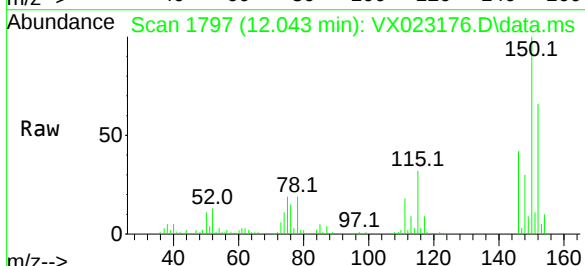


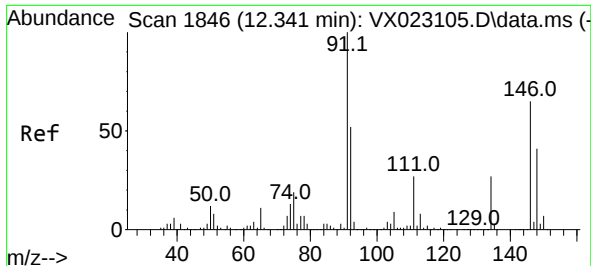

#91
1,2-Dichlorobenzene
Concen: 1.048 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Instrument :
MSVOA_X
ClientSampled :

Tgt Ion:146 Resp: 4771
Ion Ratio Lower Upper
146 100
111 37.5 20.8 62.2
148 56.0 31.9 95.5

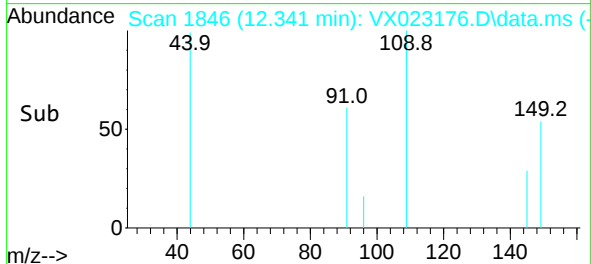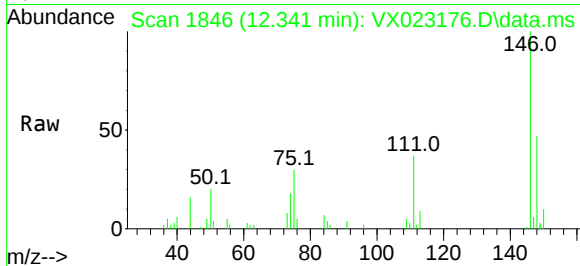

#95
Naphthalene
Concen: 1.298 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX023176.D
Acq: 07 Jul 2021 16:39

Tgt Ion:128 Resp: 236
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 0.0 8.8 13.2#

