

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070721\  
 Data File : VX023174.D  
 Acq On : 07 Jul 2021 15:51  
 Operator : JC/MD  
 Sample : M2948-03  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X070221W.M

Title : SW846 8260

Signal : TIC: VX023174.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.397       | 693           | 707         | 723          | rBV2     | 134975         | 387102        | 33.57%          | 6.396%        |
| 2         | 5.562       | 723           | 734         | 748          | rVV      | 240019         | 675077        | 58.54%          | 11.154%       |
| 3         | 5.964       | 788           | 800         | 814          | rBV      | 149874         | 402290        | 34.88%          | 6.647%        |
| 4         | 6.769       | 922           | 932         | 947          | rBV      | 369126         | 866003        | 75.09%          | 14.309%       |
| 5         | 8.653       | 1231          | 1241        | 1255         | rBV      | 736140         | 1153231       | 100.00%         | 19.055%       |
| 6         | 10.055      | 1465          | 1471        | 1484         | rBV      | 707100         | 986561        | 85.55%          | 16.301%       |
| 7         | 11.085      | 1634          | 1640        | 1652         | rBV      | 589239         | 742002        | 64.34%          | 12.260%       |
| 8         | 12.024      | 1789          | 1794        | 1803         | rBV      | 677378         | 839810        | 72.82%          | 13.876%       |




Sum of corrected areas: 6052076

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070721\  
Data File : VX023174.D  
Acq On : 07 Jul 2021 15:51  
Operator : JC/MD  
Sample : M2948-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X070221W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

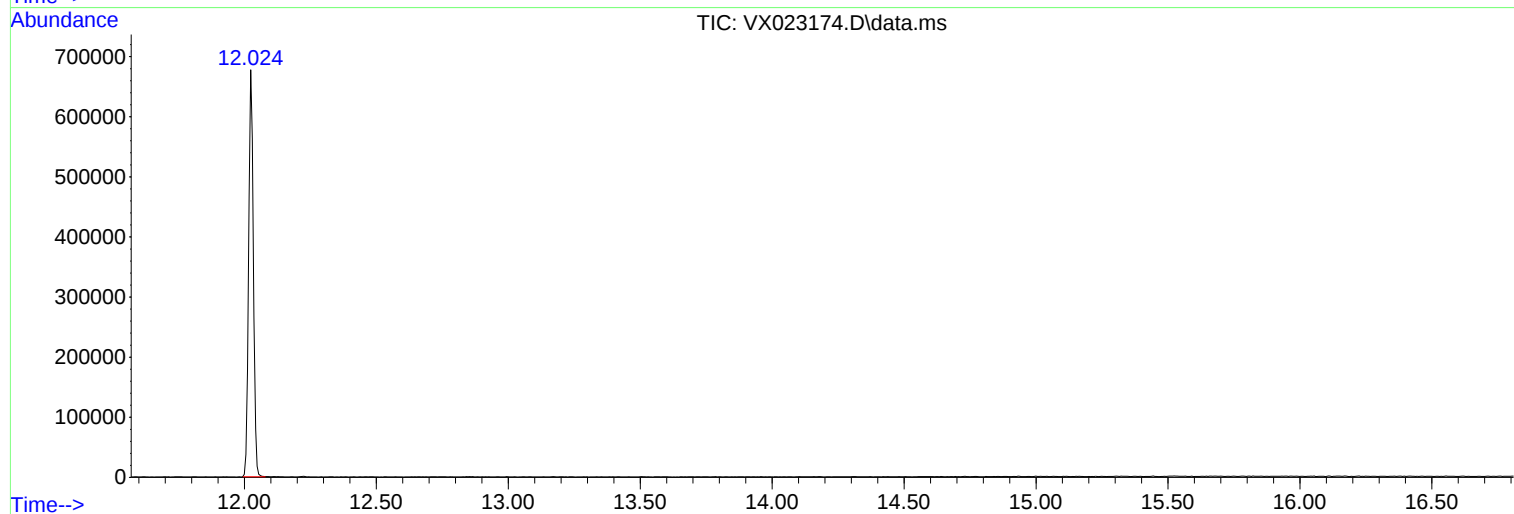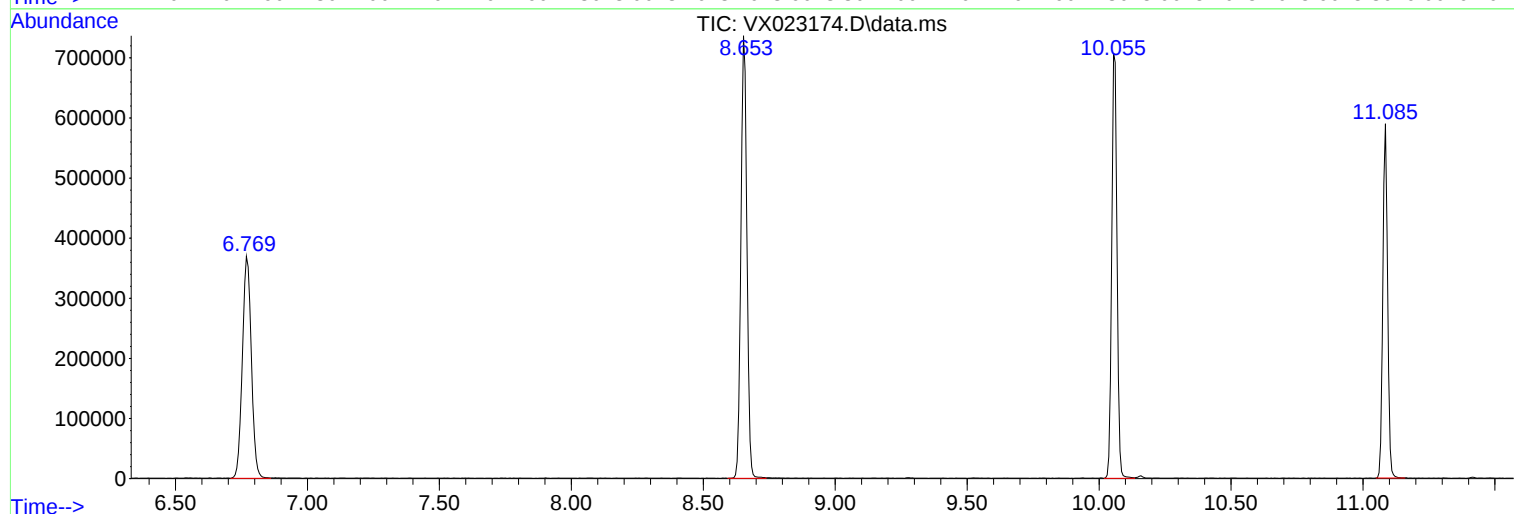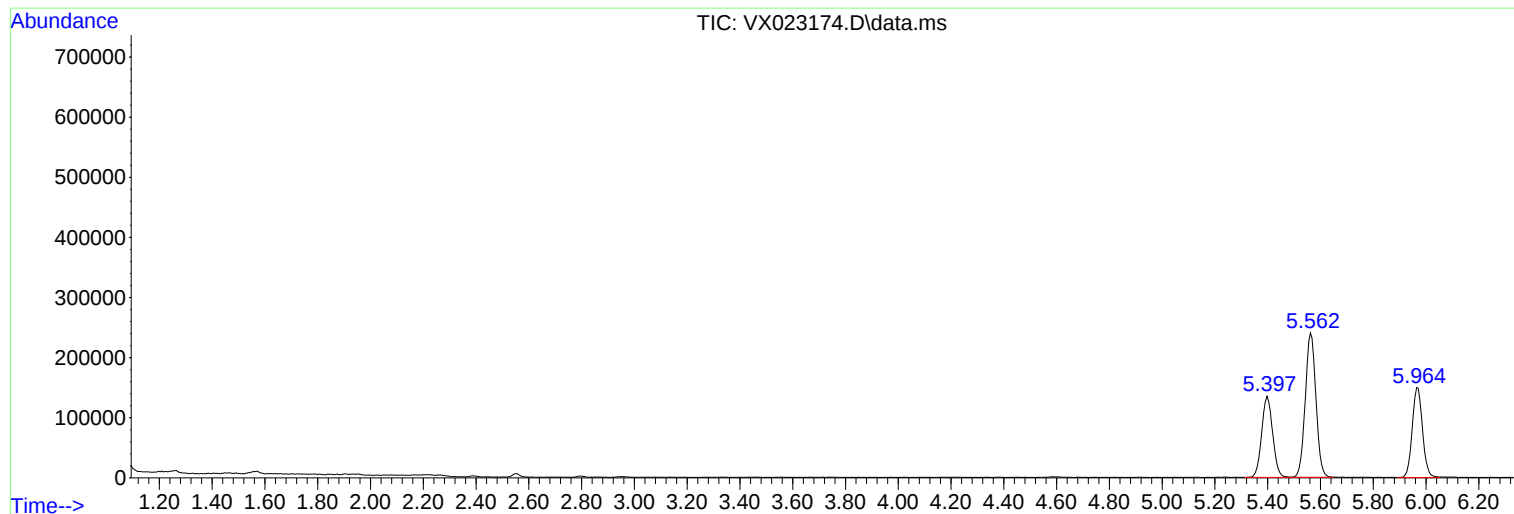

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070721\  
Data File : VX023174.D  
Acq On : 07 Jul 2021 15:51  
Operator : JC/MD  
Sample : M2948-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X070221W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070721\  
Data File : VX023174.D  
Acq On : 07 Jul 2021 15:51  
Operator : JC/MD  
Sample : M2948-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X070221W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----