

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
 Data File : VX036456.D
 Acq On : 07 Jul 2023 13:29
 Operator : JC/MD
 Sample : 03494-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M

Title : SW846 8260

Signal : TIC: VX036456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.648	84	92	94	rBV7	3637	9554	1.03%	0.192%
2	2.593	237	247	263	rBV2	3530	17299	1.86%	0.347%
3	4.574	560	572	585	rBV2	8471	30431	3.27%	0.611%
4	5.391	692	706	721	rBV2	105020	306323	32.95%	6.153%
5	5.556	721	733	749	rVB	189201	528176	56.81%	10.609%
6	5.958	788	799	811	rBV	119670	318414	34.25%	6.396%
7	6.763	920	931	947	rBV	289242	687859	73.99%	13.816%
8	8.647	1233	1240	1252	rBV	582495	929643	100.00%	18.672%
9	10.055	1465	1471	1481	rBV	626405	816233	87.80%	16.394%
10	11.079	1634	1639	1653	rBV	461813	605855	65.17%	12.169%
11	12.024	1788	1794	1805	rBV	582855	728916	78.41%	14.641%




Sum of corrected areas: 4978703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036456.D
Acq On : 07 Jul 2023 13:29
Operator : JC/MD
Sample : 03494-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

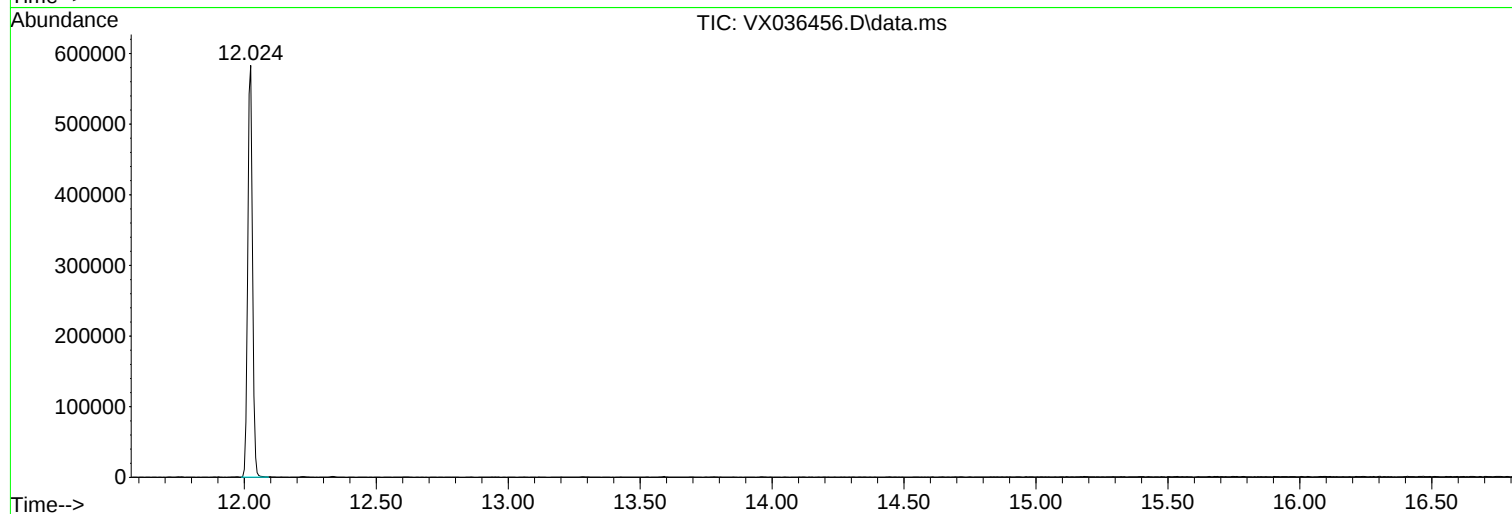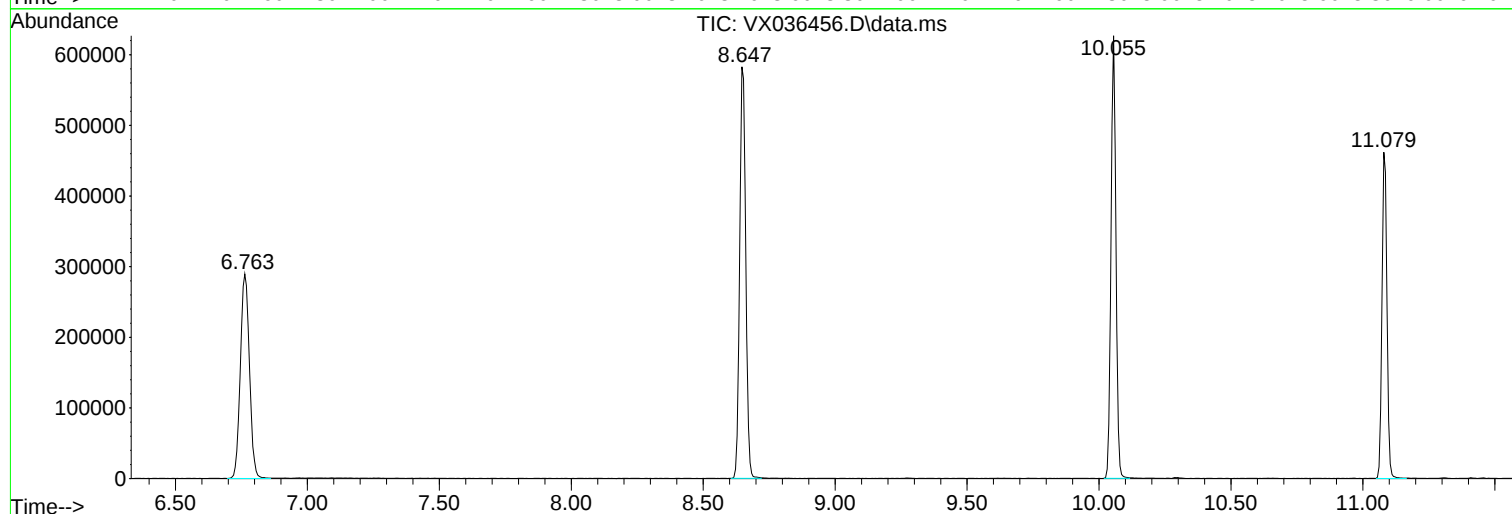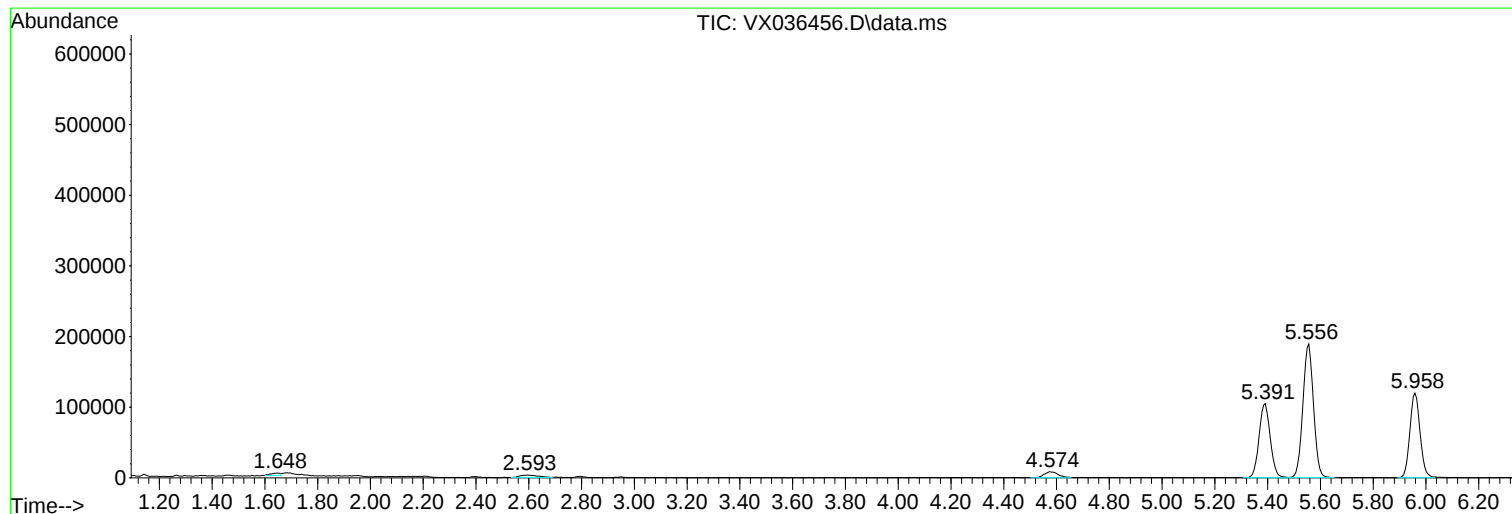

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036456.D
Acq On : 07 Jul 2023 13:29
Operator : JC/MD
Sample : 03494-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036456.D
Acq On : 07 Jul 2023 13:29
Operator : JC/MD
Sample : 03494-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------