

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036457.D
Acq On : 07 Jul 2023 13:53
Operator : JC/MD
Sample : 03494-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M

Title : SW846 8260

Signal : TIC: VX036457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.642	79	91	93	rBV5	5331	13454	1.51%	0.283%
2	2.599	237	248	249	rBV2	3718	9272	1.04%	0.195%
3	4.574	563	572	574	rBV	10016	21370	2.40%	0.450%
4	5.391	693	706	721	rBV	100318	291236	32.71%	6.131%
5	5.556	722	733	748	rVB	177462	502342	56.42%	10.576%
6	5.958	789	799	816	rBV2	115657	304849	34.24%	6.418%
7	6.763	920	931	946	rBV	280029	660034	74.13%	13.895%
8	8.653	1233	1241	1249	rBV	553717	890373	100.00%	18.745%
9	10.055	1465	1471	1478	rBV	584593	776954	87.26%	16.357%
10	11.079	1634	1639	1647	rBV	452921	581829	65.35%	12.249%
11	12.024	1788	1794	1804	rBV	536206	698279	78.43%	14.701%




Sum of corrected areas: 4749992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036457.D
Acq On : 07 Jul 2023 13:53
Operator : JC/MD
Sample : 03494-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

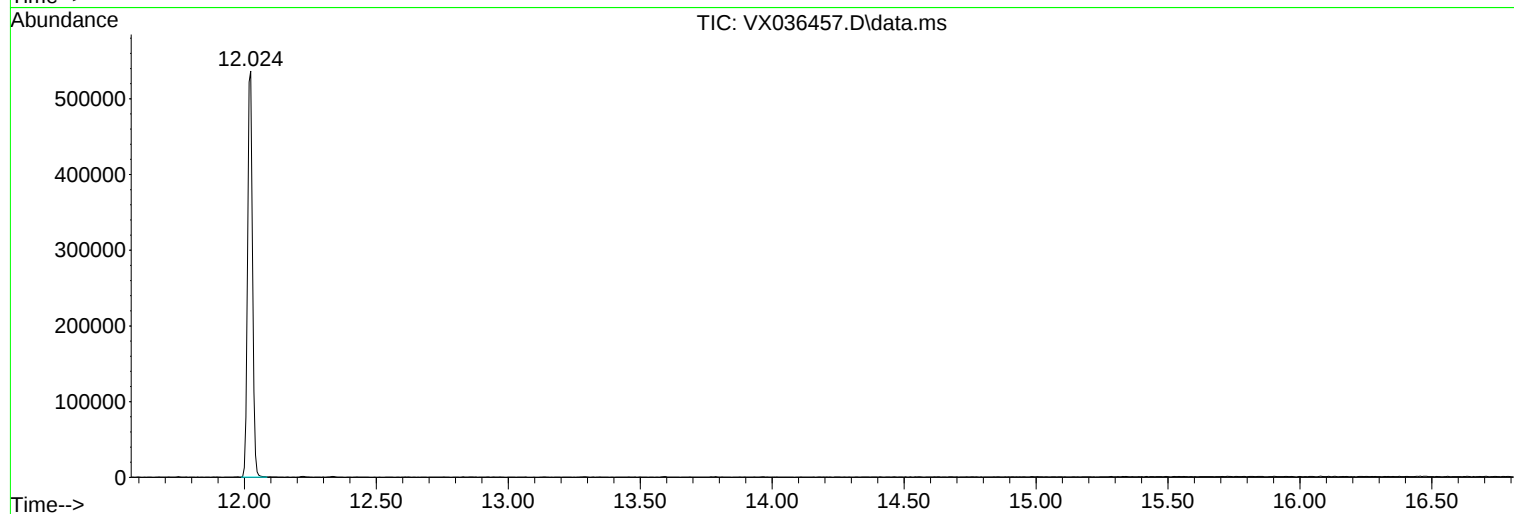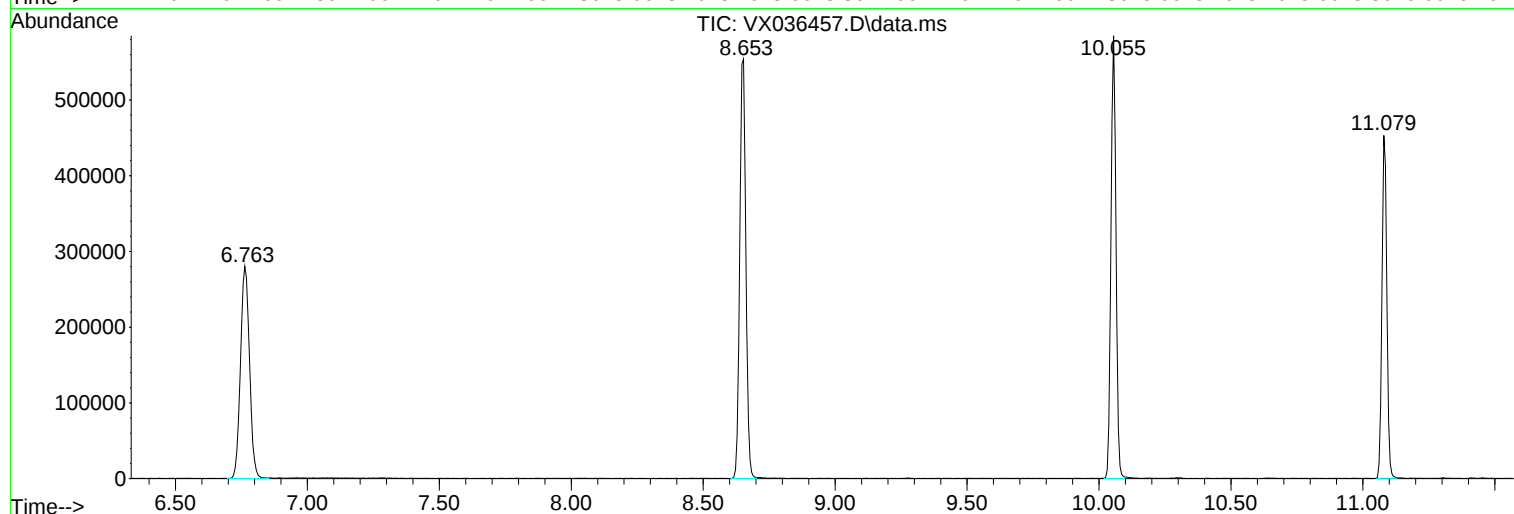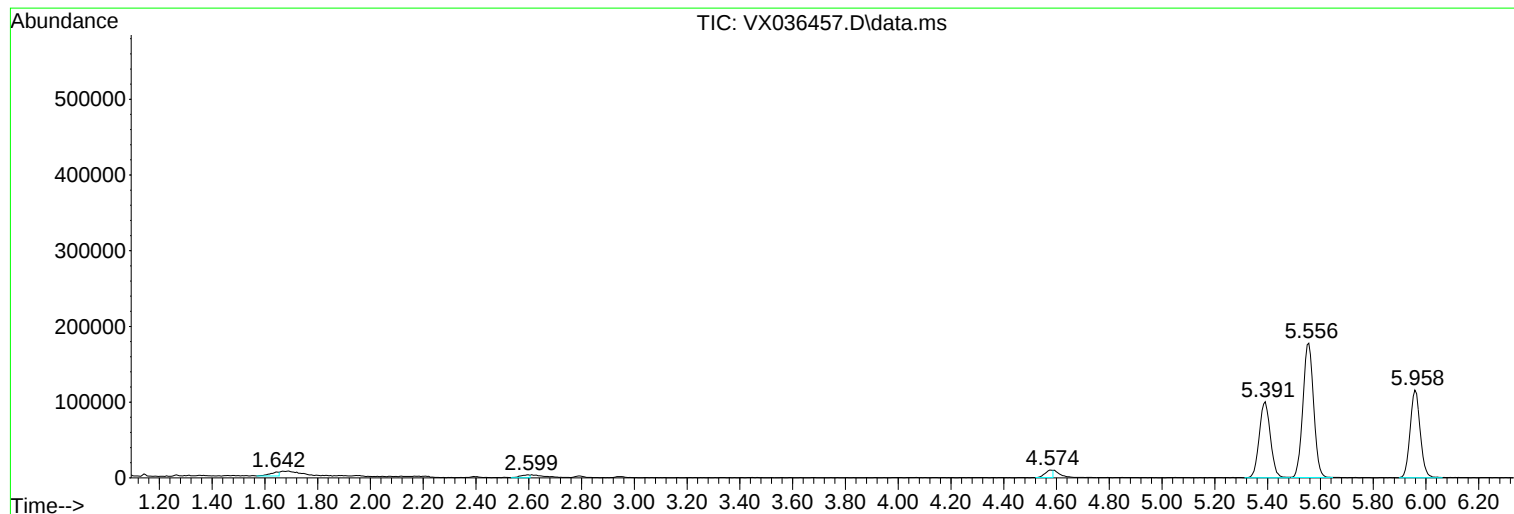

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036457.D
Acq On : 07 Jul 2023 13:53
Operator : JC/MD
Sample : 03494-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036457.D
Acq On : 07 Jul 2023 13:53
Operator : JC/MD
Sample : 03494-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------