

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070723\  
Data File : VX036463.D  
Acq On : 07 Jul 2023 16:15  
Operator : JC/MD  
Sample : 03546-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1675

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X062323W.M

Title : SW846 8260

Signal : TIC: VX036463.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.630       | 81            | 89          | 90           | rBV5     | 4926           | 9149          | 1.06%           | 0.201%        |
| 2         | 2.392       | 207           | 214         | 225          | rBV2     | 9623           | 20384         | 2.37%           | 0.447%        |
| 3         | 5.391       | 694           | 706         | 720          | rBV      | 97915          | 280805        | 32.64%          | 6.158%        |
| 4         | 5.550       | 722           | 732         | 749          | rVB      | 168275         | 478533        | 55.62%          | 10.494%       |
| 5         | 5.958       | 786           | 799         | 814          | rBV2     | 109965         | 296524        | 34.47%          | 6.503%        |
| 6         | 6.763       | 921           | 931         | 942          | rBV      | 266181         | 630340        | 73.27%          | 13.823%       |
| 7         | 8.653       | 1234          | 1241        | 1251         | rBV      | 536163         | 860344        | 100.00%         | 18.867%       |
| 8         | 10.055      | 1465          | 1471        | 1485         | rBV      | 584183         | 754148        | 87.66%          | 16.538%       |
| 9         | 11.079      | 1634          | 1639        | 1655         | rVB      | 440612         | 558162        | 64.88%          | 12.240%       |
| 10        | 12.024      | 1788          | 1794        | 1803         | rBV      | 539585         | 671656        | 78.07%          | 14.729%       |




Sum of corrected areas: 4560045

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070723\  
Data File : VX036463.D  
Acq On : 07 Jul 2023 16:15  
Operator : JC/MD  
Sample : 03546-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X062323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

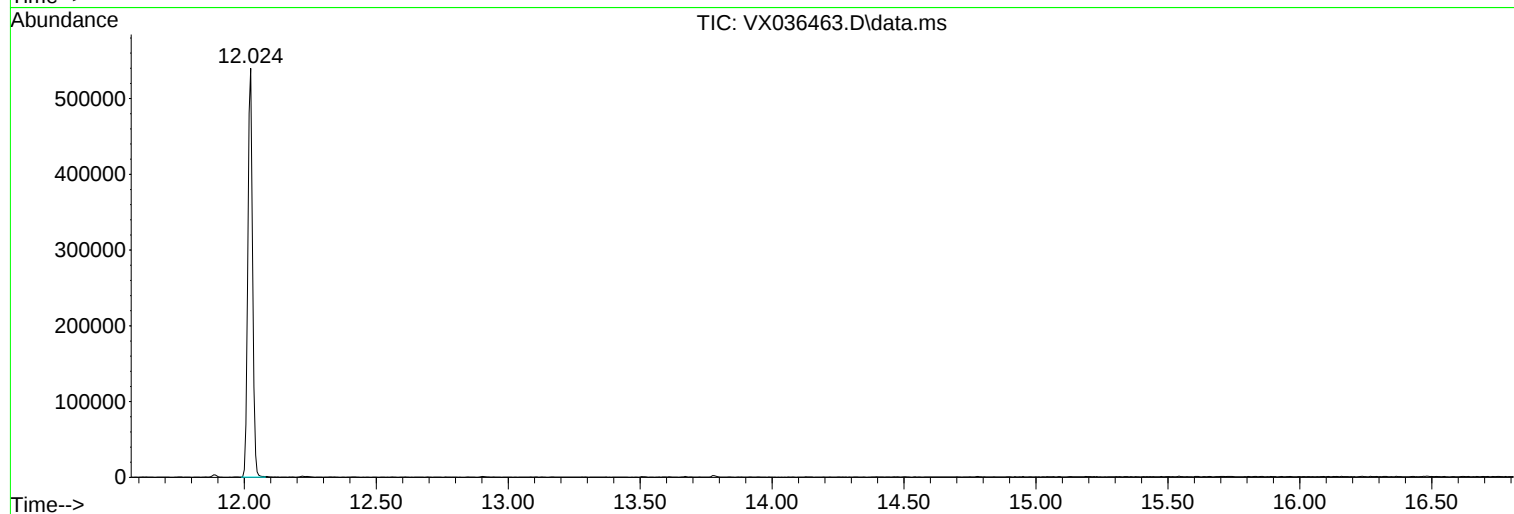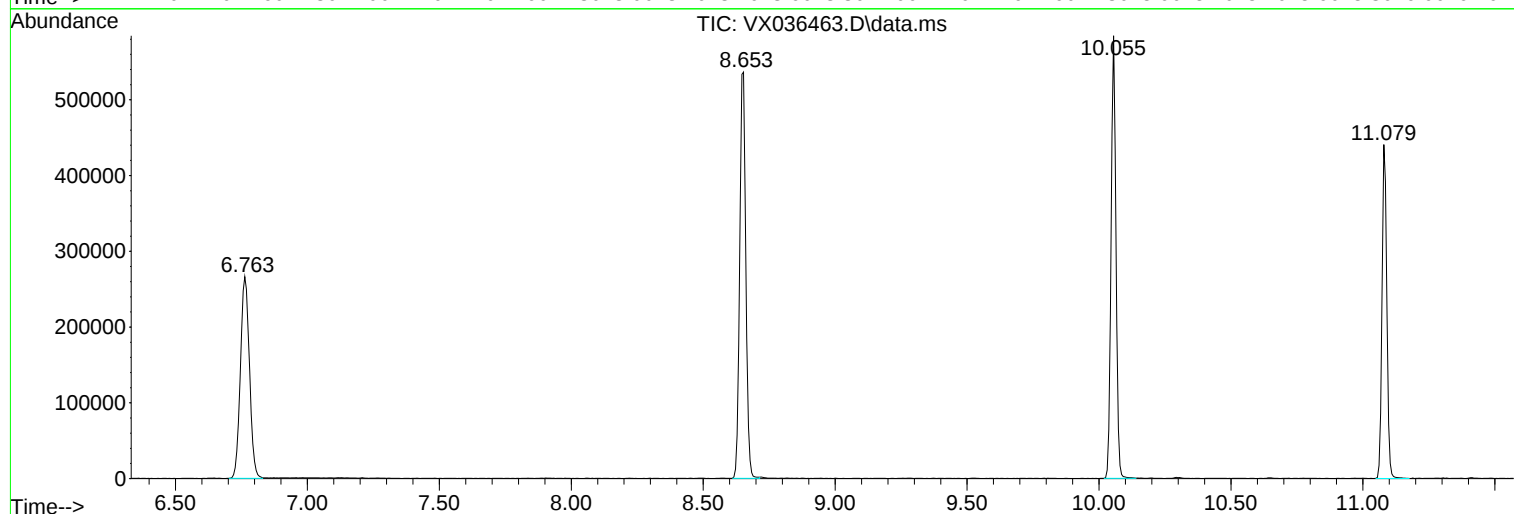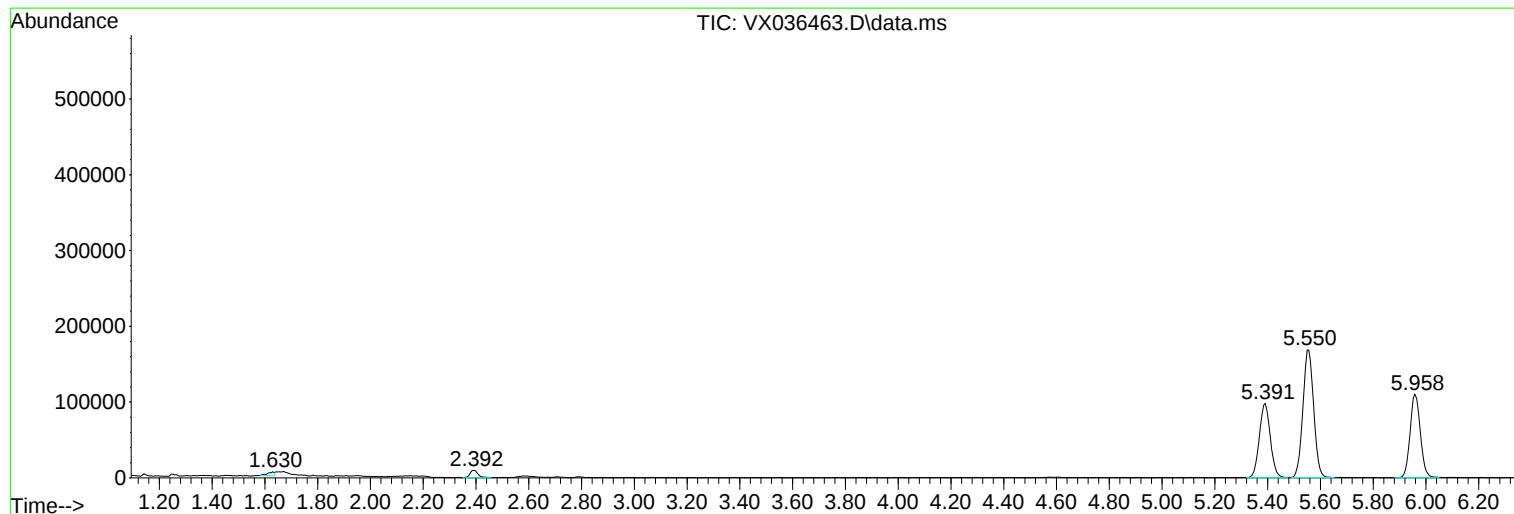

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070723\  
Data File : VX036463.D  
Acq On : 07 Jul 2023 16:15  
Operator : JC/MD  
Sample : 03546-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X062323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070723\  
Data File : VX036463.D  
Acq On : 07 Jul 2023 16:15  
Operator : JC/MD  
Sample : 03546-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X062323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|