

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
 Data File : VX036466.D
 Acq On : 07 Jul 2023 17:27
 Operator : JC/MD
 Sample : 03525-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50054

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Title : SW846 8260

Signal : TIC: VX036466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.624	76	88	89	rBV2	8035	19181	2.23%	0.393%
2	5.391	692	706	718	rBV	97522	278952	32.40%	5.716%
3	5.550	721	732	748	rVV	165600	471958	54.82%	9.671%
4	5.958	789	799	812	rBV2	111980	296075	34.39%	6.067%
5	6.763	921	931	945	rBV	264809	630776	73.27%	12.926%
6	8.653	1234	1241	1253	rBV	540139	860862	100.00%	17.640%
7	10.055	1465	1471	1487	rBV	567491	752025	87.36%	15.410%
8	11.079	1634	1639	1651	rBV	435932	560009	65.05%	11.475%
9	12.024	1788	1794	1804	rBV	555320	690686	80.23%	14.153%
10	13.268	1992	1998	2005	rBV2	6691	9993	1.16%	0.205%
11	14.036	2121	2124	2127	rVB	11214	11556	1.34%	0.237%
12	14.207	2147	2152	2163	rVB	4112	12267	1.42%	0.251%
13	14.323	2167	2171	2175	rVB5	6886	8702	1.01%	0.178%
14	14.377	2175	2180	2183	rBV3	11864	16715	1.94%	0.343%
15	14.487	2192	2198	2203	rBV7	10200	21366	2.48%	0.438%
16	14.615	2215	2219	2221	rBV2	13436	16947	1.97%	0.347%
17	14.670	2225	2228	2232	rVB2	19505	25454	2.96%	0.522%
18	14.755	2239	2242	2245	rBV	15000	15171	1.76%	0.311%
19	14.816	2249	2252	2254	rVV3	7565	8900	1.03%	0.182%
20	14.847	2255	2257	2261	rVB4	10542	11288	1.31%	0.231%
21	14.914	2262	2268	2272	rBV3	12855	22787	2.65%	0.467%
22	15.042	2282	2289	2295	rBV4	8493	18922	2.20%	0.388%
23	15.182	2308	2312	2315	rBV3	19033	27575	3.20%	0.565%
24	15.371	2339	2343	2346	rBV5	7731	10631	1.23%	0.218%
25	15.487	2358	2362	2365	rBV5	8514	11804	1.37%	0.242%
26	15.530	2365	2369	2373	rBV5	6048	11755	1.37%	0.241%
27	15.609	2378	2382	2388	rVV3	14749	31272	3.63%	0.641%
28	15.658	2388	2390	2397	rVB6	7473	11864	1.38%	0.243%
29	15.853	2415	2422	2424	rBV6	7493	14550	1.69%	0.298%




Sum of corrected areas: 4880043

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036466.D
Acq On : 07 Jul 2023 17:27
Operator : JC/MD
Sample : 03525-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50054

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

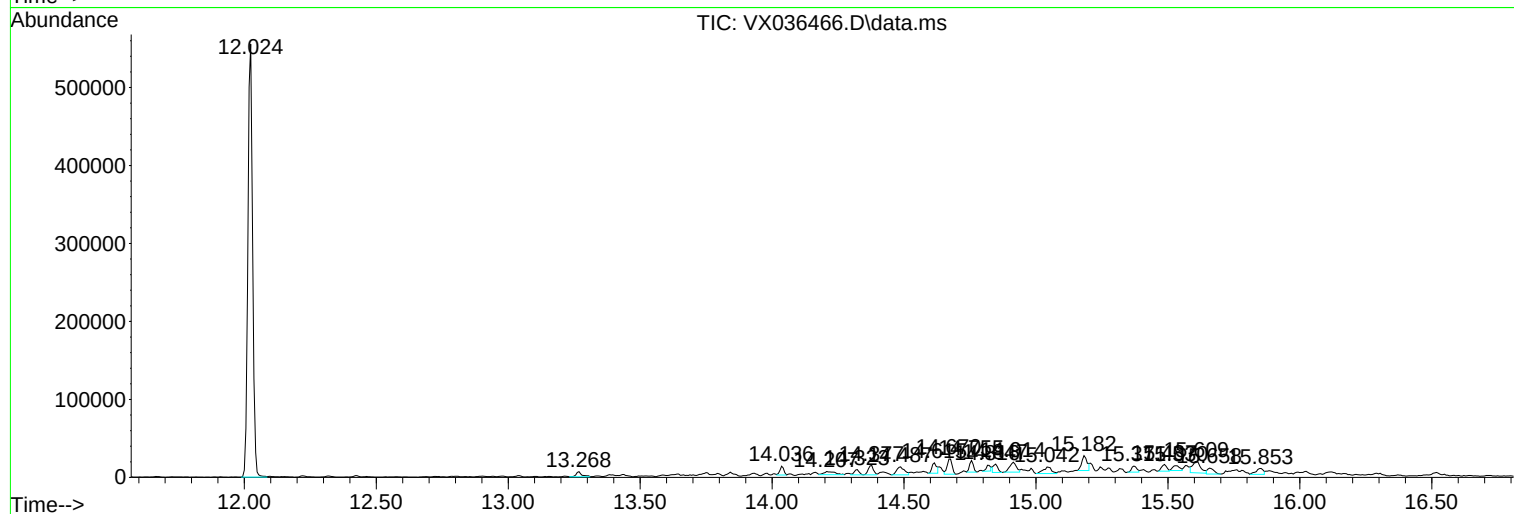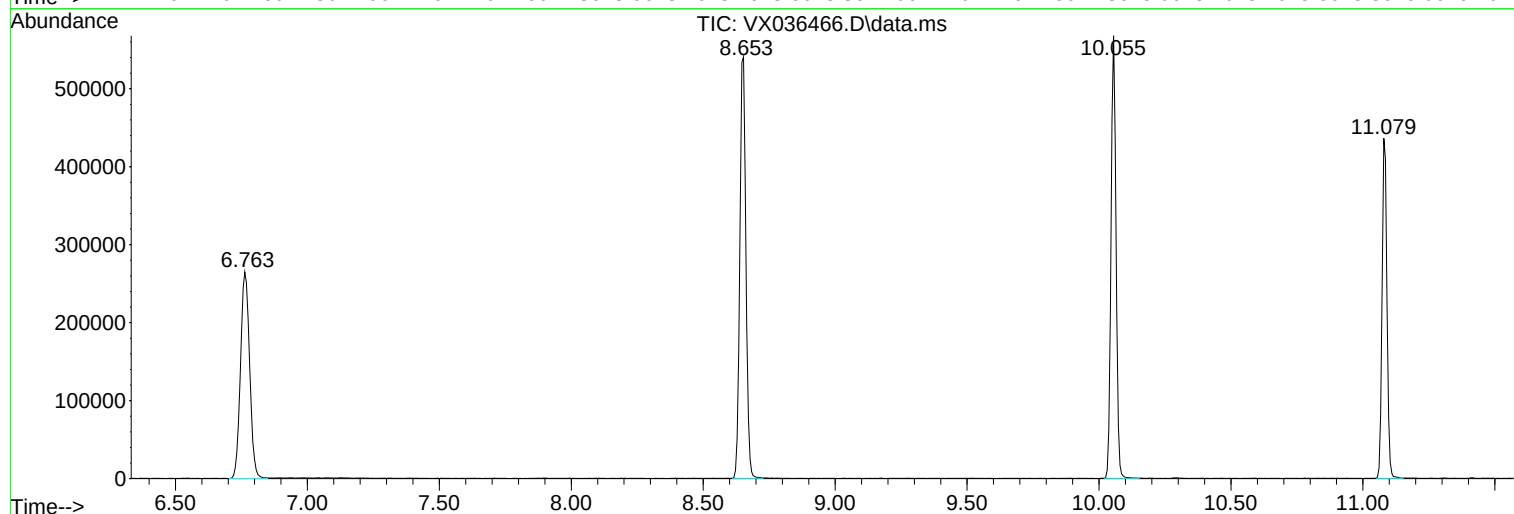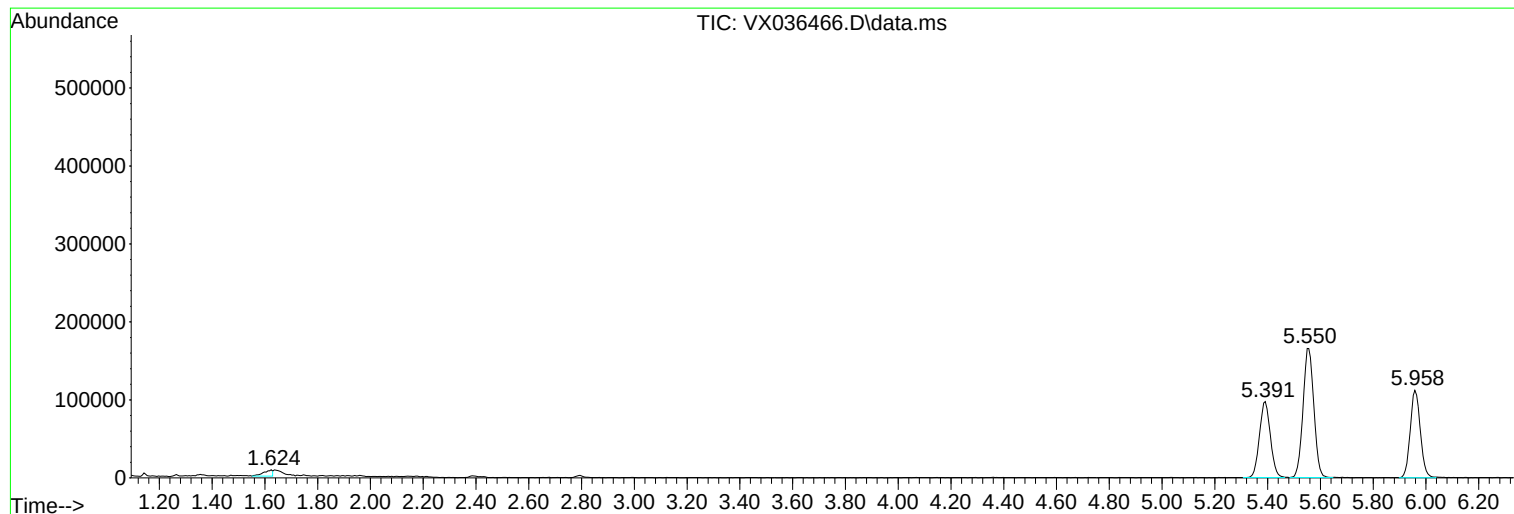

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036466.D
Acq On : 07 Jul 2023 17:27
Operator : JC/MD
Sample : 03525-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50054

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036466.D
Acq On : 07 Jul 2023 17:27
Operator : JC/MD
Sample : 03525-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50054

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------