

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
 Data File : VX036470.D
 Acq On : 07 Jul 2023 19:25
 Operator : JC/MD
 Sample : 03563-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 HOUSE-BASEMENT

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Title : SW846 8260

Signal : TIC: VX036470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.551	72	76	81	rBV	22111	28392	3.02%	0.445%
2	2.392	207	214	217	rBV	17742	32748	3.48%	0.514%
3	2.422	217	219	229	rVB	16619	23005	2.45%	0.361%
4	3.447	380	387	394	rVB4	4782	10519	1.12%	0.165%
5	5.391	693	706	720	rBV	105326	307205	32.67%	4.819%
6	5.556	720	733	748	rVB	182618	518671	55.15%	8.136%
7	5.958	789	799	814	rBV2	121050	319314	33.95%	5.009%
8	6.763	919	931	947	rBV	287892	684802	72.82%	10.741%
9	8.653	1233	1241	1247	rBV	590323	940465	100.00%	14.752%
10	8.720	1247	1252	1260	rVB	194930	295931	31.47%	4.642%
11	9.573	1388	1392	1393	rBV	13887	17268	1.84%	0.271%
12	10.055	1462	1471	1484	rBV	632263	844666	89.81%	13.249%
13	11.079	1634	1639	1649	rVB	506220	650913	69.21%	10.210%
14	11.805	1753	1758	1762	rBV	33893	43094	4.58%	0.676%
15	11.860	1764	1767	1775	rVB3	7763	12461	1.32%	0.195%
16	12.024	1788	1794	1802	rBV	660189	839096	89.22%	13.162%
17	12.219	1822	1826	1840	rBV	38836	57729	6.14%	0.906%
18	12.542	1872	1879	1881	rBV4	6794	11838	1.26%	0.186%
19	12.573	1881	1884	1890	rVB4	10801	17797	1.89%	0.279%
20	12.768	1909	1916	1922	rBV3	33718	51545	5.48%	0.809%
21	12.963	1944	1948	1955	rBV	57565	70694	7.52%	1.109%
22	13.061	1959	1964	1967	rVV	41723	52288	5.56%	0.820%
23	13.085	1967	1968	1974	rVB2	11492	11795	1.25%	0.185%
24	13.335	2005	2009	2013	rBV	36286	45884	4.88%	0.720%
25	13.384	2013	2017	2024	rVB	26719	39743	4.23%	0.623%
26	13.506	2032	2037	2044	rBV6	9354	15128	1.61%	0.237%
27	13.585	2044	2050	2059	rBV	127394	167326	17.79%	2.625%
28	13.664	2059	2063	2069	rVB2	22927	31559	3.36%	0.495%
29	13.743	2074	2076	2085	rVB6	7436	12867	1.37%	0.202%
30	13.841	2087	2092	2097	rBV7	6986	13282	1.41%	0.208%
31	13.981	2110	2115	2123	rBV	28842	47480	5.05%	0.745%
32	14.451	2187	2192	2197	rBV2	16286	22225	2.36%	0.349%
33	14.591	2209	2215	2220	rBV5	8259	15653	1.66%	0.246%
34	14.664	2220	2227	2230	rVB8	5076	12182	1.30%	0.191%
35	15.213	2309	2317	2321	rVB4	10089	15201	1.62%	0.238%
36	15.493	2358	2363	2369	rBV9	6726	15294	1.63%	0.240%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036470.D
Acq On : 07 Jul 2023 19:25
Operator : JC/MD
Sample : 03563-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HOUSE-BASEMENT

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Title : SW846 8260

37	16.097	2455	2462	2469	rBV5	19203	48944	5.20%	0.768%
38	16.273	2489	2491	2500	rVB10	5474	13884	1.48%	0.218%
39	16.700	2558	2561	2567	rVB7	8214	16481	1.75%	0.259%




Sum of corrected areas: 6375369

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036470.D
Acq On : 07 Jul 2023 19:25
Operator : JC/MD
Sample : 03563-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HOUSE-BASEMENT

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

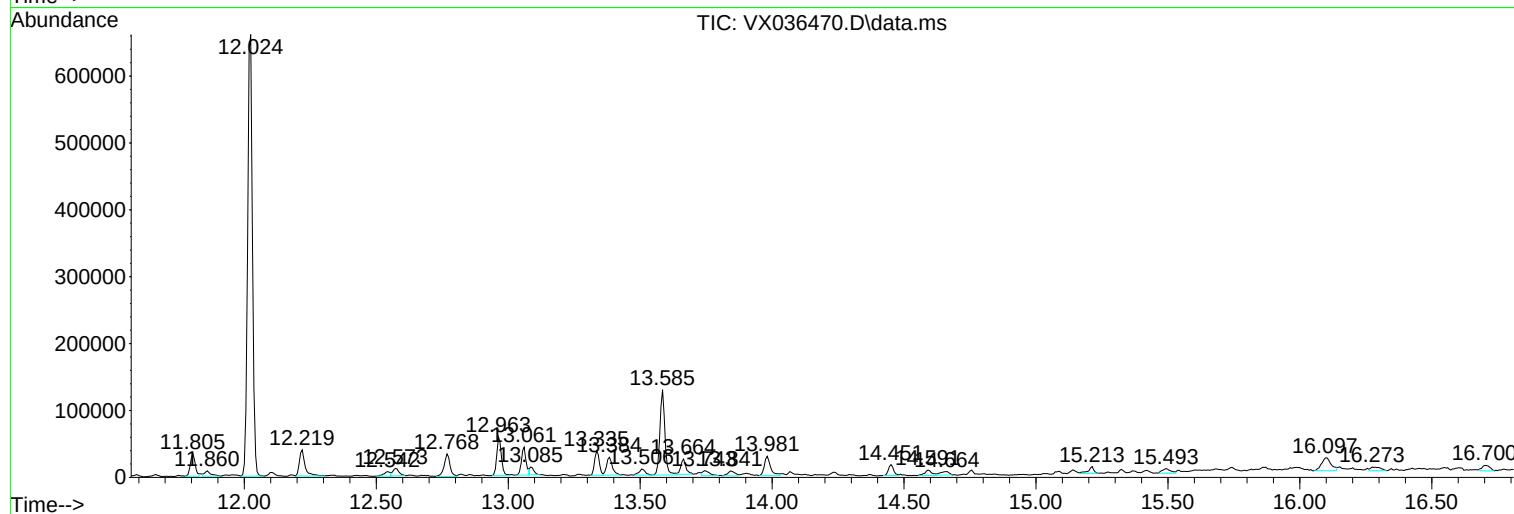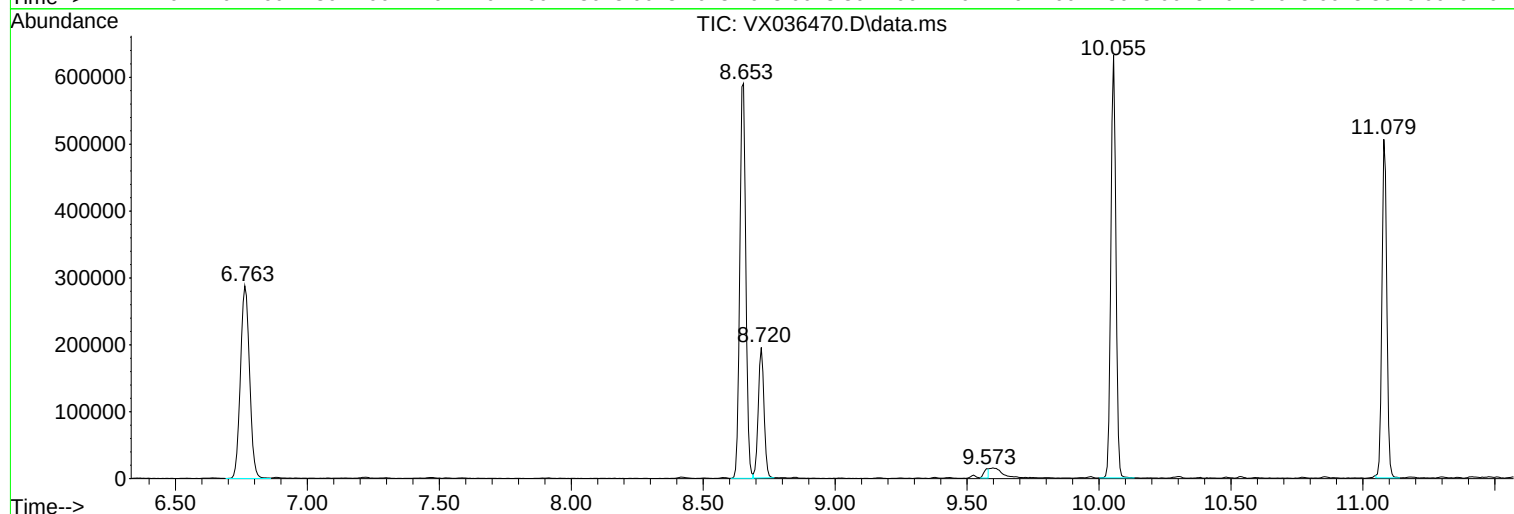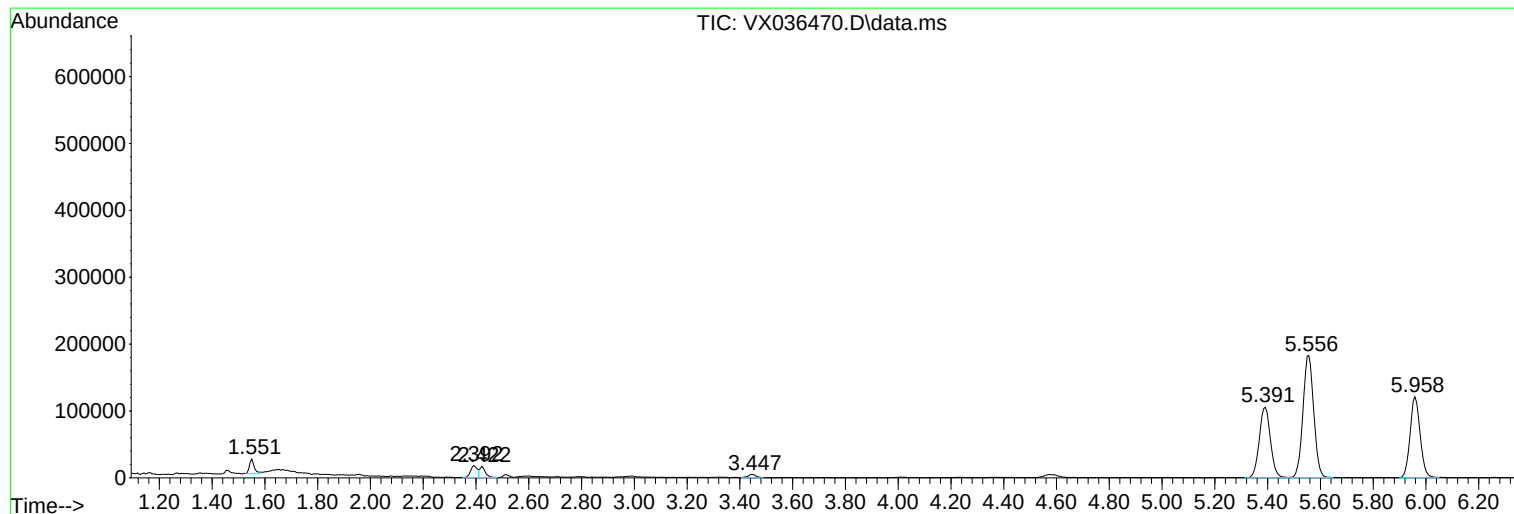

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036470.D
Acq On : 07 Jul 2023 19:25
Operator : JC/MD
Sample : 03563-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HOUSE-BASEMENT










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 ortho tert-Butyl cyclohexyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.585	9.97 ug/l	167326	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			ortho tert-Butyl cyclohexyl acetate	198	C12H22O2	000088-41-5	80
2			Cyclohexanol, 2-(1,1-dimethyleth...	156	C10H20O	013491-79-7	80
3			Cyclohexanol, 2-(1,1-dimethyleth...	156	C10H20O	005448-22-6	72
4			cis-3-Hexenyl-.alpha.-methylbuty...	184	C11H20O2	053398-85-9	58
5			cis-2-tert-Butylcyclohexanol, tr...	252	C12H19F3O2	1000467-27-6	53

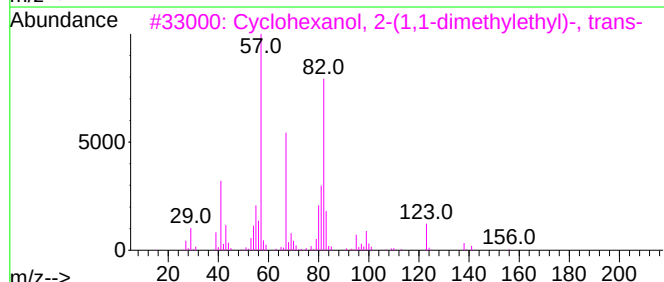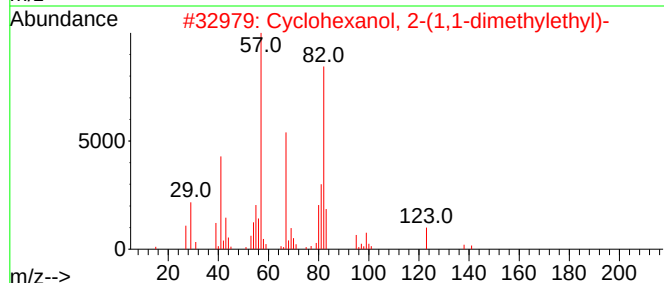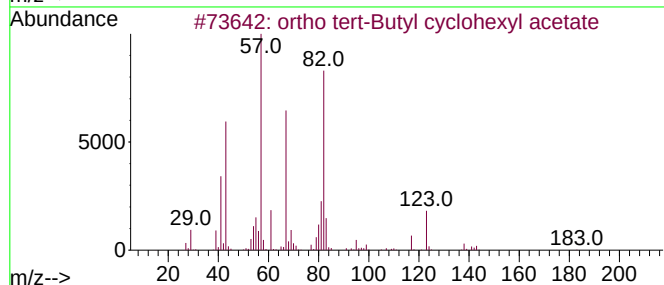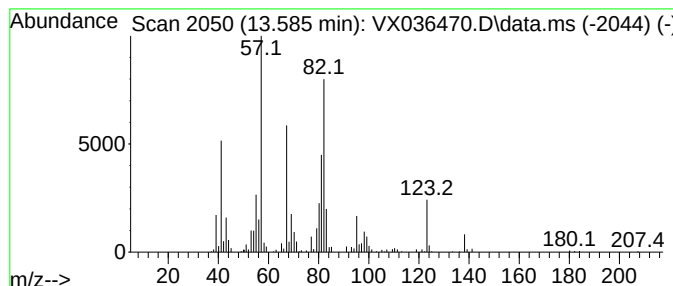

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036470.D
Acq On : 07 Jul 2023 19:25
Operator : JC/MD
Sample : 03563-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HOUSE-BASEMENT

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
ortho tert-Buty...	13.585	10.0	ug/l	167326	4	12.024	839096	50.0