
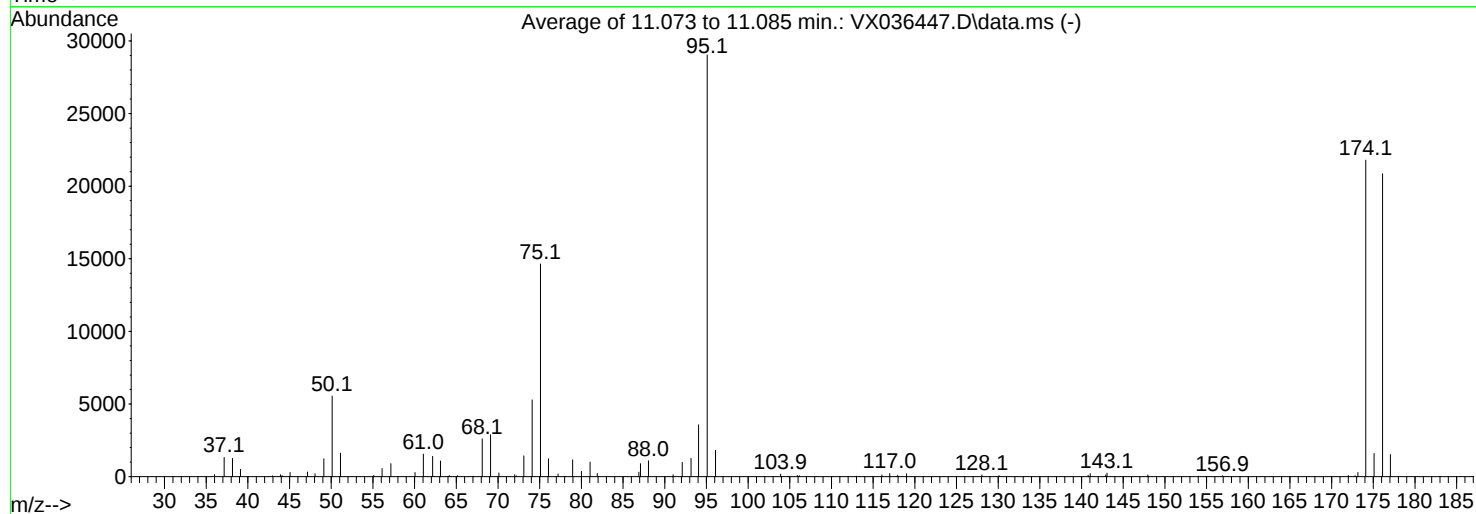


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070723\
Data File : VX036447.D
Acq On : 07 Jul 2023 09:11
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Title : SW846 8260
Last Update : Fri Jun 23 15:03:28 2023

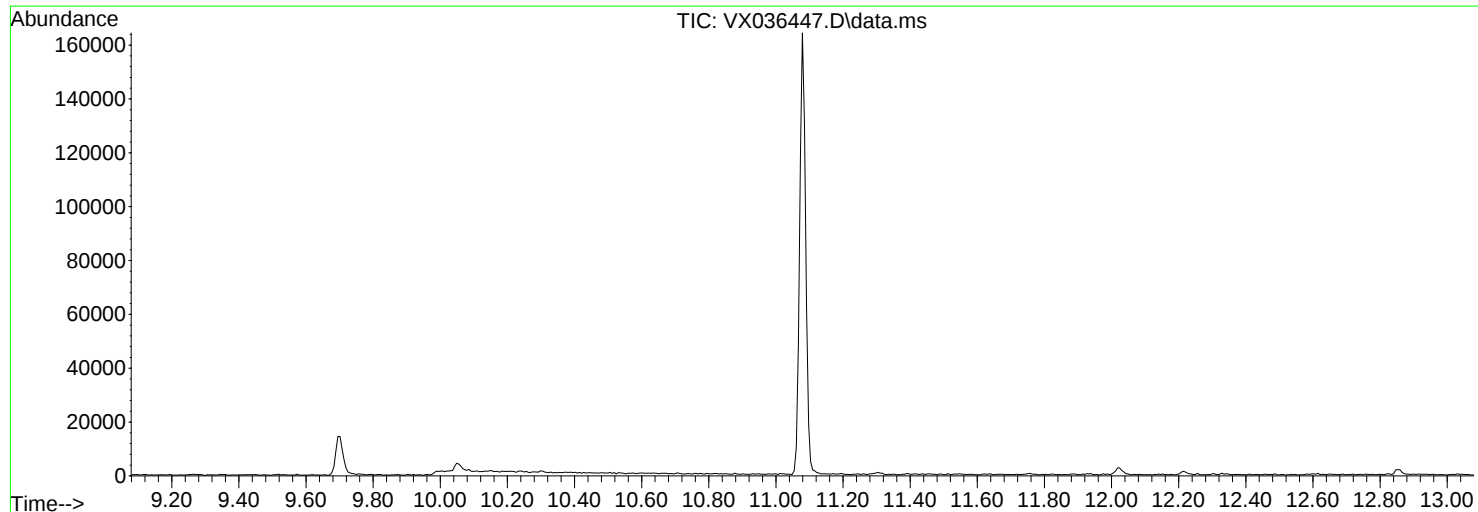

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	5548	PASS
75	95	30	60	50.4	14637	PASS
95	95	100	100	100.0	29043	PASS
96	95	5	9	6.2	1805	PASS
173	174	0.00	2	1.3	290	PASS
174	95	50	100	75.1	21797	PASS
175	174	5	9	7.3	1594	PASS
176	174	95	101	95.7	20855	PASS
177	176	5	9	7.3	1518	PASS