


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX070819\
Data File : VX010684.D
Acq On : 08 Jul 2019 09:23
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260
Last Update : Thu Jun 20 03:31:56 2019

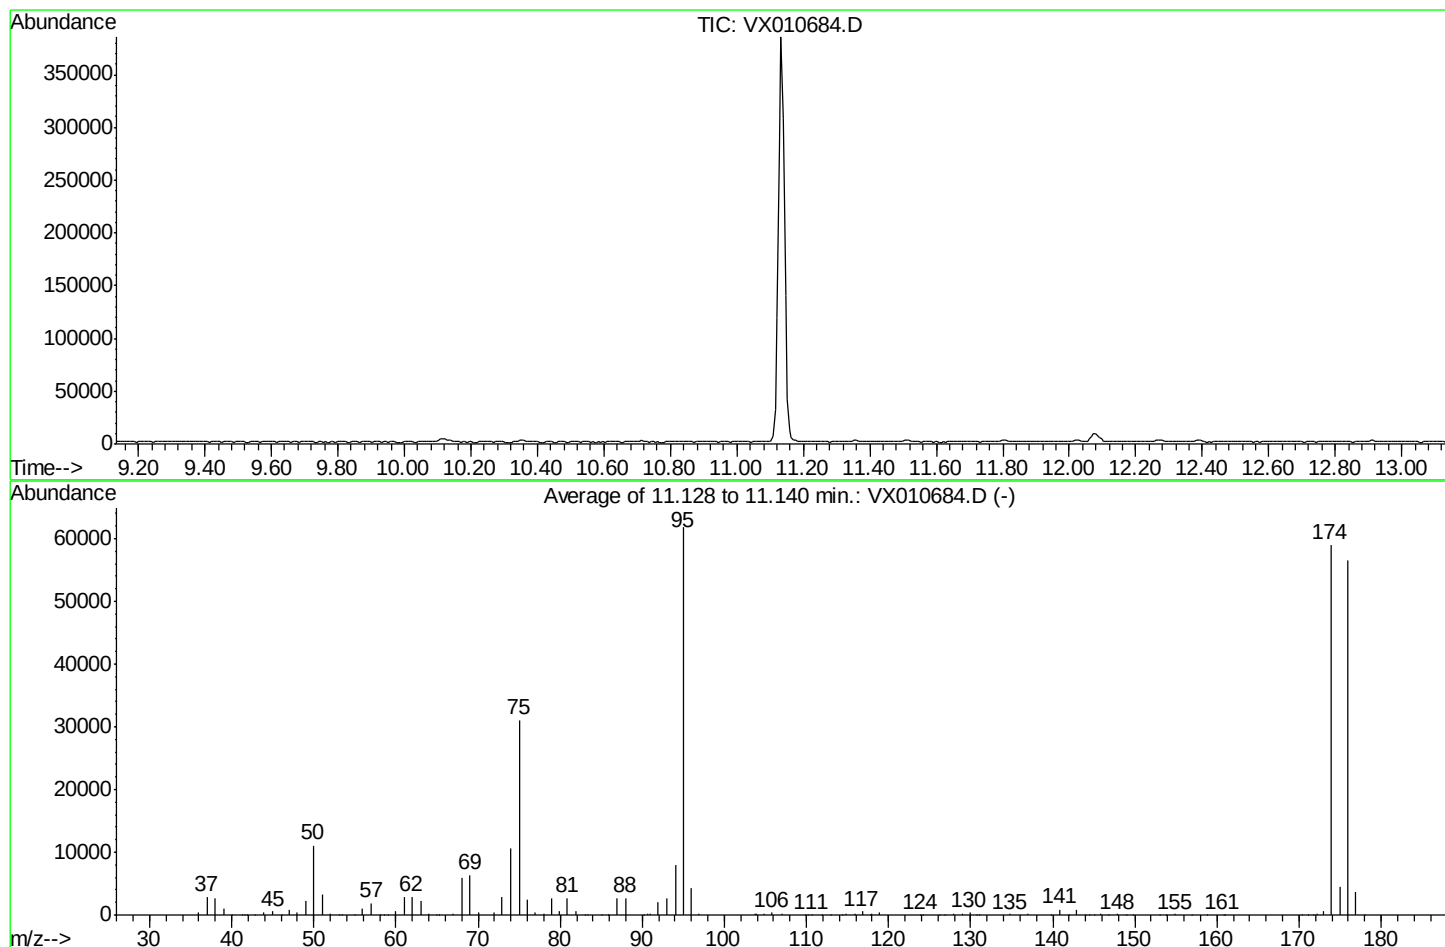

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	11092	PASS
75	95	30	60	50.2	31061	PASS
95	95	100	100	100.0	61818	PASS
96	95	5	9	6.9	4265	PASS
173	174	0.00	2	1.2	708	PASS
174	95	50	100	95.5	59045	PASS
175	174	5	9	7.7	4556	PASS
176	174	95	101	95.8	56581	PASS
177	176	5	9	6.5	3689	PASS