


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX070819\
Data File : VX010710.D
Acq On : 08 Jul 2019 21:15
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260
Last Update : Thu Jun 20 03:31:56 2019

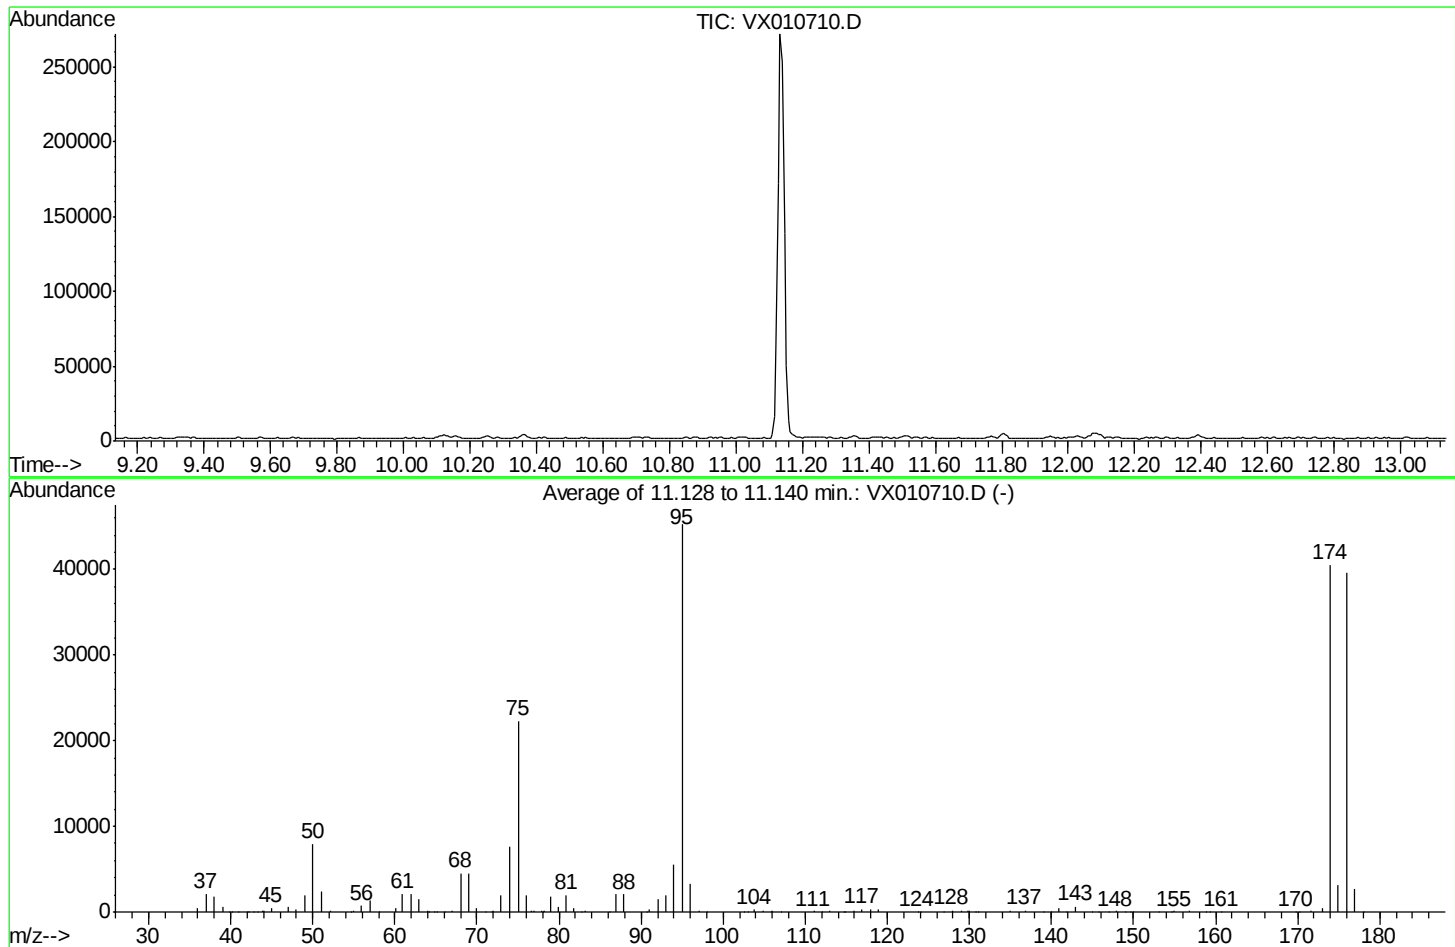

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	7973	PASS
75	95	30	60	49.3	22325	PASS
95	95	100	100	100.0	45258	PASS
96	95	5	9	7.1	3226	PASS
173	174	0.00	2	1.2	472	PASS
174	95	50	100	89.5	40512	PASS
175	174	5	9	7.9	3211	PASS
176	174	95	101	97.9	39674	PASS
177	176	5	9	6.7	2639	PASS