

Data File : VX017249.D
Acq On : 08 Jul 2020 12:51
Operator : JC/SP
Sample : L3232-05DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1005-MW-03ADL

Quant Time: Jul 09 02:29:41 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 29 17:10:38 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	256770	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	417673	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	428735	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	218771	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	164620	52.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.02%	
35) Dibromofluoromethane	5.46	113	142938	54.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.20%	
50) Toluene-d8	8.70	98	508540	52.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.10%	
62) 4-Bromofluorobenzene	11.12	95	203110	53.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.36%	


Target Compounds				Qvalue		
5) Bromomethane	1.64	94	668	0.453	ug/l #	35
8) Diethyl Ether	2.16	74	43	0.396	ug/l #	1
10) Methyl Iodide	2.50	142	724	0.227	ug/l #	61
11) Tert butyl alcohol	3.00	59	331	0.548	ug/l #	22
13) Acrolein	2.29	56	629	1.742	ug/l	89
15) Acrylonitrile	3.14	53	444	0.306	ug/l #	66
16) Acetone	2.42	43	3219	2.718	ug/l	100
17) Carbon Disulfide	2.55	76	1593	0.247	ug/l #	63
18) Methyl Acetate	2.75	43	798	0.258	ug/l #	70
20) Methylene Chloride	2.84	84	1479	Below Cal	#	76
21) trans-1,2-Dichloroethene	3.15	96	4686	1.662	ug/l	97
25) 2-Butanone	4.64	43	1411	0.715	ug/l #	63
27) cis-1,2-Dichloroethene	4.57	96	79718	24.956	ug/l	90
31) Cyclohexane	5.63	56	4943	1.157	ug/l #	1
38) Carbon Tetrachloride	5.63	117	24740	5.690	ug/l #	18
40) Benzene	6.12	78	2438	0.210	ug/l #	88
44) Trichloroethene	7.19	130	73317	22.739	ug/l	97
49) 1,4-Dioxane	7.95	88	20	0.279	ug/l #	1
51) 4-Methyl-2-Pentanone	8.63	43	801	0.202	ug/l	99
55) 1,1,2-Trichloroethane	9.31	97	2059	0.696	ug/l #	15
60) Dibromochloromethane	9.32	129	218951	63.716	ug/l #	11
64) Tetrachloroethene	9.32	164	237748	68.710	ug/l	95
76) 1,2,3-Trichloropropane	11.12	75	100976	23.472	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	100976	60.784	ug/l #	13
88) 1,4-Dichlorobenzene	12.01	146	851	Below Cal		90
94) Hexachlorobutadiene	13.76	225	298	1.013	ug/l	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX017249.D
Acq On : 08 Jul 2020 12:51
Operator : JC/SP
Sample : L3232-05DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1005-MW-03ADL

Quant Time: Jul 09 02:29:41 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 29 17:10:38 2020
Response via : Initial Calibration

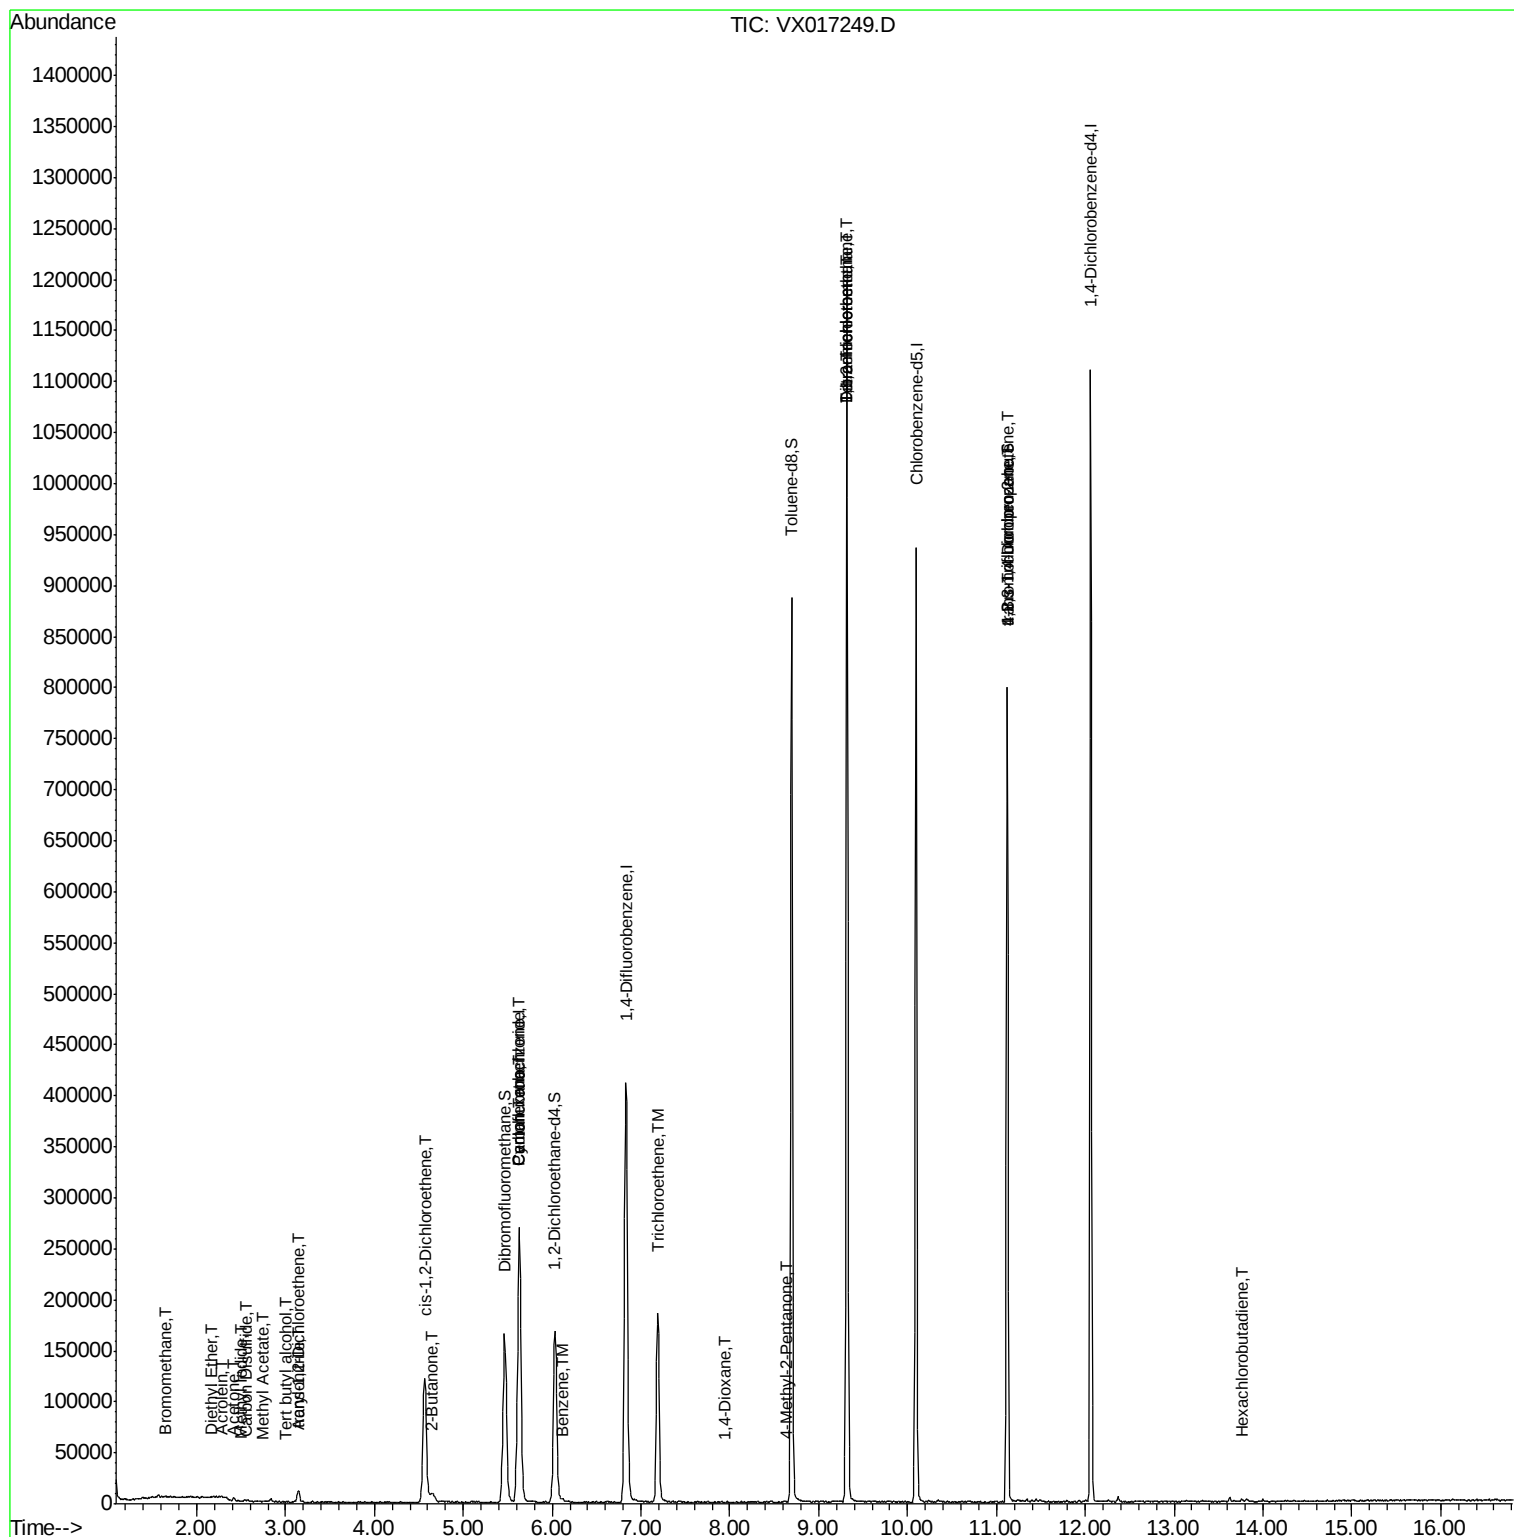



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :


1005-MW-03ADL

Tgt Ion:168 Resp: 256770

Ion Ratio Lower Upper

168 100

99 54.1 42.6 64.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

100000

80000



60000

40000

20000

0

Time-->



#5

Bromomethane

Concen: 0.453 ug/l

RT: 1.64 min Scan# 90

Delta R.T. 0.01 min

Lab File: VX017249.D


Acq: 08 Jul 2020 12:51

Tgt Ion: 94 Resp: 668

Ion Ratio Lower Upper

94 100

96 31.3 75.0 112.4#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

400


300


200

100

0

Time-->





#8

Diethyl Ether

Concen: 0.396 ug/l

RT: 2.16 min Scan# 176

Delta R.T. -0.01 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :


1005-MW-03ADL

Tgt Ion: 74 Resp: 43

Ion Ratio Lower Upper




74 100

45 414.0 49.8 149.3#

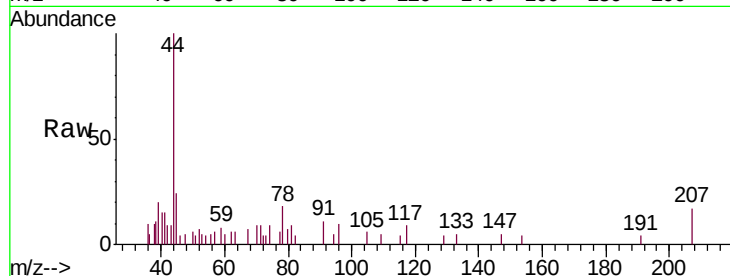

Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

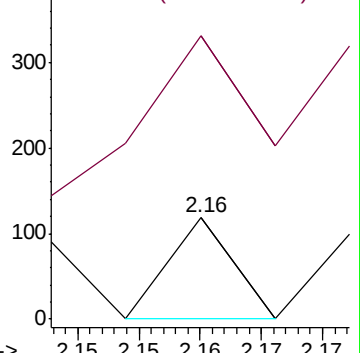

#10

Methyl Iodide

Concen: 0.227 ug/l

RT: 2.50 min Scan# 231

Delta R.T. 0.01 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51


Tgt Ion: 142 Resp: 724

Ion Ratio Lower Upper

142 100

127 14.2 36.6 54.8#



141 9.9 11.6 17.4#




Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

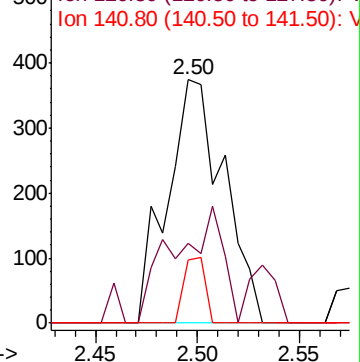




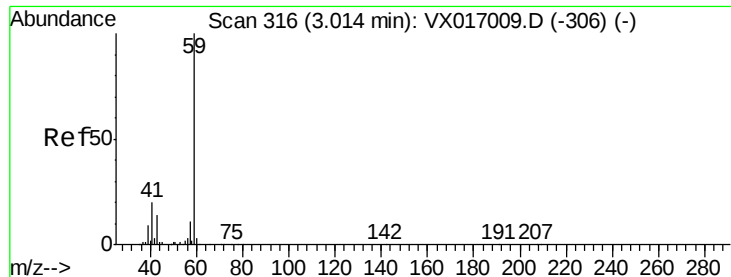


#11

Tert butyl alcohol
Concen: 0.548 ug/l
RT: 3.00 min Scan# 314
Delta R.T. -0.01 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51

Instrument :
MSVOA_X
ClientSampleId :
1005-MW-03ADL




Tgt Ion: 59 Resp: 331
Ion Ratio Lower Upper
59 100
57 39.3 8.2 12.2#

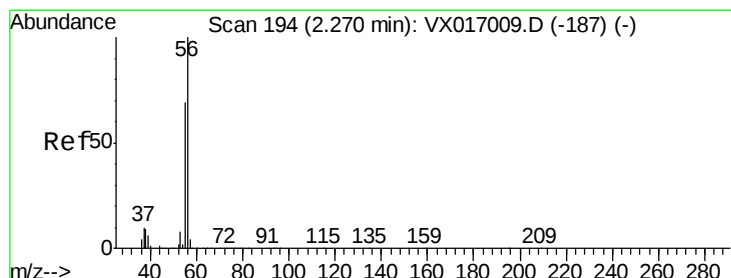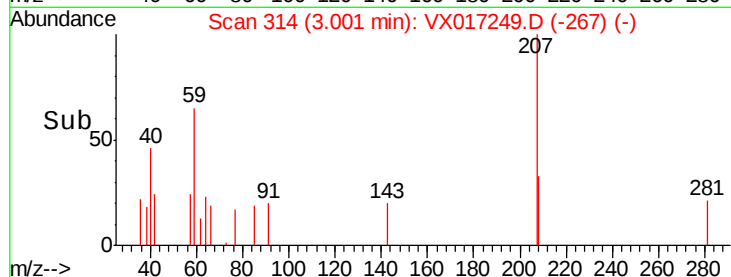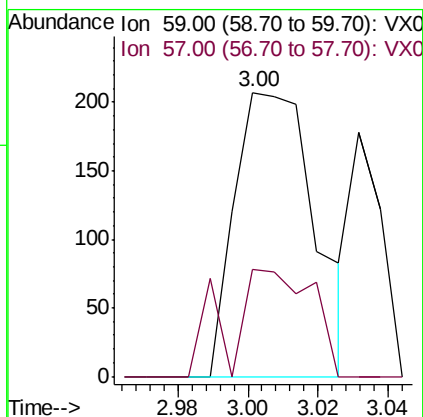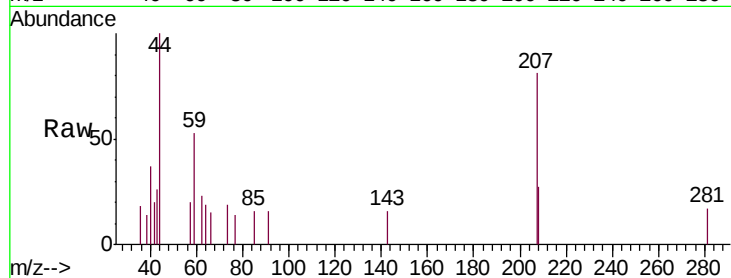


#13

Acrolein
Concen: 1.742 ug/l
RT: 2.29 min Scan# 197
Delta R.T. 0.02 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51

Tgt Ion: 56 Resp: 629
Ion Ratio Lower Upper
56 100
55 60.3 55.7 83.5

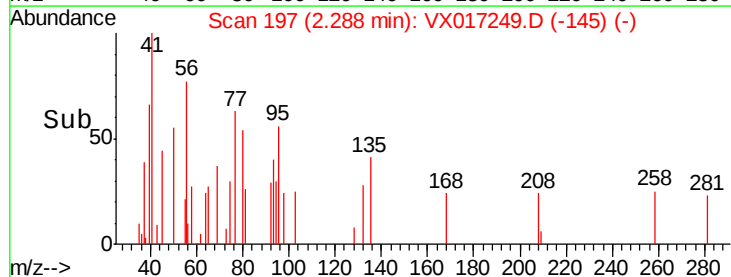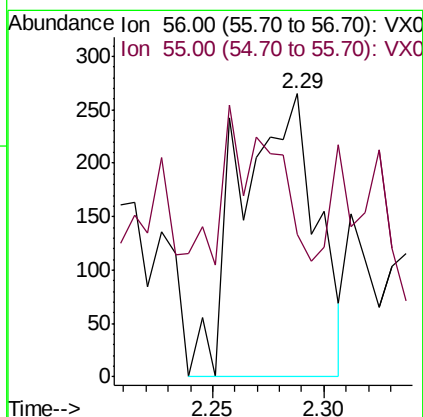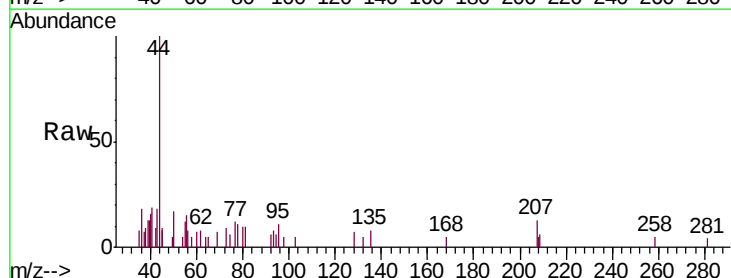



#15

Acrylonitrile

Concen: 0.306 ug/l

RT: 3.14 min Scan# 336

Delta R.T. 0.02 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :

1005-MW-03ADL


Tgt Ion: 53 Resp: 444

Ion Ratio Lower Upper

53 100

52 61.9 65.6 98.4#




51 0.0 28.3 42.5#

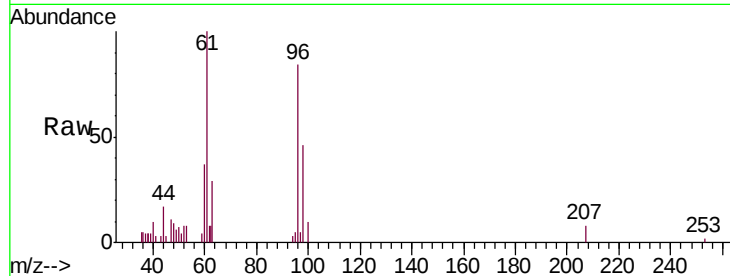

Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

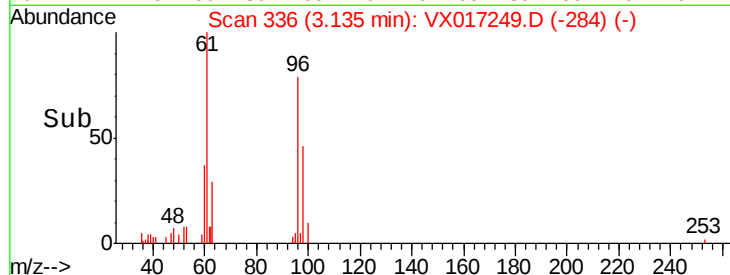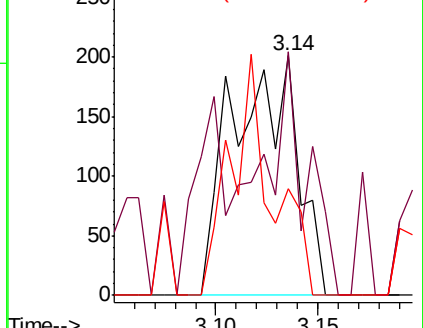

#16

Acetone

Concen: 2.718 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.01 min

Lab File: VX017249.D


Acq: 08 Jul 2020 12:51

Tgt Ion: 43 Resp: 3219

Ion Ratio Lower Upper



43 100


58 32.2 25.7 38.5



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




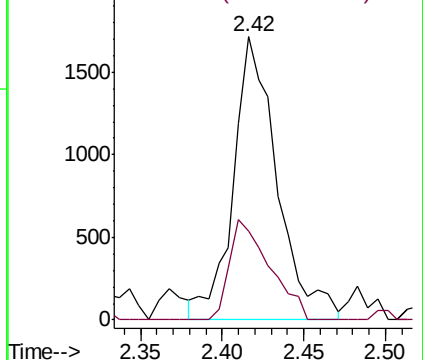


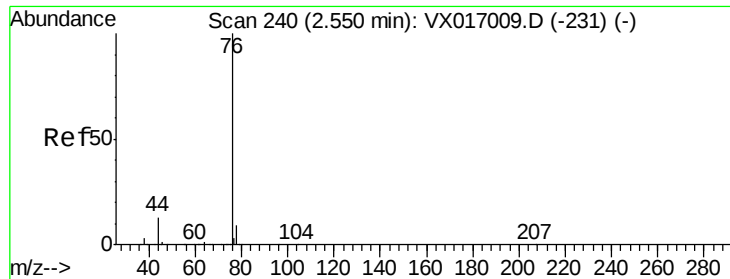

#17
Carbon Disulfide
Concen: 0.247 ug/l
RT: 2.55 min Scan# 240
Delta R.T. 0.00 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51




Instrument :
MSVOA_X
ClientSampleId :
1005-MW-03ADL


Tgt Ion: 76 Resp: 1593
Ion Ratio Lower Upper
76 100
78 22.5 7.2 10.8#

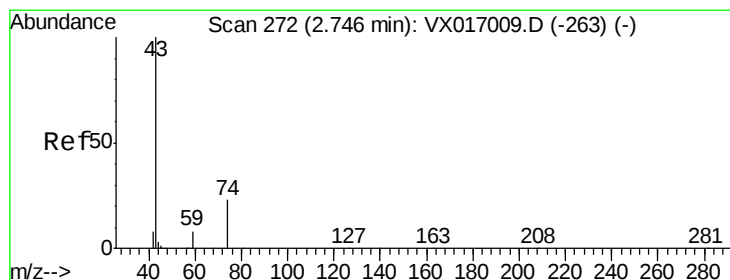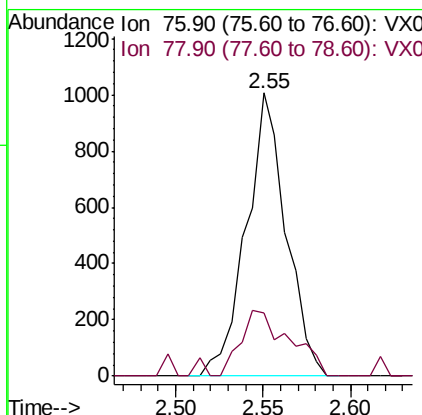

#18
Methyl Acetate
Concen: 0.258 ug/l
RT: 2.75 min Scan# 273
Delta R.T. 0.01 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51

Tgt Ion: 43 Resp: 798
Ion Ratio Lower Upper
43 100
74 9.4 19.3 28.9#



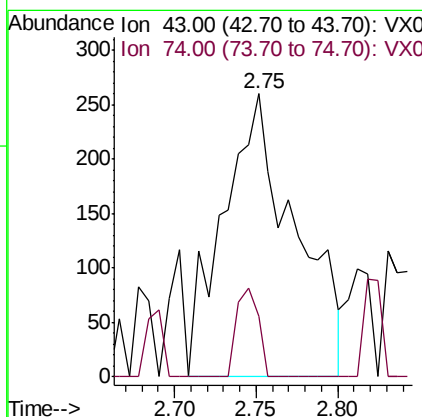
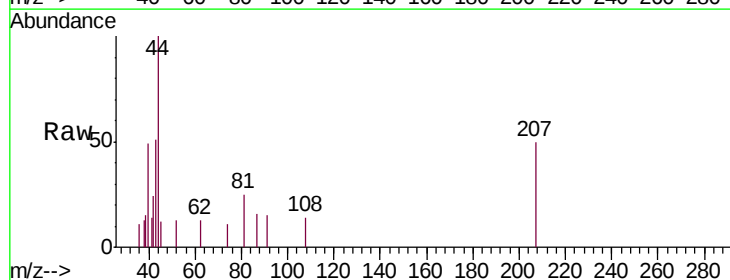


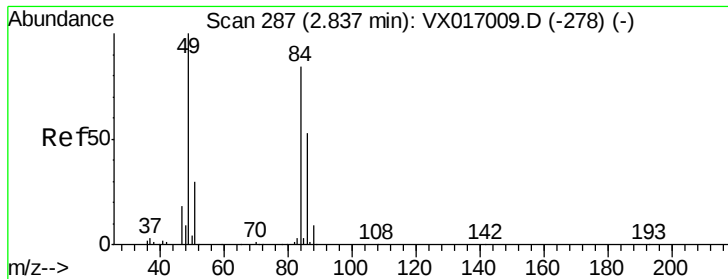

#20
Methylene Chloride
Concen: Below Cal
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51




Instrument :
MSVOA_X
ClientSampleId :
1005-MW-03ADL


Tgt Ion: 84 Resp: 1479
Ion Ratio Lower Upper
84 100
49 85.8 94.7 142.1#
51 29.6 28.6 42.8
86 46.7 50.5 75.7#

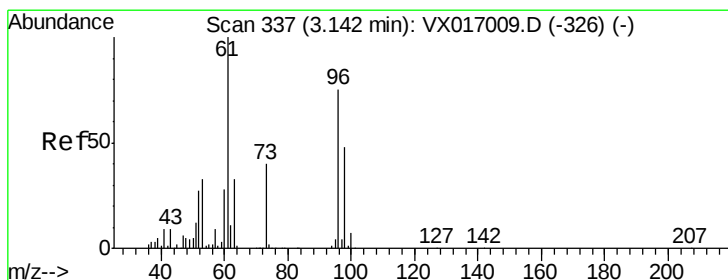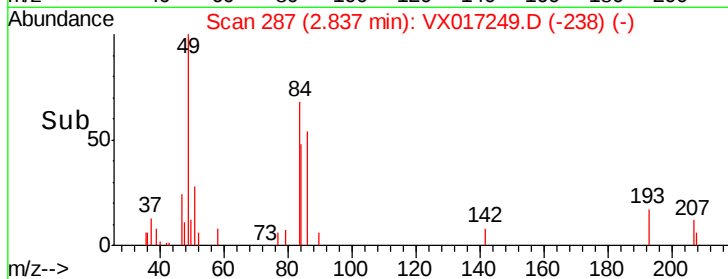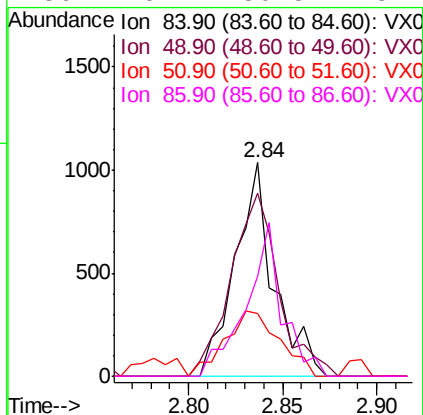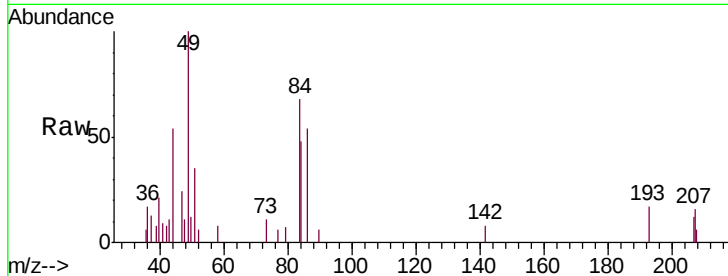

#21
trans-1,2-Dichloroethene
Concen: 1.662 ug/l
RT: 3.15 min Scan# 338
Delta R.T. 0.01 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51

Tgt Ion: 96 Resp: 4686
Ion Ratio Lower Upper
96 100
61 134.7 107.0 160.6
98 69.7 51.6 77.4

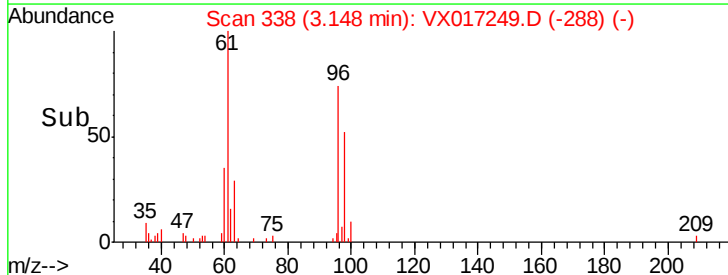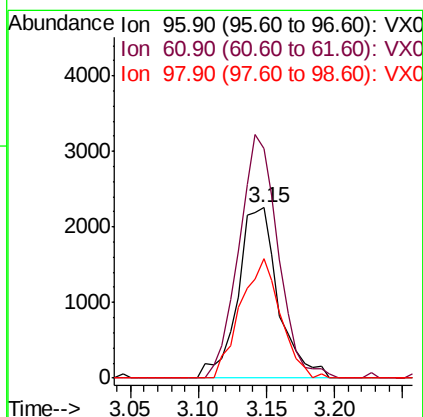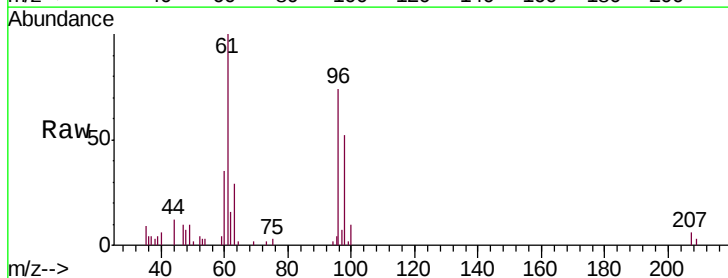



#25

2-Butanone

Concen: 0.715 ug/l

RT: 4.64 min Scan# 583

Delta R.T. 0.01 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :


1005-MW-03ADL

Tgt Ion: 43 Resp: 1411

Ion Ratio Lower Upper




43 100

72 7.2 20.8 31.2#

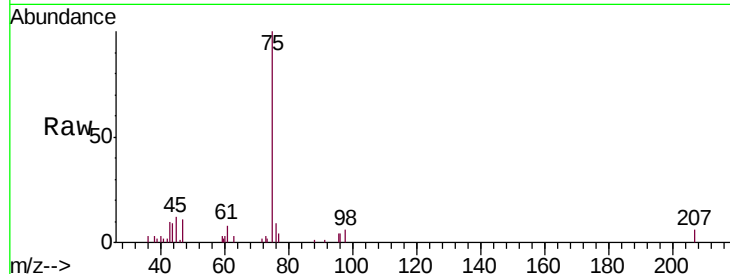

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

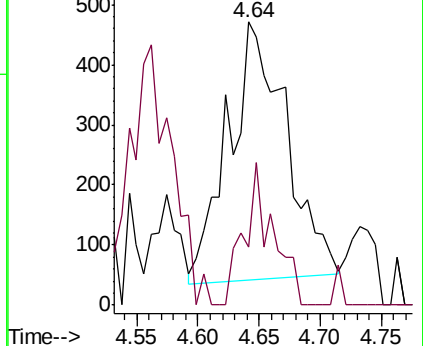

#27

cis-1,2-Dichloroethene

Concen: 24.956 ug/l

RT: 4.57 min Scan# 571

Delta R.T. 0.01 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51


Tgt Ion: 96 Resp: 79718

Ion Ratio Lower Upper

96 100

61 125.2 0.0 282.8



98 64.9 0.0 127.6

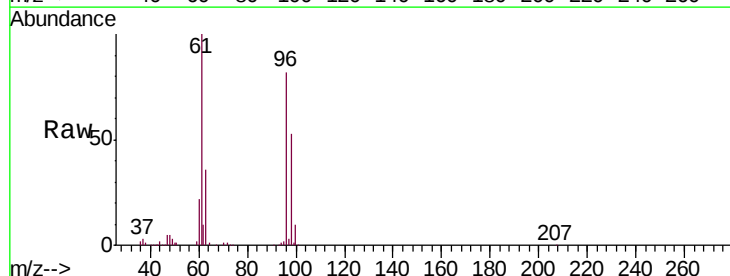


Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

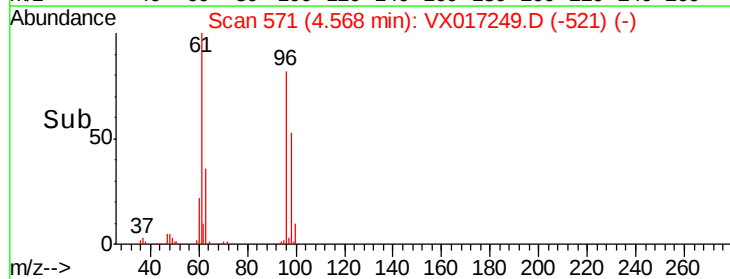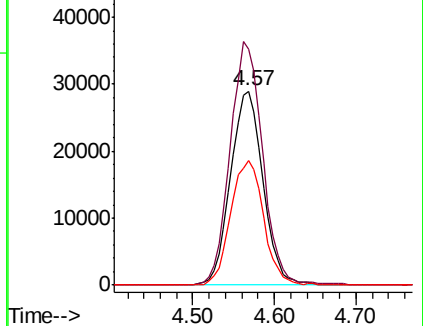


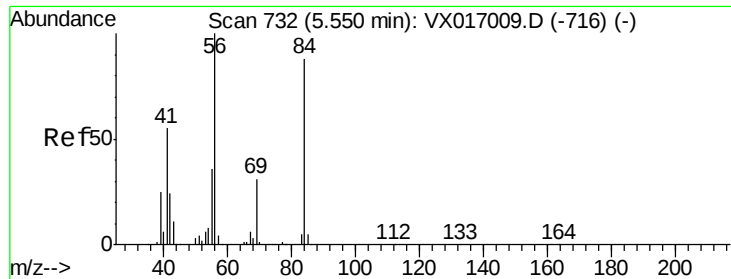




#31
Cyclohexane
Concen: 1.157 ug/l
RT: 5.63 min Scan# 745
Delta R.T. 0.08 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51

Instrument :
MSVOA_X
ClientSampleId :
1005-MW-03ADL

Tgt Ion: 56 Resp: 4943
Ion Ratio Lower Upper
56 100
69 193.2 25.0 37.4#
84 119.2 69.1 103.7#

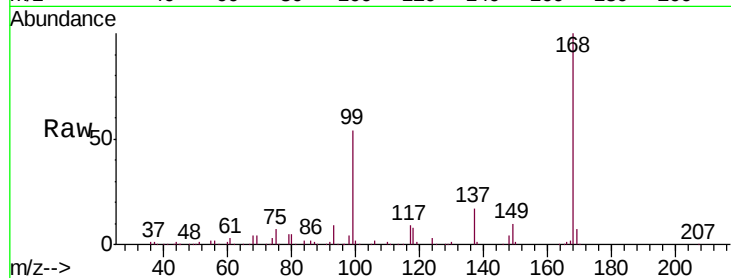


Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0

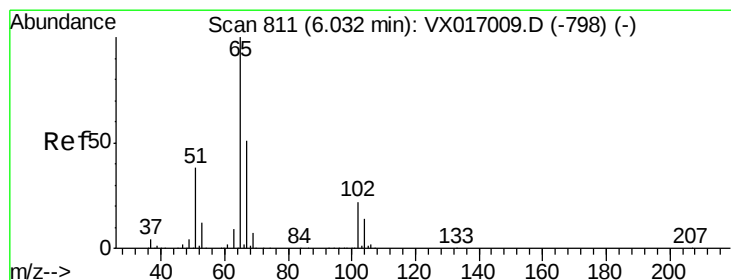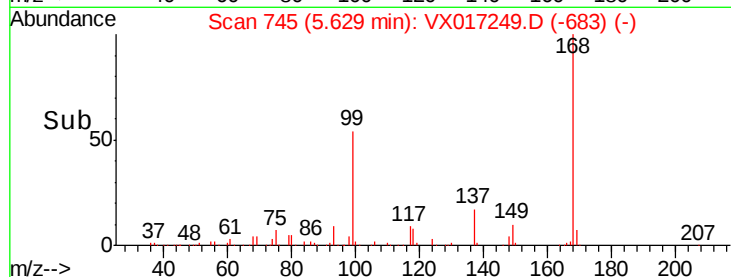
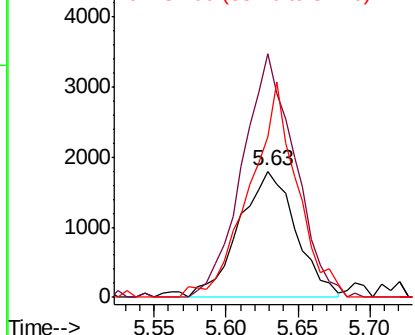



#33
1,2-Dichloroethane-d4
Concen: 52.005 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51

Tgt Ion: 65 Resp: 164620
Ion Ratio Lower Upper
65 100
67 51.7 0.0 103.8

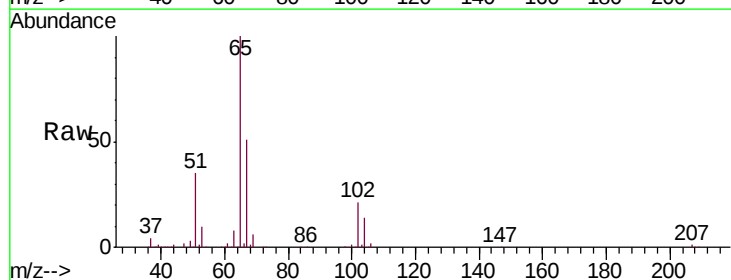

Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0

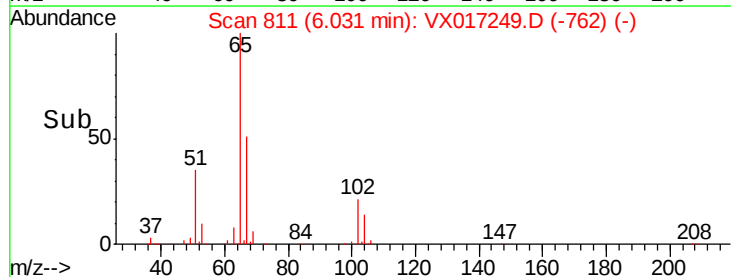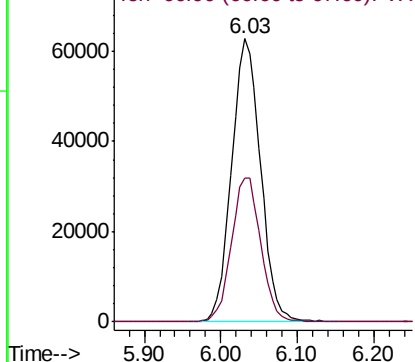

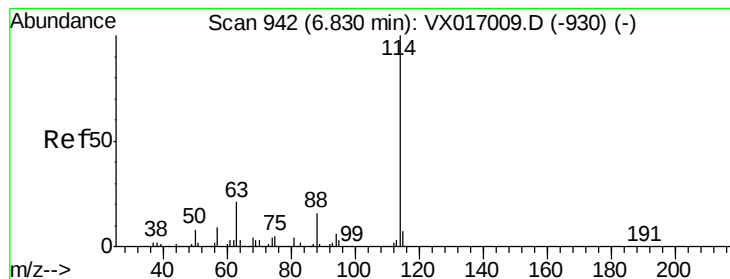

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :

1005-MW-03ADL


Tgt Ion:114 Resp: 417673

Ion Ratio Lower Upper

114 100

63 19.7 0.0 41.4




88 15.7 0.0 32.4

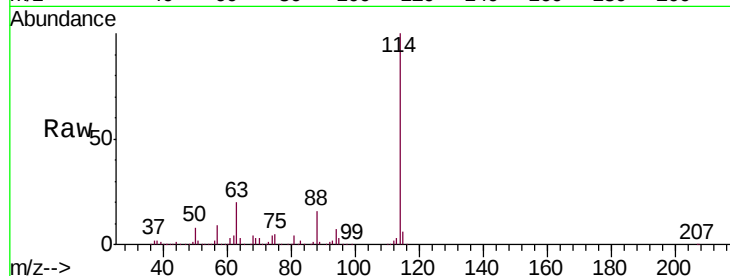

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

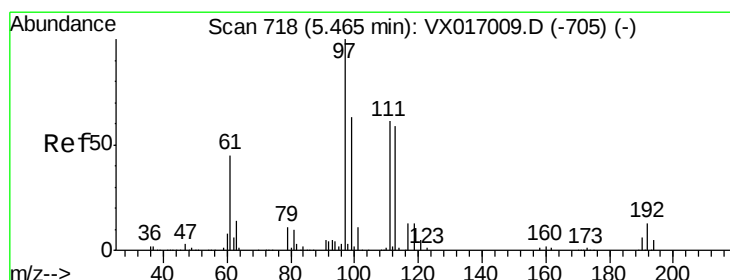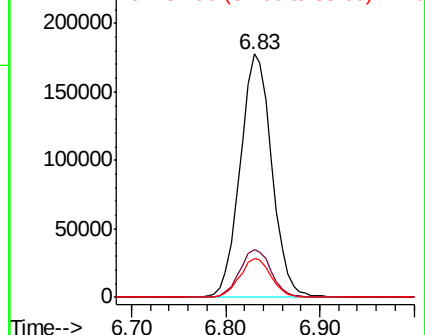

#35

Dibromofluoromethane

Concen: 54.101 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51


Tgt Ion:113 Resp: 142938

Ion Ratio Lower Upper

113 100

111 101.1 81.9 122.9



192 21.7 16.7 25.1




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

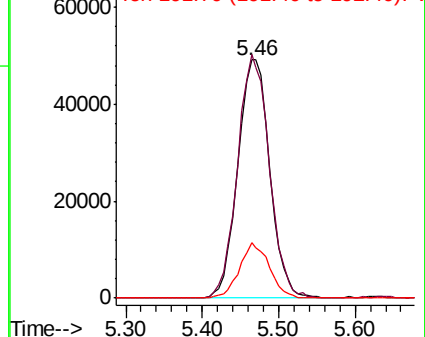

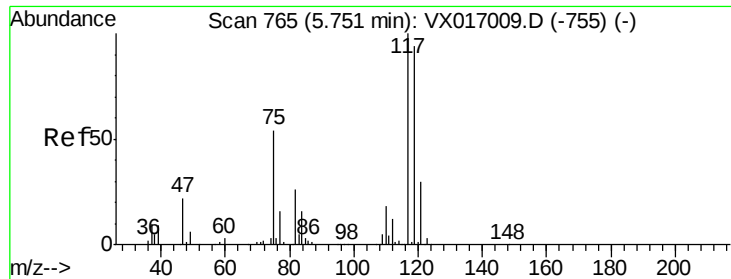

#38

Carbon Tetrachloride

Concen: 5.690 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.12 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :

1005-MW-03ADL


Tgt Ion:117 Resp: 24740

Ion Ratio Lower Upper

117 100

119 7.3 75.4 113.0#




121 0.0 23.8 35.6#

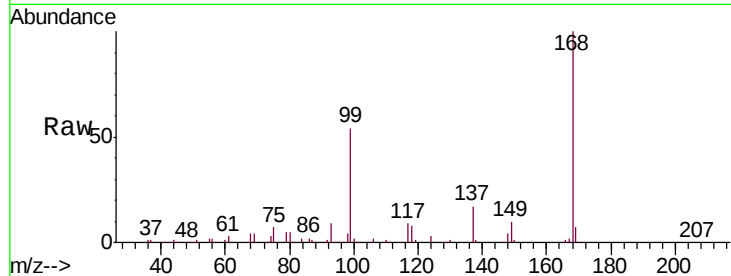

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

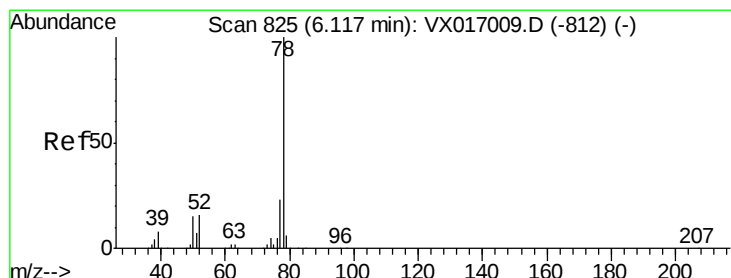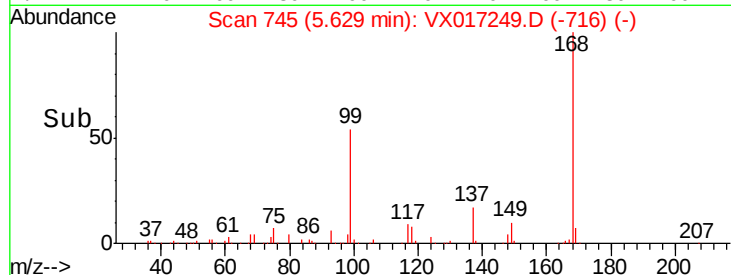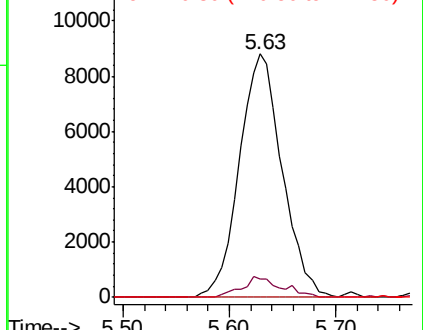

#40

Benzene

Concen: 0.210 ug/l

RT: 6.12 min Scan# 825

Delta R.T. -0.00 min

Lab File: VX017249.D


Acq: 08 Jul 2020 12:51

Tgt Ion: 78 Resp: 2438

Ion Ratio Lower Upper



78 100


77 28.9 18.3 27.5#

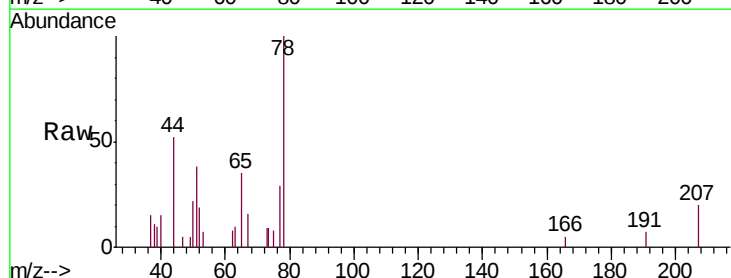

Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

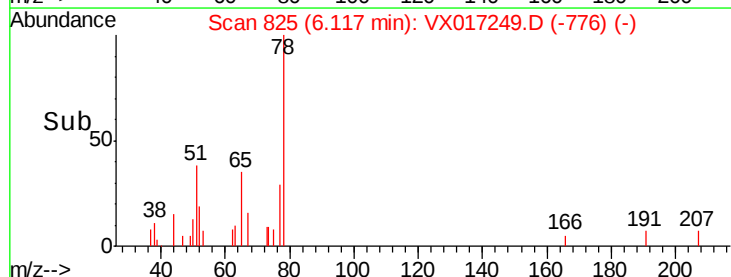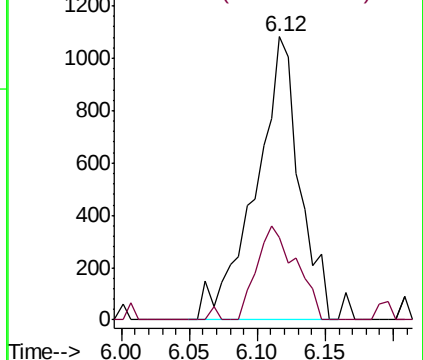

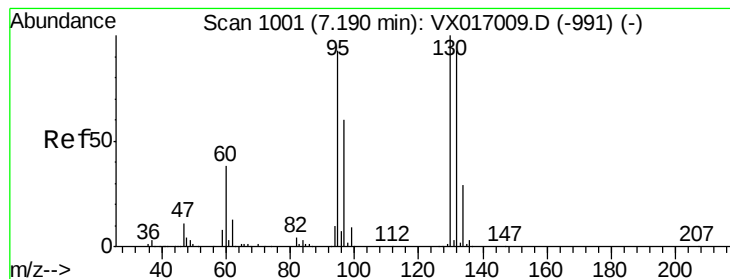

#44

Trichloroethene

Concen: 22.739 ug/l

RT: 7.19 min Scan# 1001

Delta R.T. 0.00 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :


1005-MW-03ADL

Tgt Ion:130 Resp: 73317

Ion Ratio Lower Upper

130 100

95 95.6 0.0 185.0



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

7.19

40000

30000



20000

10000

0

Time-->

7.10 7.15 7.20 7.25 7.30

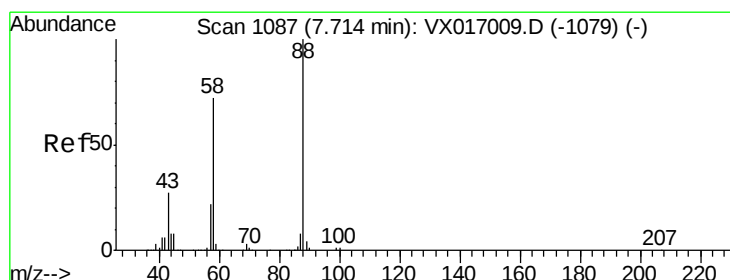

#49

1,4-Dioxane

Concen: 0.279 ug/l

RT: 7.95 min Scan# 1125

Delta R.T. 0.23 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51


Tgt Ion: 88 Resp: 20

Ion Ratio Lower Upper

88 100

43 1145.0 25.8 38.8#

58 0.0 54.8 82.2#



Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

150


100


50

0

Time-->

7.93 7.94 7.95 7.96





#50

Toluene-d8

Concen: 52.052 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :





1005-MW-03ADL

Tgt Ion: 98 Resp: 508540

Ion Ratio Lower Upper

98 100

100 66.2 53.8 80.6

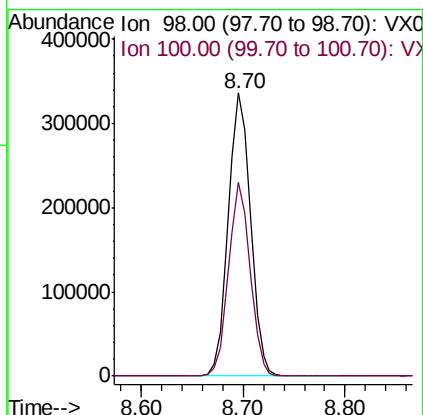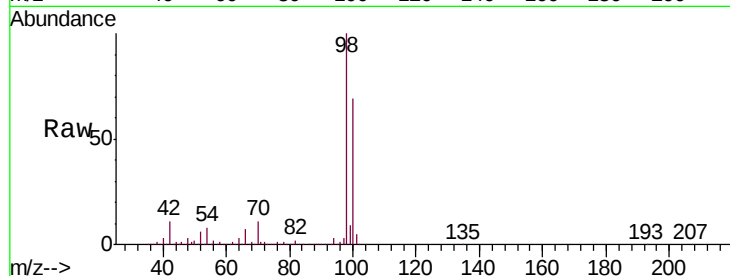

#51

4-Methyl-2-Pentanone

Concen: 0.202 ug/l

RT: 8.63 min Scan# 1237

Delta R.T. 0.01 min

Lab File: VX017249.D




Acq: 08 Jul 2020 12:51


Tgt Ion: 43 Resp: 801

Ion Ratio Lower Upper

43 100

58 39.5 31.9 47.9


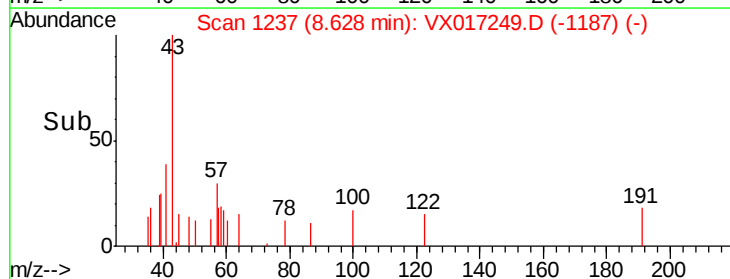
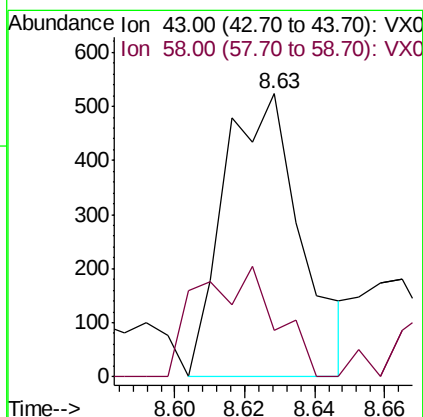



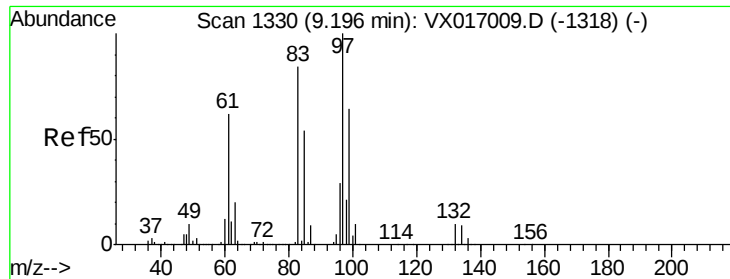

#55
 1,1,2-Trichloroethane
 Concen: 0.696 ug/l
 RT: 9.31 min Scan# 1349
 Delta R.T. 0.12 min
 Lab File: VX017249.D
 Acq: 08 Jul 2020 12:51




Instrument :
 MSVOA_X
 ClientSampleId :
 1005-MW-03ADL


Tgt Ion:	97	Resp:	2059
Ion	Ratio	Lower	Upper
97	100		
83	195.8	67.0	100.6#
85	18.1	43.5	65.3#
99	15.5	51.0	76.6#

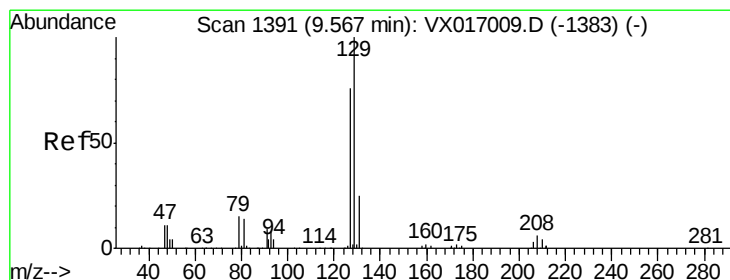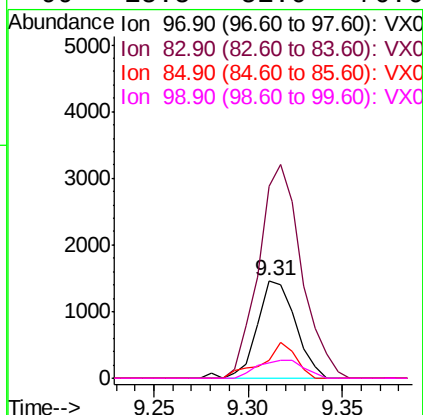

#60
 Dibromochloromethane
 Concen: 63.716 ug/l
 RT: 9.32 min Scan# 1350
 Delta R.T. -0.25 min
 Lab File: VX017249.D
 Acq: 08 Jul 2020 12:51

Tgt Ion:	129	Resp:	218951
Ion	Ratio	Lower	Upper
129	100		
127	0.2	38.9	116.7#

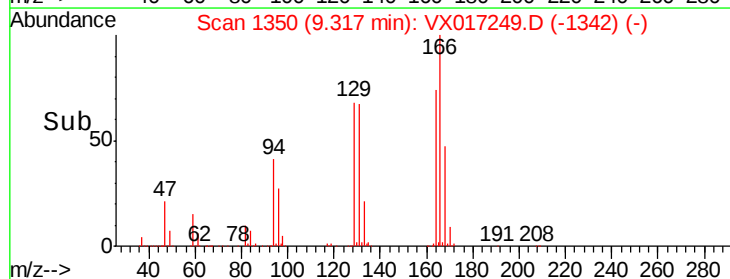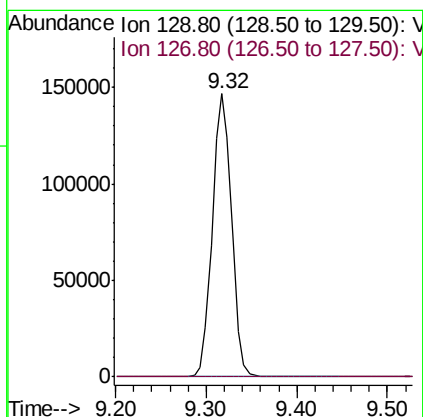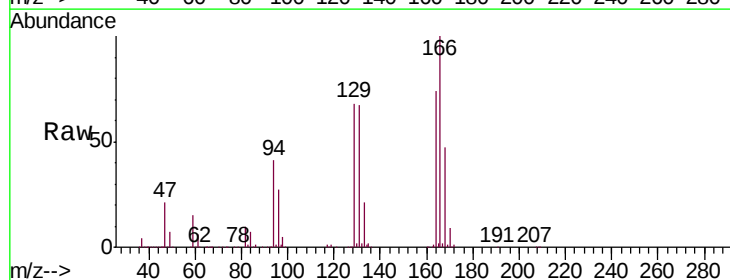



#62

4-Bromofluorobenzene

Concen: 53.182 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :

1005-MW-03ADL


Tgt Ion: 95 Resp: 203110

Ion Ratio Lower Upper

95 100

174 84.9 0.0 164.0




176 81.9 0.0 157.6

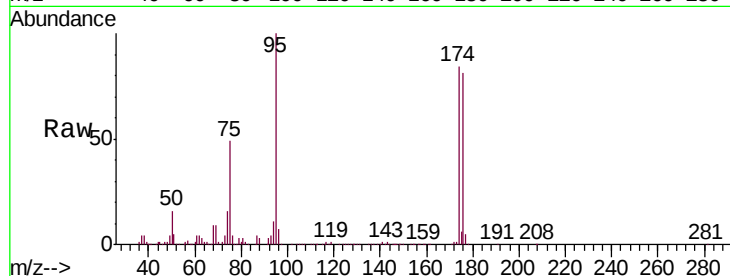

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

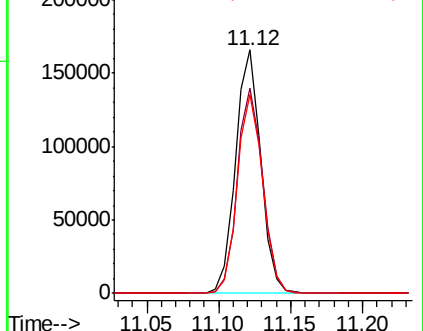

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51


Tgt Ion: 117 Resp: 428735

Ion Ratio Lower Upper

117 100

82 51.0 42.6 63.8



119 31.9 25.4 38.2




Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V



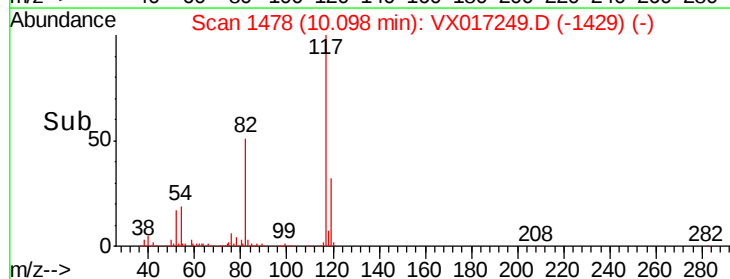
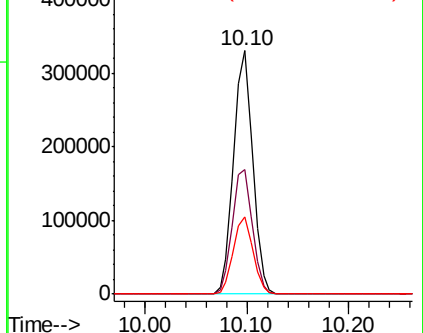


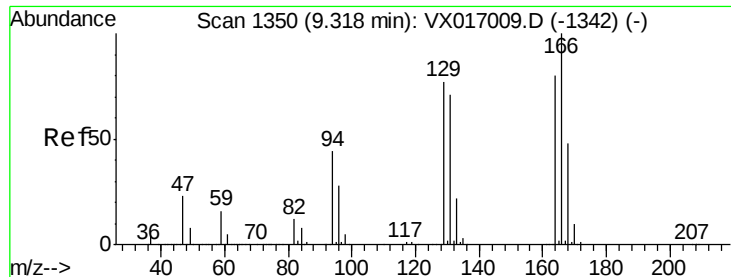

#64
Tetrachloroethene
Concen: 68.710 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.00 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51




Instrument :
MSVOA_X
ClientSampleId :
1005-MW-03ADL


Tgt Ion	Ratio	Lower	Upper
164	100		
166	134.7	99.4	149.0
129	91.3	76.3	114.5
131	89.7	70.6	105.8

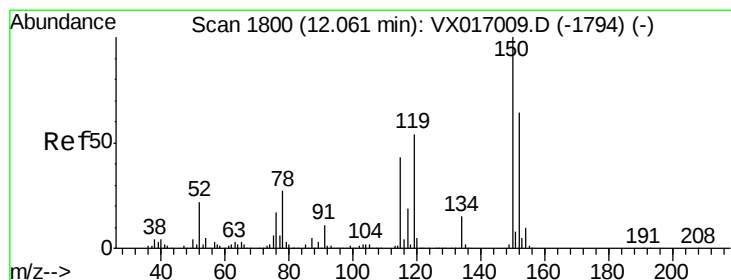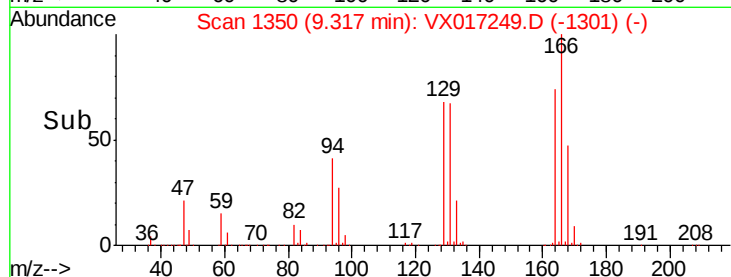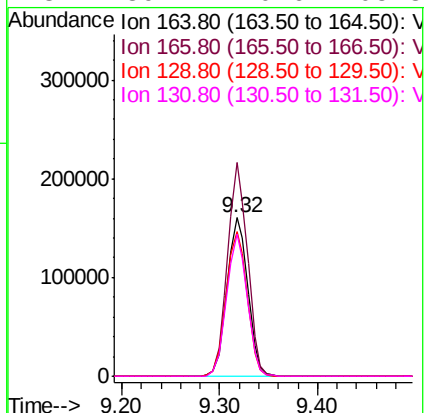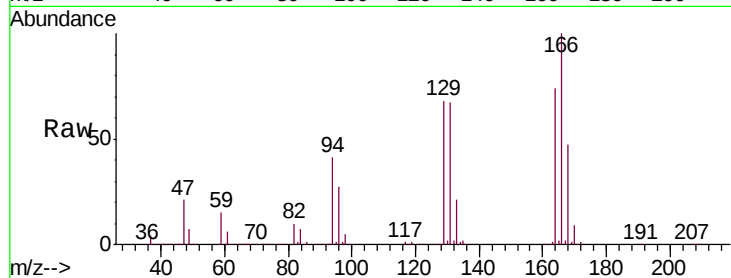

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX017249.D
Acq: 08 Jul 2020 12:51

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.9	40.9	122.7
150	155.9	0.0	351.6

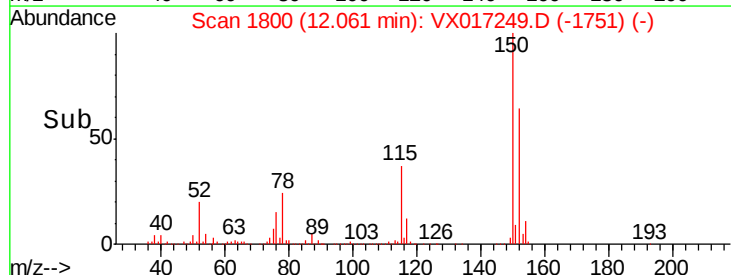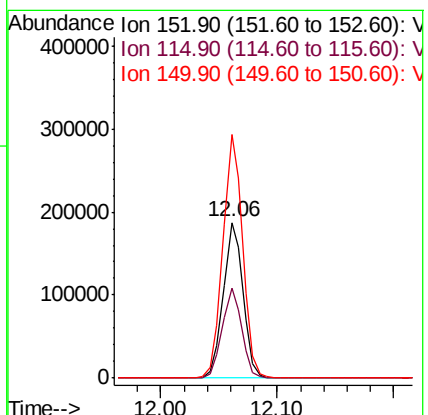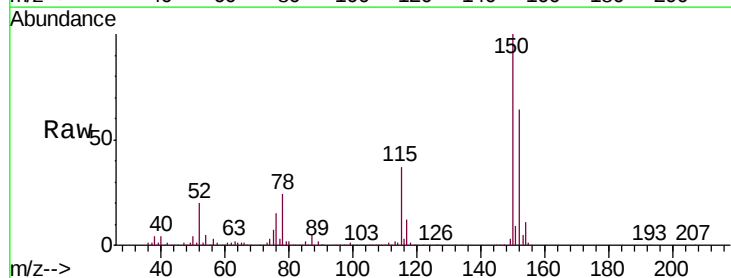



#76

1,2,3-Trichloropropane

Concen: 23.472 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :


1005-MW-03ADL

Tgt Ion: 75 Resp: 100976

Ion Ratio Lower Upper




75 100

77 1.2 20.2 60.6#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

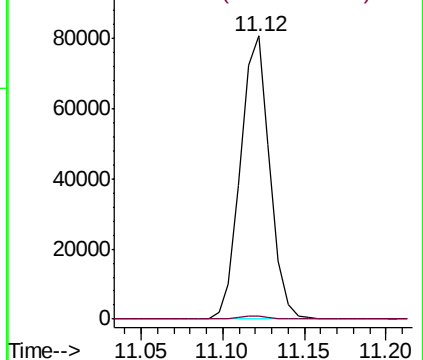

#81

trans-1,4-Dichloro-2-butene

Concen: 60.784 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51


Tgt Ion: 75 Resp: 100976

Ion Ratio Lower Upper

75 100

53 0.3 72.4 108.6#



89 0.0 37.0 55.4#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

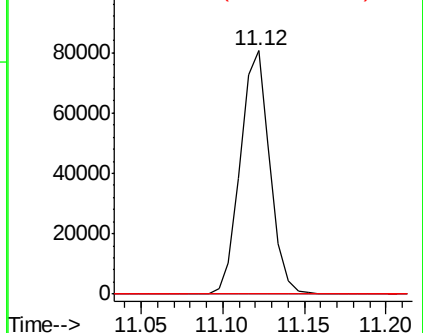

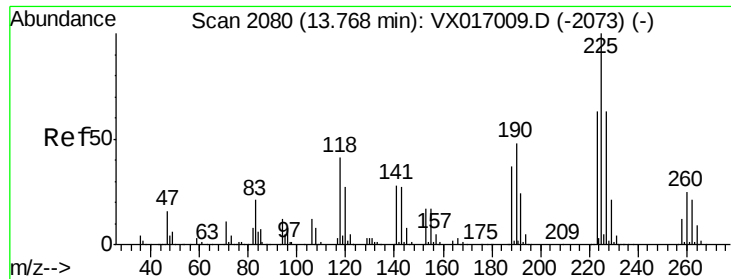

#94

Hexachlorobutadiene

Concen: 1.013 ug/l

RT: 13.76 min Scan# 2079

Delta R.T. -0.01 min

Lab File: VX017249.D

Acq: 08 Jul 2020 12:51

Instrument :

MSVOA_X

ClientSampleId :

1005-MW-03ADL



Tgt Ion: 225 Resp: 298

Ion Ratio Lower Upper

225 100

223 86.6 32.5 97.5


227 81.2 33.1 99.2

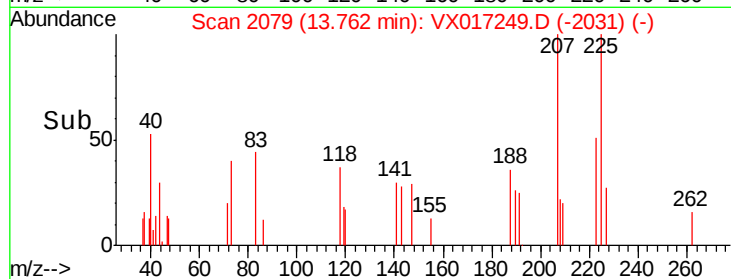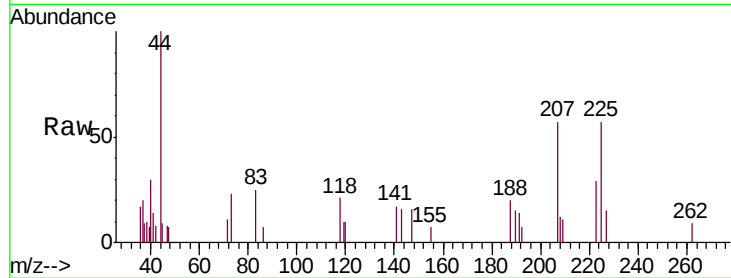

Abundance Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

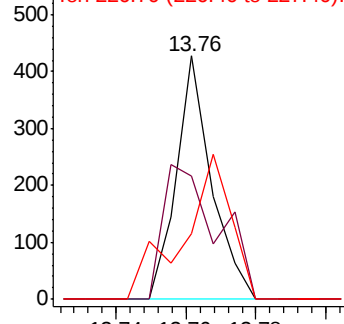

Time-->