

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070820\  
 Data File : VX017258.D  
 Acq On : 08 Jul 2020 16:16  
 Operator : JC/SP  
 Sample : L3232-01  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 1003-MW-01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X062920W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.568       | 558           | 571         | 588          | rBV      | 471919         | 1316197       | 13.94%          | 6.432%        |
| 2         | 5.464       | 707           | 718         | 731          | rBV2     | 168676         | 492902        | 5.22%           | 2.409%        |
| 3         | 5.629       | 735           | 745         | 758          | rVB      | 266860         | 746102        | 7.90%           | 3.646%        |
| 4         | 6.031       | 800           | 811         | 822          | rBV      | 173323         | 461852        | 4.89%           | 2.257%        |
| 5         | 6.836       | 932           | 943         | 955          | rBV      | 413362         | 1002164       | 10.62%          | 4.897%        |
| 6         | 7.190       | 991           | 1001        | 1018         | rBV      | 823520         | 1746737       | 18.51%          | 8.536%        |
| 7         | 8.695       | 1241          | 1248        | 1258         | rBV      | 909214         | 1385060       | 14.67%          | 6.769%        |
| 8         | 9.317       | 1342          | 1350        | 1369         | rBV      | 6397630        | 9439213       | 100.00%         | 46.128%       |
| 9         | 10.098      | 1471          | 1478        | 1488         | rBV      | 989413         | 1342551       | 14.22%          | 6.561%        |
| 10        | 11.122      | 1640          | 1646        | 1656         | rBV      | 893500         | 1098493       | 11.64%          | 5.368%        |
| 11        | 12.061      | 1795          | 1800        | 1807         | rBV      | 1156484        | 1431687       | 15.17%          | 6.996%        |


Sum of corrected areas: 20462958

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070820\  
Data File : VX017258.D  
Acq On : 08 Jul 2020 16:16  
Operator : JC/SP  
Sample : L3232-01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1003-MW-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X062920W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

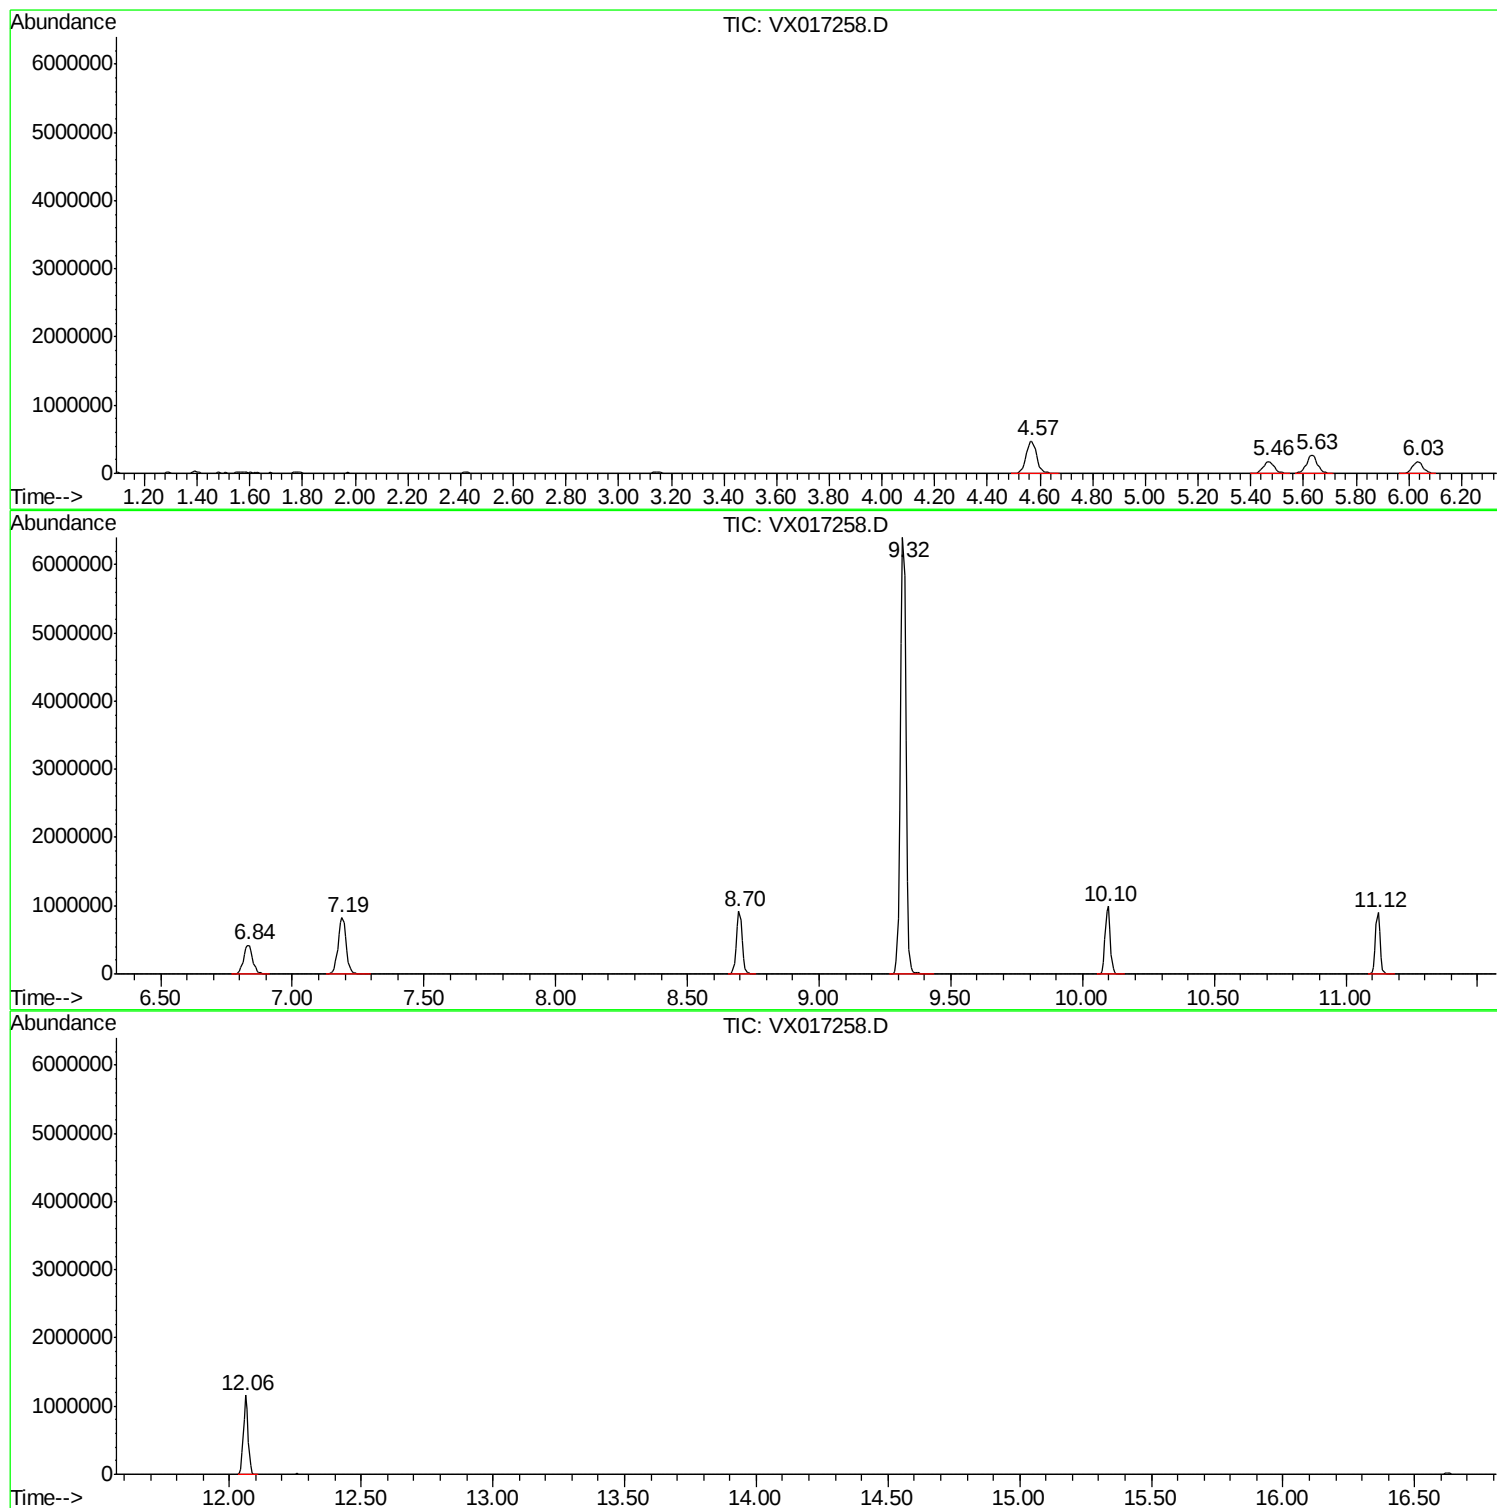

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX070820\  
Data File : VX017258.D  
Acq On : 08 Jul 2020 16:16  
Operator : JC/SP  
Sample : L3232-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1003-MW-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X062920W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX070820\  
Data File : VX017258.D  
Acq On : 08 Jul 2020 16:16  
Operator : JC/SP  
Sample : L3232-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1003-MW-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X062920W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |