

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070821\
 Data File : VX023187.D
 Acq On : 08 Jul 2021 10:14
 Operator : JC/MD
 Sample : VX0708MBL01
 Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0708MBL01

Quant Time: Jul 09 02:08:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 02 14:29:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	239171	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	388416	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	346837	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	147545	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	158041	49.166	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.340%
35) Dibromofluoromethane	5.397	113	124093	49.474	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.940%
50) Toluene-d8	8.653	98	461720	49.349	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.700%
62) 4-Bromofluorobenzene	11.085	95	168200	46.566	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070821\
Data File : VX023187.D
Acq On : 08 Jul 2021 10:14
Operator : JC/MD
Sample : VX0708MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0708MBL01

Quant Time: Jul 09 02:08:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 02 14:29:42 2021
Response via : Initial Calibration




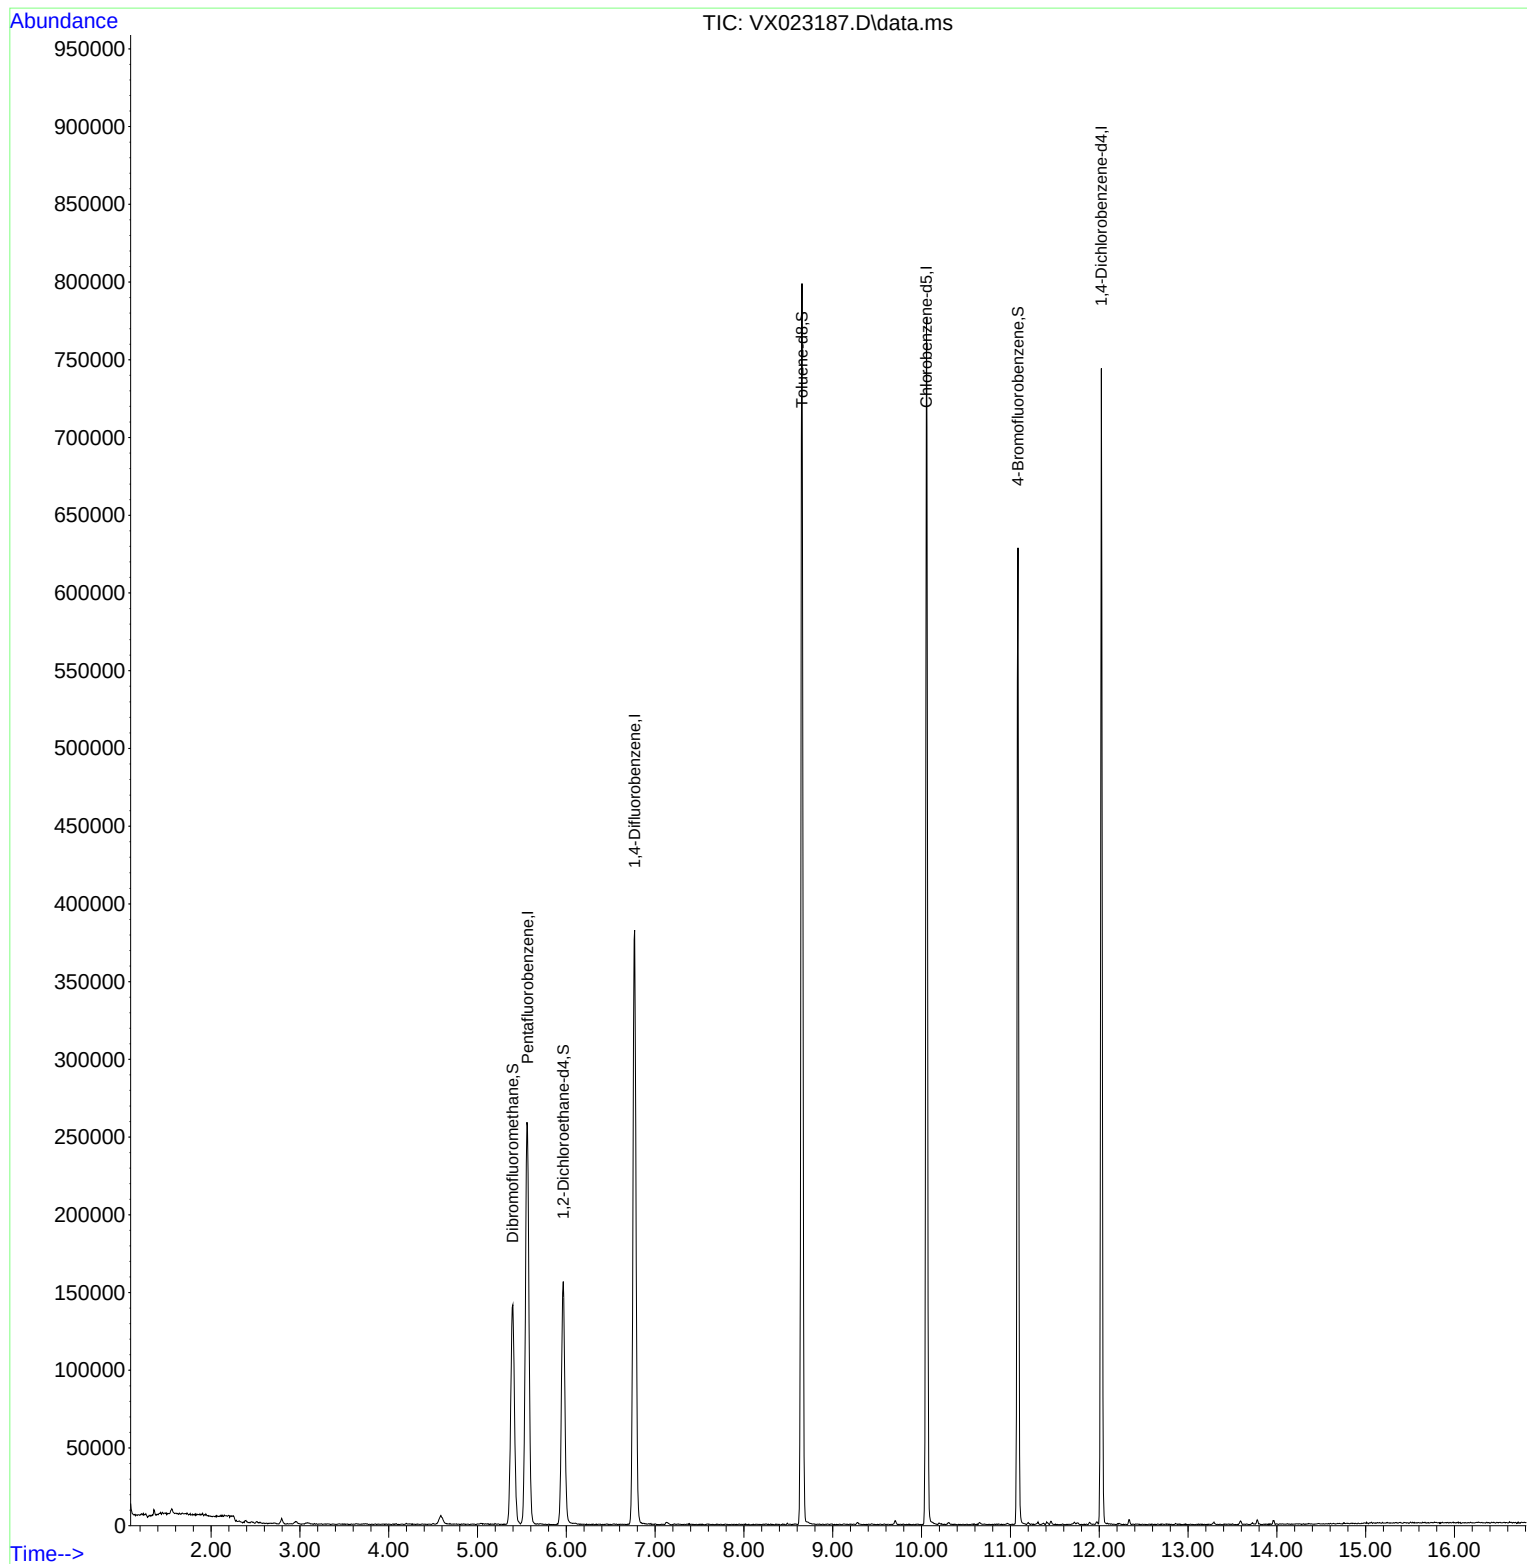


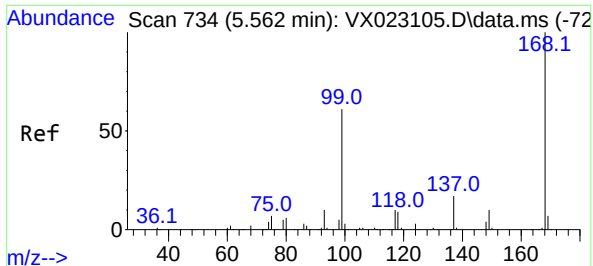

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023187.D
Acq: 08 Jul 2021 10:14




Instrument :
MSVOA_X
ClientSampleId :
VX0708MBL01


Tgt Ion:168 Resp: 239171
Ion Ratio Lower Upper
168 100
99 57.9 45.8 68.6

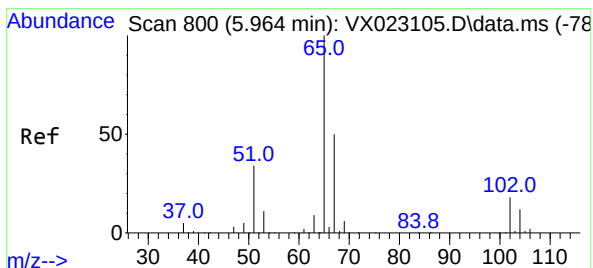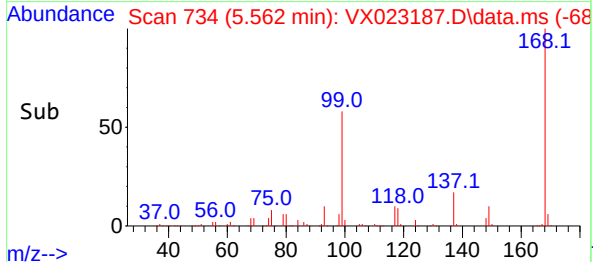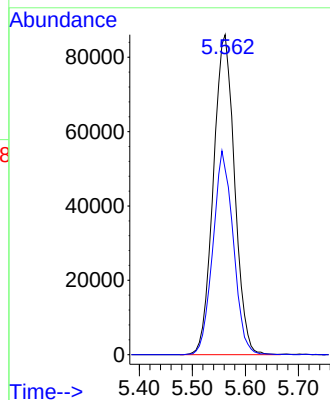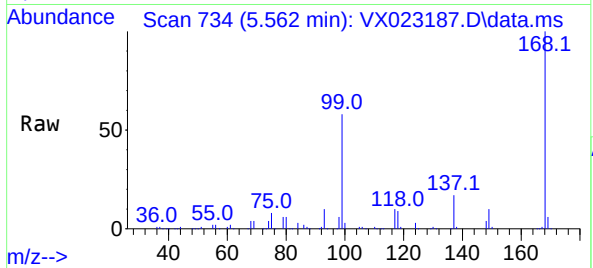

#33
1,2-Dichloroethane-d4
Concen: 49.166 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023187.D
Acq: 08 Jul 2021 10:14

Tgt Ion: 65 Resp: 158041
Ion Ratio Lower Upper
65 100
67 50.9 0.0 105.4


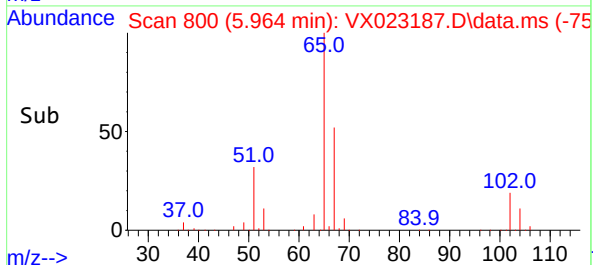
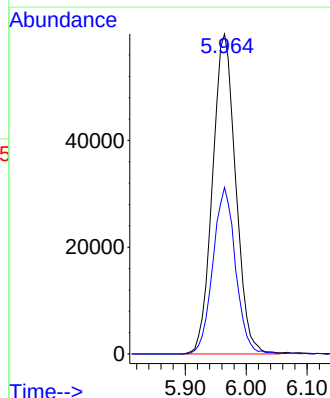
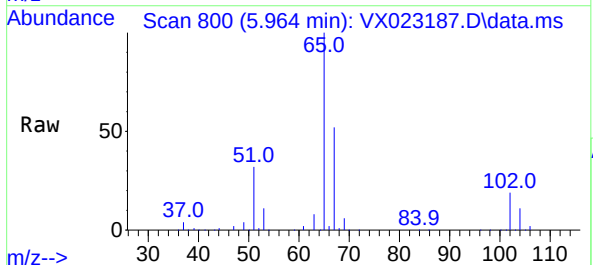


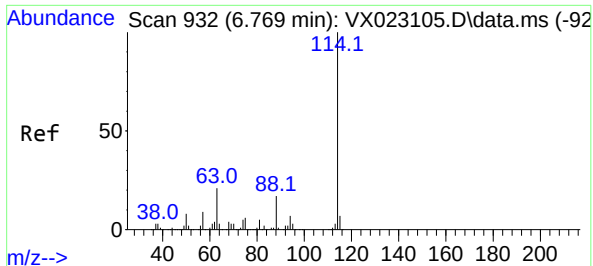

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX023187.D
Acq: 08 Jul 2021 10:14




Instrument :
MSVOA_X
ClientSampleId :
VX0708MBL01


Tgt Ion:114 Resp: 388416
Ion Ratio Lower Upper
114 100
63 21.5 0.0 40.8
88 17.2 0.0 32.8

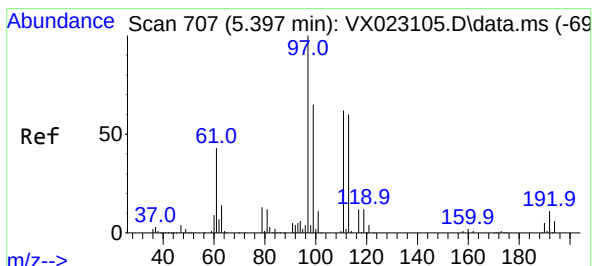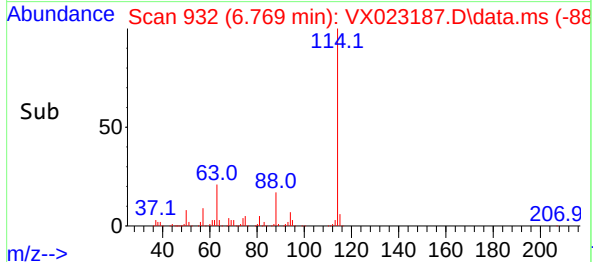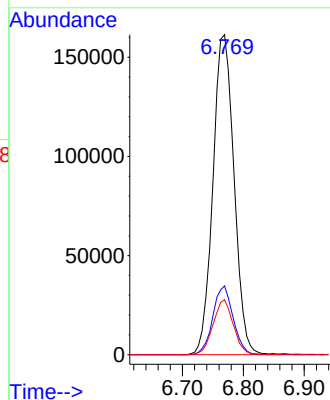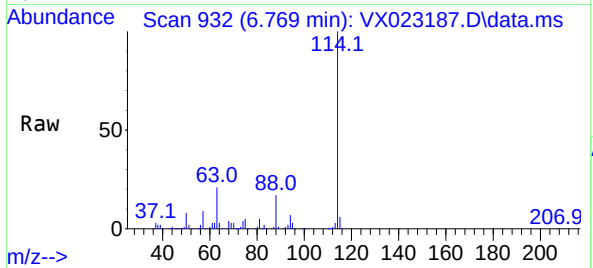

#35
Dibromofluoromethane
Concen: 49.474 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023187.D
Acq: 08 Jul 2021 10:14

Tgt Ion:113 Resp: 124093
Ion Ratio Lower Upper
113 100
111 101.8 81.9 122.9
192 18.8 16.7 25.1


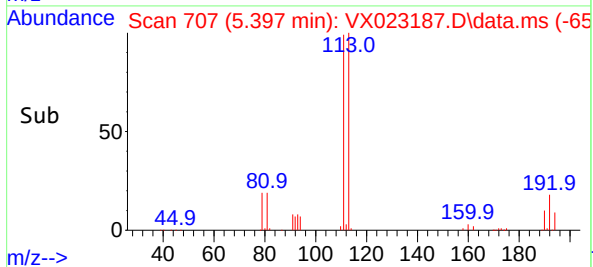
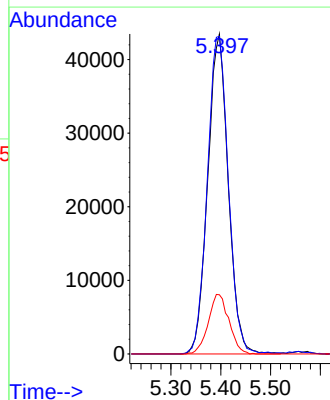
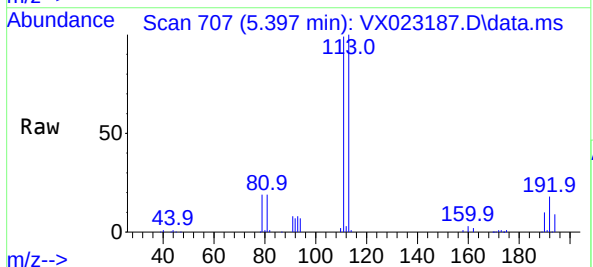


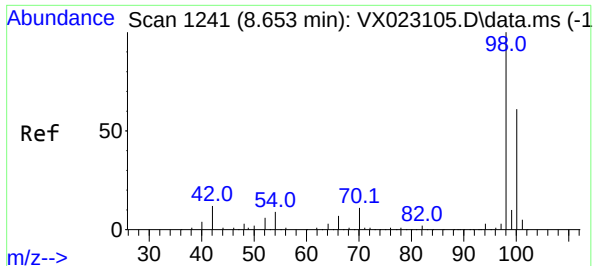

#50
Toluene-d8
Concen: 49.349 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023187.D
Acq: 08 Jul 2021 10:14




Instrument :
MSVOA_X
ClientSampleId :
VX0708MBL01


Tgt Ion: 98 Resp: 461720
Ion Ratio Lower Upper
98 100
100 63.8 51.9 77.9

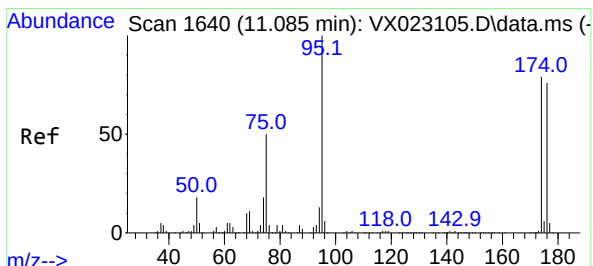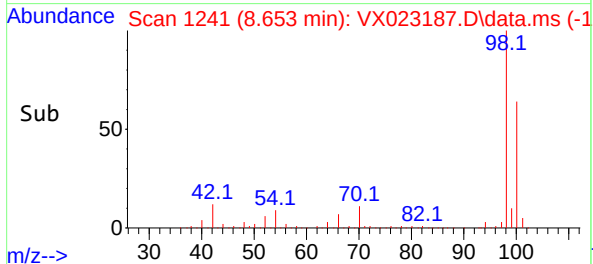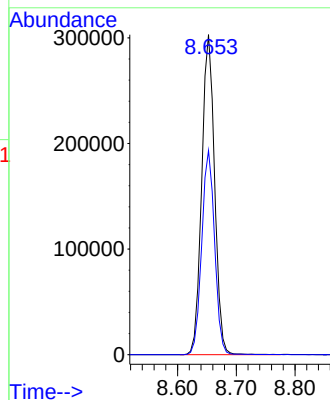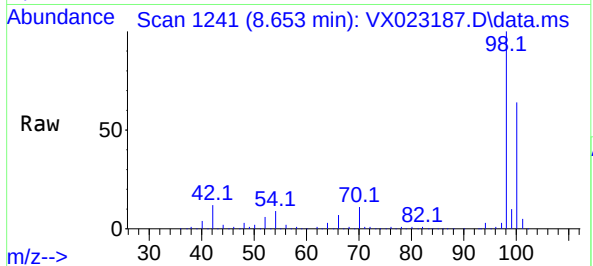

#62
4-Bromofluorobenzene
Concen: 46.566 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023187.D
Acq: 08 Jul 2021 10:14

Tgt Ion: 95 Resp: 168200
Ion Ratio Lower Upper
95 100
174 76.2 0.0 154.6
176 73.4 0.0 155.8


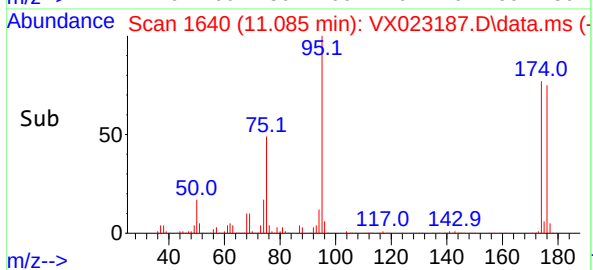
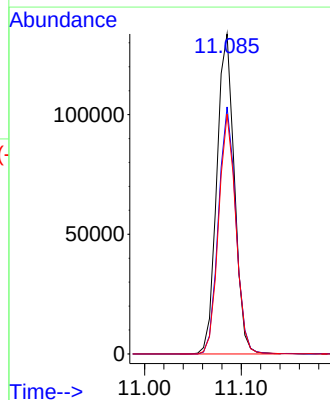
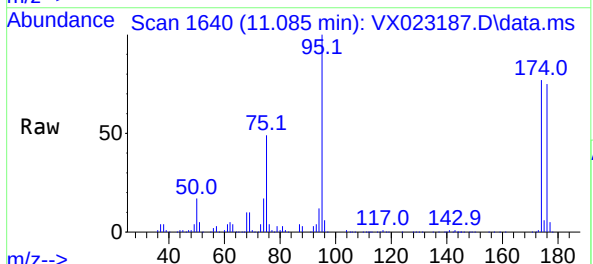


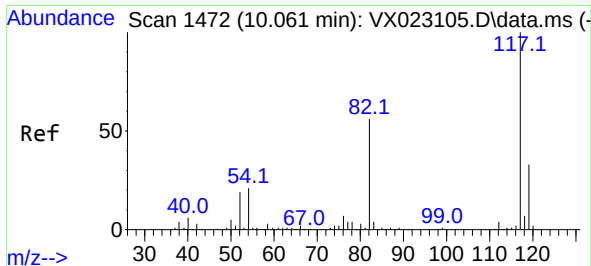

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023187.D
Acq: 08 Jul 2021 10:14

Instrument :
MSVOA_X
ClientSampleId :
VX0708MBL01

Tgt Ion:117 Resp: 346837
Ion Ratio Lower Upper
117 100
82 58.3 47.4 71.2
119 31.5 26.6 39.8

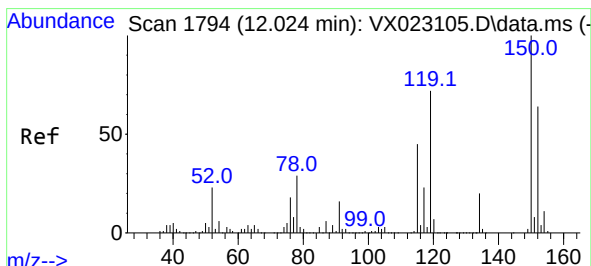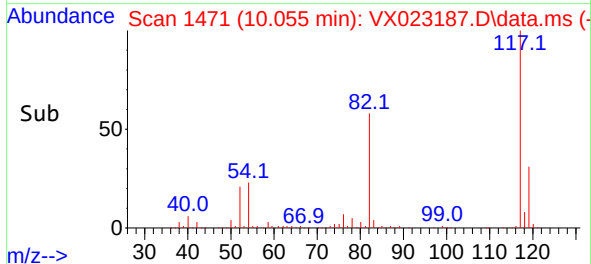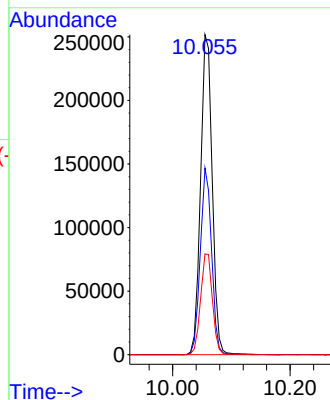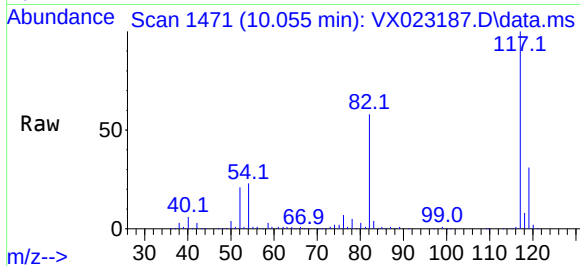

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023187.D
Acq: 08 Jul 2021 10:14

Tgt Ion:152 Resp: 147545
Ion Ratio Lower Upper
152 100
115 62.2 41.1 123.3
150 157.9 0.0 349.0

