
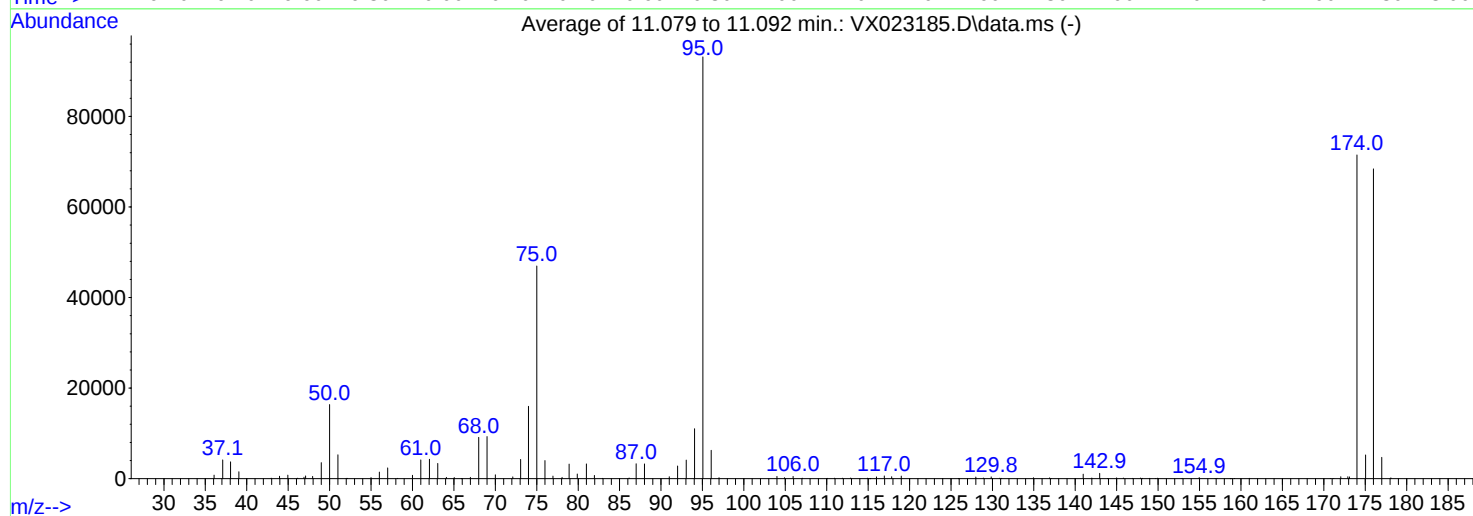


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070821\
 Data File : VX023185.D
 Acq On : 08 Jul 2021 08:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Title : SW846 8260
 Last Update : Fri Jul 02 14:29:42 2021

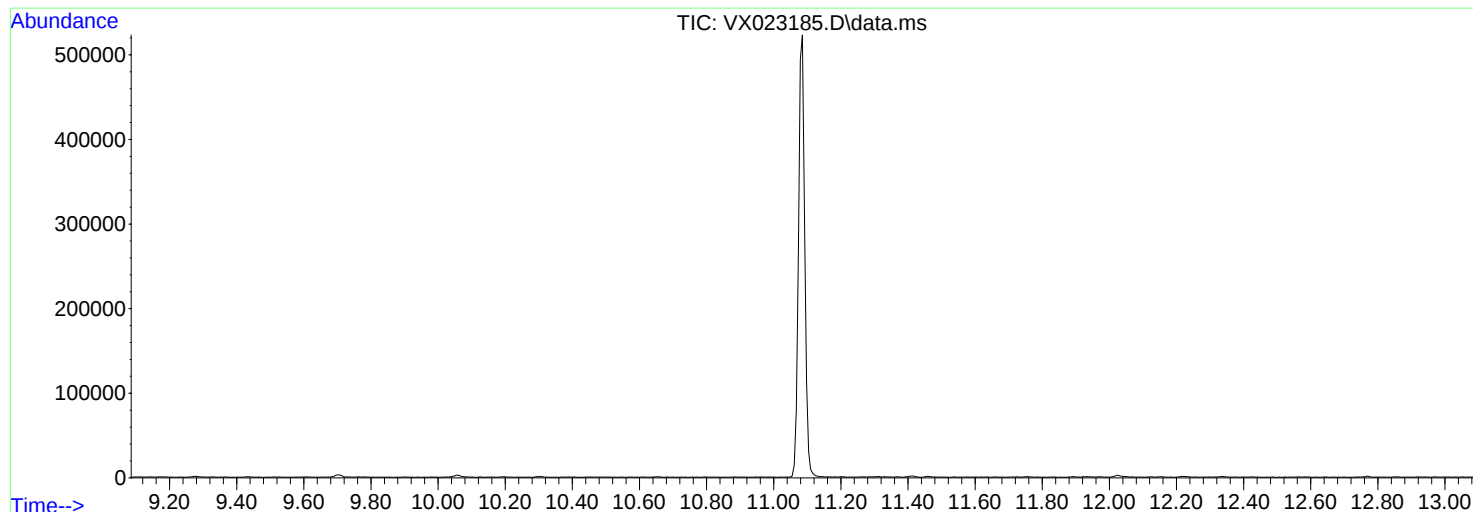

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	16360	PASS
75	95	30	60	50.4	46981	PASS
95	95	100	100	100.0	93163	PASS
96	95	5	9	6.7	6265	PASS
173	174	0.00	2	0.6	430	PASS
174	95	50	100	76.7	71496	PASS
175	174	5	9	7.3	5238	PASS
176	174	95	101	95.7	68427	PASS
177	176	5	9	6.9	4695	PASS