

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070822\
 Data File : VX029970.D
 Acq On : 08 Jul 2022 13:43
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X070822W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX029970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.325	197	203	209	rVB7	4567	9642	1.49%	0.358%
2	2.514	229	234	240	rVB	8694	13054	2.01%	0.485%
3	2.947	295	305	313	rBV	11239	26215	4.04%	0.974%
4	3.093	320	329	335	rBV4	5664	14574	2.25%	0.541%
5	4.580	564	573	585	rBV2	7218	24551	3.79%	0.912%
6	4.904	615	626	641	rBV2	73082	213738	32.98%	7.940%
7	5.696	750	756	766	rVB9	2719	8024	1.24%	0.298%
8	5.964	789	800	811	rBV	84325	225404	34.78%	8.373%
9	6.763	922	931	947	rBV	165001	399384	61.63%	14.836%
10	7.129	985	991	1000	rBV5	5214	12278	1.89%	0.456%
11	7.385	1026	1033	1039	rBV8	3347	8014	1.24%	0.298%
12	8.251	1170	1175	1181	rBV3	4458	7886	1.22%	0.293%
13	8.653	1234	1241	1249	rBV	410568	648085	100.00%	24.074%
14	9.275	1336	1343	1347	rBV5	6951	10067	1.55%	0.374%
15	10.055	1465	1471	1483	rVB	330870	450842	69.57%	16.747%
16	10.305	1505	1512	1518	rBV	11333	17008	2.62%	0.632%
17	10.659	1563	1570	1575	rBV4	6370	12412	1.92%	0.461%
18	10.963	1616	1620	1626	rVB	6351	7563	1.17%	0.281%
19	11.085	1634	1640	1647	rBV	293320	380163	58.66%	14.122%
20	11.311	1672	1677	1680	rBV	7695	10164	1.57%	0.378%
21	11.366	1682	1686	1691	rVB3	5352	6996	1.08%	0.260%
22	11.457	1696	1701	1708	rVB3	14011	20810	3.21%	0.773%
23	11.713	1740	1743	1746	rBV2	6252	8112	1.25%	0.301%
24	11.756	1746	1750	1755	rVB2	6352	9233	1.42%	0.343%
25	11.890	1768	1772	1779	rBV	7210	10828	1.67%	0.402%
26	11.969	1781	1785	1789	rVV2	9611	12808	1.98%	0.476%
27	12.006	1789	1791	1794	rVV	9101	11999	1.85%	0.446%
28	12.043	1794	1797	1807	rVB2	11125	14392	2.22%	0.535%
29	12.335	1841	1845	1851	rBV2	16964	22595	3.49%	0.839%
30	13.286	1997	2001	2009	rVB2	8049	10680	1.65%	0.397%
31	13.591	2046	2051	2058	rBV2	12574	16547	2.55%	0.615%
32	13.725	2069	2073	2077	rBV3	15441	18795	2.90%	0.698%
33	13.780	2077	2082	2088	rVV2	10159	14413	2.22%	0.535%
34	13.963	2107	2112	2119	rBV	10976	14746	2.28%	0.548%

Sum of corrected areas: 2692022




Instrument :
MSVOA_X
ClientSampleId :
IBLK

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070822\
Data File : VX029970.D
Acq On : 08 Jul 2022 13:43
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X070822W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

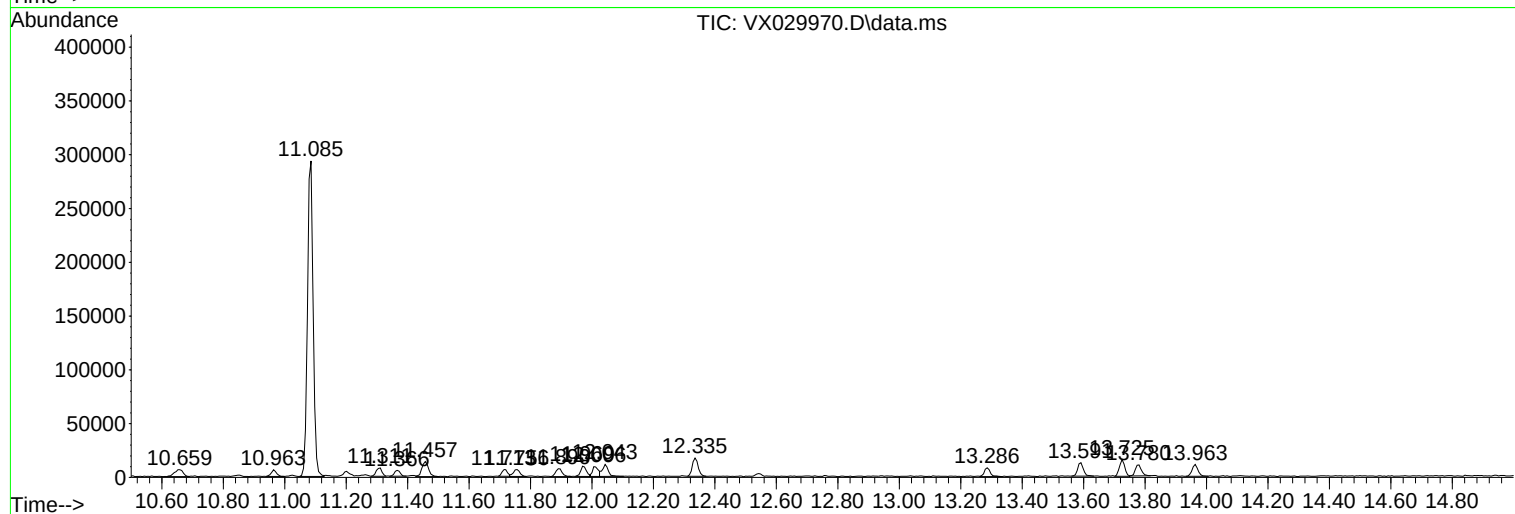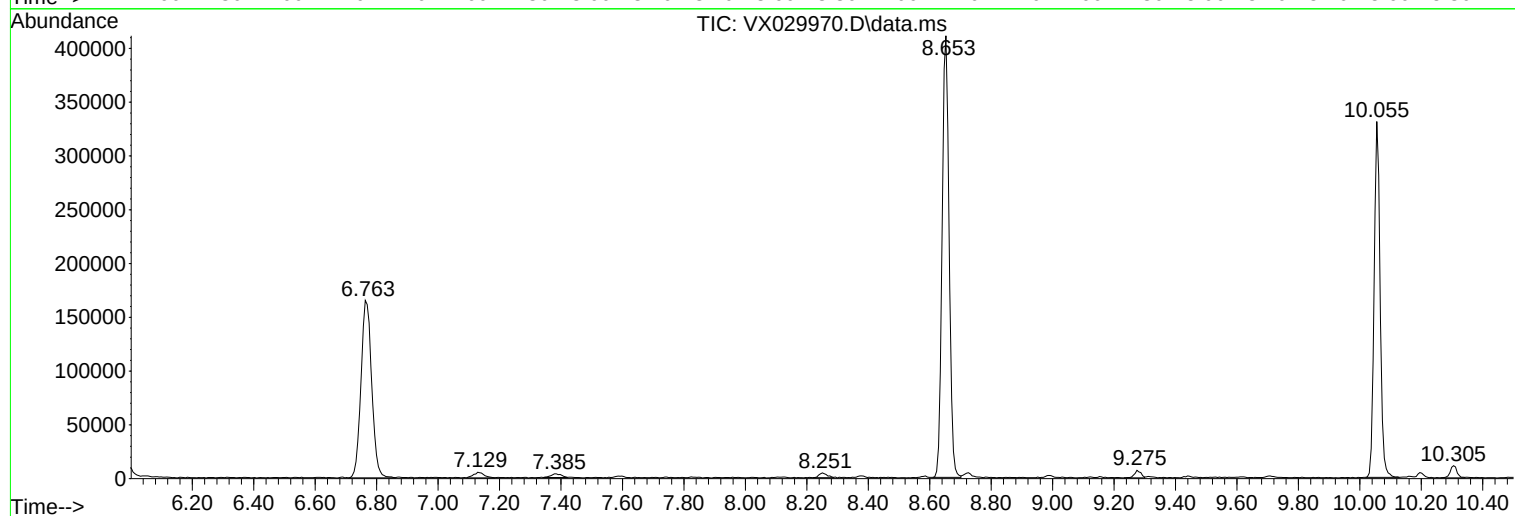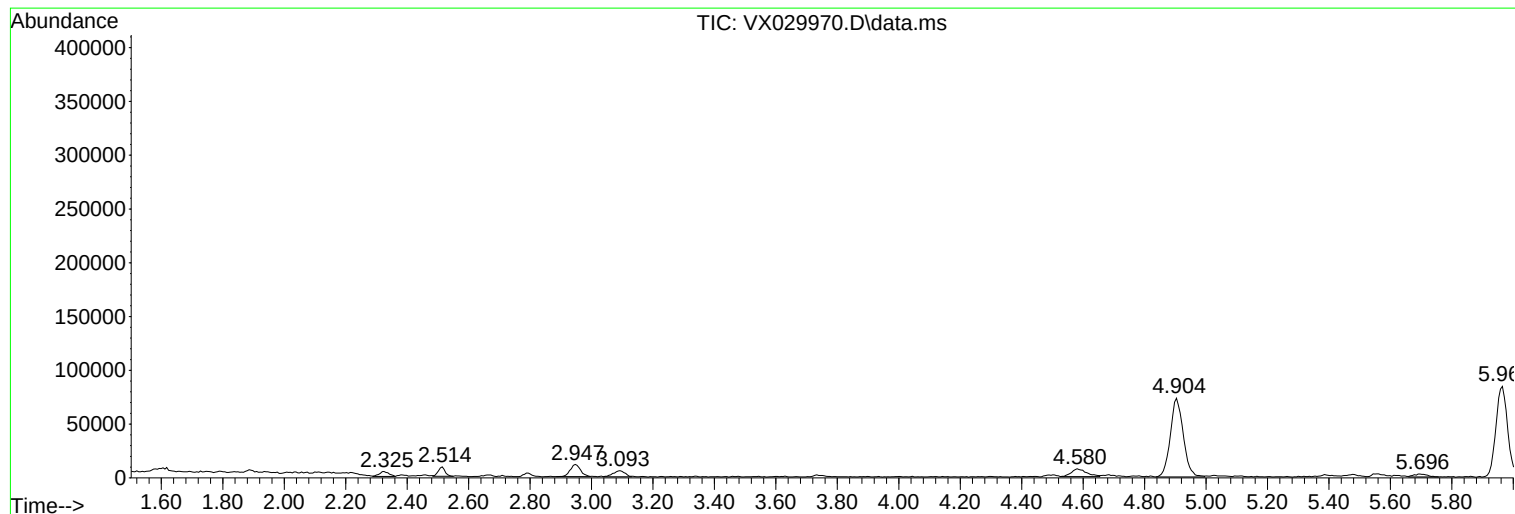

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070822\
Data File : VX029970.D
Acq On : 08 Jul 2022 13:43
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X070822W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070822\
Data File : VX029970.D
Acq On : 08 Jul 2022 13:43
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X070822W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc