
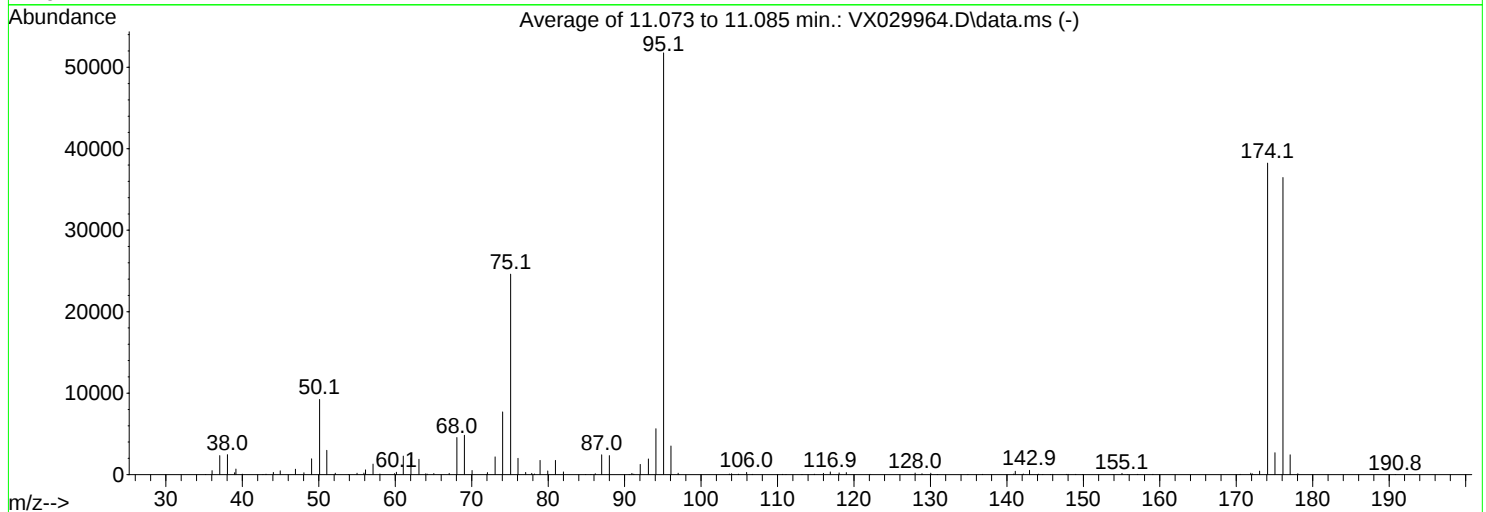


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070822\
 Data File : VX029964.D
 Acq On : 08 Jul 2022 11:20
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Title : SFAM01.0
 Last Update : Fri Jul 08 23:21:00 2022

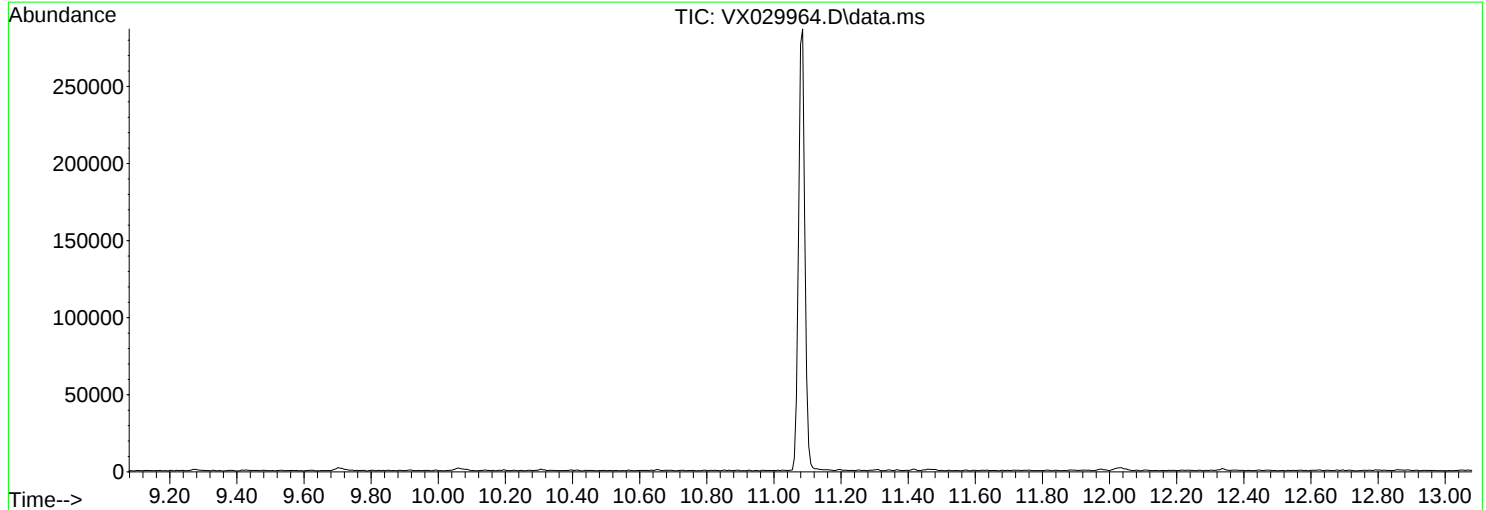

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	9235	PASS
75	95	30	80	47.5	24605	PASS
95	95	100	100	100.0	51771	PASS
96	95	5	9	6.8	3519	PASS
173	174	0.00	2	1.1	430	PASS
174	95	50	120	73.9	38243	PASS
175	174	5	9	7.0	2693	PASS
176	174	95	105	95.4	36475	PASS
177	176	5	10	6.7	2440	PASS