

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
 Data File : VX042230.D
 Acq On : 08 Jul 2024 11:50
 Operator : JC/MD
 Sample : P3100-17ME
 Misc : 4.21g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 09 02:36:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 09 02:35:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	266804	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	243720	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	123063	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.575	65	68	0.044	ug/L	0.21
Spiked Amount	50.000	Range	60 - 135	Recovery	=	0.080%#
7) Chloroethane-d5	1.648	69	6397	6.542	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	13.080%#
11) 1,1-Dichloroethene-d2	2.276	65	21629	31.823	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.640%
21) 2-Butanone-d5	4.489	46	91985	82.193	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.190%
24) Chloroform-d	5.056	84	112955	36.175	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.340%
26) 1,2-Dichloroethane-d4	5.952	65	74229	40.276	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.560%
32) Benzene-d6	5.964	84	242949	38.566	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.140%
36) 1,2-Dichloropropane-d6	7.305	67	76566	40.387	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.780%
41) Toluene-d8	8.647	98	226551	38.591	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.180%#
43) trans-1,3-Dichloroprop...	8.951	79	29858	36.441	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.880%
47) 2-Hexanone-d5	9.390	63	74210	86.236	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.240%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	110264	39.341	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.680%
66) 1,2-Dichlorobenzene-d4	12.323	152	97689	40.869	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.740%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.721	43	41022	21.148	ug/L	100
48) 2-Hexanone	9.390	43	8467	4.323	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
Data File : VX042230.D
Acq On : 08 Jul 2024 11:50
Operator : JC/MD
Sample : P3100-17ME
Misc : 4.21g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 09 02:36:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 09 02:35:21 2024
Response via : Initial Calibration

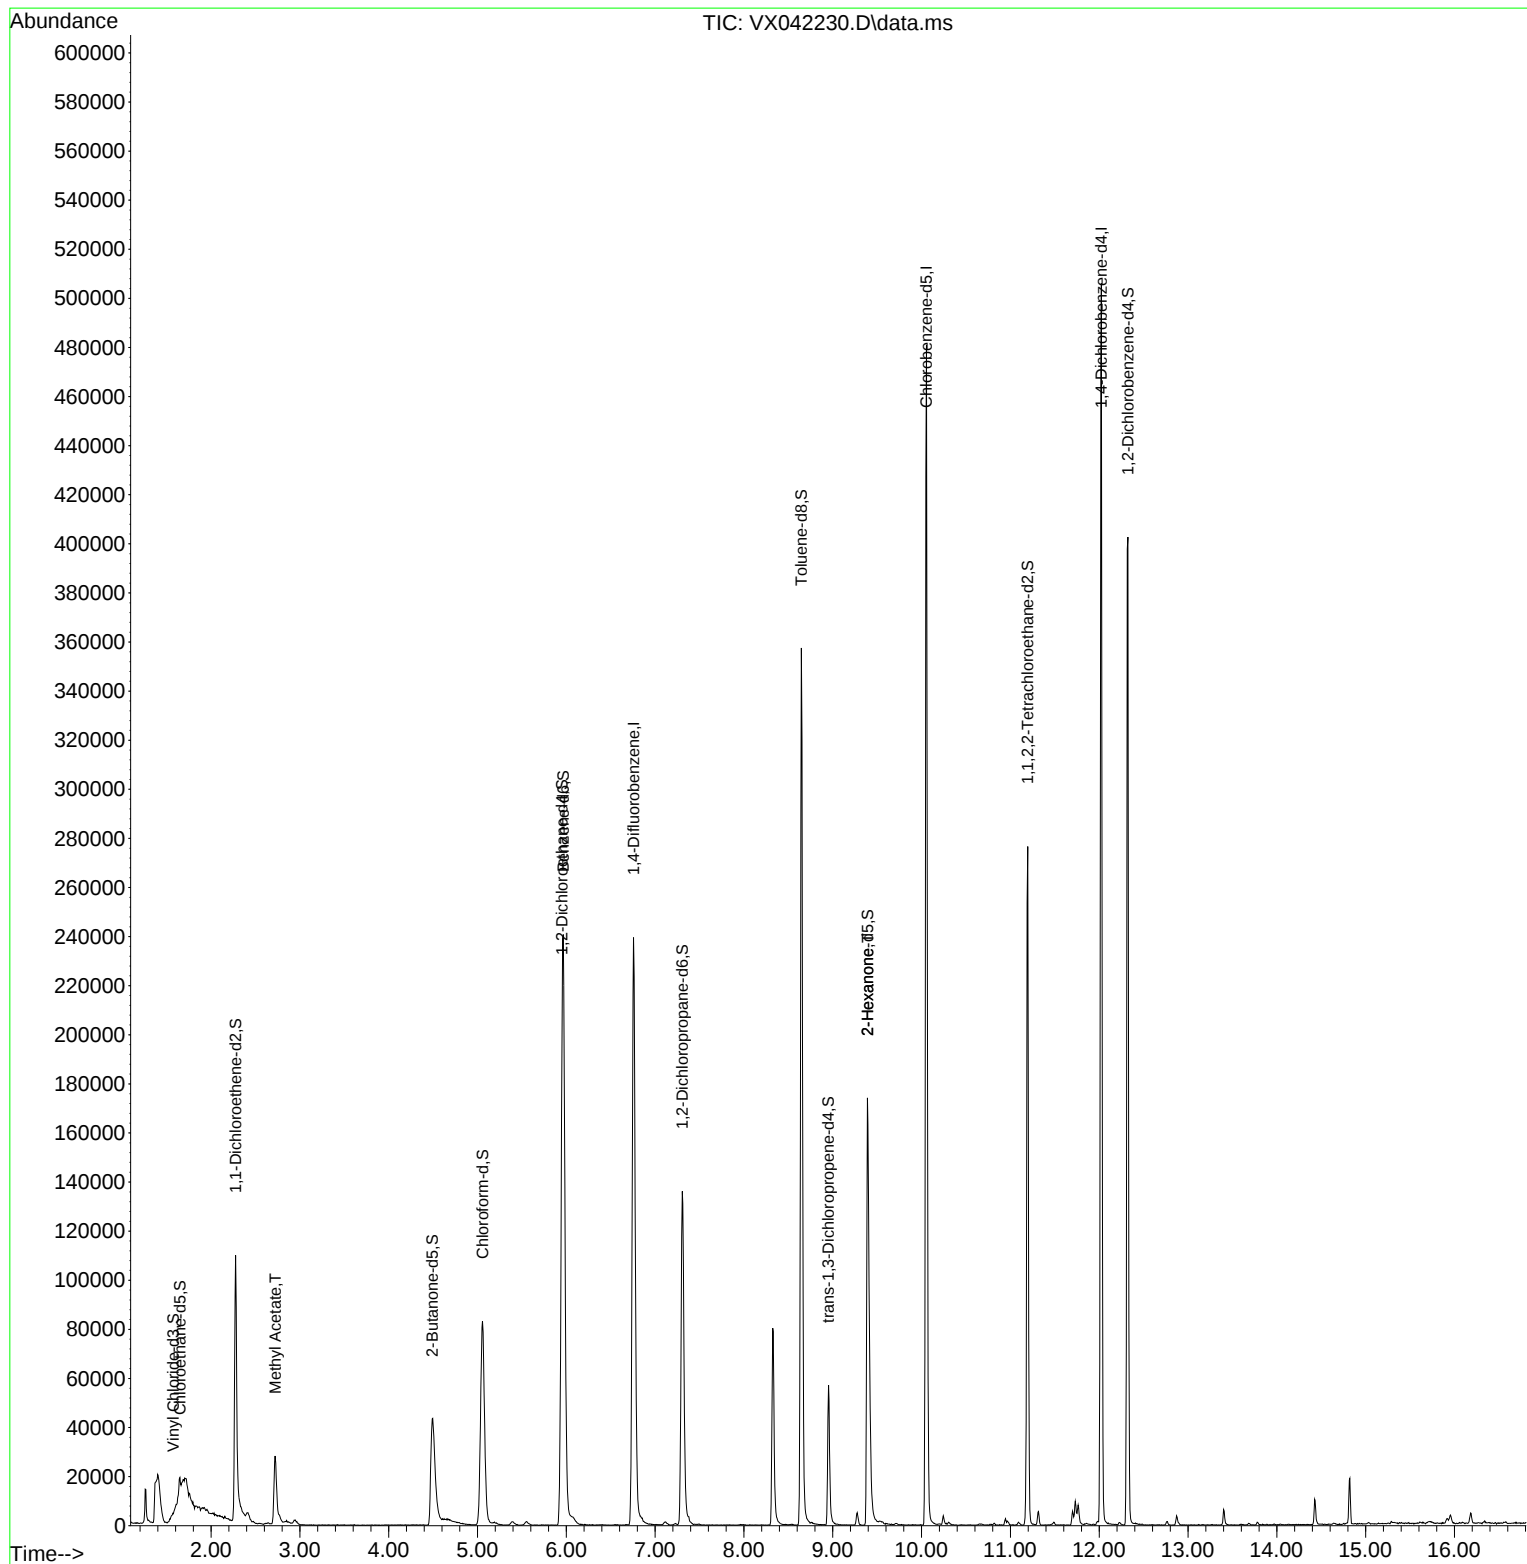

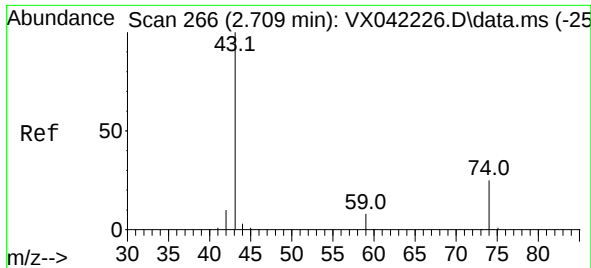

#15

Methyl Acetate

Concen: 21.148 ug/L

RT: 2.721 min Scan# 2

Delta R.T. 0.012 min

Lab File: VX042230.D

Acq: 08 Jul 2024 11:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 41022

Ion Ratio Lower Upper

43 100

74 25.1 20.1 30.1

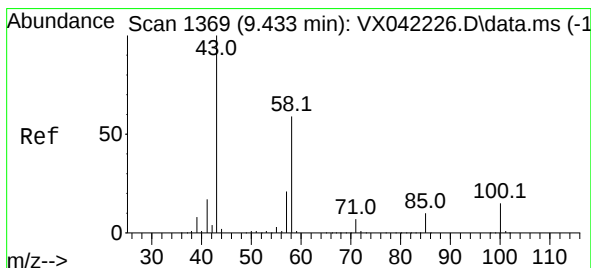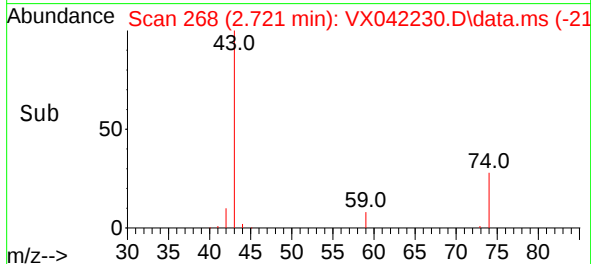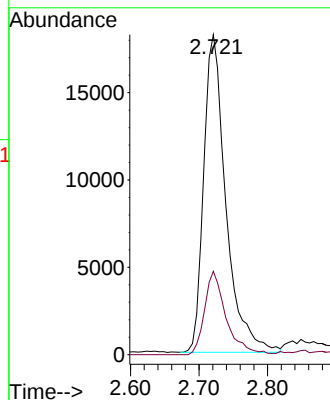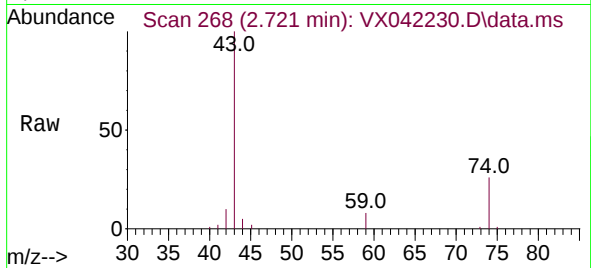

#48

2-Hexanone

Concen: 4.323 ug/L

RT: 9.390 min Scan# 1362

Delta R.T. -0.043 min

Lab File: VX042230.D

Acq: 08 Jul 2024 11:50

Tgt Ion: 43 Resp: 8467

Ion Ratio Lower Upper

43 100

58 28.9 46.4 69.6#

57 25.1 16.3 24.5#

100 0.0 12.1 18.1#

