




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
Data File : VX042229.D
Acq On : 08 Jul 2024 11:27
Operator : JC/MD
Sample : P3100-16ME
Misc : 4.48g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D07ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/09/2024
Supervised By :Mahesh Dadoda 07/09/2024

Quant Time: Jul 09 02:36:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 09 02:35:21 2024
Response via : Initial Calibration

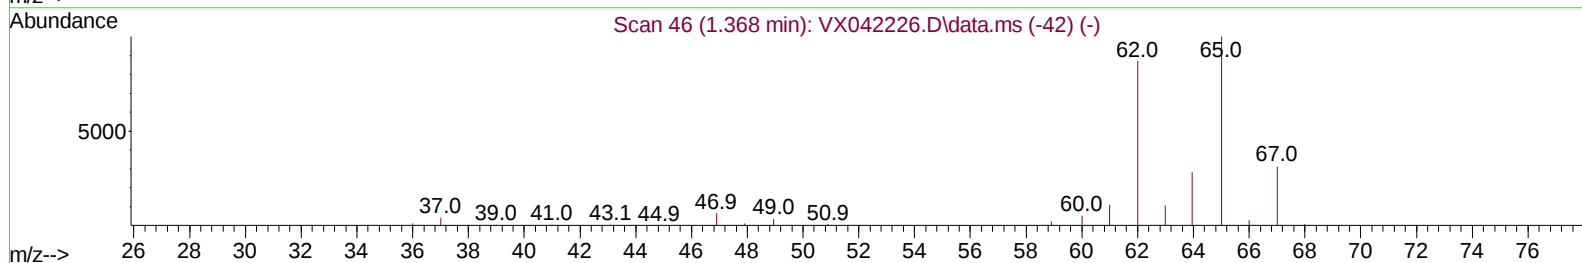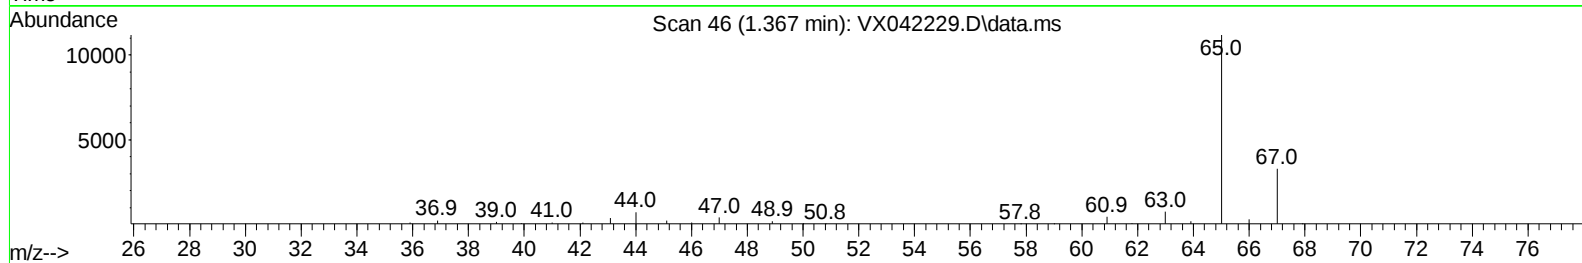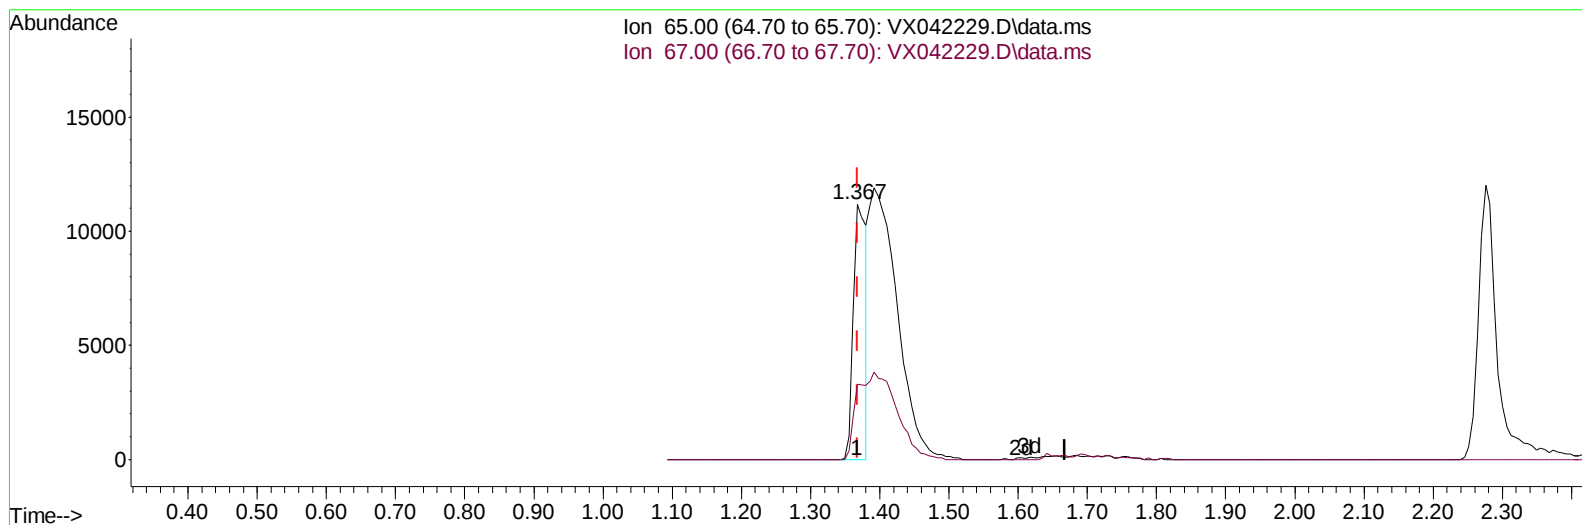

TIC: VX042229.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.367min (-0.000) 9.20 ug/L

response 14421

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.70	30.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
Data File : VX042229.D
Acq On : 08 Jul 2024 11:27
Operator : JC/MD
Sample : P3100-16ME
Misc : 4.48g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D07ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/09/2024
Supervised By :Mahesh Dadoda 07/09/2024

Quant Time: Jul 09 02:36:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 09 02:35:21 2024
Response via : Initial Calibration

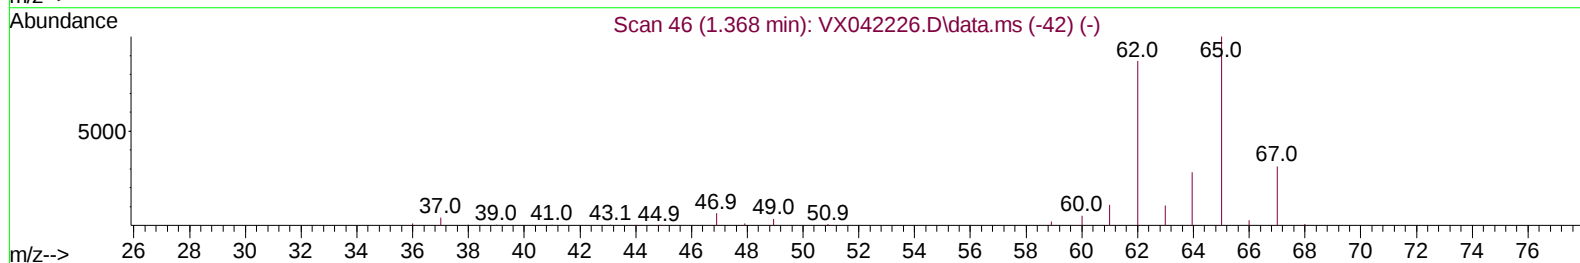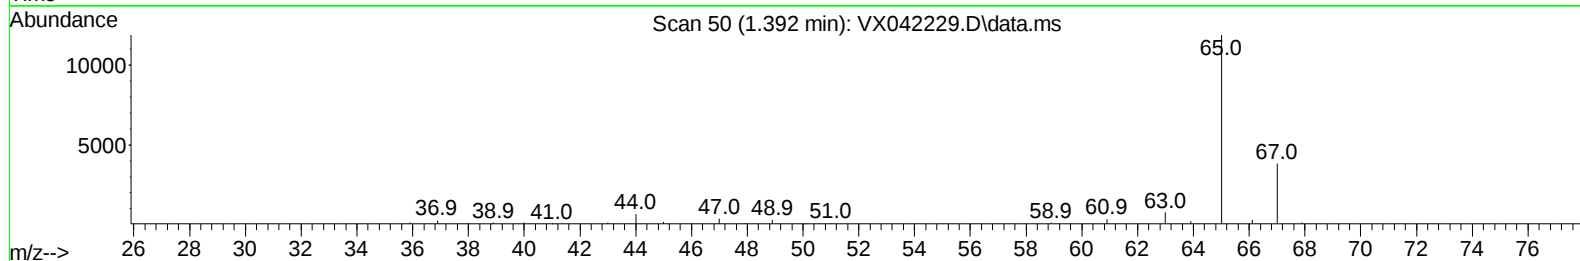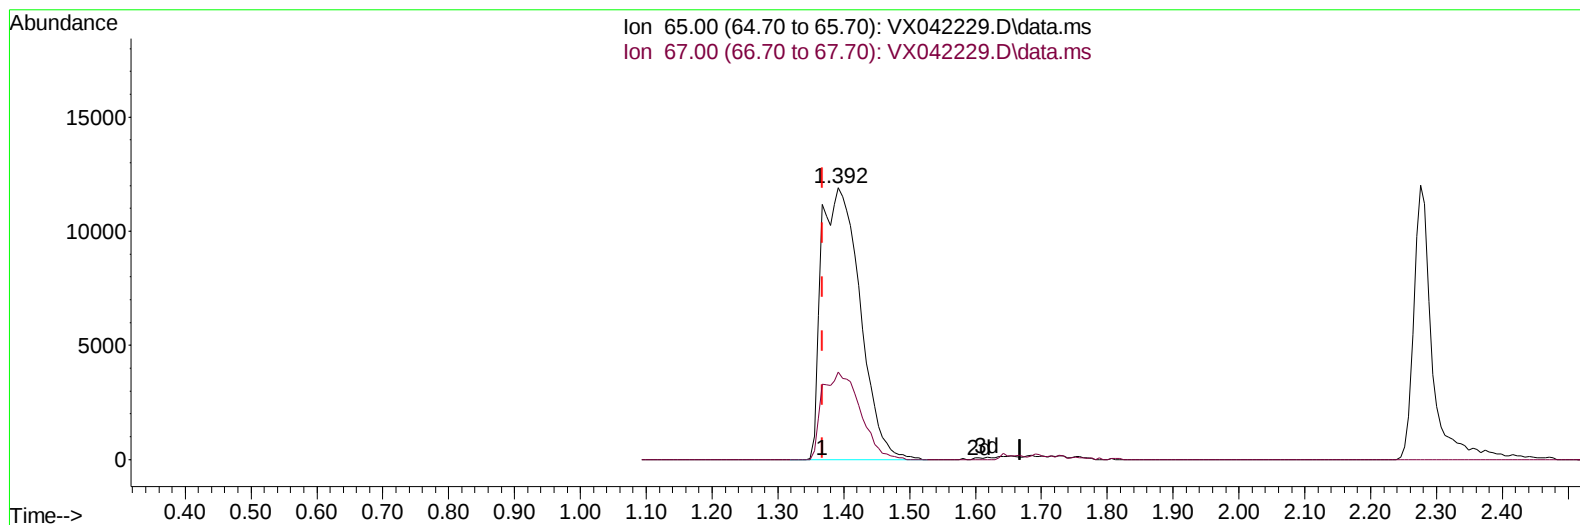

TIC: VX042229.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.392min (+ 0.024) 30.81 ug/L m

response 48275

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.70	9.10#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
Data File : VX042229.D
Acq On : 08 Jul 2024 11:27
Operator : JC/MD
Sample : P3100-16ME
Misc : 4.48g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D07ME

Manual IntegrationsAPPROVED

Quant Time: Jul 09 02:36:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 09 02:35:21 2024
Response via : Initial Calibration

Reviewed By :John Carlone 07/09/2024
Supervised By :Mahesh Dadoda 07/09/2024

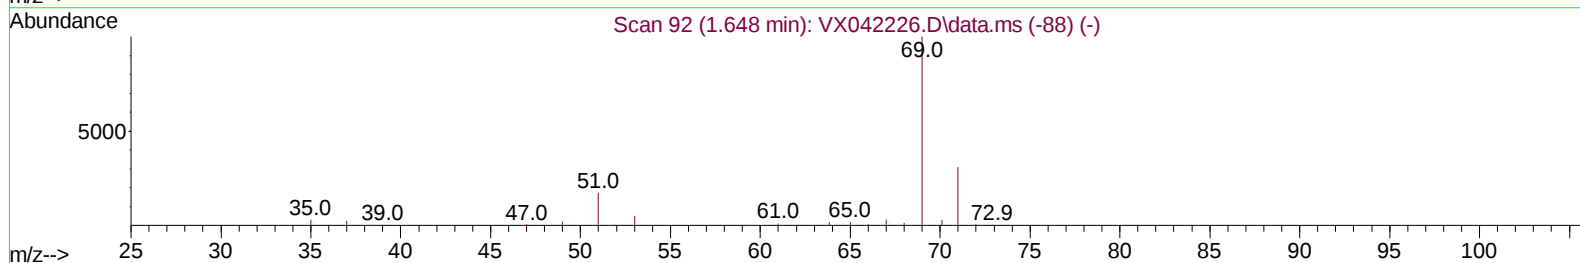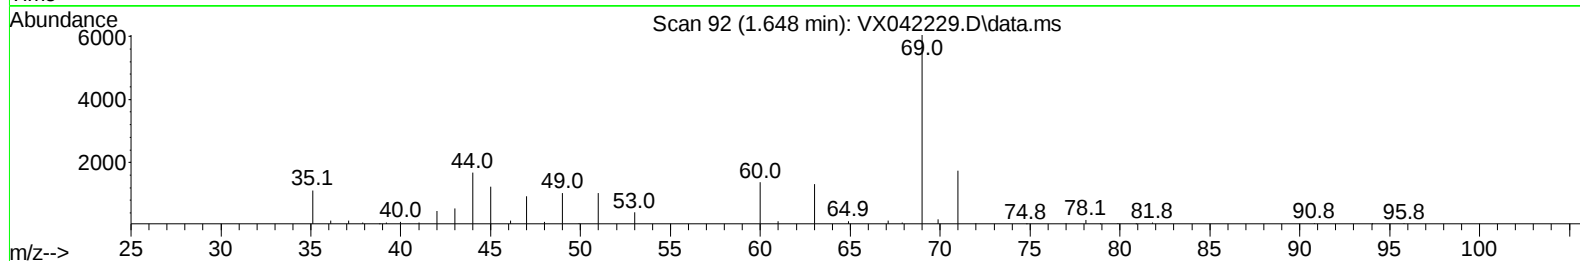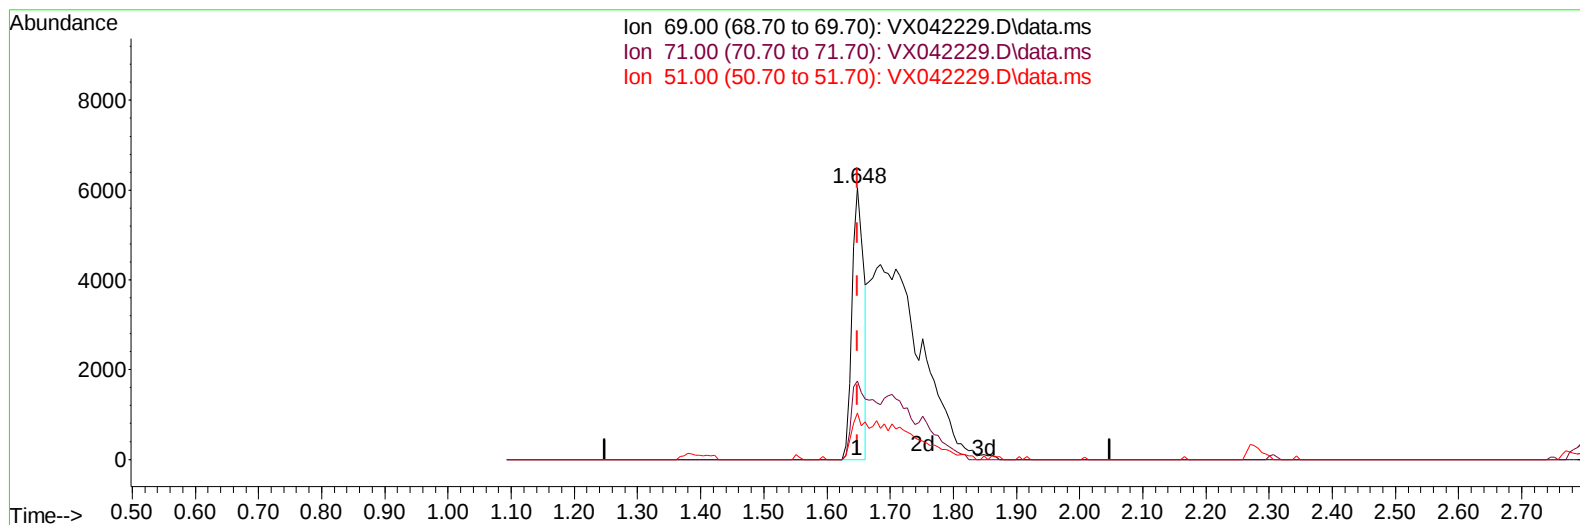

TIC: VX042229.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 8.02 ug/L

response 7908

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	38.11
51.00	12.70	21.38#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
Data File : VX042229.D
Acq On : 08 Jul 2024 11:27
Operator : JC/MD
Sample : P3100-16ME
Misc : 4.48g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D07ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/09/2024
Supervised By :Mahesh Dadoda 07/09/2024

Quant Time: Jul 09 02:36:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 09 02:35:21 2024
Response via : Initial Calibration

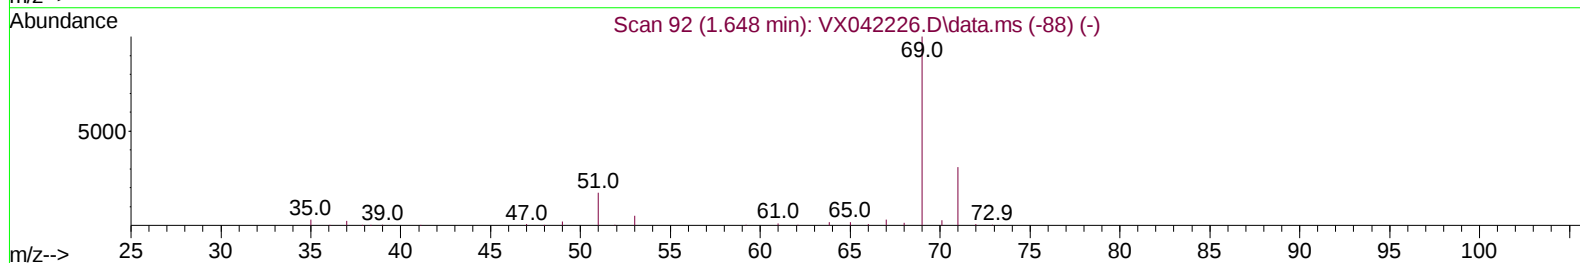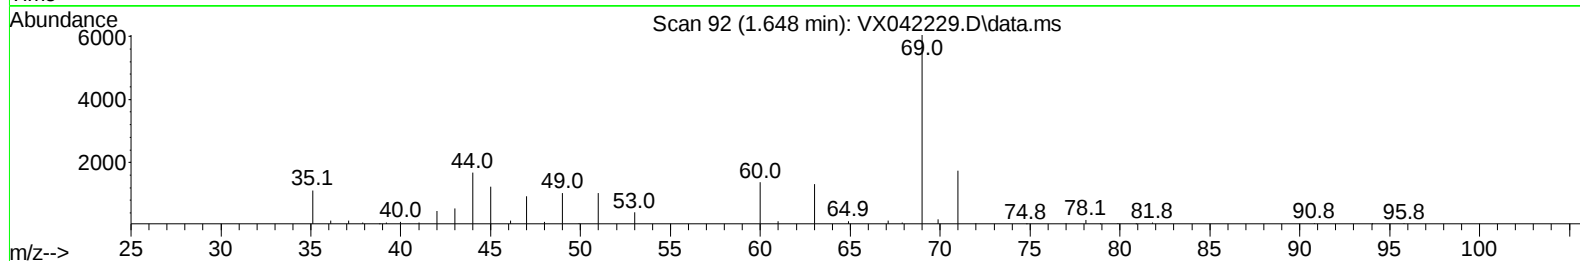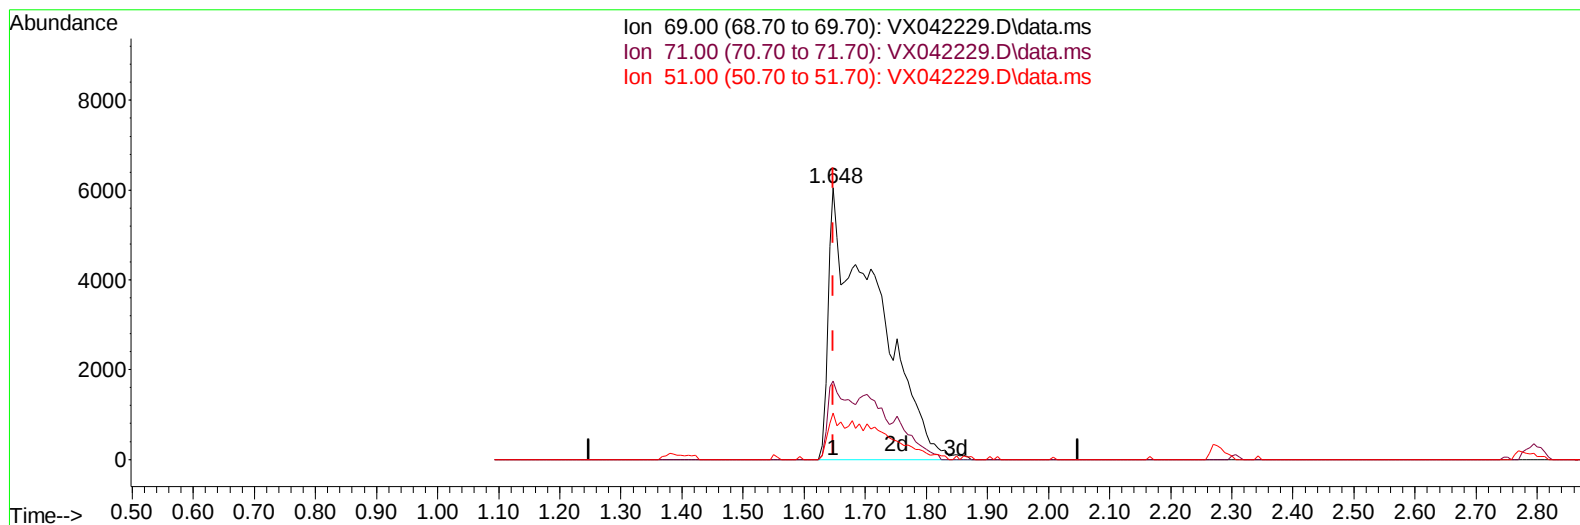

TIC: VX042229.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 33.24 ug/L m

response 32798

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	9.19#
51.00	12.70	5.16#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
 Data File : VX042229.D
 Acq On : 08 Jul 2024 11:27
 Operator : JC/MD
 Sample : P3100-16ME
 Misc : 4.48g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4D07ME

Manual IntegrationsAPPROVED

Quant Time: Jul 09 02:36:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 09 02:35:21 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 07/09/2024
 Supervised By :Mahesh Dadoda 07/09/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	269204	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	245571	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	124814	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.392	65	48275m	30.809	ug/L	0.02
Spiked Amount 50.000	Range 60	- 135	Recovery	=	61.620%	
7) Chloroethane-d5	1.648	69	32798m	33.244	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	66.480%#	
11) 1,1-Dichloroethene-d2	2.276	65	22189	32.356	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	64.720%	
21) 2-Butanone-d5	4.489	46	86513	76.615	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	76.610%	
24) Chloroform-d	5.056	84	112793	35.801	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	71.600%	
26) 1,2-Dichloroethane-d4	5.952	65	73984	39.785	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	79.560%	
32) Benzene-d6	5.964	84	241160	37.993	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	75.980%	
36) 1,2-Dichloropropane-d6	7.305	67	75081	39.305	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	78.620%	
41) Toluene-d8	8.647	98	225911	38.192	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	76.380%#	
43) trans-1,3-Dichloroprop...	8.951	79	30215	36.599	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	73.200%	
47) 2-Hexanone-d5	9.390	63	69998	80.729	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	80.730%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	110043	38.966	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	77.940%	
66) 1,2-Dichlorobenzene-d4	12.323	152	97777	40.332	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	80.660%	
Target Compounds						
					Qvalue	
29) Cyclohexane	5.452	56	3453	1.301	ug/L	98
35) Methylcyclohexane	7.372	83	10510	3.853	ug/L	97
46) Tetrachloroethene	9.275	164	10796	6.412	ug/L	96
53) m,p-Xylene	10.305	106	3975	1.240	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
Data File : VX042229.D
Acq On : 08 Jul 2024 11:27
Operator : JC/MD
Sample : P3100-16ME
Misc : 4.48g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4D07ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/09/2024
Supervised By :Mahesh Dadoda 07/09/2024

Quant Time: Jul 09 02:36:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 09 02:35:21 2024
Response via : Initial Calibration

