
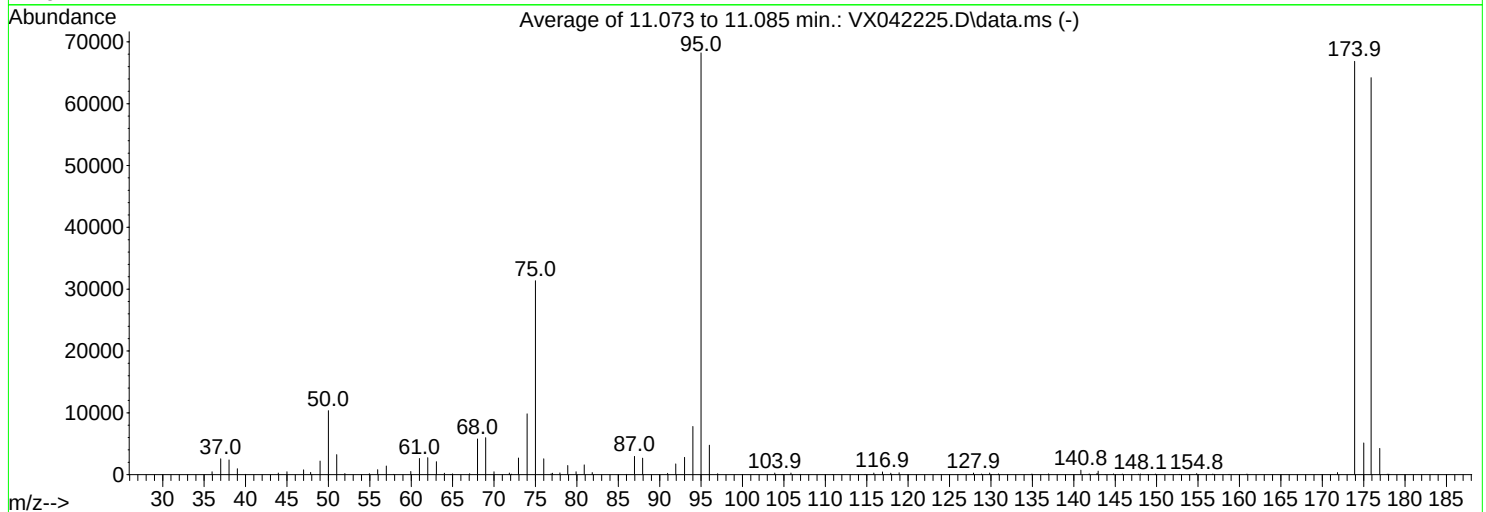


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070824\
Data File : VX042225.D
Acq On : 08 Jul 2024 07:40
Operator : JC/MD
Sample : BFB679
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB679

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM070324WMA.M
Title : VOC Analysis
Last Update : Tue Jul 09 02:35:21 2024

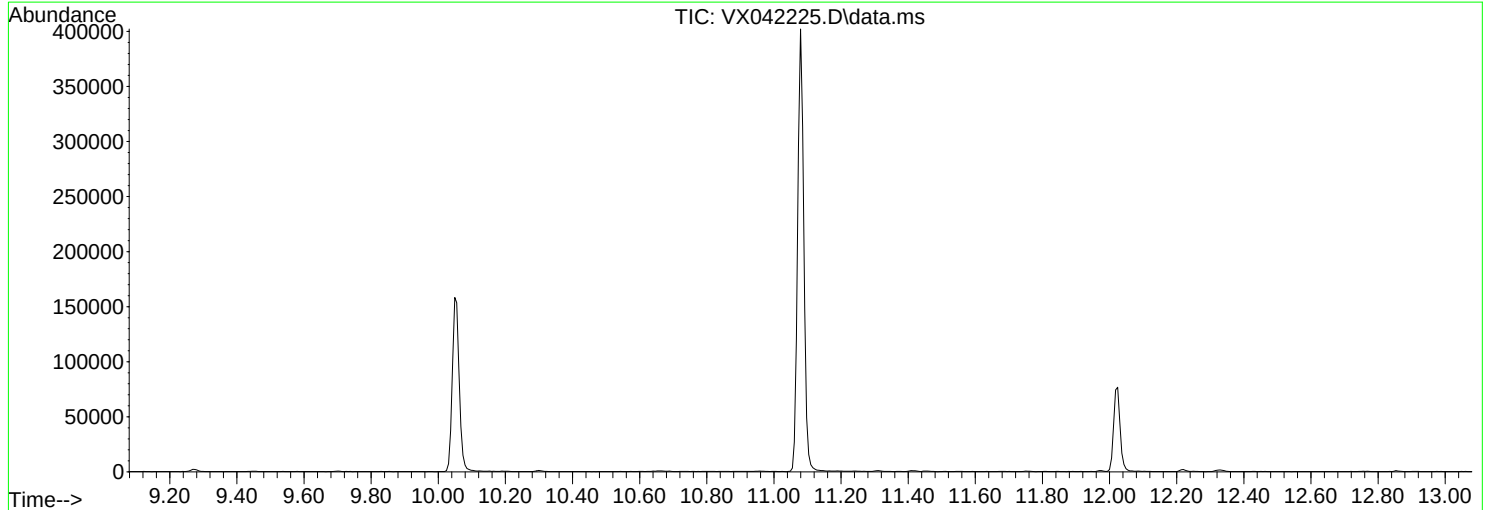

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.2	10341	PASS
75	95	30	80	46.0	31376	PASS
95	95	100	100	100.0	68221	PASS
96	95	5	9	7.0	4760	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.0	66848	PASS
175	174	5	9	7.7	5132	PASS
176	174	95	101	96.0	64200	PASS
177	176	5	9	6.6	4246	PASS

m/z	Abundance
35.90	79.0
40.10	132.0
44.00	197.0

Instrument :
MSVOA_X
ClientSampleId :
BFB679

m/z	Abundance
36.00	624.0
37.00	2697.0
38.00	2640.0
39.00	1039.0
40.10	213.0
43.90	506.0
45.00	458.0
47.00	714.0
47.90	413.0
49.00	2274.0
50.00	10159.0
51.00	3173.0
52.00	182.0
55.00	172.0
56.00	769.0
57.00	1492.0
57.90	76.0
60.00	513.0
61.00	2507.0
62.00	2636.0
63.10	2033.0
64.00	253.0
64.80	195.0
67.10	170.0
68.00	5510.0
69.00	5919.0
70.00	396.0
71.80	320.0
72.90	2596.0
74.00	9504.0
75.00	29712.0
76.00	2493.0
76.90	395.0
78.00	242.0
78.90	1287.0
79.90	382.0
80.90	1447.0
81.90	310.0
86.00	54.0
87.00	2753.0
88.00	2342.0
91.10	194.0
92.00	1652.0
93.00	2723.0
94.00	7284.0
95.00	63440.0
96.00	4597.0
97.00	177.0
104.00	251.0
105.80	207.0
110.90	62.0
114.80	68.0
115.80	243.0
117.00	340.0
118.00	193.0
118.90	286.0
127.90	242.0
128.90	91.0
129.80	204.0
130.90	147.0
135.00	65.0
136.90	115.0
140.90	577.0
141.90	84.0
142.80	597.0
144.70	84.0
145.90	56.0
148.10	114.0
149.90	74.0
152.80	55.0
154.80	120.0
156.80	104.0
160.80	70.0
171.90	277.0
173.90	52520.0
175.00	4366.0
175.90	49512.0
176.90	3364.0
177.90	82.0

Instrument :
MSVOA_X
ClientSampleId :
BFB679

m/z	Abundance
36.00	688.0
37.00	2882.0
38.00	2621.0
39.00	1098.0
40.00	230.0
44.00	423.0
45.00	599.0
47.00	994.0
47.80	447.0
49.00	2723.0
50.00	12398.0
51.00	3962.0
52.00	215.0
55.00	198.0
55.90	900.0
57.00	1570.0
57.90	76.0
59.90	679.0
61.00	3286.0
62.00	3230.0
63.00	2500.0
64.00	218.0
65.00	195.0
67.00	171.0
68.00	6920.0
69.00	6975.0
70.00	616.0
71.90	443.0
73.00	3259.0
74.00	11993.0
75.00	38208.0
76.00	3032.0
77.10	360.0
77.90	405.0
78.90	1923.0
79.90	652.0
80.90	1866.0
81.90	460.0
87.00	3492.0
88.00	3185.0
90.90	248.0
92.00	2055.0
93.00	3332.0
94.00	9349.0
95.00	80168.0
96.00	5703.0
97.00	218.0
103.80	312.0
104.80	75.0
105.90	339.0
107.00	74.0
114.80	89.0
115.90	314.0
116.90	485.0
117.80	273.0
118.90	338.0
127.90	275.0
128.80	116.0
129.90	273.0
130.90	145.0
134.90	100.0
137.00	112.0
140.80	836.0
141.90	183.0
143.00	1019.0
143.80	61.0
144.80	190.0
145.90	142.0
148.00	211.0
149.80	103.0
152.80	70.0
154.90	265.0
156.80	99.0
158.80	89.0
160.90	146.0
171.90	424.0
173.90	80152.0
175.00	5757.0
175.90	76440.0
177.00	5252.0
177.80	134.0
178.10	123.0

Instrument :
MSVOA_X
ClientSampleId :
BFB679

m/z	Abundance
36.00	317.0
37.00	2137.0
38.00	1859.0
39.00	746.0
39.90	136.0
44.00	426.0
45.10	330.0
47.00	643.0
47.90	272.0
49.00	1643.0
50.00	8465.0
51.00	2590.0
52.00	133.0
54.90	142.0
56.00	731.0
57.00	1158.0
60.00	367.0
61.00	2084.0
62.00	2412.0
63.00	1768.0
64.00	230.0
65.00	202.0
67.00	111.0
68.00	4909.0
69.00	5080.0
70.00	413.0
72.10	217.0
73.00	2211.0
74.00	8005.0
75.00	26208.0
76.00	2148.0
77.00	375.0
77.90	212.0
78.90	1191.0
79.90	397.0
80.90	1413.0
81.80	283.0
86.00	101.0
86.90	2626.0
87.90	2464.0
90.90	178.0
91.90	1513.0
93.00	2359.0
94.00	6738.0
95.00	61056.0
96.00	3981.0
97.00	91.0
103.90	244.0
104.80	97.0
105.90	260.0
106.90	53.0
115.90	215.0
116.80	476.0
117.90	260.0
118.90	323.0
127.90	281.0
128.90	107.0
129.90	288.0
130.80	80.0
134.90	135.0
136.90	134.0
140.90	784.0
141.80	98.0
142.90	713.0
144.90	85.0
145.80	142.0
147.80	231.0
148.90	52.0
149.80	99.0
153.90	53.0
154.90	200.0
156.80	123.0
157.00	122.0
158.70	66.0
161.00	80.0
171.80	327.0
173.90	67872.0
175.00	5273.0
175.90	66648.0
177.00	4121.0
178.00	139.0

Instrument :
MSVOA_X
ClientSampleId :
BFB679