

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070825\
 Data File : VX046912.D
 Acq On : 08 Jul 2025 11:11
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Jul 09 05:10:43 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 09 05:05:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	357622	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	624792	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	577142	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	283637	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	242709	51.372	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	102.740%
35) Dibromofluoromethane	5.397	113	200504	47.276	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.560%
50) Toluene-d8	8.652	98	753404	50.349	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.700%
62) 4-Bromofluorobenzene	11.079	95	285439	50.192	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.380%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070825\
Data File : VX046912.D
Acq On : 08 Jul 2025 11:11
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Jul 09 05:10:43 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 09 05:05:09 2025
Response via : Initial Calibration




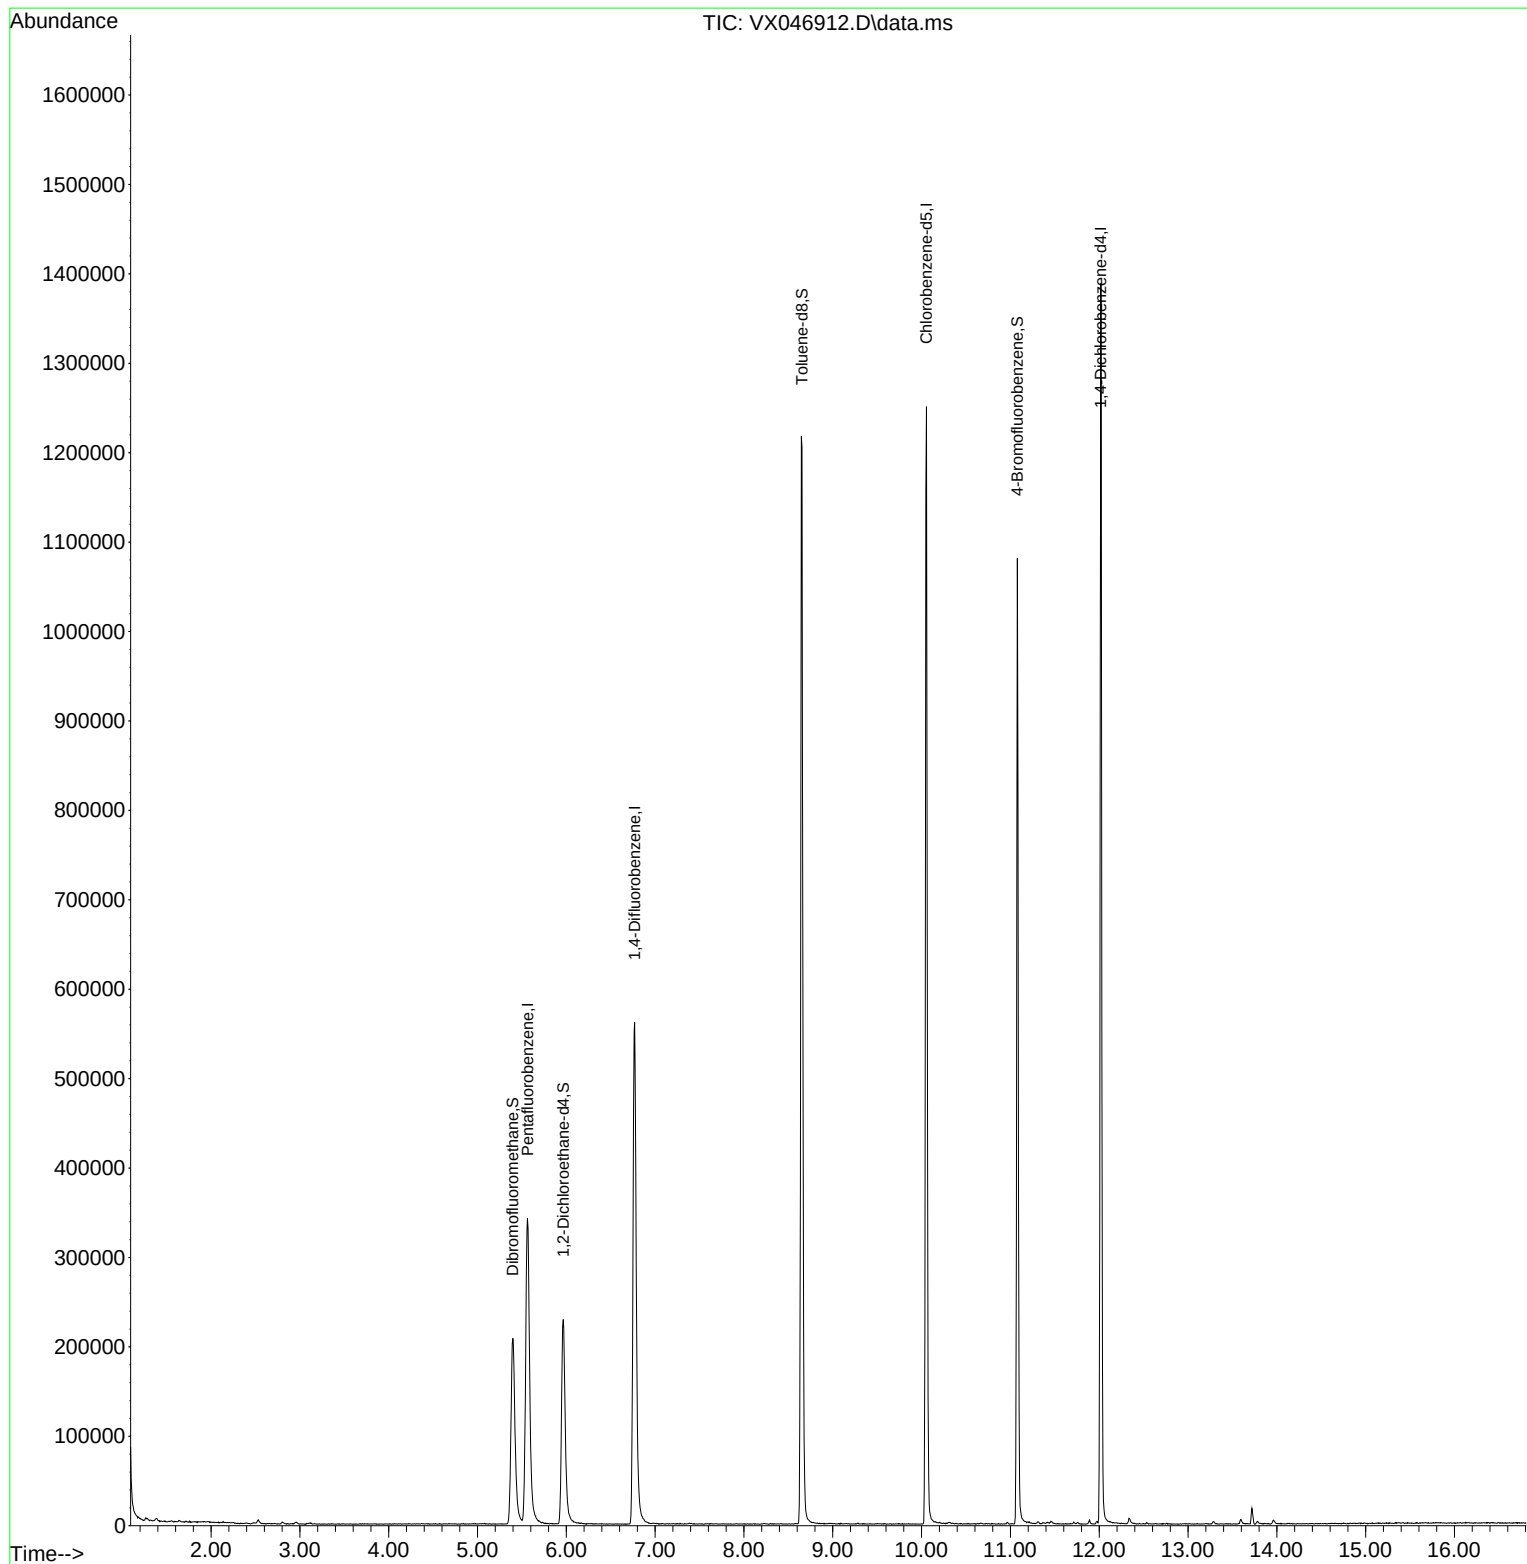


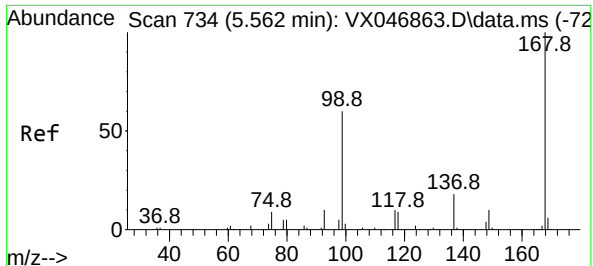

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX046912.D
Acq: 08 Jul 2025 11:11




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 357622
Ion Ratio Lower Upper
168 100
99 59.5 48.8 73.2

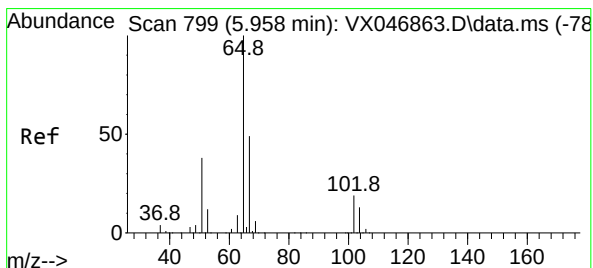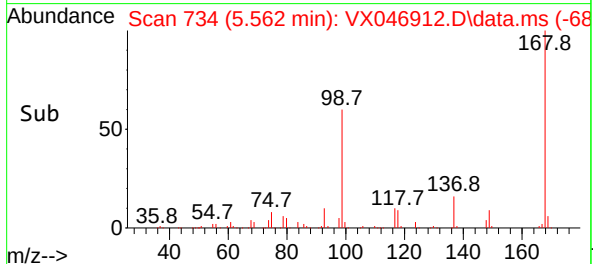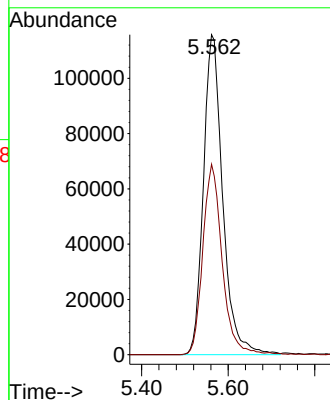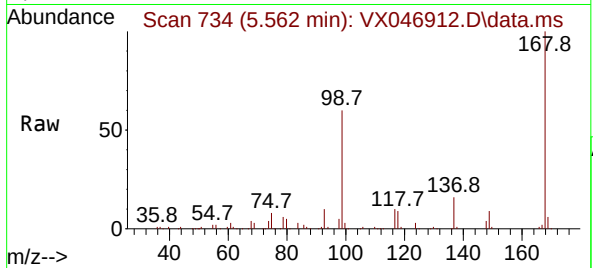

#33
1,2-Dichloroethane-d4
Concen: 51.372 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.006 min
Lab File: VX046912.D
Acq: 08 Jul 2025 11:11

Tgt Ion: 65 Resp: 242709
Ion Ratio Lower Upper
65 100
67 52.2 0.0 105.2


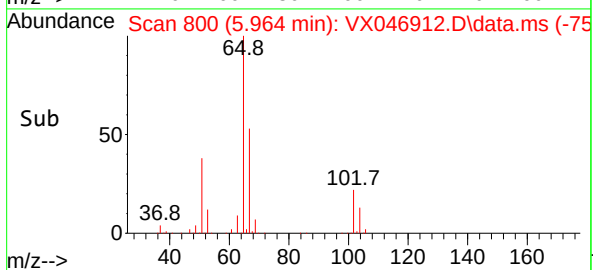
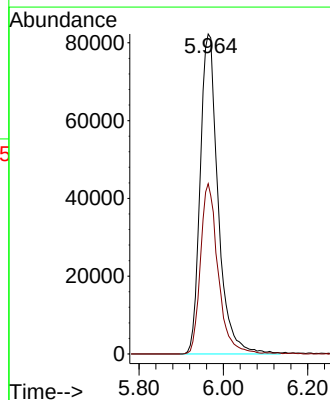
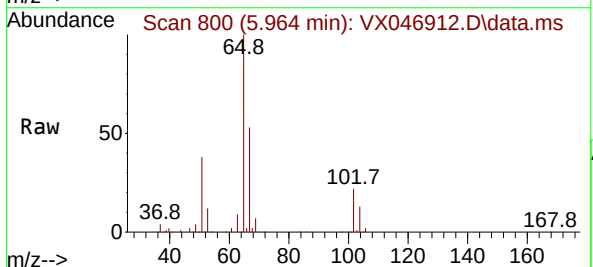


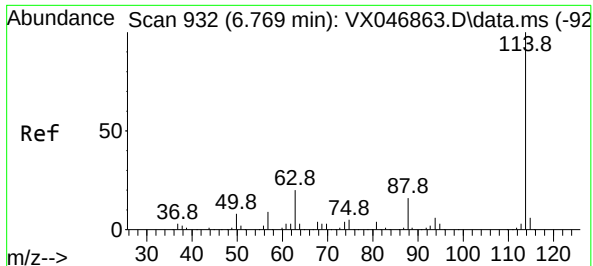

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 912
Delta R.T. -0.000 min
Lab File: VX046912.D
Acq: 08 Jul 2025 11:11




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 624792
Ion Ratio Lower Upper
114 100
63 21.3 0.0 40.4
88 16.1 0.0 31.0

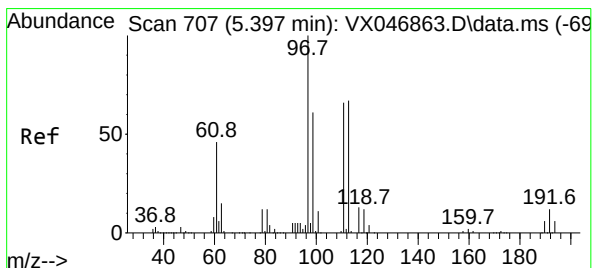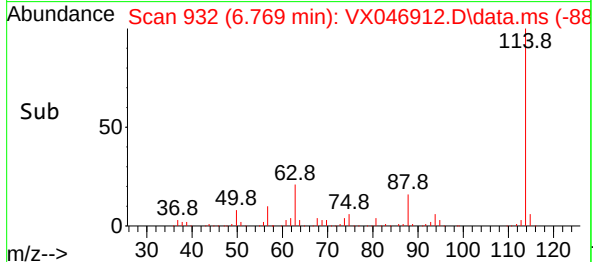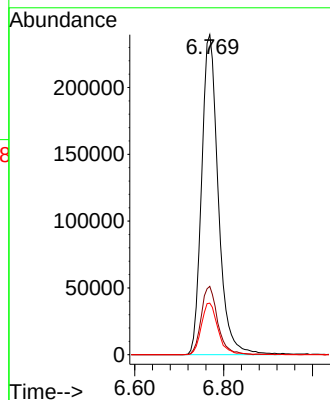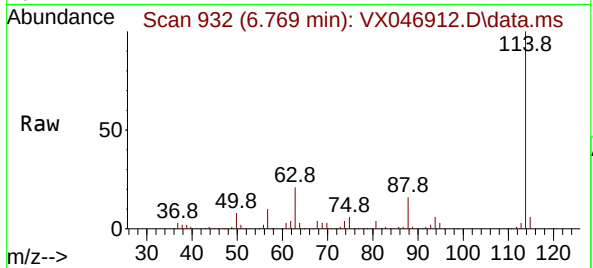

#35
Dibromofluoromethane
Concen: 47.276 ug/l
RT: 5.397 min Scan# 707
Delta R.T. -0.000 min
Lab File: VX046912.D
Acq: 08 Jul 2025 11:11

Tgt Ion:113 Resp: 200504
Ion Ratio Lower Upper
113 100
111 105.9 81.2 121.8
192 19.0 15.3 22.9


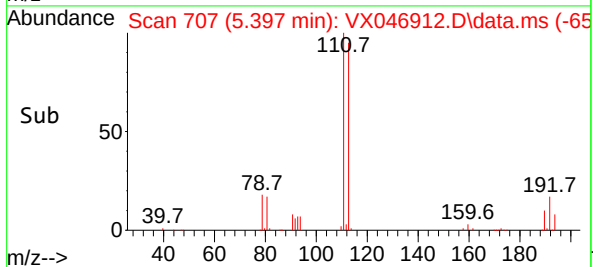
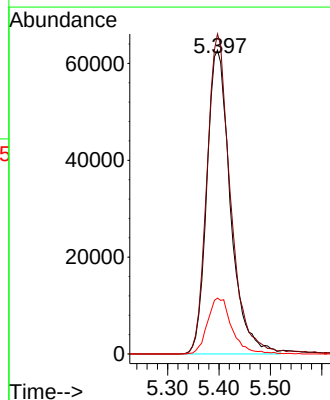
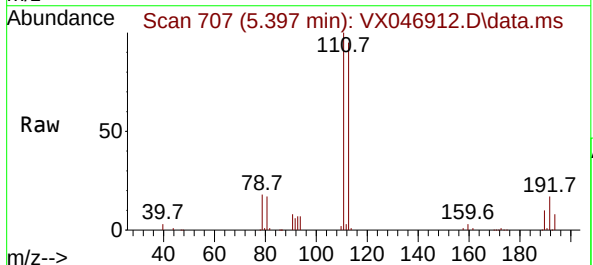


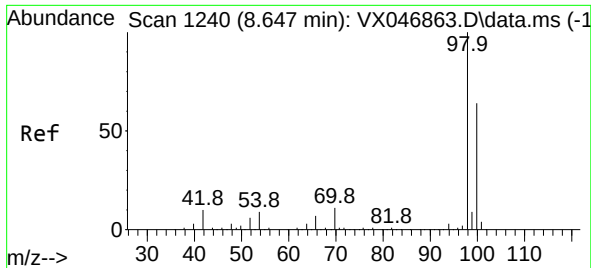

#50
Toluene-d8
Concen: 50.349 ug/l
RT: 8.652 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046912.D
Acq: 08 Jul 2025 11:11




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 753404
Ion Ratio Lower Upper
98 100
100 66.7 53.0 79.6

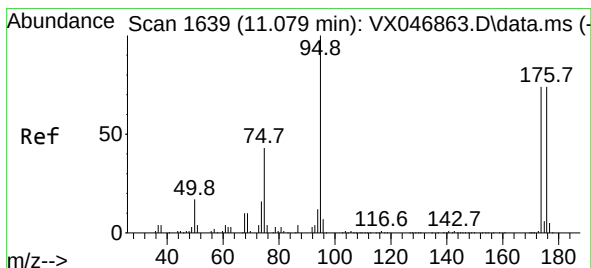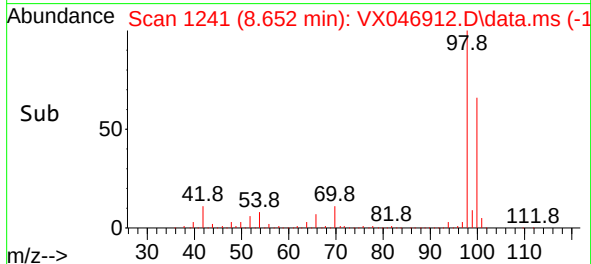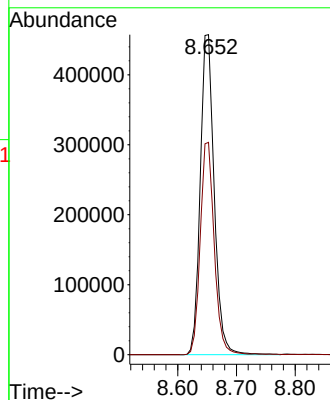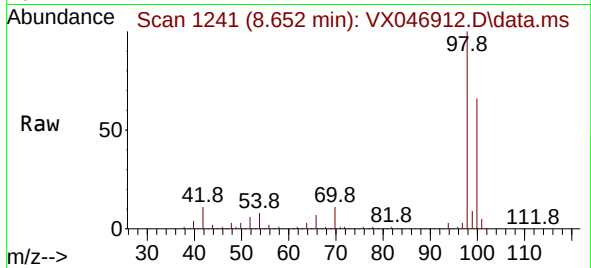

#62
4-Bromofluorobenzene
Concen: 50.192 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX046912.D
Acq: 08 Jul 2025 11:11

Tgt Ion: 95 Resp: 285439
Ion Ratio Lower Upper
95 100
174 75.5 0.0 152.0
176 72.6 0.0 145.2


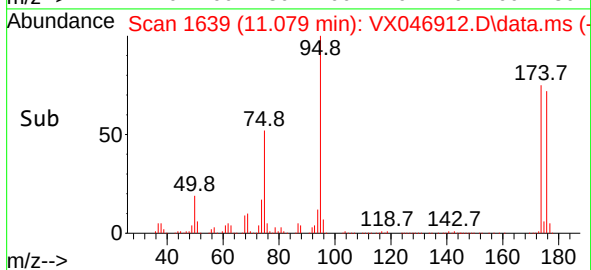
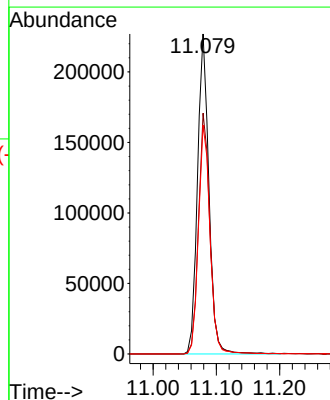
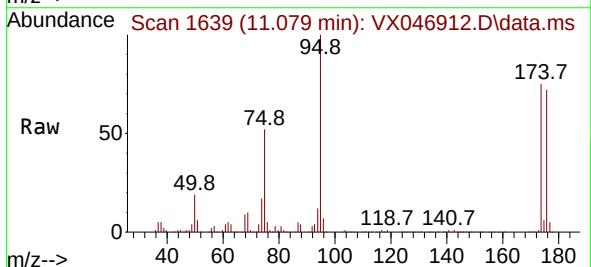


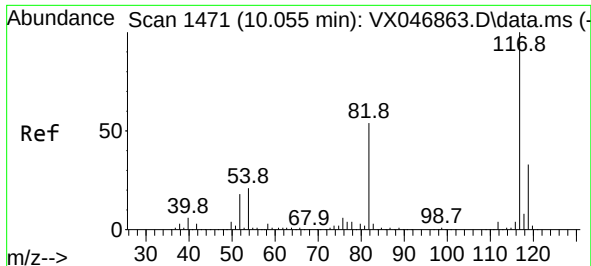

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX046912.D
Acq: 08 Jul 2025 11:11

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 577142
Ion Ratio Lower Upper
117 100
82 54.8 43.3 64.9
119 32.1 26.4 39.6

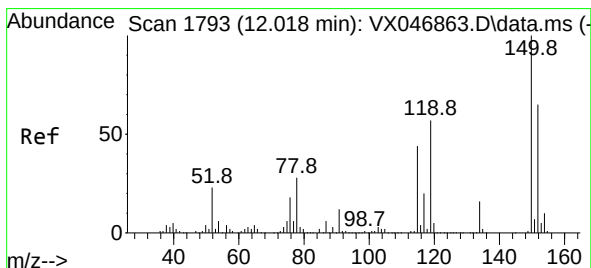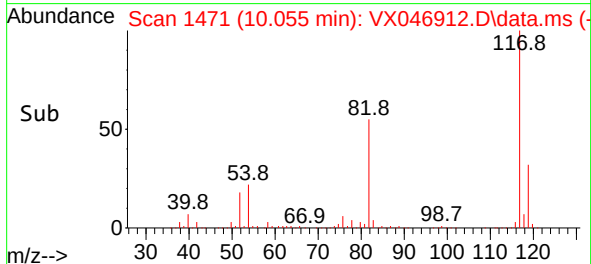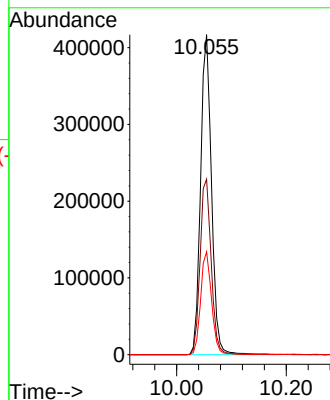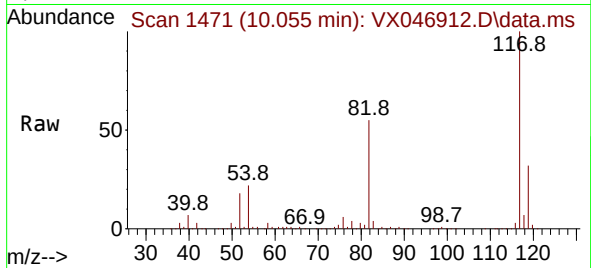

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX046912.D
Acq: 08 Jul 2025 11:11

Tgt Ion:152 Resp: 283637
Ion Ratio Lower Upper
152 100
115 60.6 42.4 127.1
150 157.7 0.0 349.2

