

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070825\
 Data File : VX046913.D
 Acq On : 08 Jul 2025 11:32
 Operator : JC/MD
 Sample : Q2126-09 0.2PPB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Quant Time: Jul 09 05:11:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 09 05:05:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	374336	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	638116	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	589137	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	304916	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	258374	52.246	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 104.500%			
35) Dibromofluoromethane	5.397	113	214838	49.598	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.200%			
50) Toluene-d8	8.647	98	746478	48.845	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 97.680%			
62) 4-Bromofluorobenzene	11.079	95	300130	51.673	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 103.340%			
Target Compounds						Qvalue
3) Chloromethane	1.307	50	989	0.253	ug/l #	85
5) Bromomethane	1.630	94	1397	0.510	ug/l #	55
6) Chloroethane	1.703	64	1205	0.428	ug/l #	70
10) Methyl Iodide	2.483	142	1466	0.321	ug/l #	63
12) 1,1-Dichloroethene	2.337	96	899	0.221	ug/l #	89
13) Acrolein	2.252	56	401	1.035	ug/l #	40
15) Acrylonitrile	3.099	53	1285	0.685	ug/l #	76
16) Acetone	2.392	43	2085	1.357	ug/l	89
17) Carbon Disulfide	2.532	76	2978	0.280	ug/l #	93
20) Methylene Chloride	2.806	84	1827	0.402	ug/l #	92
23) Vinyl Acetate	3.770	43	8420m	0.805	ug/l	
29) Tetrahydrofuran	5.056	42	1380m	1.056	ug/l	
36) 1,1-Dichloropropene	5.733	75	1574m	0.269	ug/l	
38) Carbon Tetrachloride	5.690	117	1410m	0.228	ug/l	
39) Methylcyclohexane	7.385	83	1474	0.202	ug/l	91
42) 1,2-Dichloroethane	6.105	62	1642m	0.274	ug/l	
51) 4-Methyl-2-Pentanone	8.580	43	3178	0.706	ug/l	97
58) 2-Chloroethyl Vinyl ether	8.281	63	2082m	0.654	ug/l	
59) 2-Hexanone	9.476	43	1827m	0.612	ug/l	
64) Tetrachloroethene	9.281	164	824	0.210	ug/l #	82
65) Chlorobenzene	10.079	112	2736	0.215	ug/l	90
68) m/p-Xylenes	10.305	106	2615	0.318	ug/l	98
71) Bromoform	10.799	173	707	0.222	ug/l #	75
74) N-amyl acetate	10.860	43	1972m	0.271	ug/l	
87) 1,3-Dichlorobenzene	11.975	146	2122	0.213	ug/l	94
88) 1,4-Dichlorobenzene	12.043	146	2508m	0.241	ug/l	
93) 1,2,4-Trichlorobenzene	13.597	180	1583	0.241	ug/l	87
94) Hexachlorobutadiene	13.719	225	1369	0.552	ug/l	95
96) 1,2,3-Trichlorobenzene	13.963	180	1504	0.242	ug/l	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070825\
Data File : VX046913.D
Acq On : 08 Jul 2025 11:32
Operator : JC/MD
Sample : Q2126-09 0.2PPB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025

Quant Time: Jul 09 05:11:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 09 05:05:09 2025
Response via : Initial Calibration




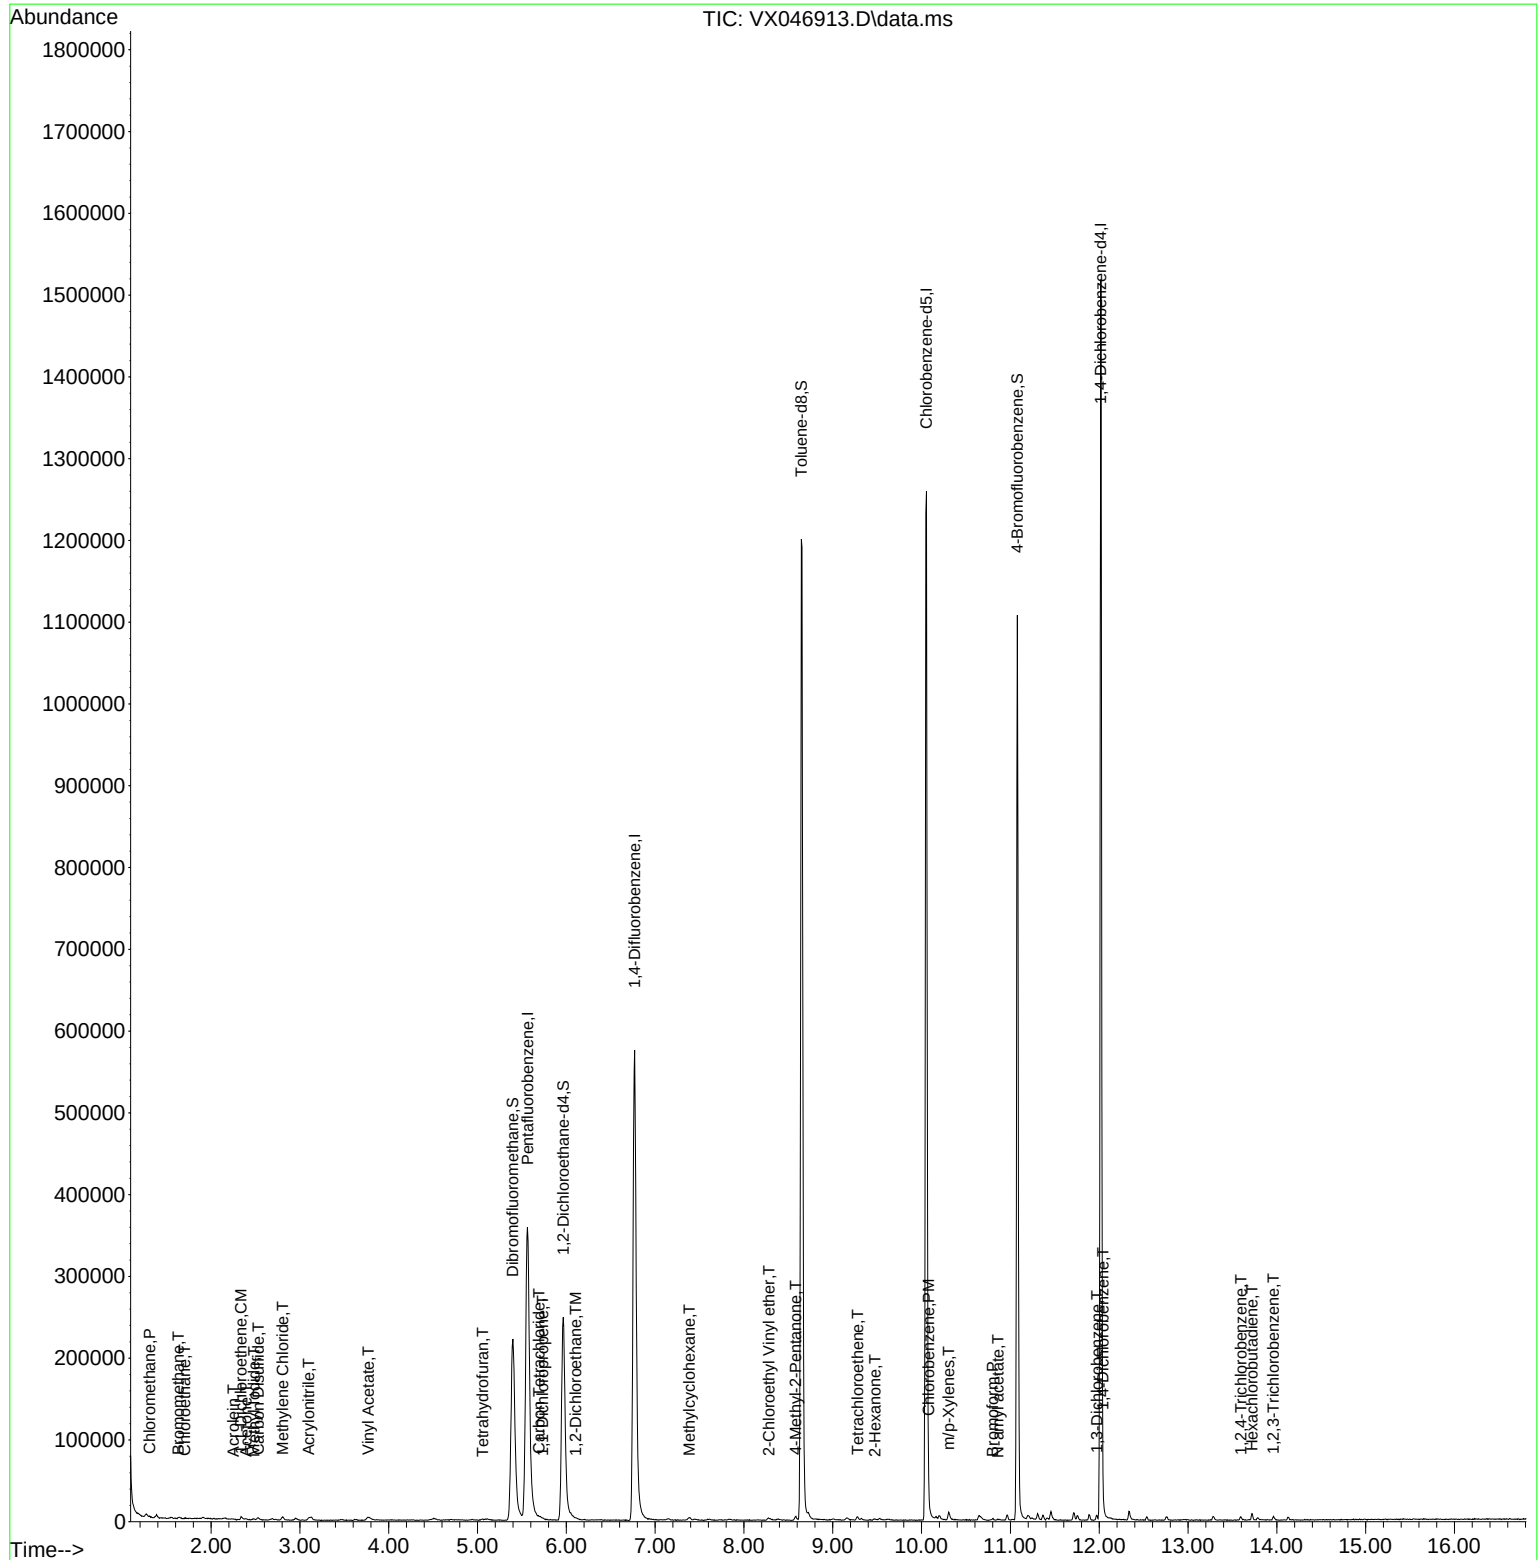




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion:168 Resp: 374336
Ion Ratio Lower Upper
168 100
99 58.8 48.8 73.2

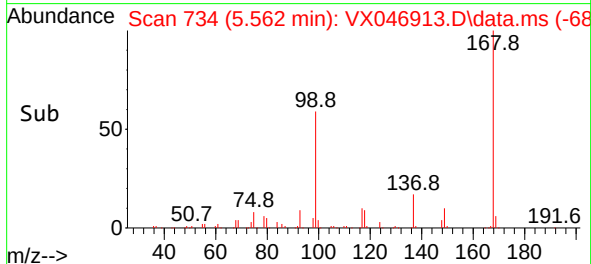

#3
Chloromethane
Concen: 0.253 ug/l
RT: 1.307 min Scan# 36
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32


Tgt Ion: 50 Resp: 989
Ion Ratio Lower Upper
50 100
52 23.0 25.0 37.4#

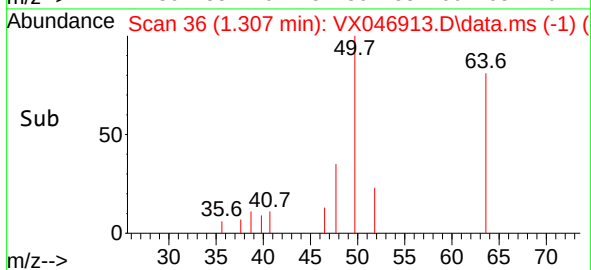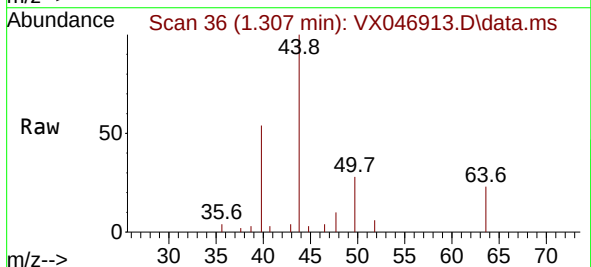



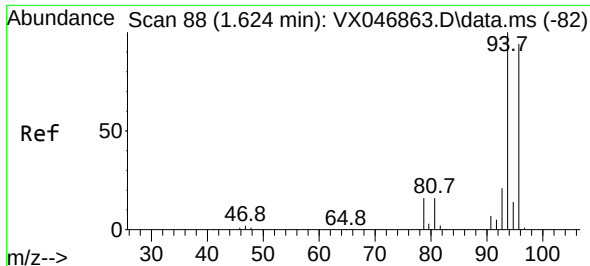


#5
Bromomethane
Concen: 0.510 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.006 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025



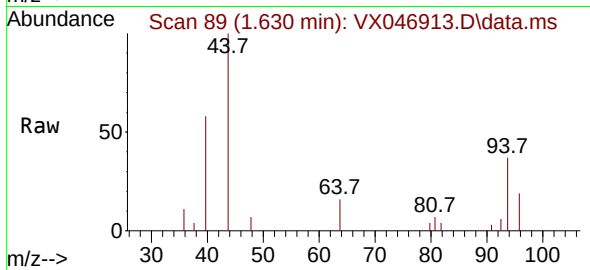



Tgt Ion: 94 Resp: 1397
Ion Ratio Lower Upper
94 100
96 51.1 75.5 113.3#

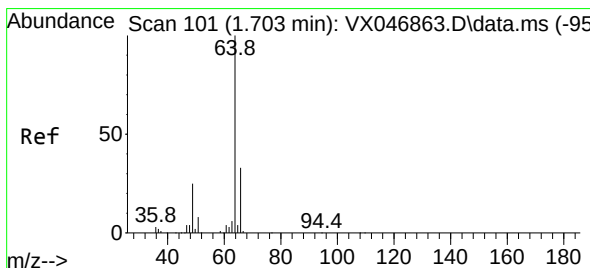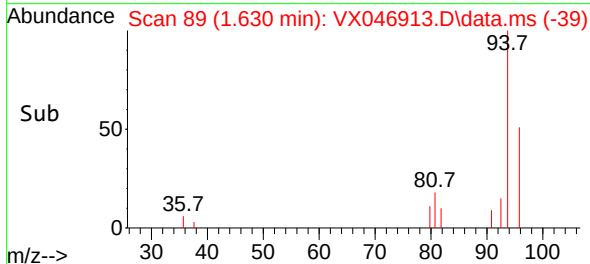

#6
Chloroethane
Concen: 0.428 ug/l
RT: 1.703 min Scan# 101
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32


Tgt Ion: 64 Resp: 1205
Ion Ratio Lower Upper
64 100
66 15.9 26.4 39.6#

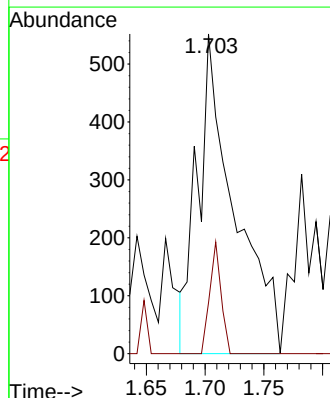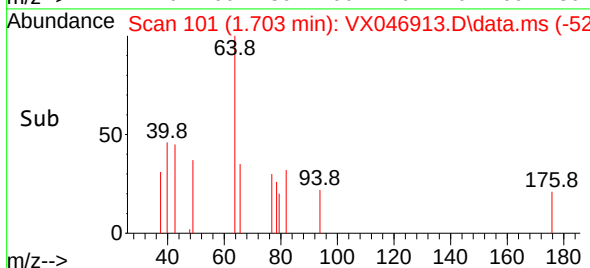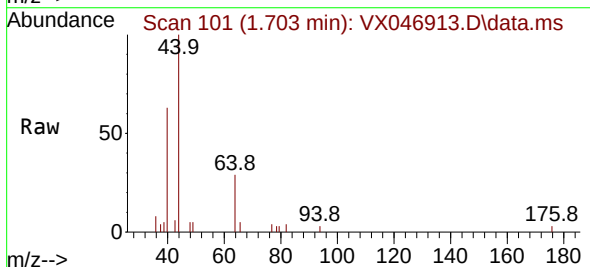






#10
Methyl Iodide
Concen: 0.321 ug/l
RT: 2.483 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32


Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025





Tgt Ion:142 Resp: 1466
Ion Ratio Lower Upper
142 100
127 72.1 34.9 52.3#
141 18.9 11.1 16.7#

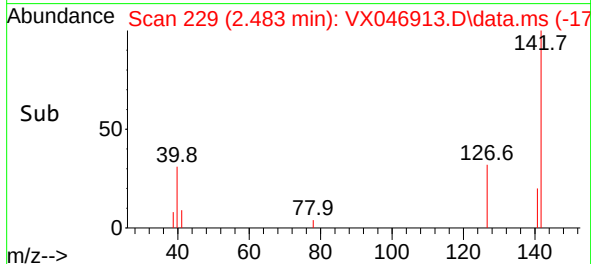


#12
1,1-Dichloroethene
Concen: 0.221 ug/l
RT: 2.337 min Scan# 205
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

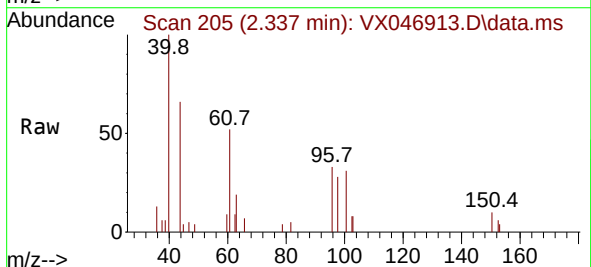

Tgt Ion: 96 Resp: 899
Ion Ratio Lower Upper
96 100
61 155.6 130.2 195.4
98 83.9 51.3 76.9#



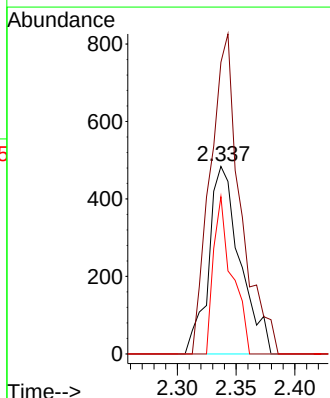
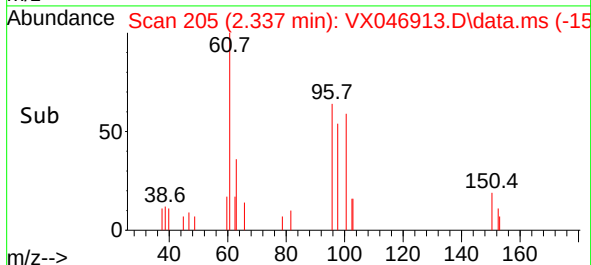




#13
Acrolein
Concen: 1.035 ug/l
RT: 2.252 min Scan# 14
Delta R.T. 0.006 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument : MSVOA_X
ClientSampleId : MDL-WATER-03-QT2-2025


Tgt Ion: 56 Resp: 401
Ion Ratio Lower Upper
56 100
55 118.7 55.5 83.3#

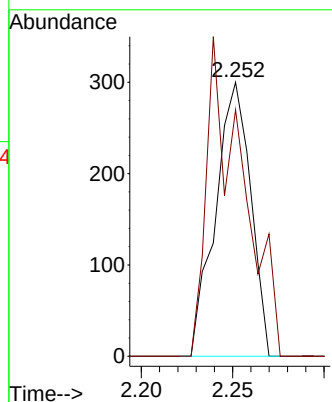

#15
Acrylonitrile
Concen: 0.685 ug/l
RT: 3.099 min Scan# 330
Delta R.T. 0.024 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion: 53 Resp: 1285
Ion Ratio Lower Upper
53 100
52 102.3 66.0 99.0#
51 19.5 28.6 43.0#


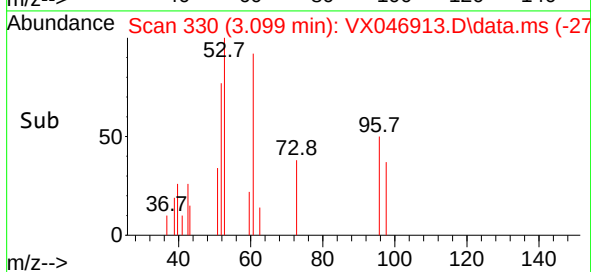
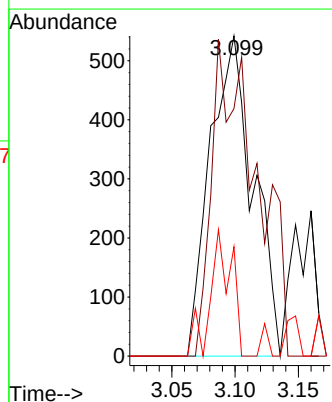
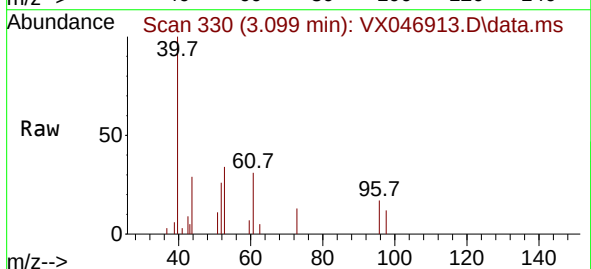




#16
Acetone
Concen: 1.357 ug/l
RT: 2.392 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion: 43 Resp: 2085
Ion Ratio Lower Upper
43 100
58 25.8 25.8 38.6

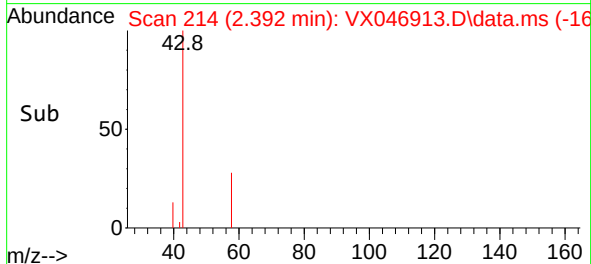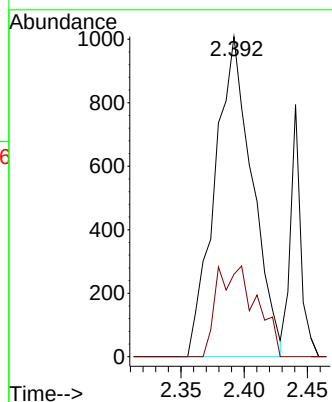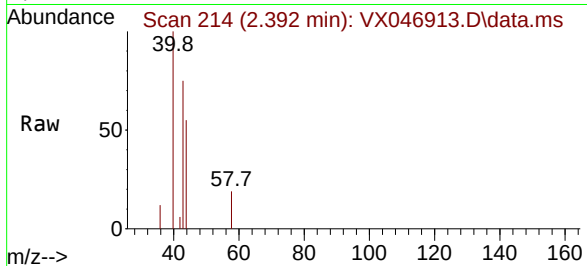

#17
Carbon Disulfide
Concen: 0.280 ug/l
RT: 2.532 min Scan# 237
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32


Tgt Ion: 76 Resp: 2978
Ion Ratio Lower Upper
76 100
78 6.9 7.4 11.2#

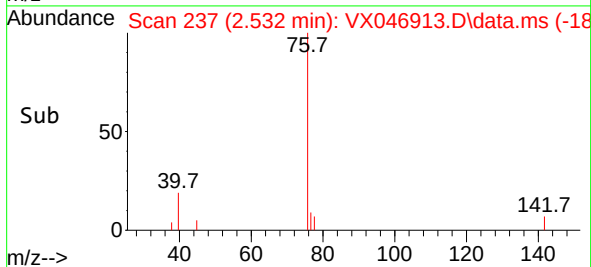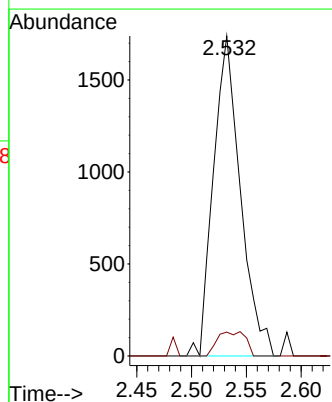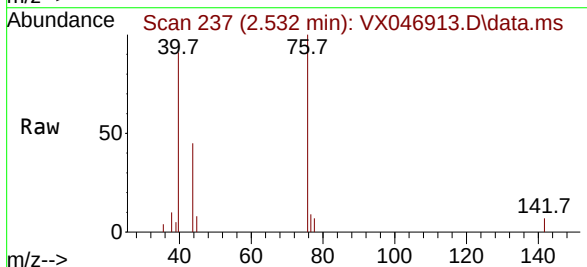



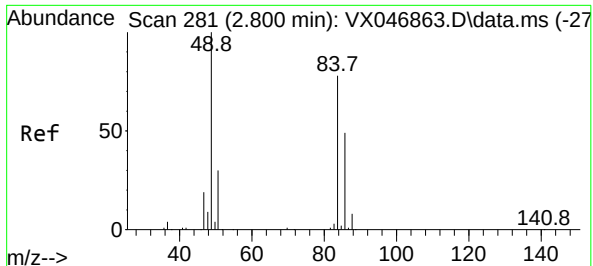


#20
Methylene Chloride
Concen: 0.402 ug/l
RT: 2.806 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025



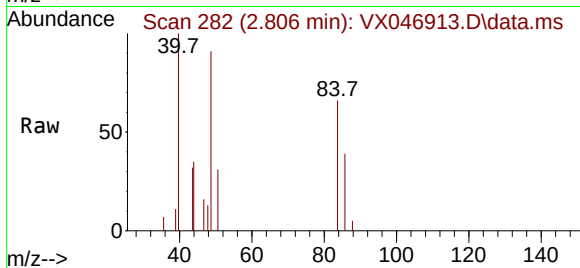



Tgt Ion: 84 Resp: 1827
Ion Ratio Lower Upper
84 100
49 136.7 102.8 154.2
51 46.8 31.1 46.7#
86 59.1 50.6 75.8

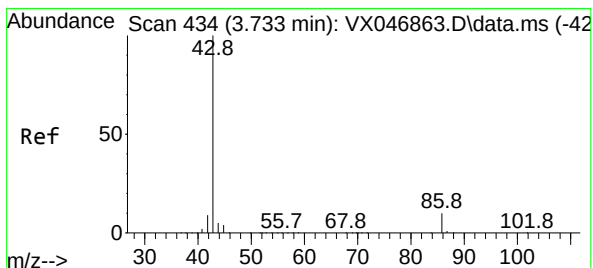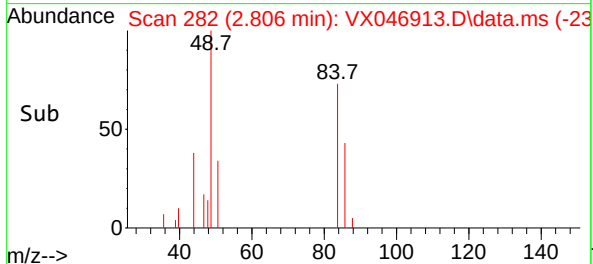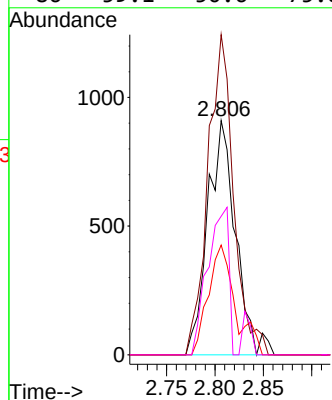

#23
Vinyl Acetate
Concen: 0.805 ug/l m
RT: 3.770 min Scan# 440
Delta R.T. 0.037 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion: 43 Resp: 8420
Ion Ratio Lower Upper
43 100
86 10.4 8.2 12.4

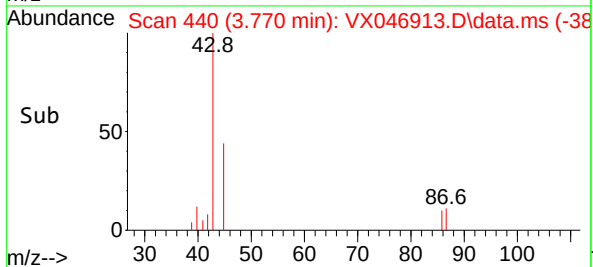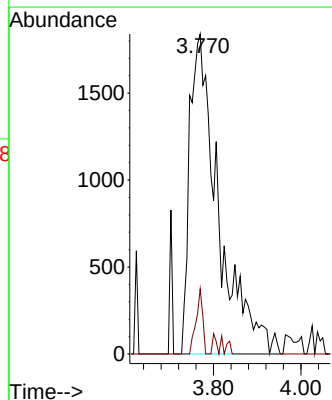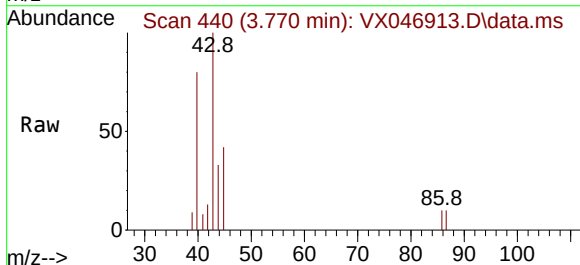



#29

Tetrahydrofuran

Concen: 1.056 ug/l m

RT: 5.056 min Scan# 61

Delta R.T. 0.049 min

Lab File: VX046913.D

Acq: 08 Jul 2025 11:32

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-03-QT2-2025





Tgt Ion: 42 Resp: 1380

Ion Ratio Lower Upper

42 100

72 17.3 35.1 52.7#

71 6.5 31.9 47.9#

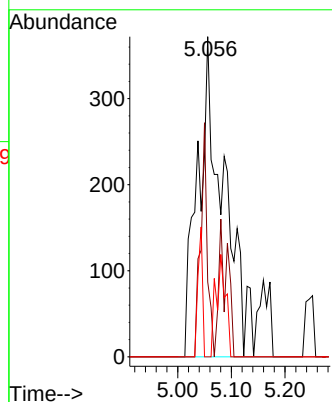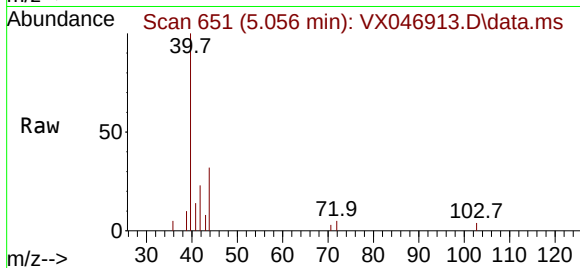

#33

1,2-Dichloroethane-d4

Concen: 52.246 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.006 min

Lab File: VX046913.D




Acq: 08 Jul 2025 11:32


Tgt Ion: 65 Resp: 258374

Ion Ratio Lower Upper

65 100

67 52.6 0.0 105.2

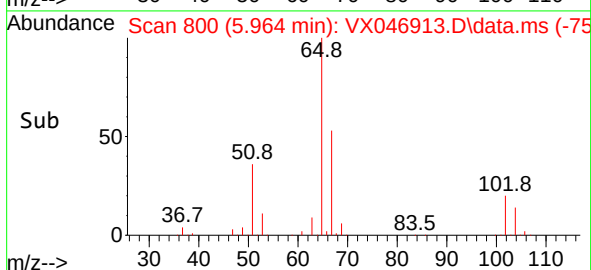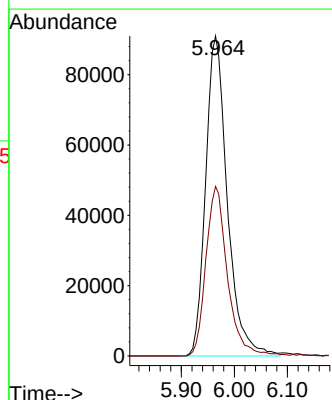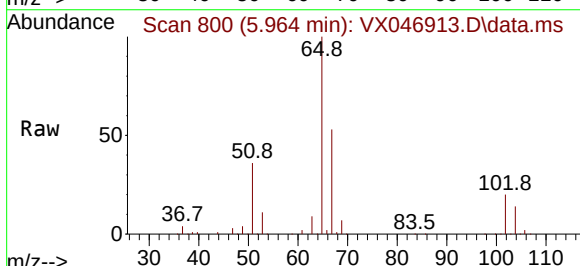



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX046913.D

Acq: 08 Jul 2025 11:32

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-03-QT2-2025





Tgt Ion:114 Resp: 638116

Ion Ratio Lower Upper

114 100

63 20.8 0.0 40.4

88 15.1 0.0 31.0

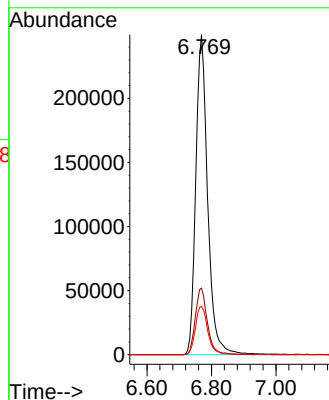

#35

Dibromofluoromethane

Concen: 49.598 ug/l

RT: 5.397 min Scan# 707

Delta R.T. -0.000 min

Lab File: VX046913.D

Acq: 08 Jul 2025 11:32




Tgt Ion:113 Resp: 214838


Ion Ratio Lower Upper

113 100

111 102.9 81.2 121.8

192 18.6 15.3 22.9



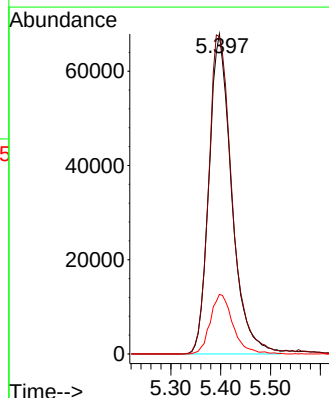
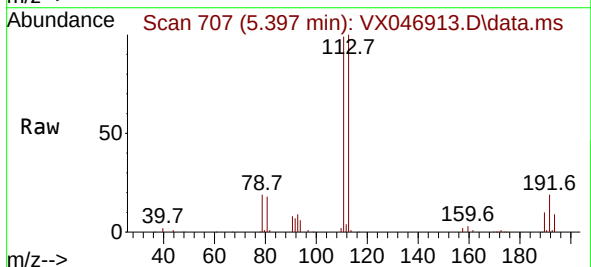




#36
1,1-Dichloropropene
Concen: 0.269 ug/l m
RT: 5.733 min Scan# 762
Delta R.T. 0.030 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion: 75 Resp: 1574
Ion Ratio Lower Upper
75 100
110 103.0 17.3 51.9#
77 0.0 24.2 36.4#

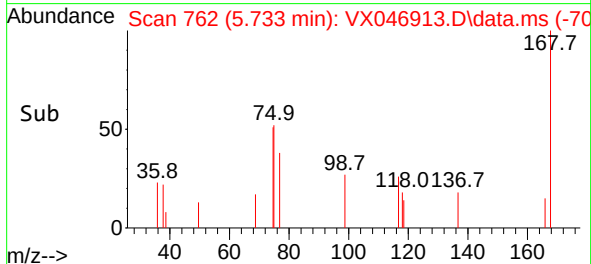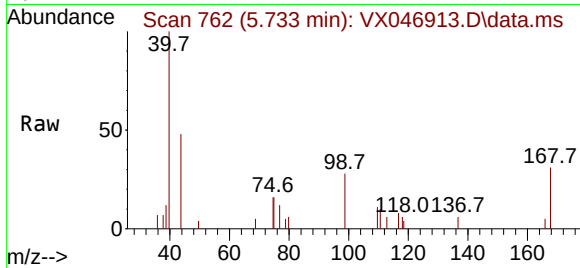

#38
Carbon Tetrachloride
Concen: 0.228 ug/l m
RT: 5.690 min Scan# 755
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion: 117 Resp: 1410
Ion Ratio Lower Upper
117 100
119 99.3 76.6 114.8
121 30.8 24.1 36.1

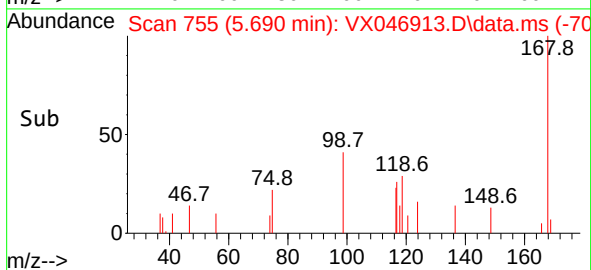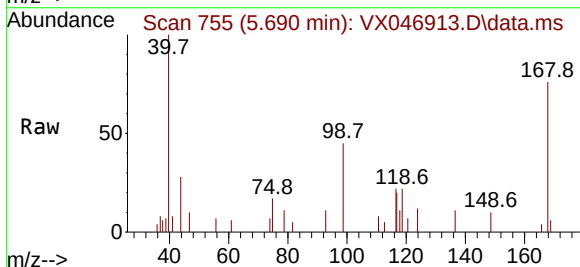

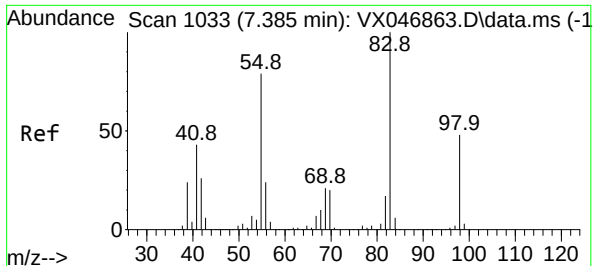

#39

Methylcyclohexane

Concen: 0.202 ug/l

RT: 7.385 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046913.D

Acq: 08 Jul 2025 11:32

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-03-QT2-2025





Tgt Ion: 83 Resp: 1474

Ion Ratio Lower Upper

83 100

55 73.5 63.0 94.4

98 38.9 38.5 57.7

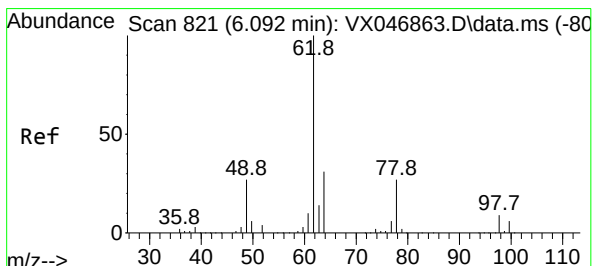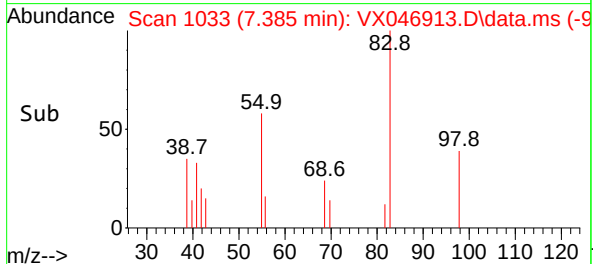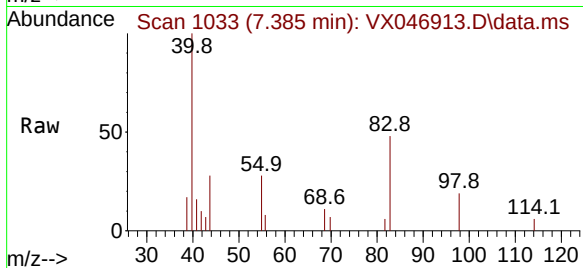

#42

1,2-Dichloroethane

Concen: 0.274 ug/l m

RT: 6.105 min Scan# 823

Delta R.T. 0.012 min

Lab File: VX046913.D




Acq: 08 Jul 2025 11:32


Tgt Ion: 62 Resp: 1642

Ion Ratio Lower Upper

62 100

98 4.9 0.0 19.4


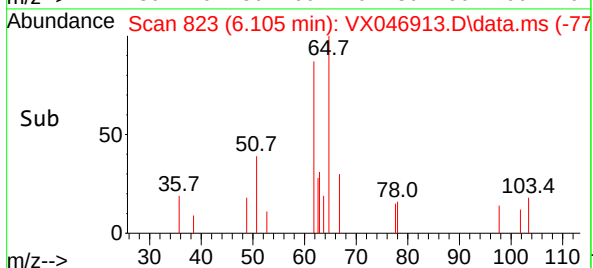
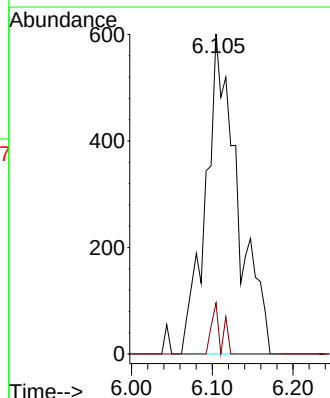
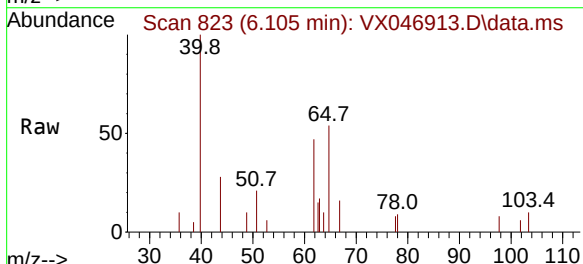


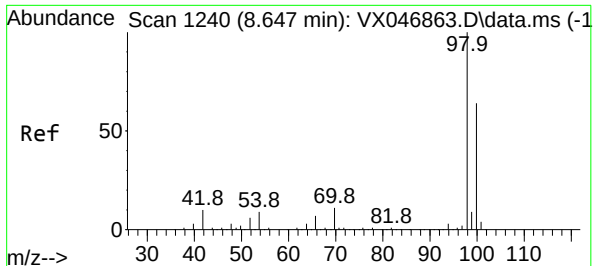

#50
Toluene-d8
Concen: 48.845 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion: 98 Resp: 746478
Ion Ratio Lower Upper
98 100
100 67.2 53.0 79.6

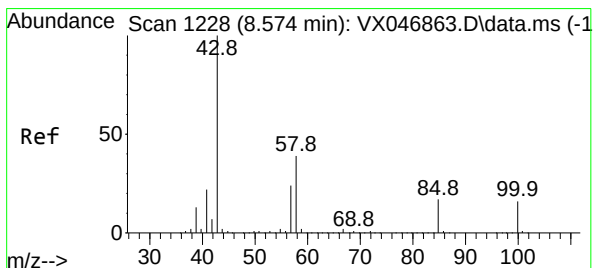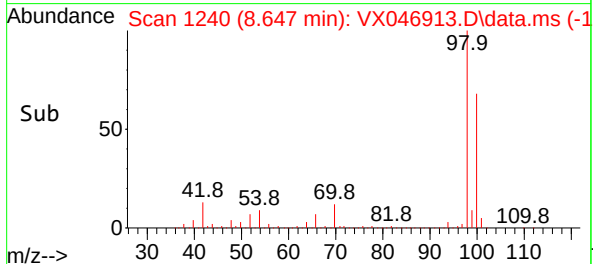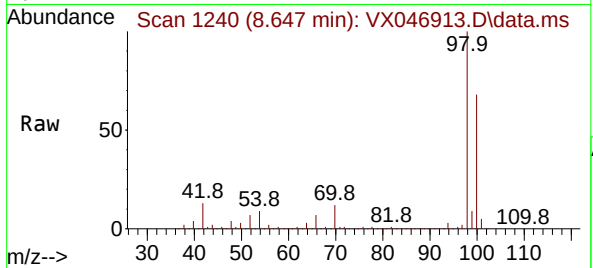

#51
4-Methyl-2-Pentanone
Concen: 0.706 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion: 43 Resp: 3178
Ion Ratio Lower Upper
43 100
58 39.9 30.4 45.6


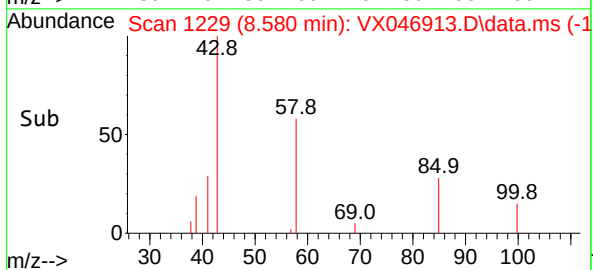

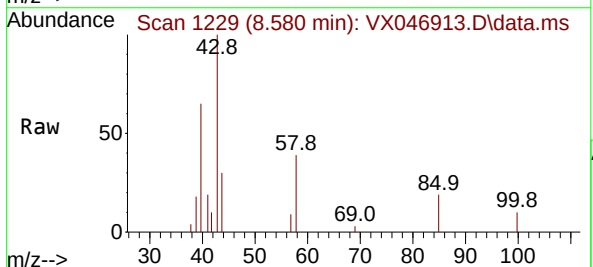


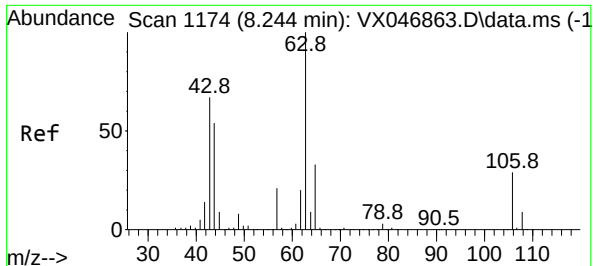

#58
2-Chloroethyl Vinyl ether
Concen: 0.654 ug/l m
RT: 8.281 min Scan# 1174
Delta R.T. 0.037 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion: 63 Resp: 2082
Ion Ratio Lower Upper
63 100
106 17.3 22.6 33.8#

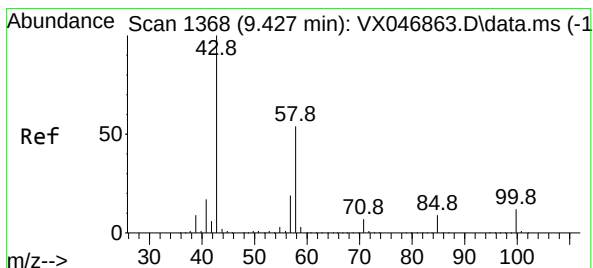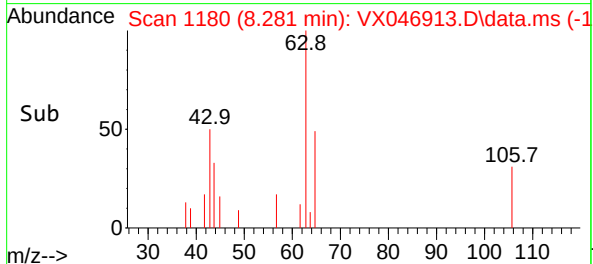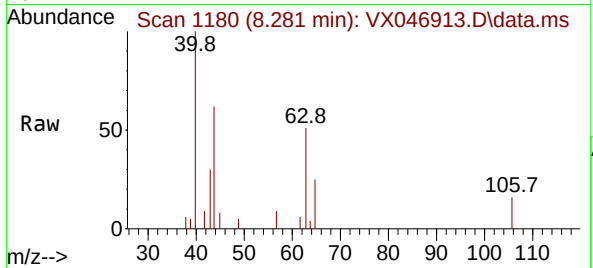

#59
2-Hexanone
Concen: 0.612 ug/l m
RT: 9.476 min Scan# 1376
Delta R.T. 0.049 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion: 43 Resp: 1827
Ion Ratio Lower Upper
43 100
58 33.1 27.1 81.3


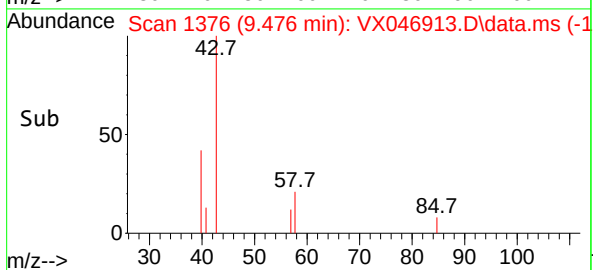

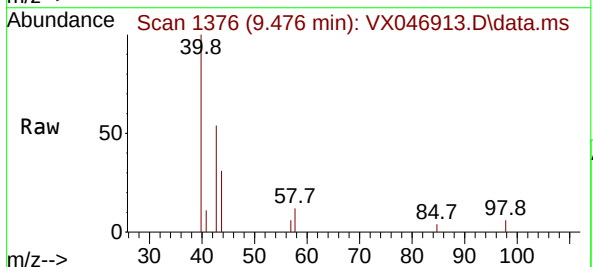




#62
4-Bromofluorobenzene
Concen: 51.673 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion: 95 Resp: 300130
Ion Ratio Lower Upper
95 100
174 76.1 0.0 152.0
176 71.9 0.0 145.2

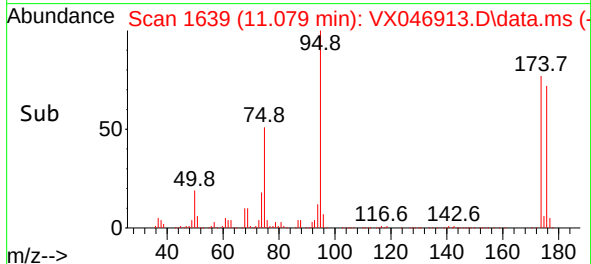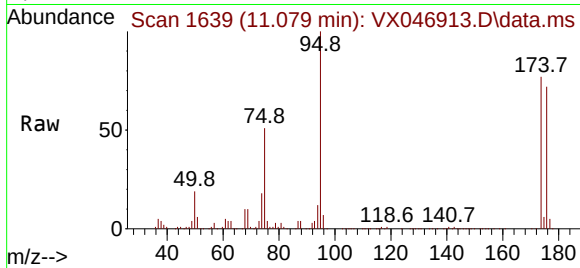

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion: 117 Resp: 589137
Ion Ratio Lower Upper
117 100
82 54.1 43.3 64.9
119 32.0 26.4 39.6



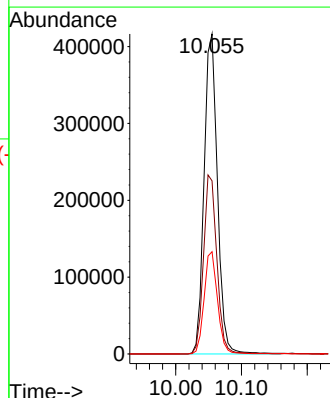
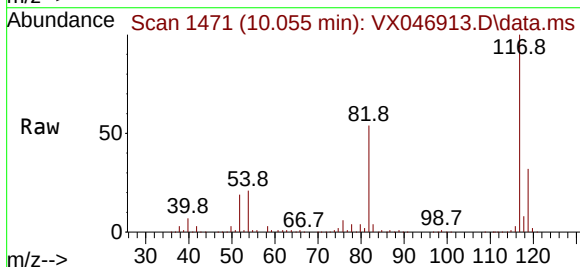




#64
Tetrachloroethene
Concen: 0.210 ug/l
RT: 9.281 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion:164 Resp: 824
Ion Ratio Lower Upper
164 100
166 105.3 107.0 160.6#
129 88.8 79.7 119.5
131 80.9 77.1 115.7

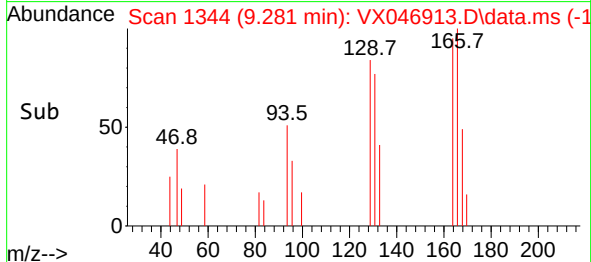

#65
Chlorobenzene
Concen: 0.215 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion:112 Resp: 2736
Ion Ratio Lower Upper
112 100
114 27.0 26.3 39.5


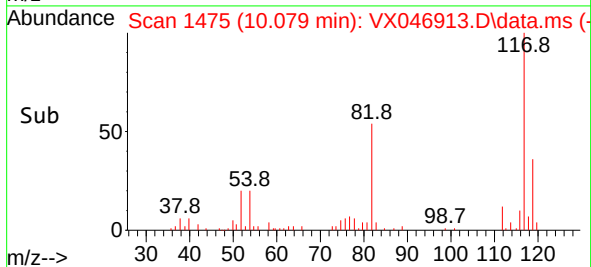

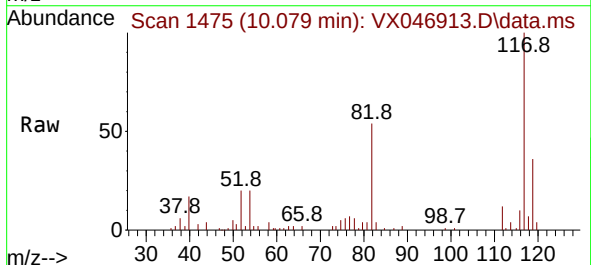




#68
m/p-Xylenes
Concen: 0.318 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion:106 Resp: 2615
Ion Ratio Lower Upper
106 100
91 202.8 164.6 246.8

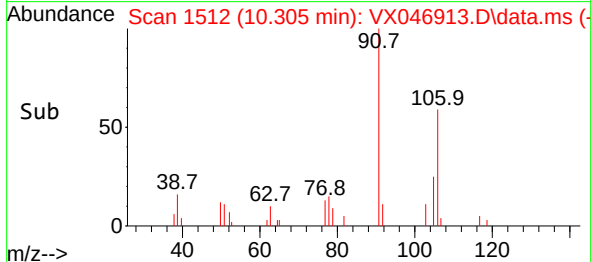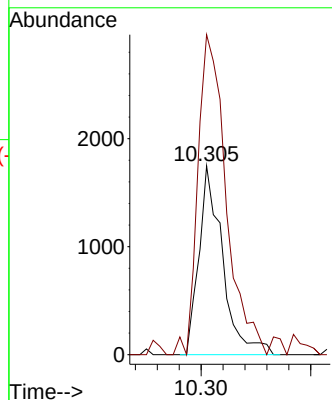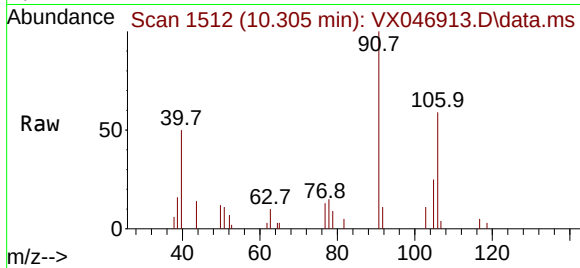

#71
Bromoform
Concen: 0.222 ug/l
RT: 10.799 min Scan# 1593
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion:173 Resp: 707
Ion Ratio Lower Upper
173 100
175 64.8 23.8 71.5
254 0.0 0.1 0.1#


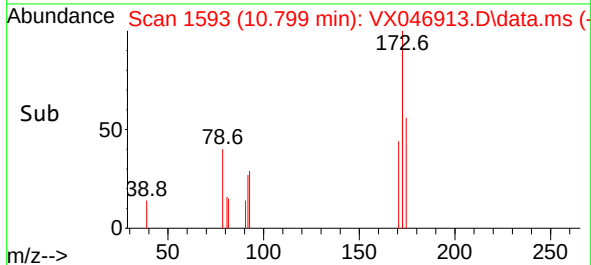
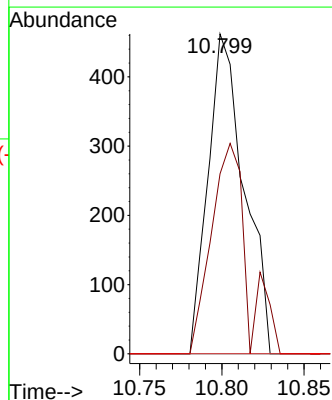
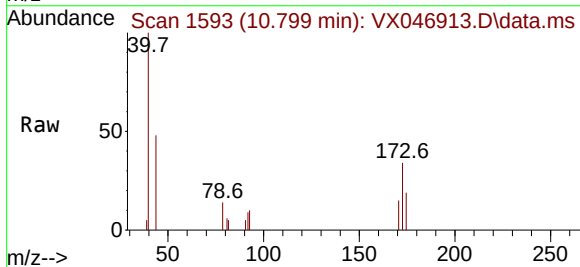




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX046913.D
 Acq: 08 Jul 2025 11:32




Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-03-QT2-2025


Tgt Ion:152 Resp: 304916
 Ion Ratio Lower Upper
 152 100
 115 59.8 42.4 127.1
 150 158.4 0.0 349.2

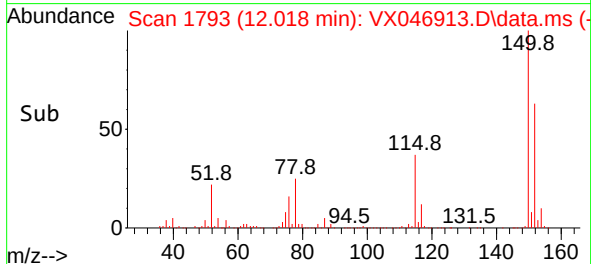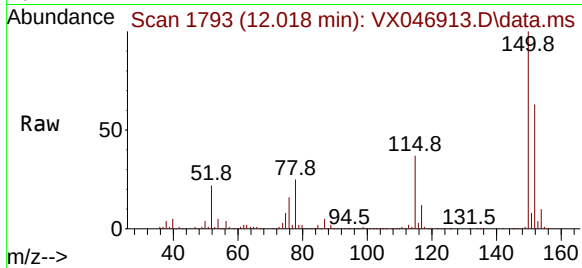

#74
 N-ethyl acetate
 Concen: 0.271 ug/l m
 RT: 10.860 min Scan# 1603
 Delta R.T. 0.018 min
 Lab File: VX046913.D
 Acq: 08 Jul 2025 11:32

Tgt Ion: 43 Resp: 1972
 Ion Ratio Lower Upper
 43 100
 70 0.0 33.4 50.2#
 55 0.0 19.6 29.4#
 61 0.0 18.9 28.3#


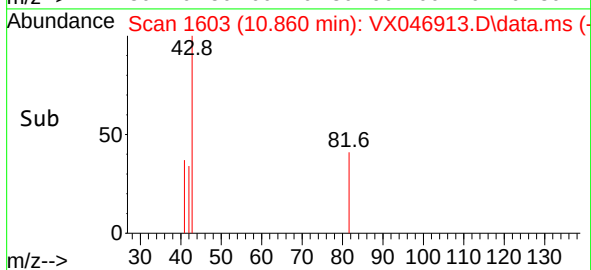

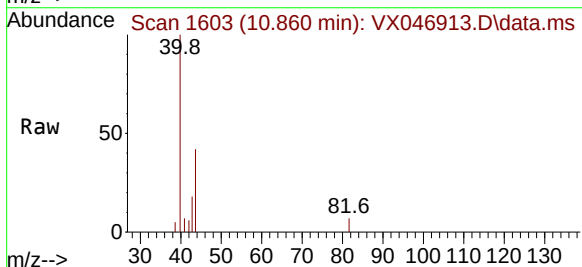




#87
1,3-Dichlorobenzene
Concen: 0.213 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.012 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion:146 Resp: 2122
Ion Ratio Lower Upper
146 100
111 36.3 20.5 61.6
148 59.0 31.4 94.2

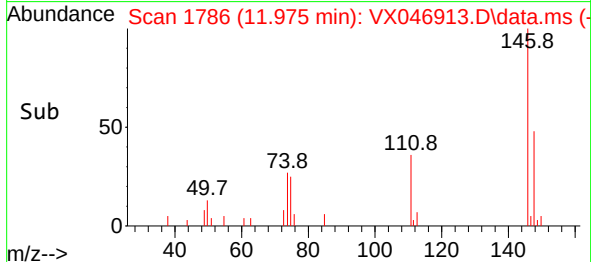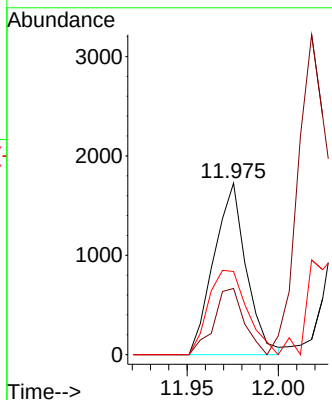

#88
1,4-Dichlorobenzene
Concen: 0.241 ug/l m
RT: 12.043 min Scan# 1797
Delta R.T. 0.006 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32

Tgt Ion:146 Resp: 2508
Ion Ratio Lower Upper
146 100
111 30.7 20.2 60.5
148 50.0 32.4 97.0


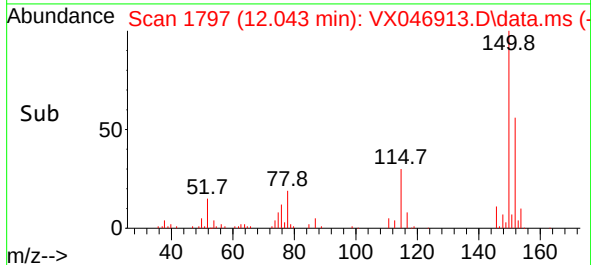
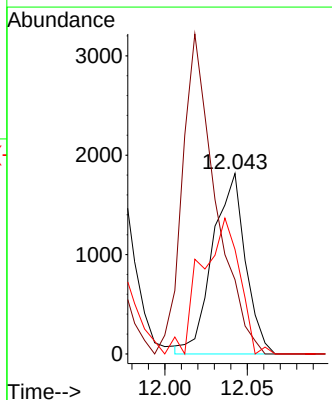
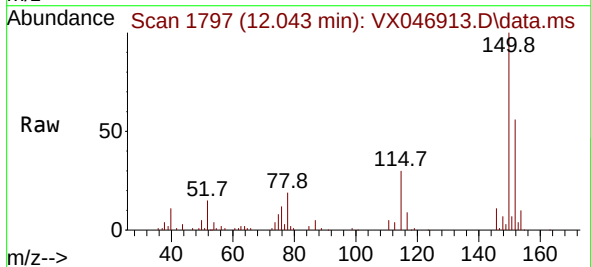




#93
1,2,4-Trichlorobenzene
Concen: 0.241 ug/l
RT: 13.597 min Scan# 2052
Delta R.T. 0.012 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT2-2025


Tgt Ion:180 Resp: 1583
Ion Ratio Lower Upper
180 100
182 107.2 47.3 141.9
145 23.9 16.1 48.2

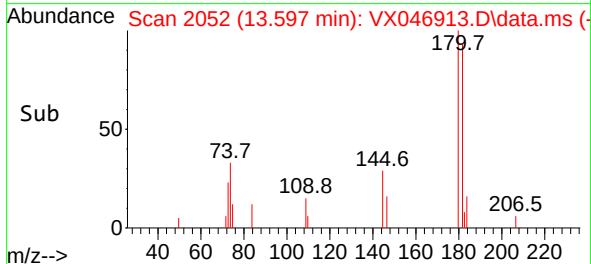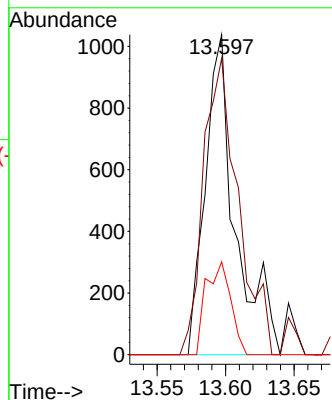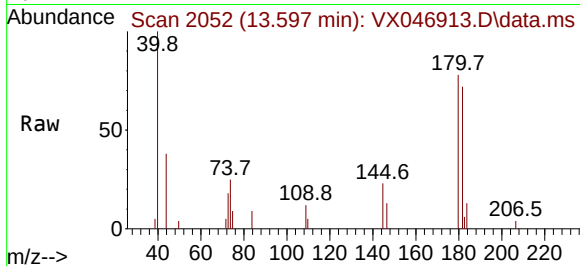

#94
Hexachlorobutadiene
Concen: 0.552 ug/l
RT: 13.719 min Scan# 2072
Delta R.T. -0.000 min
Lab File: VX046913.D
Acq: 08 Jul 2025 11:32


Tgt Ion:225 Resp: 1369
Ion Ratio Lower Upper
225 100
223 57.0 31.6 94.7
227 61.6 31.6 94.7

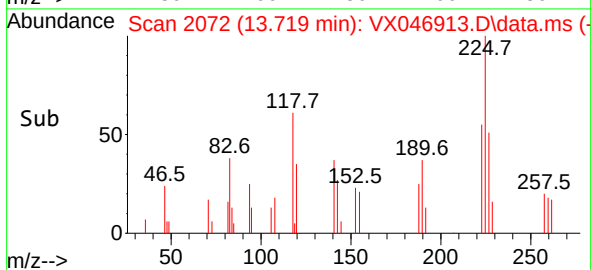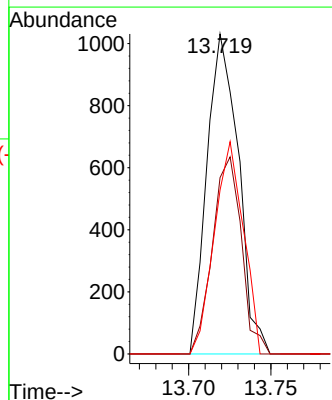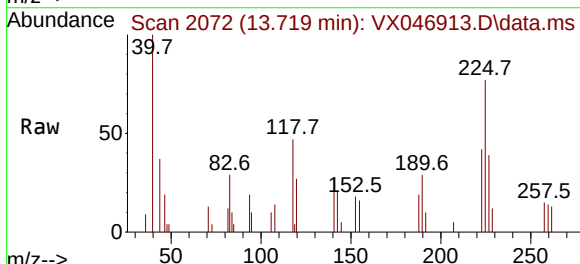



#96
 1,2,3-Trichlorobenzene
 Concen: 0.242 ug/l
 RT: 13.963 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX046913.D
 Acq: 08 Jul 2025 11:32

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-03-QT2-2025

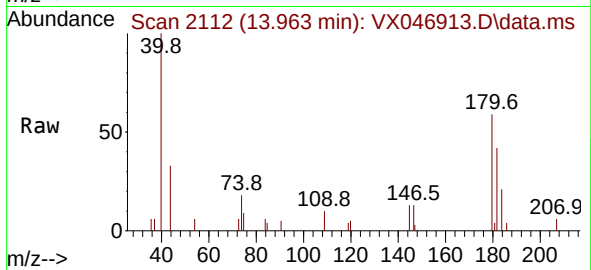

Tgt Ion:	180	Resp:	1504
Ion	Ratio	Lower	Upper
180	100		
182	70.6	46.7	140.1
145	28.3	16.8	50.3

