



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070825\
Data File : VX046906.D
Acq On : 08 Jul 2025 08:44
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Title : SW846 8260
Last Update : Thu Jul 03 05:51:11 2025

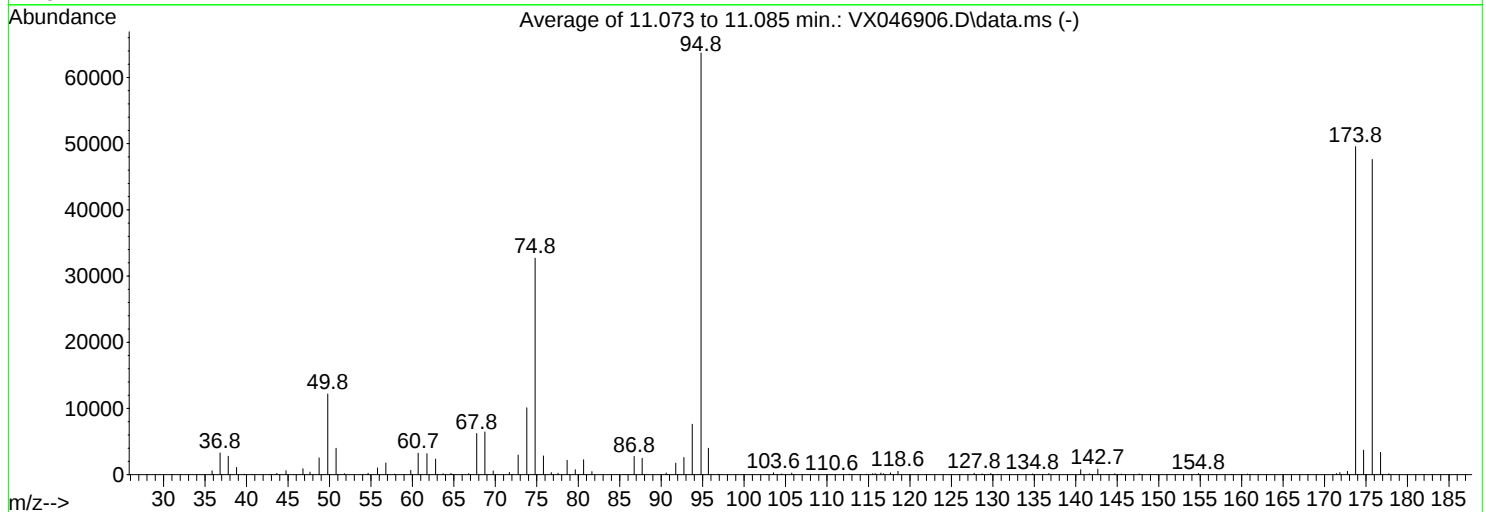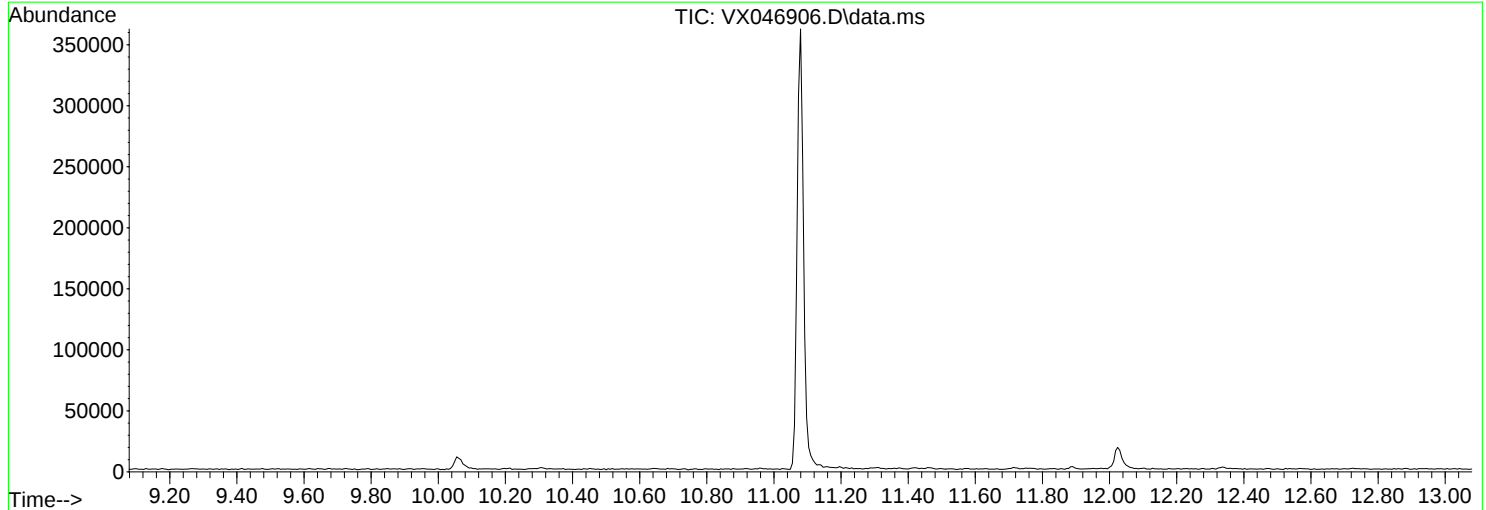

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	12177	PASS
75	95	30	60	51.3	32699	PASS
95	95	100	100	100.0	63720	PASS
96	95	5	9	6.3	3987	PASS
173	174	0.00	2	1.0	500	PASS
174	95	50	100	77.7	49541	PASS
175	174	5	9	7.5	3710	PASS
176	174	95	101	96.1	47624	PASS
177	176	5	9	7.1	3360	PASS