

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070918\
 Data File : VX003247.D
 Acq On : 09 Jul 2018 16:04
 Operator : JC/MD
 Sample : J3854-03
 Misc : 4.50µ/5mL/100µL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S5

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X070918W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.069	75	79	93	rBV	681665	902593	71.80%	11.264%
2	1.264	107	111	117	rBV	12801	19345	1.54%	0.241%
3	1.636	158	172	174	rBV5	18505	48760	3.88%	0.608%
4	2.843	365	370	382	rVB4	6099	14265	1.13%	0.178%
5	3.014	394	398	407	rVB	6265	13670	1.09%	0.171%
6	5.501	792	806	822	rBV	157679	455026	36.20%	5.678%
7	5.660	822	832	849	rVB	236807	677161	53.87%	8.450%
8	6.068	888	899	917	rVB	162637	421825	33.56%	5.264%
9	6.861	1018	1029	1043	rBV	340329	799417	63.60%	9.976%
10	7.452	1117	1126	1134	rBV4	9316	21934	1.74%	0.274%
11	8.714	1326	1333	1341	rBV	794388	1257017	100.00%	15.687%
12	8.787	1342	1345	1349	rVB	10895	16430	1.31%	0.205%
13	10.116	1557	1563	1580	rBV	694372	967806	76.99%	12.078%
14	10.360	1593	1603	1608	rBV	16865	25288	2.01%	0.316%
15	10.701	1654	1659	1668	rVB3	14539	22451	1.79%	0.280%
16	11.140	1725	1731	1745	rBV	799549	1008691	80.24%	12.588%
17	11.512	1788	1792	1801	rVB6	6959	12978	1.03%	0.162%
18	11.811	1837	1841	1850	rVB	9261	12635	1.01%	0.158%
19	12.079	1880	1885	1893	rBV	974689	1243185	98.90%	15.514%
20	12.390	1930	1936	1942	rVB5	7889	13798	1.10%	0.172%
21	13.835	2168	2173	2178	rVB	18356	25423	2.02%	0.317%
22	14.701	2305	2315	2323	rBV	13073	20791	1.65%	0.259%
23	14.841	2335	2338	2344	rVB	10113	12784	1.02%	0.160%


Sum of corrected areas: 8013273

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070918\
Data File : VX003247.D
Acq On : 09 Jul 2018 16:04
Operator : JC/MD
Sample : J3854-03
Misc : 4.50µL/5mL/100µL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X070918W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

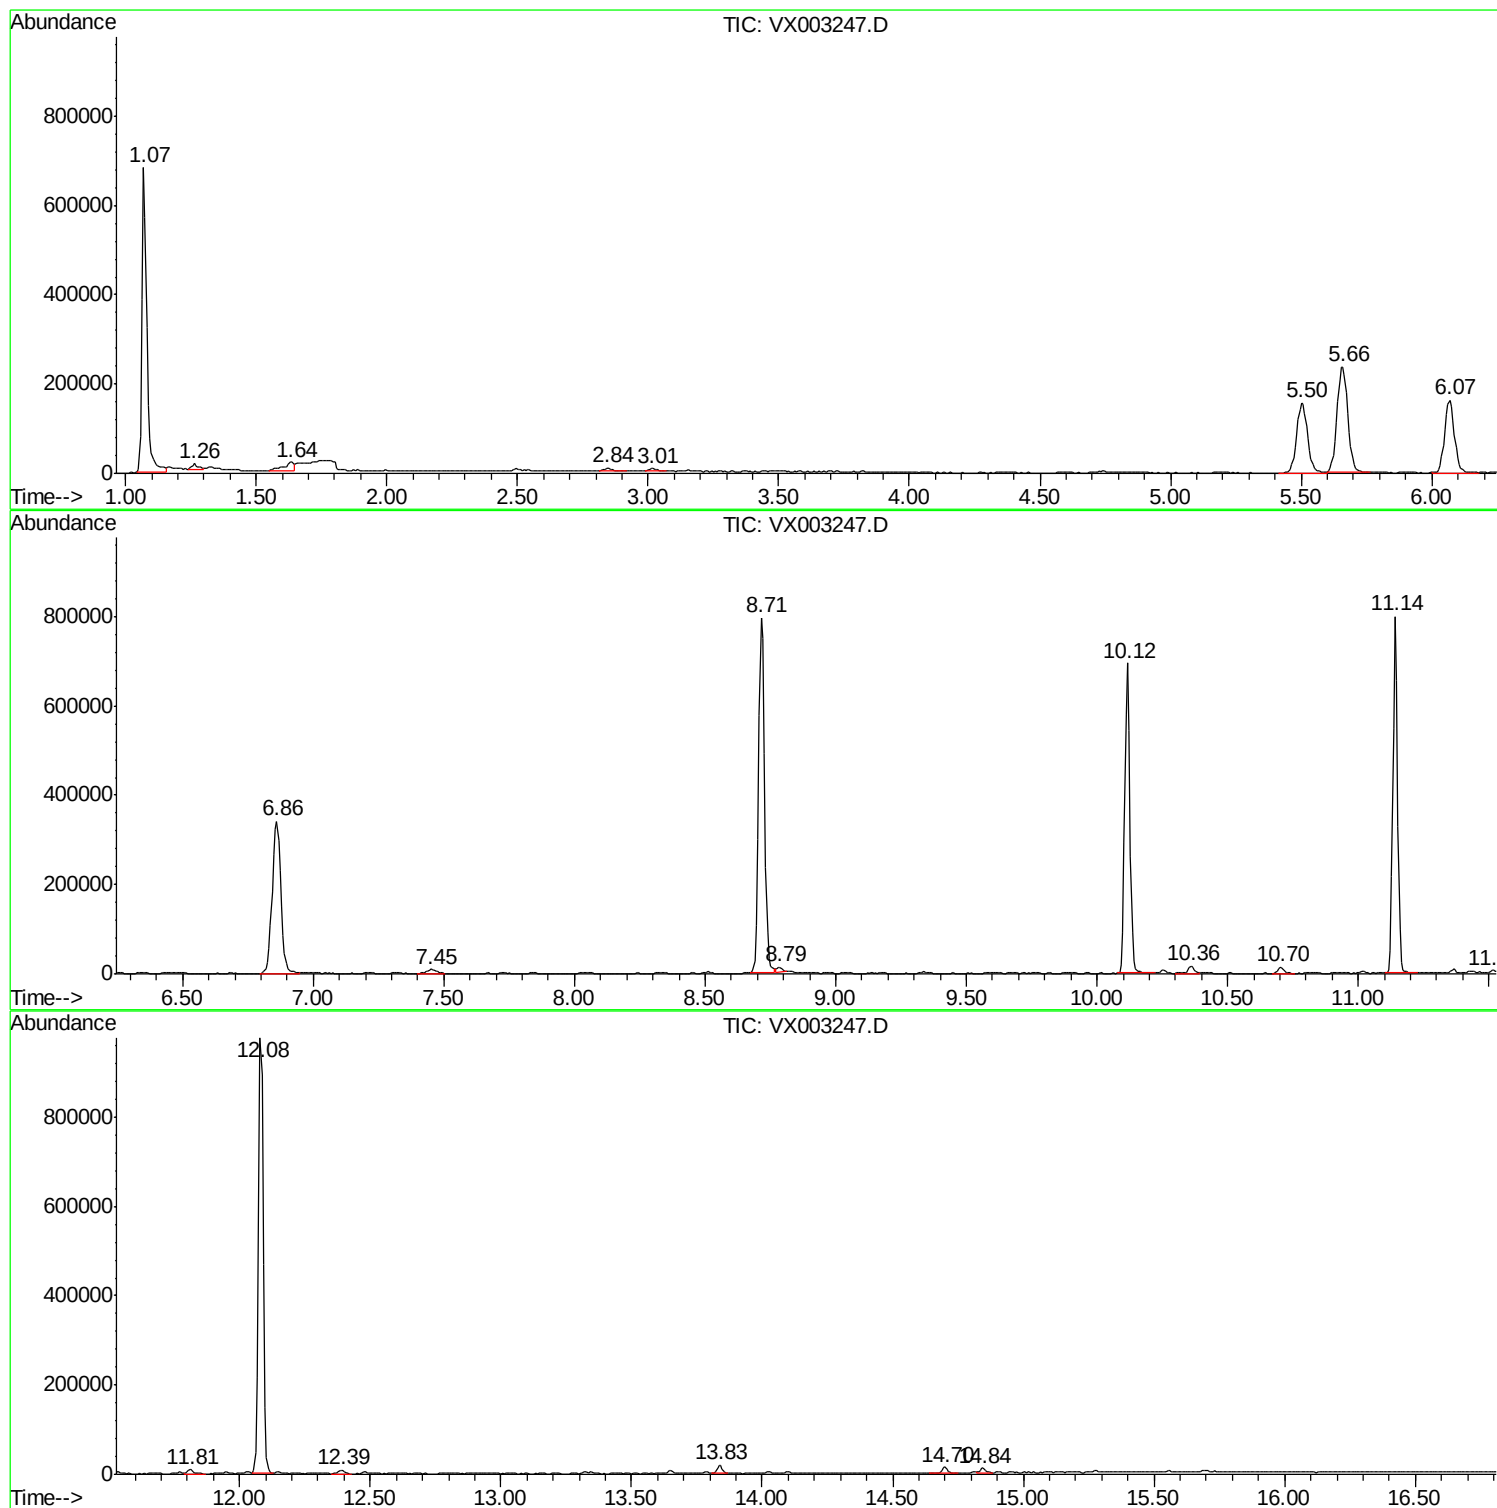

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070918\
Data File : VX003247.D
Acq On : 09 Jul 2018 16:04
Operator : JC/MD
Sample : J3854-03
Misc : 4.50g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X070918W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Carbon dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.07	66.65 ug/l	902593	Pentafluorobenzene	5.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Carbon dioxide	44	C02	000124-38-9	4
2			Ethylene oxide	44	C2H4O	000075-21-8	3
3			Nitrous oxide	44	N2O	010024-97-2	3
4			Ethyne, fluoro-	44	C2HF	002713-09-9	2
5			Acetaldehyde	44	C2H4O	000075-07-0	2

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070918\
Data File : VX003247.D
Acq On : 09 Jul 2018 16:04
Operator : JC/MD
Sample : J3854-03
Misc : 4.50g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X070918W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Carbon dioxide	1.07	66.6	ug/l	902593	1	5.66	677161	50.0