


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070918\
Data File : VX003251.D
Acq On : 09 Jul 2018 18:17
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X070918W.M
Title : SW846 8260
Last Update : Mon Jul 09 15:24:16 2018

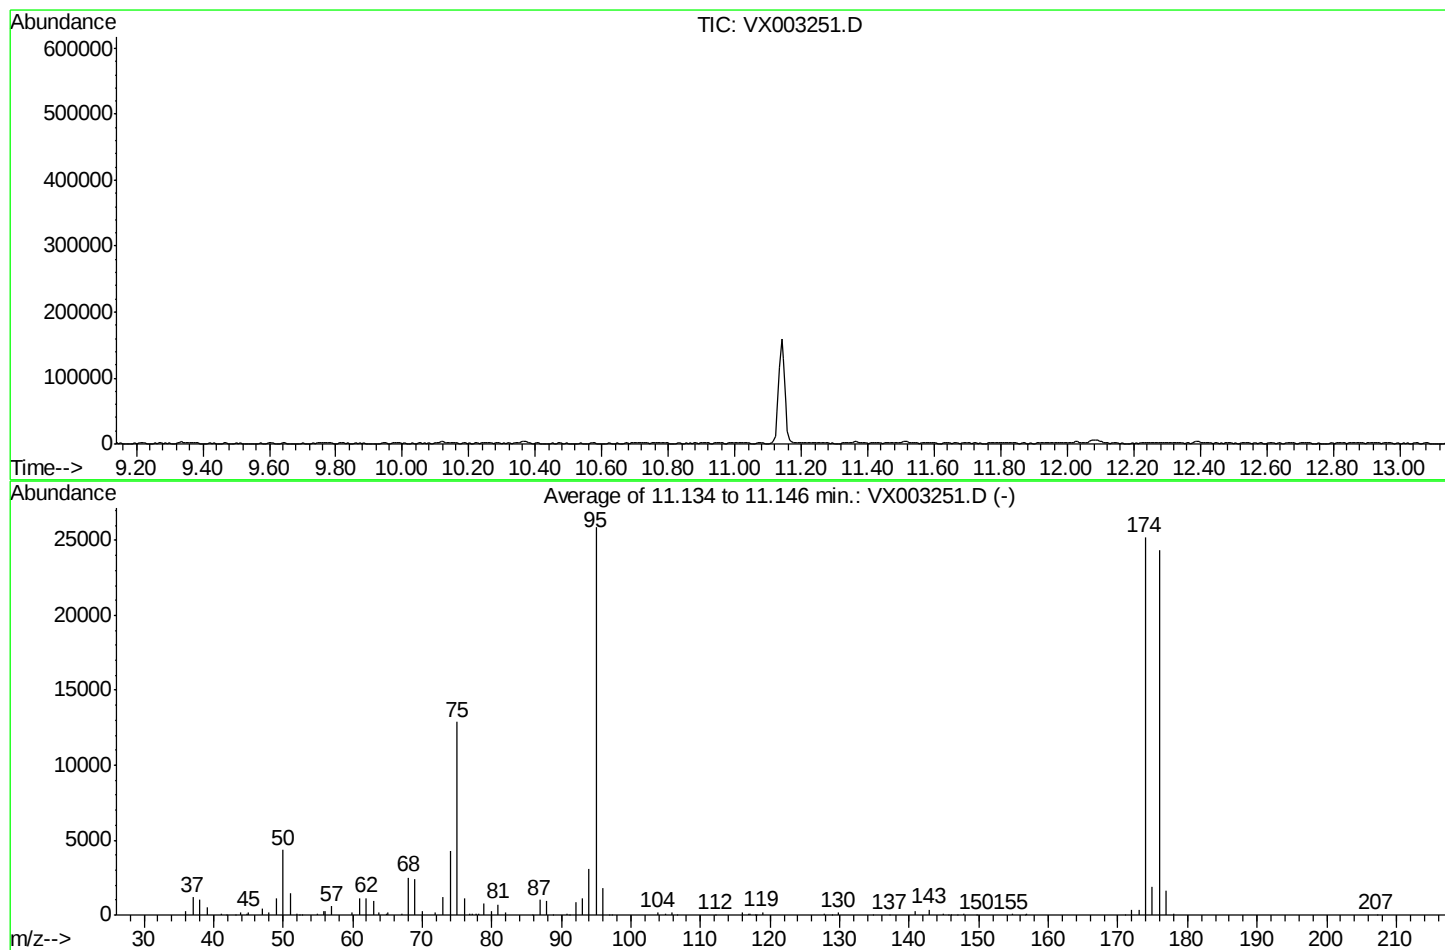

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	4329	PASS
75	95	30	60	49.8	12878	PASS
95	95	100	100	100.0	25877	PASS
96	95	5	9	7.0	1804	PASS
173	174	0.00	2	1.4	355	PASS
174	95	50	100	97.3	25181	PASS
175	174	5	9	7.6	1917	PASS
176	174	95	101	96.7	24341	PASS
177	176	5	9	6.8	1644	PASS