

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070919\
Data File : VX010742.D
Acq On : 09 Jul 2019 11:54
Operator : JC/SP
Sample : K3705-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-1-NE-BOILER-PIT

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	16	21	27	rBV	11999	18047	1.64%	0.286%
2	2.440	205	211	219	rBV	69742	114611	10.41%	1.815%
3	5.214	655	666	678	rBV	49646	147998	13.45%	2.344%
4	5.501	700	713	728	rBV	134341	388573	35.31%	6.154%
5	5.659	728	739	754	rVB	223847	632839	57.51%	10.022%
6	6.061	795	805	825	rBV	128153	337596	30.68%	5.346%
7	6.860	925	936	949	rBV	334779	799580	72.66%	12.662%
8	8.713	1233	1240	1249	rBV	719649	1100472	100.00%	17.427%
9	9.634	1387	1391	1399	rBV	54272	74311	6.75%	1.177%
10	10.110	1463	1469	1481	rBV	697943	953621	86.66%	15.102%
11	10.250	1488	1492	1499	rVB	11140	17278	1.57%	0.274%
12	10.353	1502	1509	1516	rBV	40002	58540	5.32%	0.927%
13	10.695	1560	1565	1575	rBV	17752	29761	2.70%	0.471%
14	11.134	1632	1637	1649	rBV	606683	754418	68.55%	11.947%
15	12.079	1786	1792	1798	rBV	684901	886967	80.60%	14.046%


Sum of corrected areas: 6314612

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070919\
Data File : VX010742.D
Acq On : 09 Jul 2019 11:54
Operator : JC/SP
Sample : K3705-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-1-NE-BOILER-PIT

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

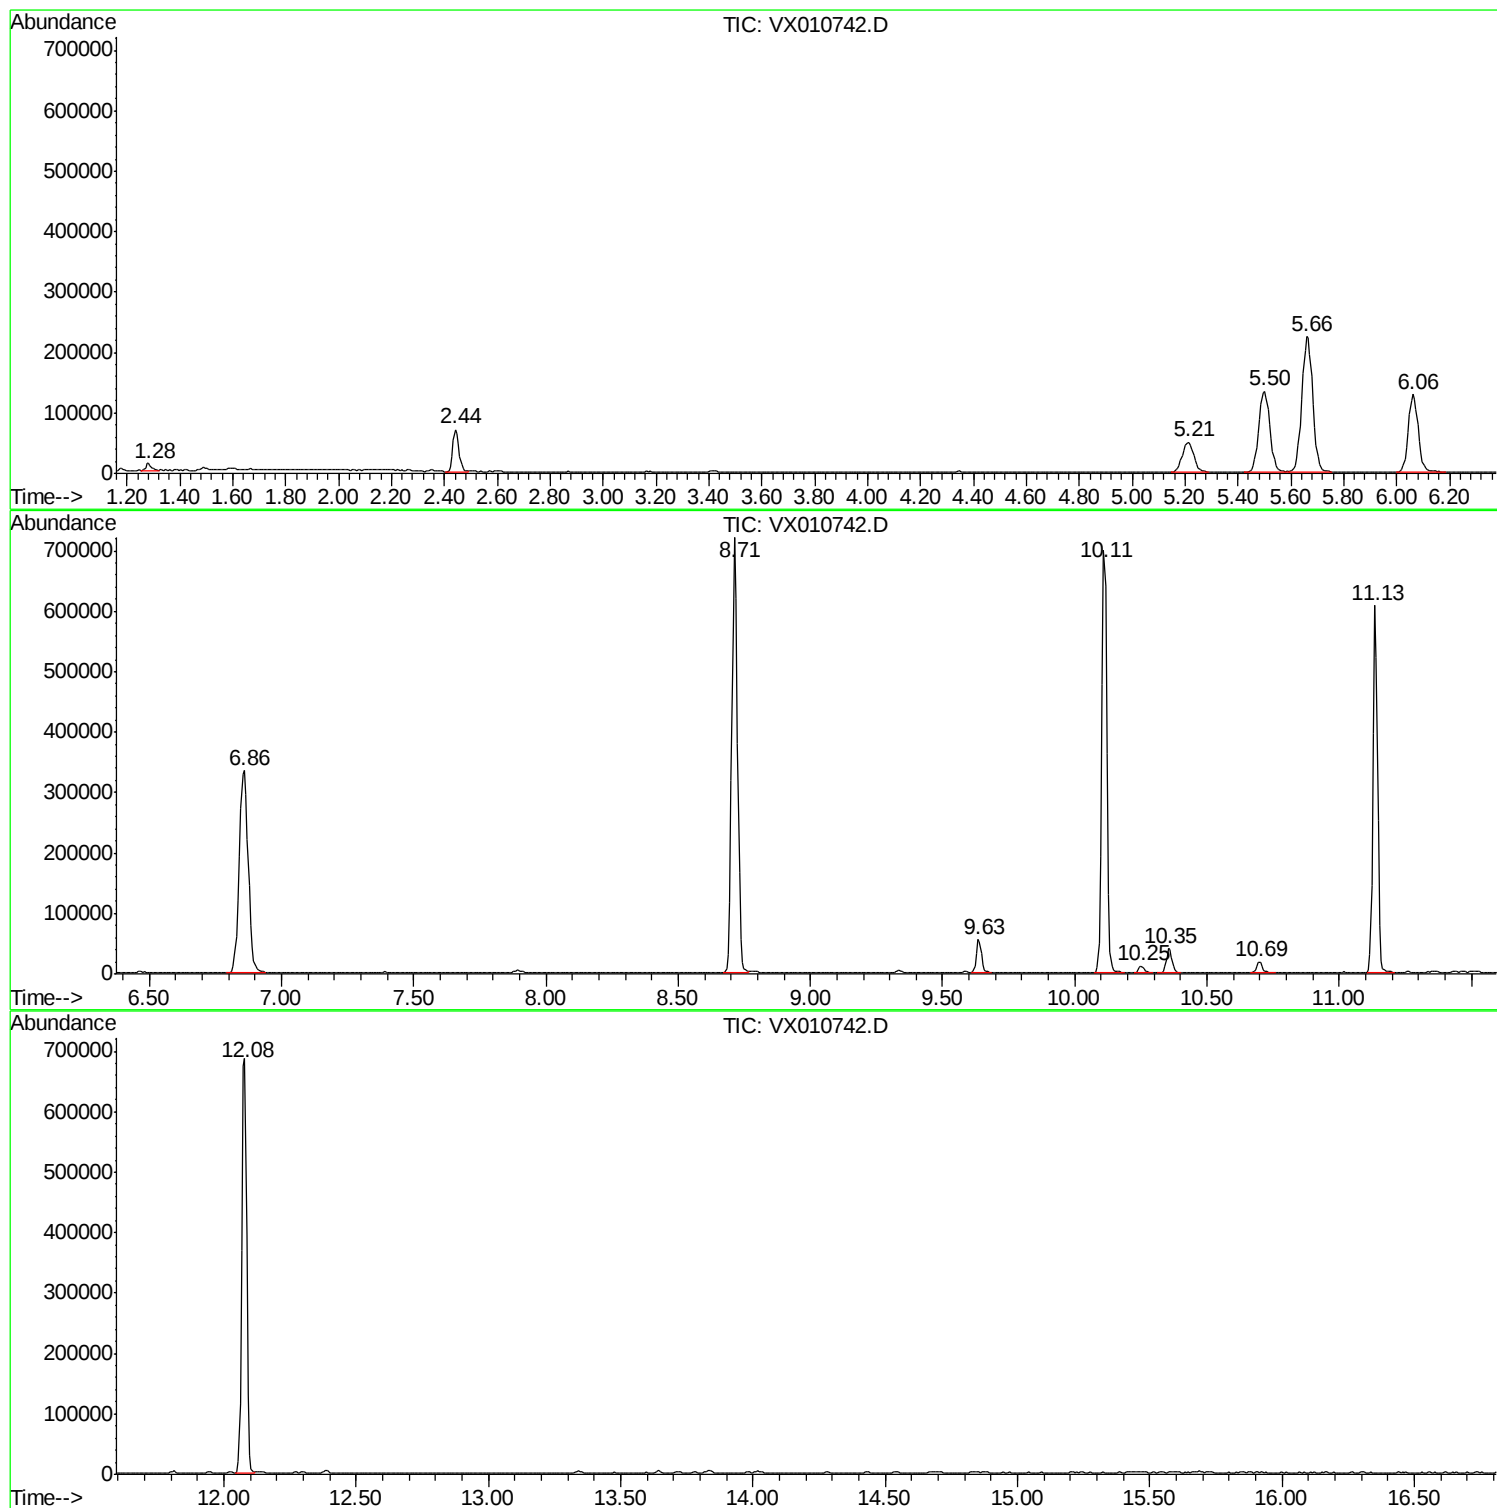

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070919\
Data File : VX010742.D
Acq On : 09 Jul 2019 11:54
Operator : JC/SP
Sample : K3705-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-1-NE-BOILER-PIT

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070919\
Data File : VX010742.D
Acq On : 09 Jul 2019 11:54
Operator : JC/SP
Sample : K3705-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-1-NE-BOILER-PIT

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc