

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070919\
 Data File : VX010750.D
 Acq On : 09 Jul 2019 15:01
 Operator : JC/SP
 Sample : K3691-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-0535-190704

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	30	rBV	51401	67789	6.46%	1.154%
2	1.410	38	42	47	rVB	15066	16978	1.62%	0.289%
3	3.019	298	306	314	rBV2	18740	45177	4.30%	0.769%
4	4.702	570	582	591	rBV2	8950	29617	2.82%	0.504%
5	5.501	701	713	725	rBV	125643	359056	34.19%	6.110%
6	5.659	728	739	750	rBV	208764	590035	56.19%	10.041%
7	6.061	795	805	815	rBV2	122902	323361	30.79%	5.503%
8	6.860	926	936	948	rBV	316534	749782	71.40%	12.759%
9	8.713	1233	1240	1249	rBV	686602	1045708	99.58%	17.795%
10	10.109	1463	1469	1483	rBV2	675901	1050084	100.00%	17.869%
11	11.134	1631	1637	1650	rBV	553048	721080	68.67%	12.271%
12	12.079	1786	1792	1801	rBV	664604	867014	82.57%	14.754%
13	12.390	1837	1843	1848	rVB3	6631	10759	1.02%	0.183%


Sum of corrected areas: 5876440

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070919\
Data File : VX010750.D
Acq On : 09 Jul 2019 15:01
Operator : JC/SP
Sample : K3691-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-0535-190704

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

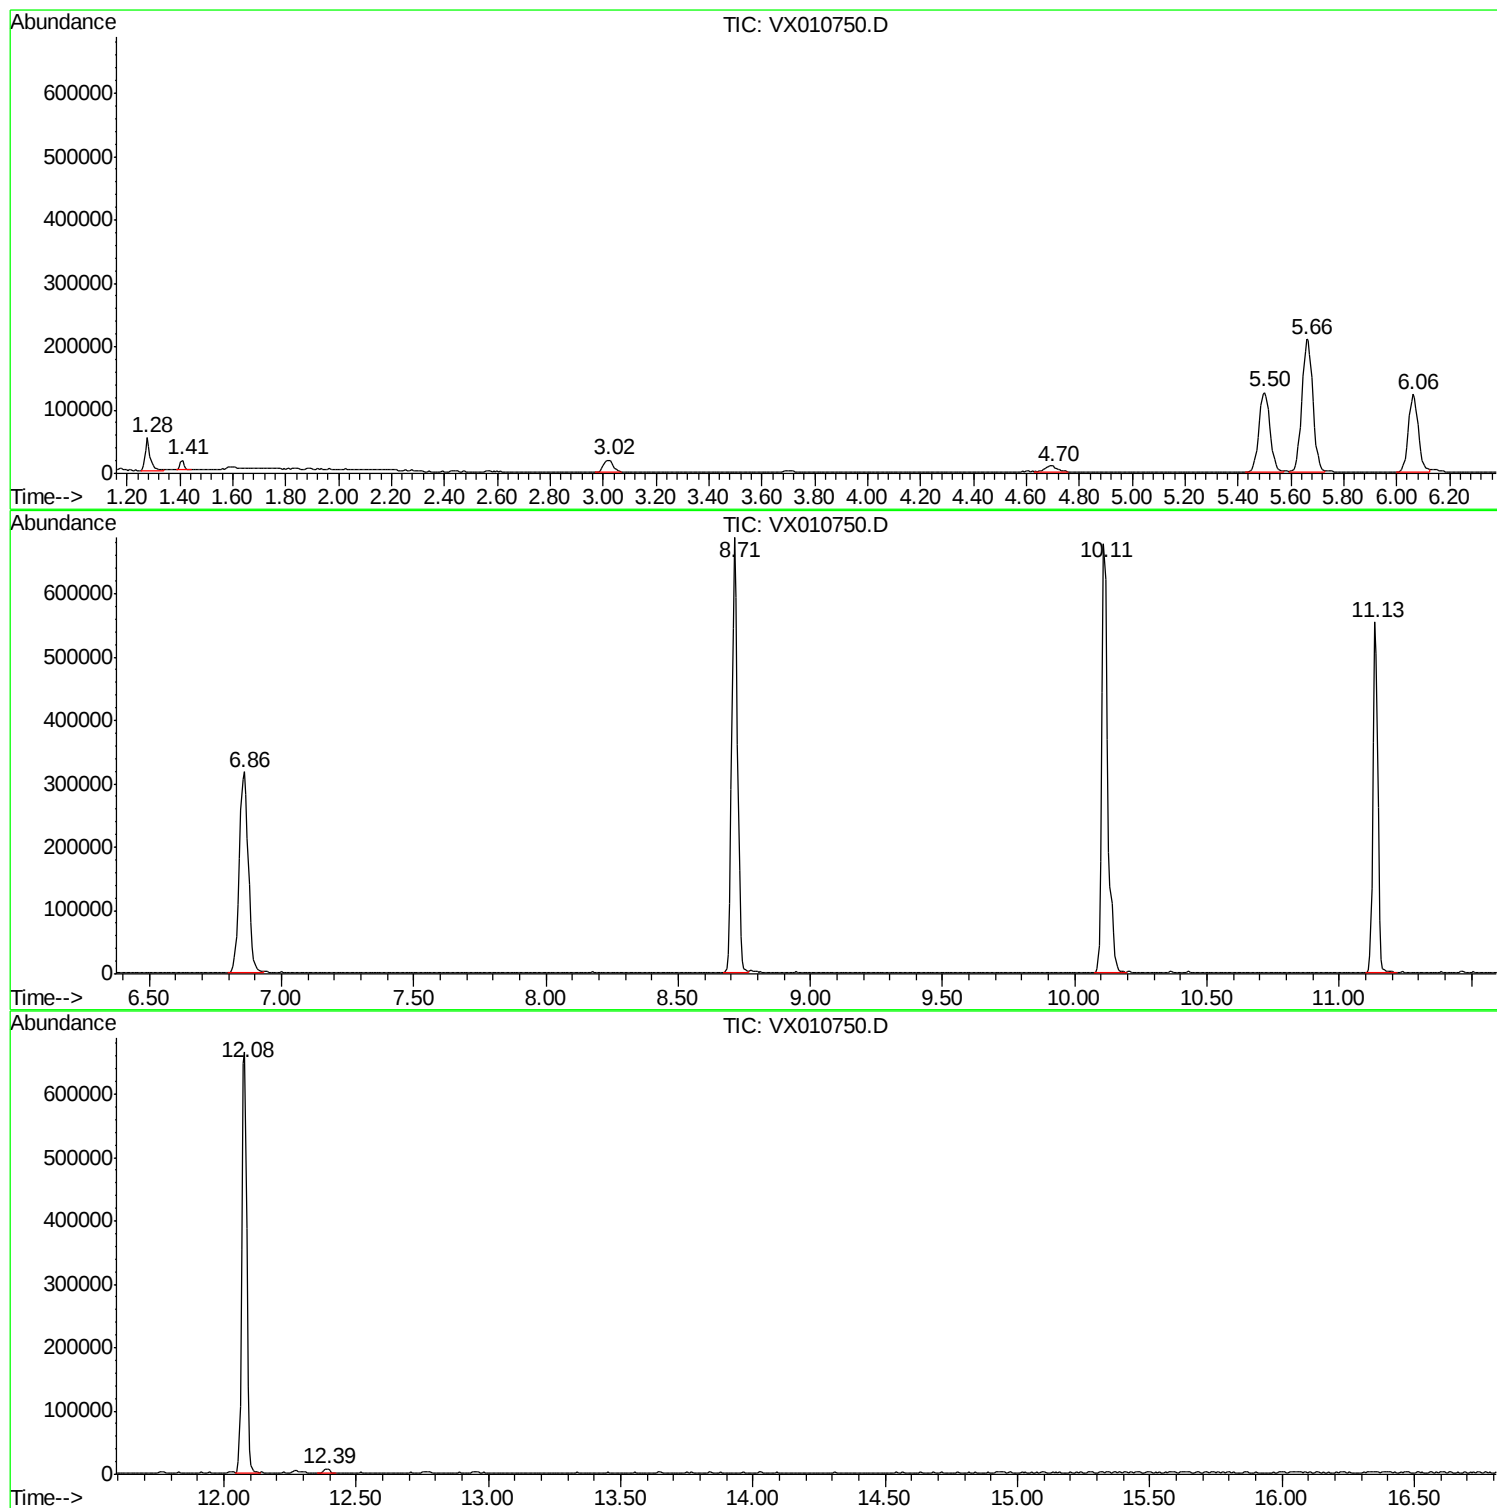

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070919\
Data File : VX010750.D
Acq On : 09 Jul 2019 15:01
Operator : JC/SP
Sample : K3691-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-0535-190704










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.28	5.74 ug/l	67789	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Sulfur dioxide	64	O2S	007446-09-5	90
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

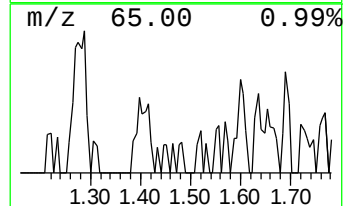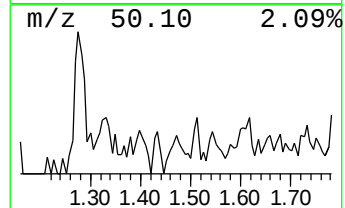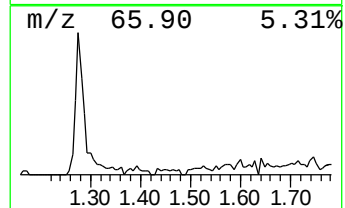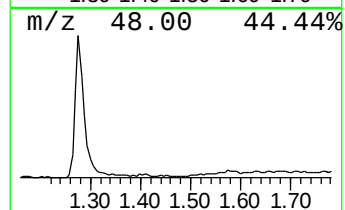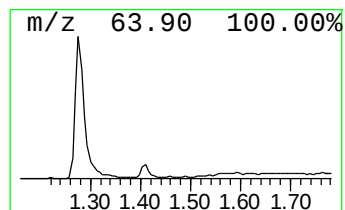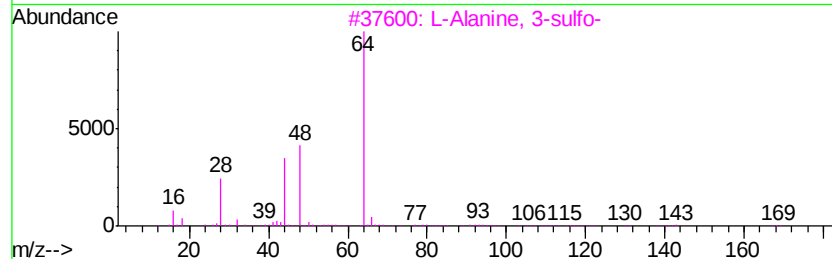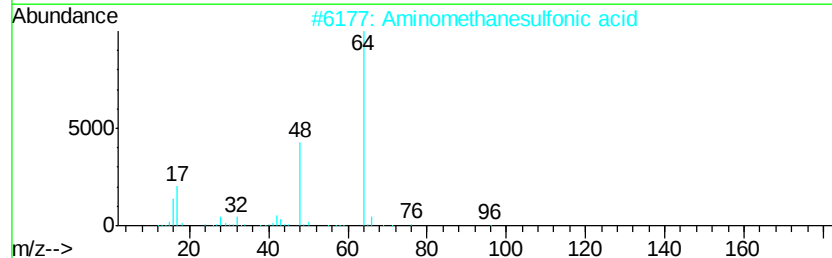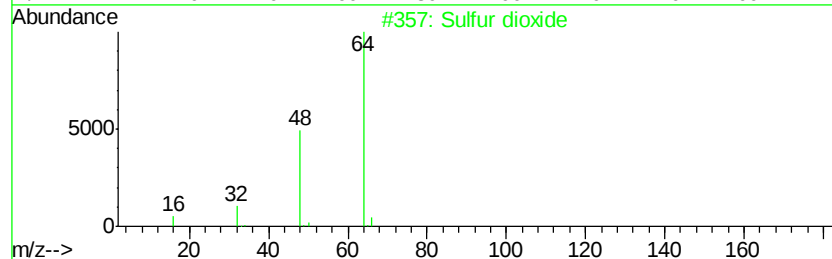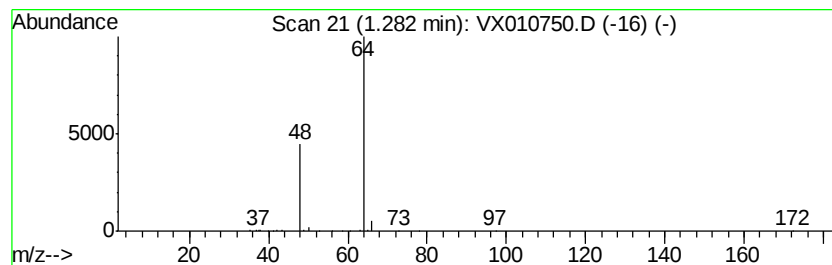

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX070919\
Data File : VX010750.D
Acq On : 09 Jul 2019 15:01
Operator : JC/SP
Sample : K3691-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-0535-190704

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.28	5.7	ug/l	67789	1	5.67	590035	50.0