

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX070920\
 Data File : VX017318.D
 Acq On : 09 Jul 2020 19:13
 Operator : JC/SP
 Sample : L3217-12 20X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E3-41-COMP-1-FLOOR

Quant Time: Jul 10 07:06:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 29 17:10:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	246102	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	402723	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	430956	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	233540	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	153561	50.61	ug/l	0.00
Spiked Amount			Recovery	=	101.22%	
35) Dibromofluoromethane	5.46	113	132213	51.90	ug/l	0.00
Spiked Amount			Recovery	=	103.80%	
50) Toluene-d8	8.70	98	494552	52.50	ug/l	0.00
Spiked Amount			Recovery	=	105.00%	
62) 4-Bromofluorobenzene	11.12	95	217741	59.13	ug/l	0.00
Spiked Amount			Recovery	=	118.26%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.31	50	624	0.217	ug/l	100
5) Bromomethane	1.62	94	413	0.292	ug/l	90
8) Diethyl Ether	2.14	74	206	0.519	ug/l	69
10) Methyl Iodide	2.49	142	1157	0.378	ug/l #	95
11) Tert butyl alcohol	3.00	59	227	0.392	ug/l #	73
13) Acrolein	2.29	56	424	1.225	ug/l #	1
15) Acrylonitrile	3.11	53	433	0.311	ug/l #	69
16) Acetone	2.43	43	2993	2.637	ug/l #	86
18) Methyl Acetate	2.75	43	870	0.294	ug/l #	77
20) Methylene Chloride	2.83	84	5743	1.446	ug/l #	93
25) 2-Butanone	4.66	43	785	0.415	ug/l #	49
29) Tetrahydrofuran	5.11	42	454	0.363	ug/l #	45
36) 1,1-Dichloropropene	5.62	75	17424	4.578	ug/l #	50
38) Carbon Tetrachloride	5.64	117	24753	5.904	ug/l #	18
43) Isopropyl Acetate	6.42	43	3374	0.526	ug/l	93
44) Trichloroethene	7.18	130	148	Below Cal		11
49) 1,4-Dioxane	7.79	88	24	0.347	ug/l #	6
51) 4-Methyl-2-Pentanone	8.60	43	3286	0.859	ug/l #	47
59) 2-Hexanone	9.52	43	990	0.354	ug/l	73
76) 1,2,3-Trichloropropane	11.12	75	106772	23.250	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	106772	60.208	ug/l #	13
88) 1,4-Dichlorobenzene	12.01	146	763	Below Cal		85
94) Hexachlorobutadiene	13.76	225	354	1.032	ug/l	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070920\
Data File : VX017318.D
Acq On : 09 Jul 2020 19:13
Operator : JC/SP
Sample : L3217-12 20X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E3-41-COMP-1-FLOOR

Quant Time: Jul 10 07:06:56 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 29 17:10:38 2020
Response via : Initial Calibration

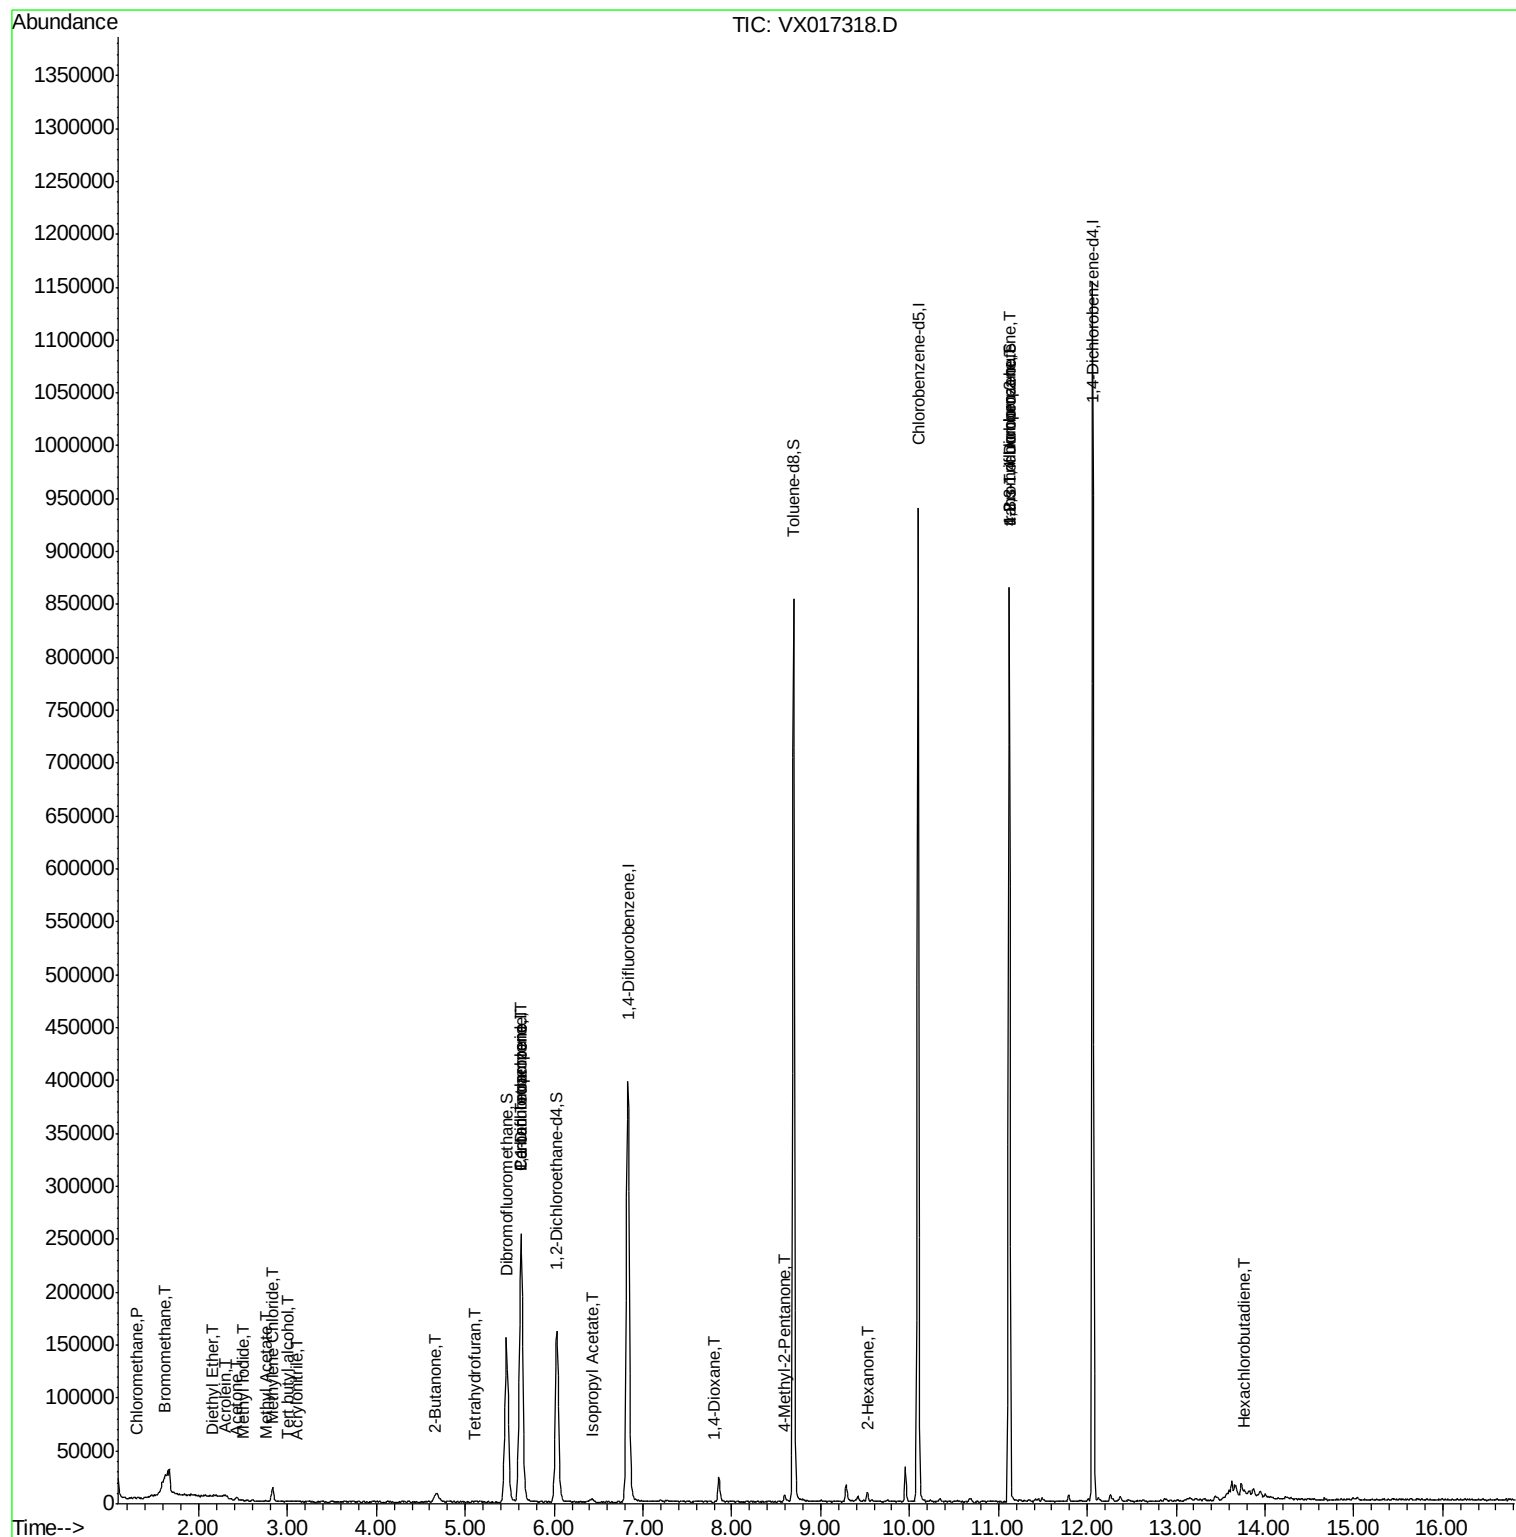



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :


E3-41-COMP-1-FLOOR

Tot Ion:168 Resp: 246102

Ion Ratio Lower Upper

168 100

99 52.8 42.6 64.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

80000



60000

40000

20000

0

Time-->



#3

Chloromethane

Concen: 0.217 ug/l

RT: 1.31 min Scan# 37

Delta R.T. -0.00 min

Lab File: VX017318.D


Acq: 09 Jul 2020 19:13

Tgt Ion: 50 Resp: 624

Ion Ratio Lower Upper

50 100

52 32.7 26.1 39.1



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.31

500

400


300


200

100

0

Time-->





#5

Bromomethane

Concen: 0.292 ug/l

RT: 1.62 min Scan# 88

Delta R.T. 0.00 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :


E3-41-COMP-1-FLOOR

Tot Ion: 94 Resp: 413

Ion Ratio Lower Upper

94 100

96 84.1 75.0 112.4




Abundance Ion 93.90 (93.60 to 94.60): VX0


Ion 95.90 (95.60 to 96.60): VX0

1.62

Time-->



Time-->



#8

Diethyl Ether

Concen: 0.519 ug/l

RT: 2.14 min Scan# 173

Delta R.T. -0.02 min

Lab File: VX017318.D


Acq: 09 Jul 2020 19:13

Tgt Ion: 74 Resp: 206

Ion Ratio Lower Upper

74 100

45 68.9 49.8 149.3




Abundance Ion 74.00 (73.70 to 74.70): VX0


Ion 45.00 (44.70 to 45.70): VX0

2.14

Time-->




Time-->






#10
Methyl Iodide
Concen: 0.378 ug/l
RT: 2.49 min Scan# 230
Delta R.T. -0.00 min
Lab File: VX017318.D
Acq: 09 Jul 2020 19:13

Instrument :
MSVOA_X
ClientSampleId :
E3-41-COMP-1-FLOOR

Tot Ion:142 Resp: 1157
Ion Ratio Lower Upper
142 100
127 46.5 36.6 54.8
141 7.7 11.6 17.4#

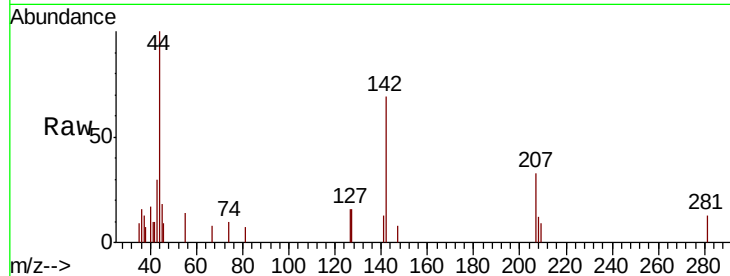


Abundance Ion 141.80 (141.50 to 142.50): V
Ion 126.80 (126.50 to 127.50): V
Ion 140.80 (140.50 to 141.50): V


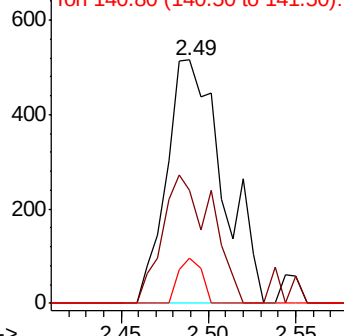



#11
Tert butyl alcohol
Concen: 0.392 ug/l
RT: 3.00 min Scan# 313
Delta R.T. -0.02 min
Lab File: VX017318.D
Acq: 09 Jul 2020 19:13

Tgt Ion: 59 Resp: 227
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#



Abundance Ion 59.00 (58.70 to 59.70): VX0
Ion 57.00 (56.70 to 57.70): VX0

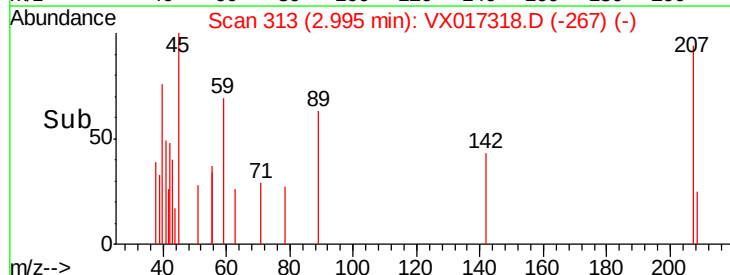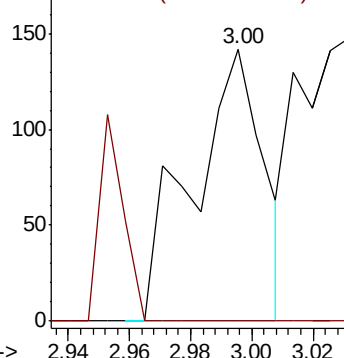



#13

Acrolein

Concen: 1.225 ug/l

RT: 2.29 min Scan# 197

Delta R.T. 0.02 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :


E3-41-COMP-1-FLOOR

Tot Ion: 56 Resp: 424

Ion Ratio Lower Upper




56 100

55 185.8 55.7 83.5#

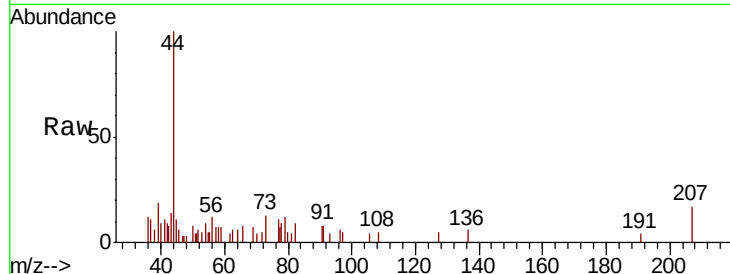

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

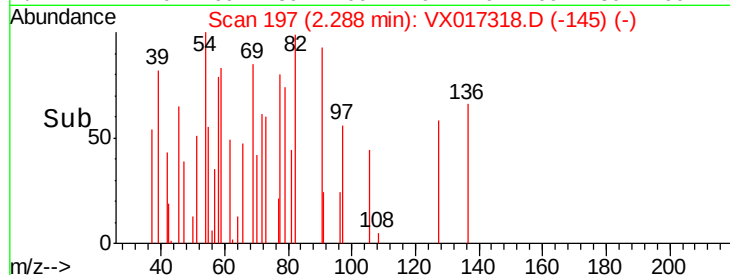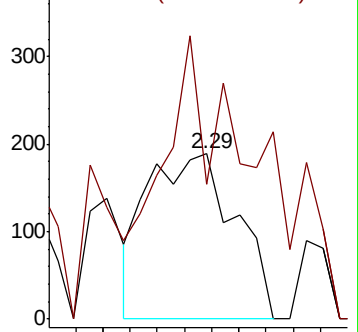

#15

Acrylonitrile

Concen: 0.311 ug/l

RT: 3.11 min Scan# 331

Delta R.T. -0.01 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13


Tgt Ion: 53 Resp: 433

Ion Ratio Lower Upper

53 100

52 65.1 65.6 98.4#



51 0.0 28.3 42.5#

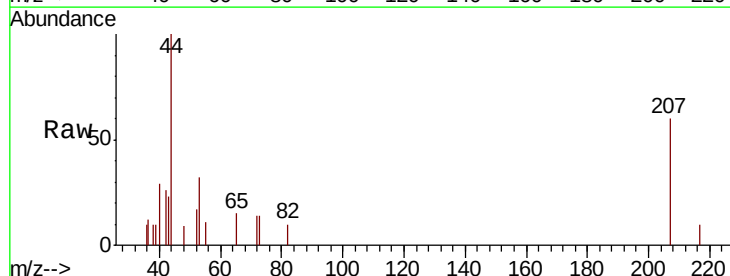


Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

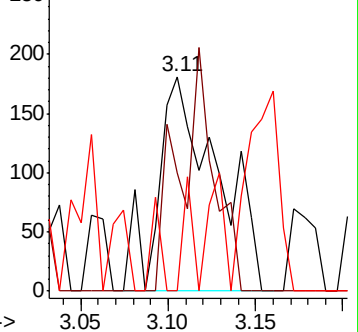



#16

Acetone

Concen: 2.637 ug/l

RT: 2.43 min Scan# 220

Delta R.T. 0.01 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :


E3-41-COMP-1-FLOOR

Tot Ion: 43 Resp: 2993

Ion Ratio Lower Upper




43 100

58 24.1 25.7 38.5#

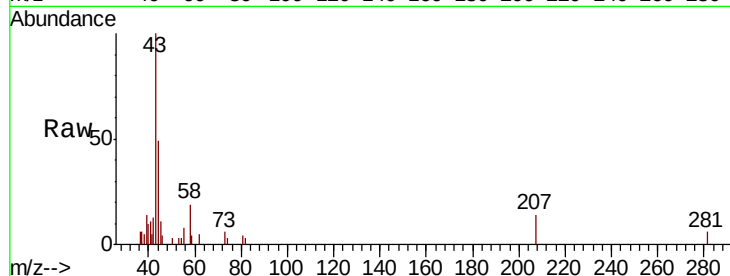

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

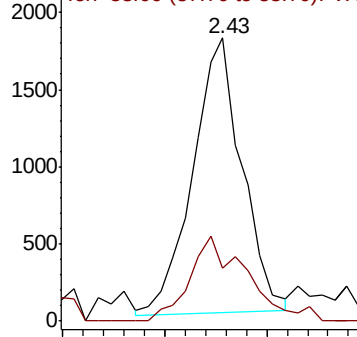

#18

Methyl Acetate

Concen: 0.294 ug/l

RT: 2.75 min Scan# 273

Delta R.T. 0.01 min

Lab File: VX017318.D


Acq: 09 Jul 2020 19:13

Tgt Ion: 43 Resp: 870

Ion Ratio Lower Upper



43 100


74 12.9 19.3 28.9#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0




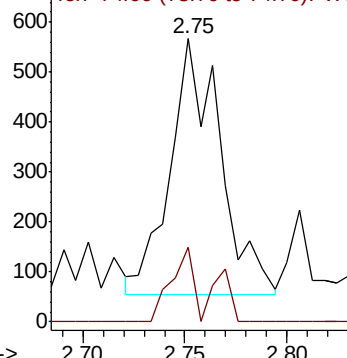


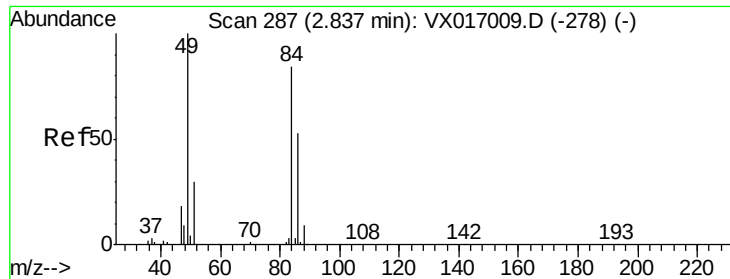

#20
Methylene Chloride
Concen: 1.446 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.01 min
Lab File: VX017318.D
Acq: 09 Jul 2020 19:13




Instrument :
MSVOA_X
ClientSampleId :
E3-41-COMP-1-FLOOR


Tot Ion: 84 Resp: 5743
Ion Ratio Lower Upper
84 100
49 119.4 94.7 142.1
51 42.7 28.6 42.8
86 76.5 50.5 75.7#

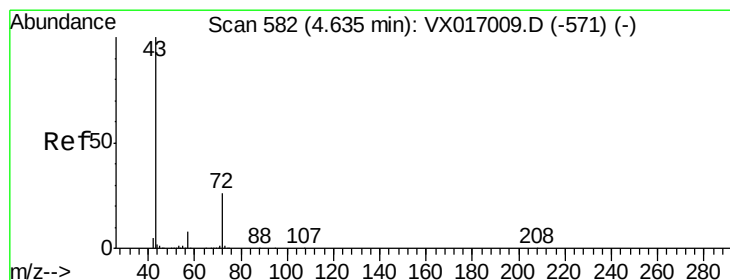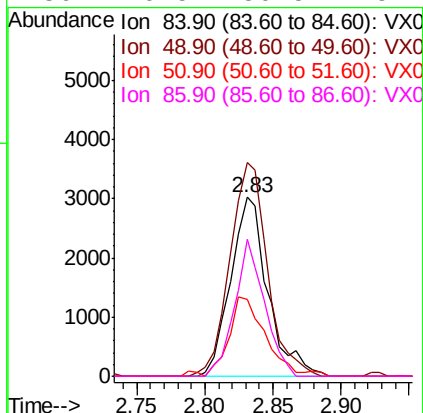

#25
2-Butanone
Concen: 0.415 ug/l
RT: 4.66 min Scan# 586
Delta R.T. 0.02 min
Lab File: VX017318.D
Acq: 09 Jul 2020 19:13

Tgt Ion: 43 Resp: 785
Ion Ratio Lower Upper
43 100
72 0.0 20.8 31.2#

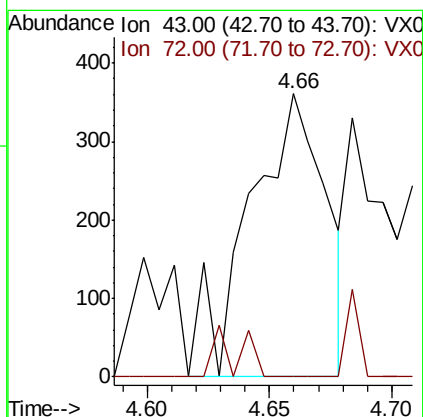

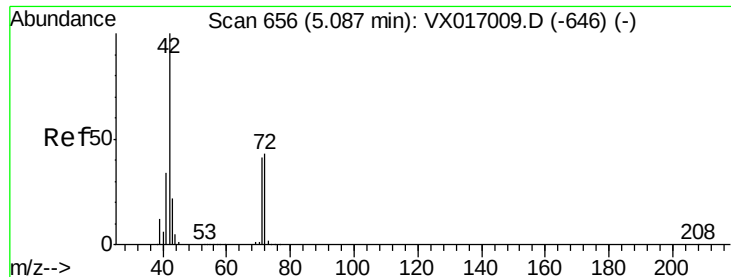

#29

Tetrahydrofuran

Concen: 0.363 ug/l

RT: 5.11 min Scan# 660

Delta R.T. 0.02 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :

E3-41-COMP-1-FLOOR


Tot Ion: 42 Resp: 454

Ion Ratio Lower Upper




42 100

72 14.5 35.3 52.9#

71 0.0 33.1 49.7#

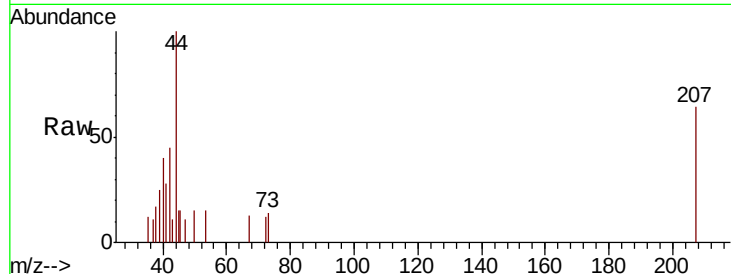

Abundance Ion 42.00 (41.70 to 42.70): VX0
Ion 72.00 (71.70 to 72.70): VX0
Ion 71.00 (70.70 to 71.70): VX0

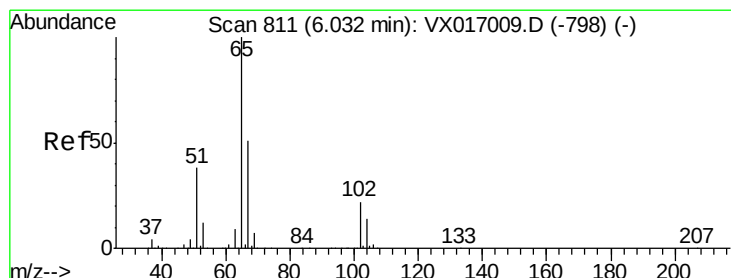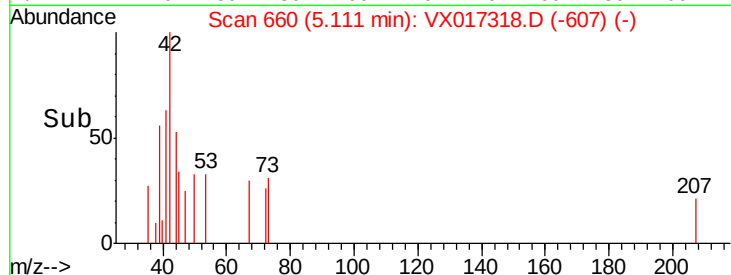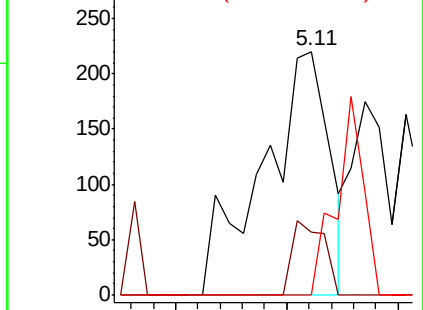

#33

1,2-Dichloroethane-d4

Concen: 50.614 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX017318.D


Acq: 09 Jul 2020 19:13

Tgt Ion: 65 Resp: 153561



Ion Ratio Lower Upper


65 100

67 52.9 0.0 103.8

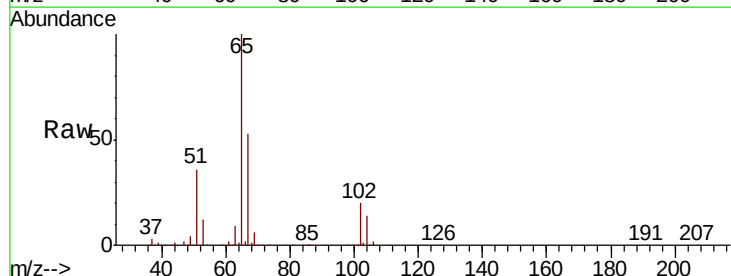

Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0

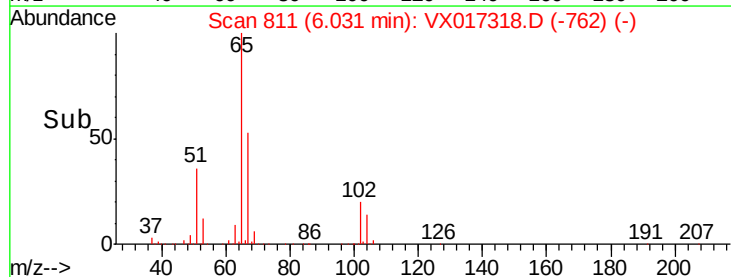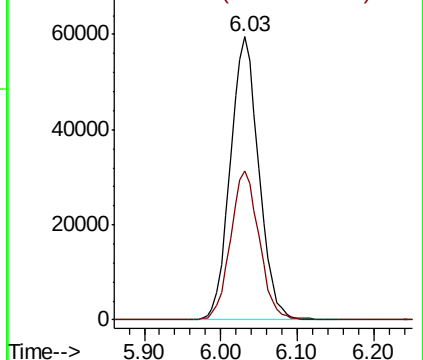



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :

E3-41-COMP-1-FLOOR


Tot Ion:114 Resp: 402723

Ion Ratio Lower Upper

114 100

63 20.4 0.0 41.4




88 16.4 0.0 32.4

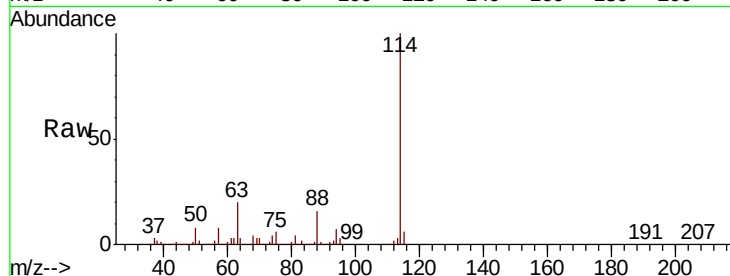

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

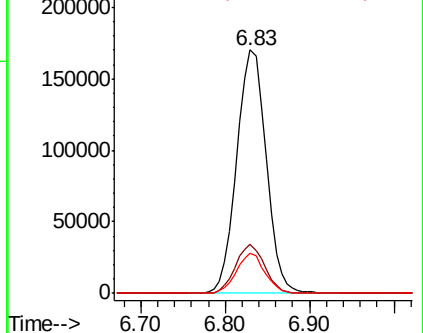

#35

Dibromofluoromethane

Concen: 51.899 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13


Tgt Ion:113 Resp: 132213

Ion Ratio Lower Upper

113 100

111 103.3 81.9 122.9



192 21.5 16.7 25.1




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

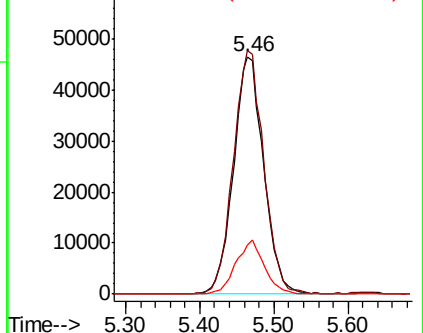


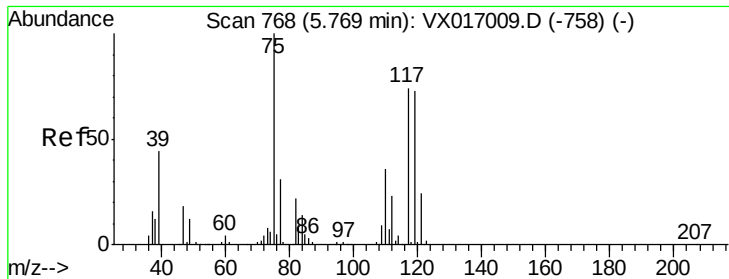




#36
 1,1-Dichloropropene
 Concen: 4.578 ug/l
 RT: 5.62 min Scan# 744
 Delta R.T. -0.15 min
 Lab File: VX017318.D
 Acq: 09 Jul 2020 19:13

Instrument :
 MSVOA_X
 ClientSampleId :
 E3-41-COMP-1-FLOOR

Tot Ion	Ratio	Lower	Upper
75	100		
110	9.1	18.1	54.1#
77	0.2	24.6	37.0#

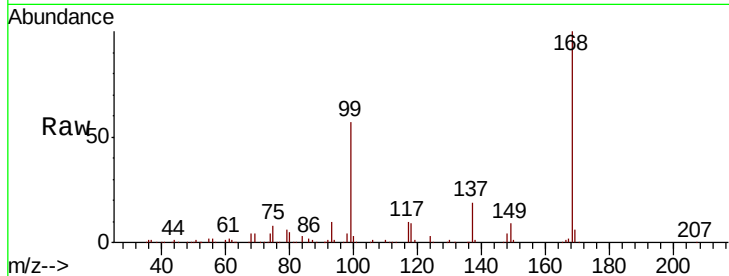


Abundance Ion 74.90 (74.60 to 75.60): VX0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VX0

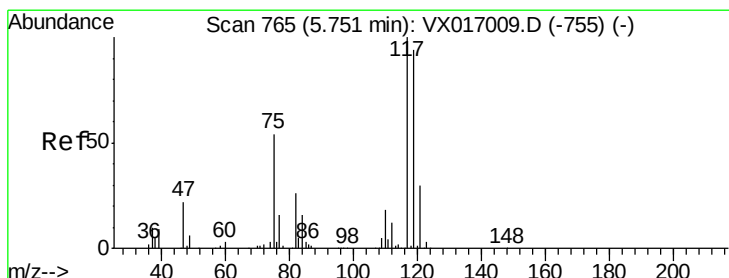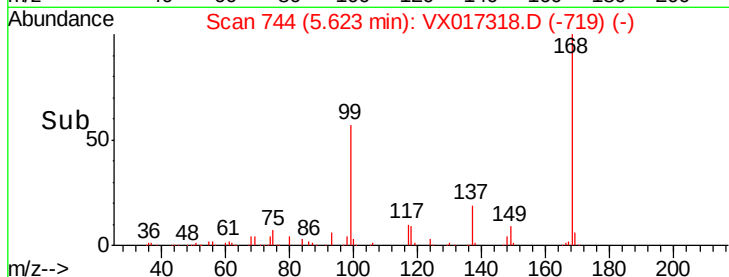
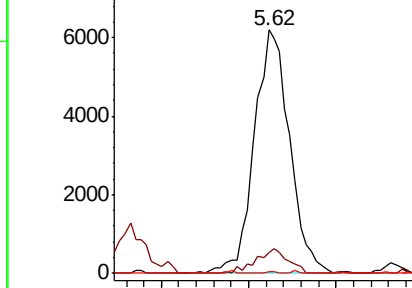



#38
 Carbon Tetrachloride
 Concen: 5.904 ug/l
 RT: 5.64 min Scan# 746
 Delta R.T. -0.12 min
 Lab File: VX017318.D
 Acq: 09 Jul 2020 19:13

Tgt Ion	Ratio	Lower	Upper
117	100		
119	6.6	75.4	113.0#
121	0.0	23.8	35.6#

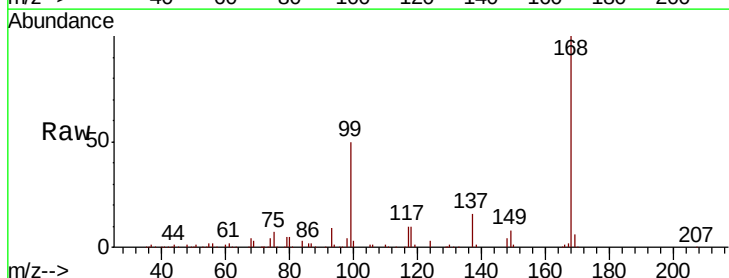

Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V

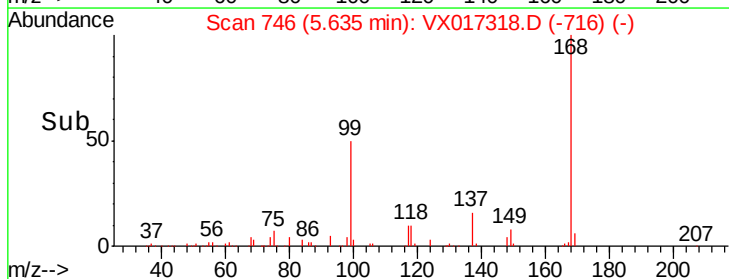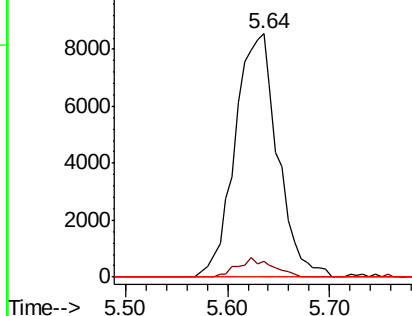



#43

Isopropyl Acetate

Concen: 0.526 ug/l

RT: 6.42 min Scan# 875

Delta R.T. 0.01 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :

E3-41-COMP-1-FLOOR


Tot Ion: 43 Resp: 3374

Ion Ratio Lower Upper




43 100

61 16.5 16.2 24.2

87 11.7 10.7 16.1

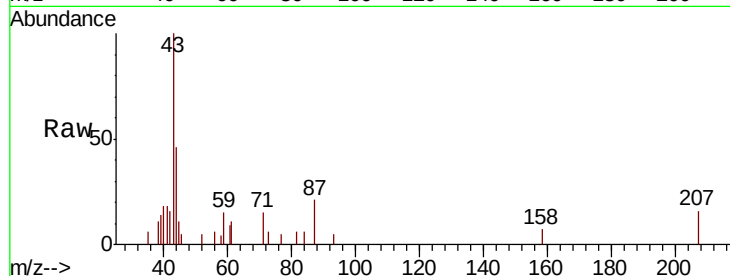

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0

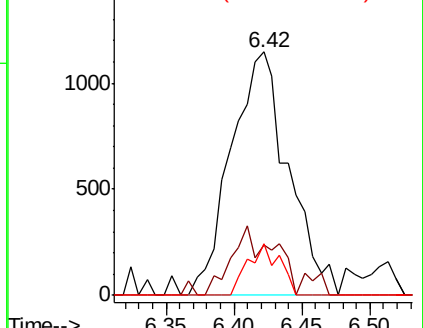

#44

Trichloroethene

Concen: Below Cal

RT: 7.18 min Scan# 999

Delta R.T. -0.01 min

Lab File: VX017318.D


Acq: 09 Jul 2020 19:13

Tgt Ion: 130 Resp: 148



Ion Ratio Lower Upper


130 100

95 7.6 0.0 185.0



Abundance Ion 129.80 (129.50 to 130.50): V
Ion 94.90 (94.60 to 95.60): VX0

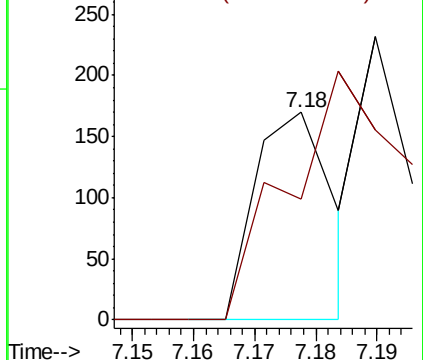


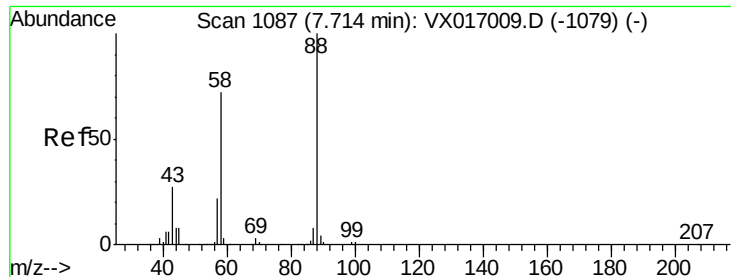




#49
1,4-Dioxane
Concen: 0.347 ug/l
RT: 7.79 min Scan# 1099
Delta R.T. 0.07 min
Lab File: VX017318.D
Acq: 09 Jul 2020 19:13

Instrument :
MSVOA_X
ClientSampleId :
E3-41-COMP-1-FLOOR

Tot Ion: 88 Resp: 24
Ion Ratio Lower Upper
88 100
43 0.0 25.8 38.8#
58 158.3 54.8 82.2#

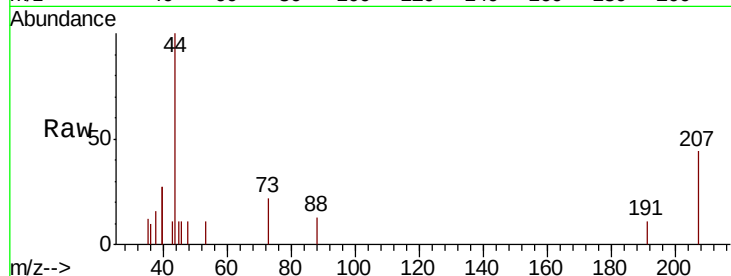


Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0

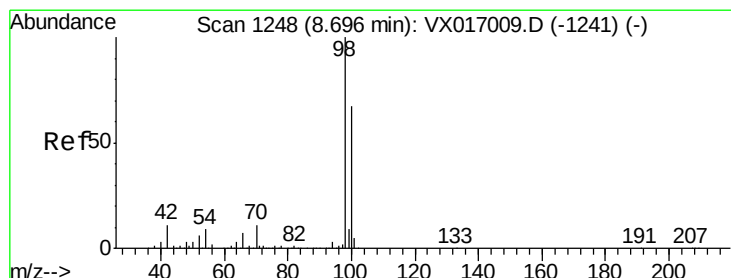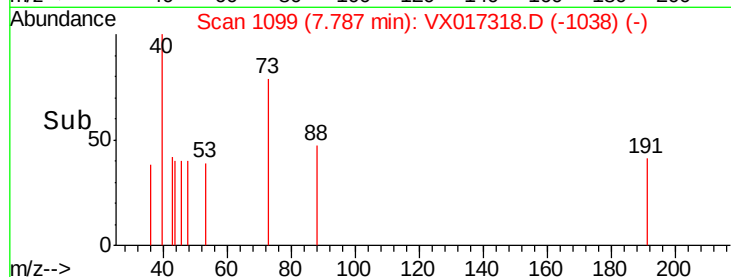
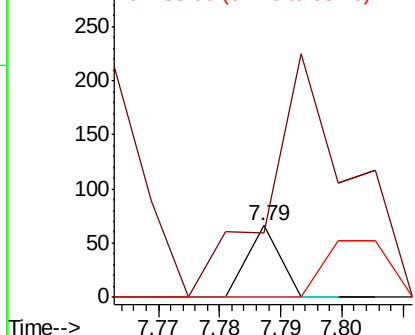



#50
Toluene-d8
Concen: 52.499 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX017318.D
Acq: 09 Jul 2020 19:13

Tgt Ion: 98 Resp: 494552
Ion Ratio Lower Upper
98 100
100 65.8 53.8 80.6

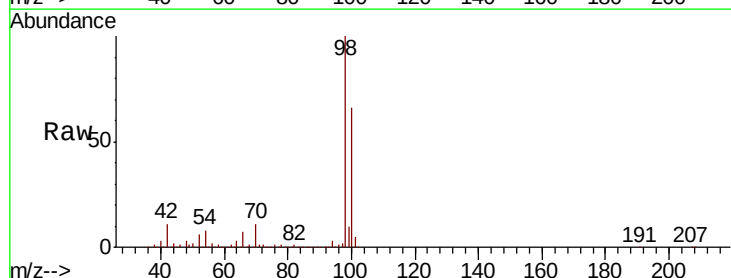

Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): V

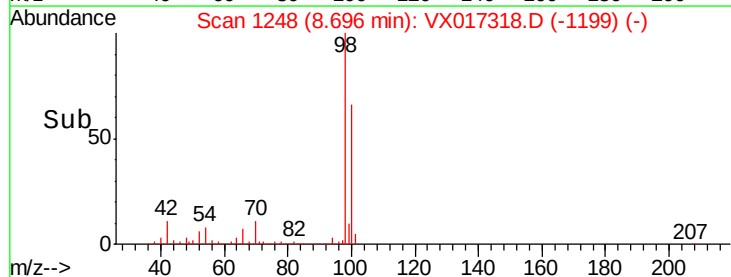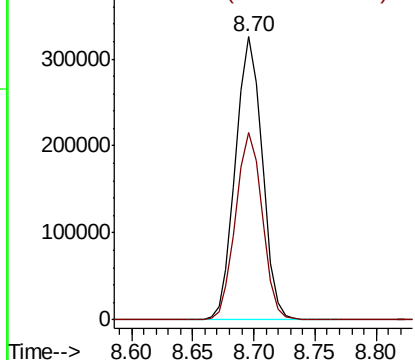



#51

4-Methyl-2-Pentanone

Concen: 0.859 ug/l

RT: 8.60 min Scan# 1232

Delta R.T. -0.02 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :


E3-41-COMP-1-FLOOR

Tot Ion: 43 Resp: 3286

Ion Ratio Lower Upper




43 100

58 7.0 31.9 47.9#

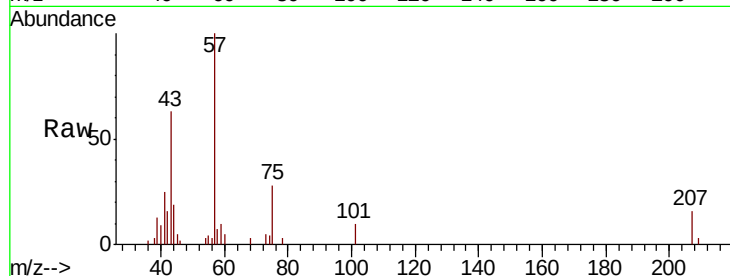

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

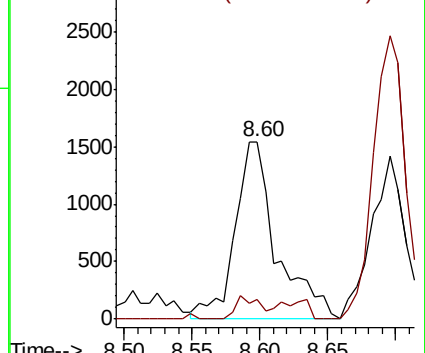

#59

2-Hexanone

Concen: 0.354 ug/l

RT: 9.52 min Scan# 1383

Delta R.T. 0.05 min

Lab File: VX017318.D


Acq: 09 Jul 2020 19:13

Tgt Ion: 43 Resp: 990

Ion Ratio Lower Upper



43 100


58 36.0 27.9 83.6



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

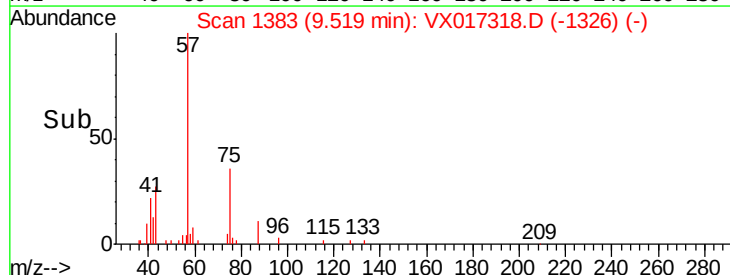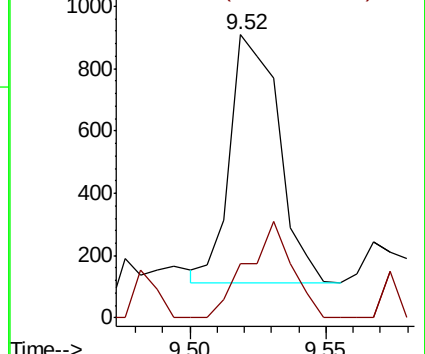

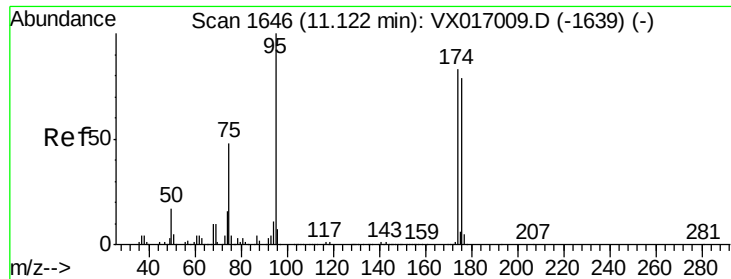

#62

4-Bromofluorobenzene

Concen: 59.129 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :

E3-41-COMP-1-FLOOR


Tot Ion: 95 Resp: 217741

Ion Ratio Lower Upper

95 100

174 85.6 0.0 164.0




176 81.4 0.0 157.6

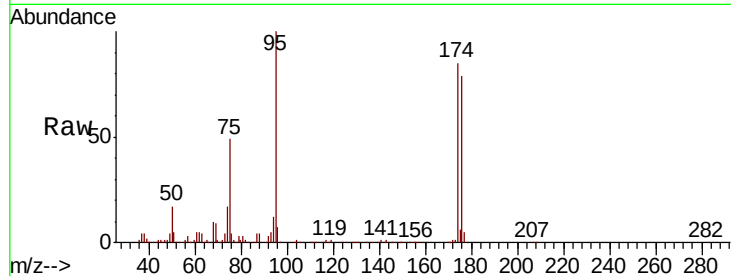

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): VX0

Ion 175.80 (175.50 to 176.50): VX0

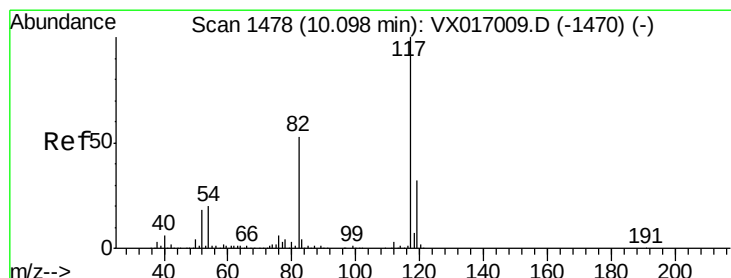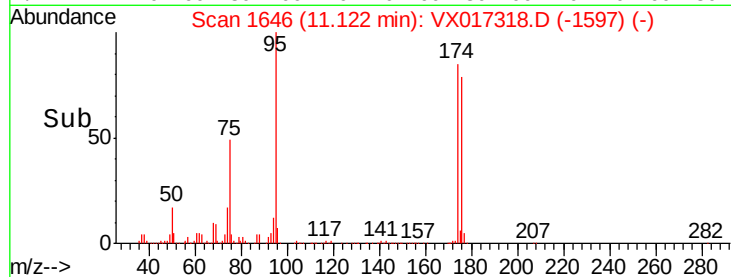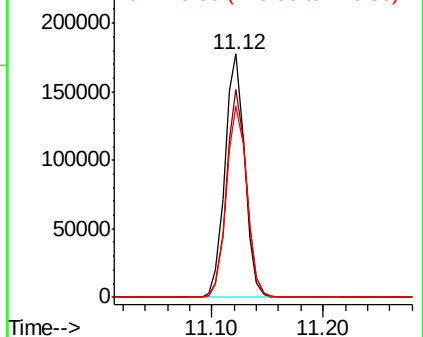

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13


Tgt Ion: 117 Resp: 430956

Ion Ratio Lower Upper

117 100

82 52.4 42.6 63.8



119 32.8 25.4 38.2

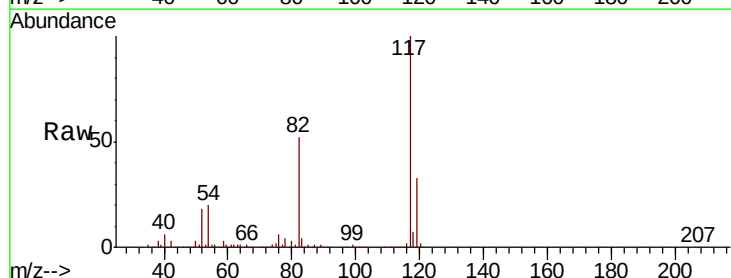


Abundance Ion 116.90 (116.60 to 117.60): VX0

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): VX0

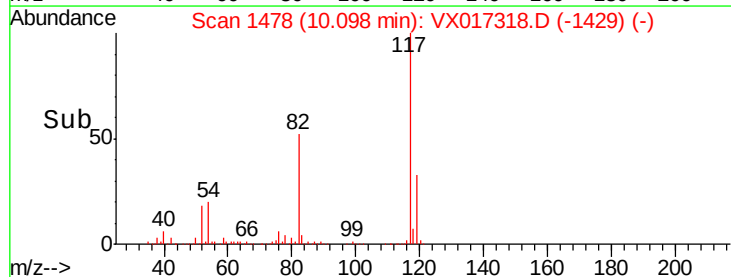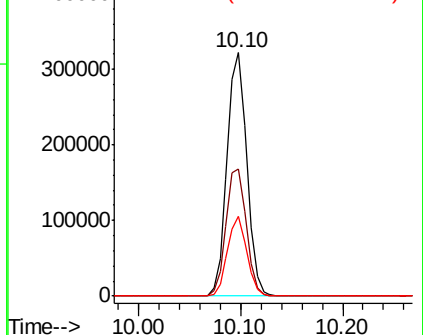



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :

E3-41-COMP-1-FLOOR


Tot Ion:152 Resp: 233540

Ion Ratio Lower Upper

152 100

115 57.9 40.9 122.7




150 156.4 0.0 351.6

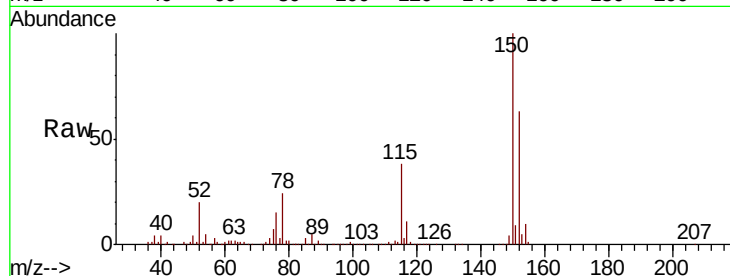

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

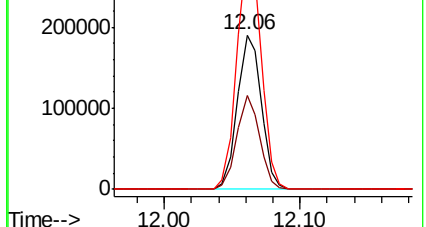

#76

1,2,3-Trichloropropane

Concen: 23.250 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017318.D


Acq: 09 Jul 2020 19:13

Tgt Ion: 75 Resp: 106772

Ion Ratio Lower Upper



75 100


77 1.4 20.2 60.6#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

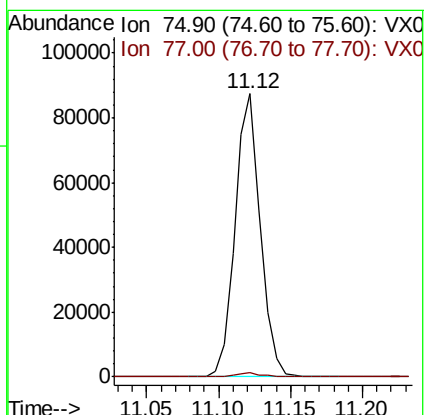

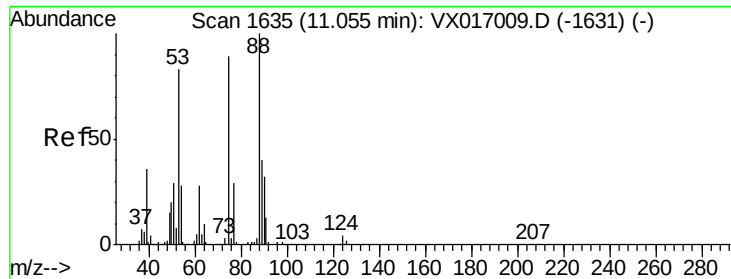

#81

trans-1,4-Dichloro-2-butene

Concen: 60.208 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13

Instrument :

MSVOA_X

ClientSampleId :

E3-41-COMP-1-FLOOR


Tot Ion: 75 Resp: 106772

Ion Ratio Lower Upper

75 100

53 0.1 72.4 108.6#

89 0.0 37.0 55.4#



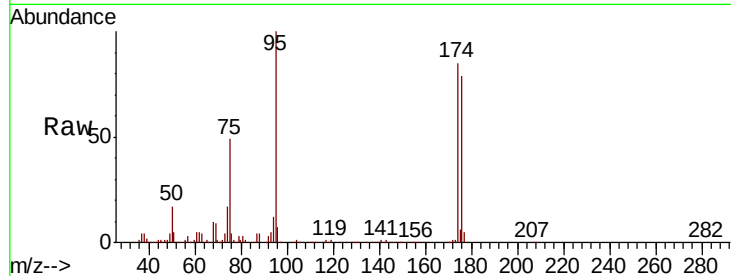


Abundance

Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

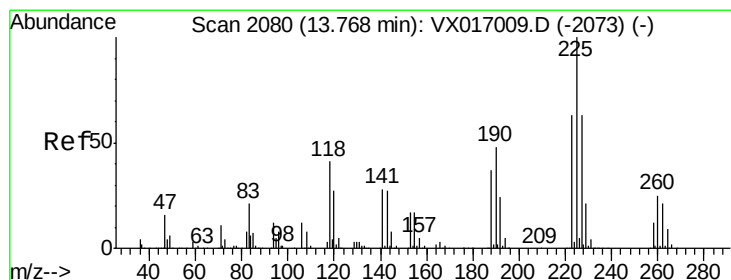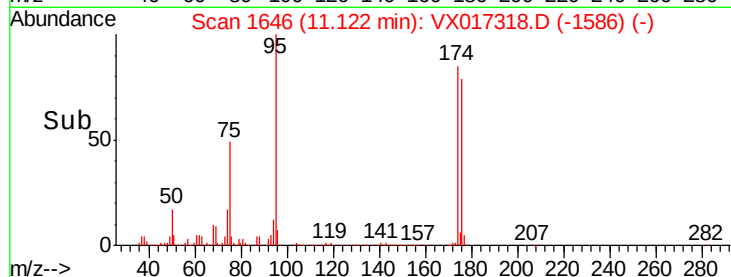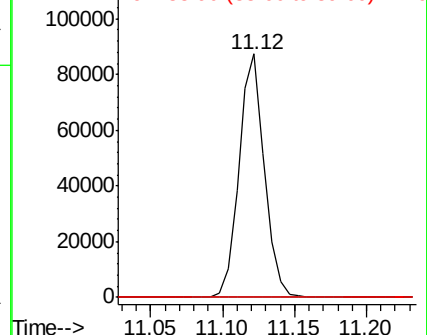

#94

Hexachlorobutadiene

Concen: 1.032 ug/l

RT: 13.76 min Scan# 2079

Delta R.T. -0.01 min

Lab File: VX017318.D

Acq: 09 Jul 2020 19:13


Tgt Ion: 225 Resp: 354

Ion Ratio Lower Upper

225 100

223 35.9 32.5 97.5

227 58.8 33.1 99.2

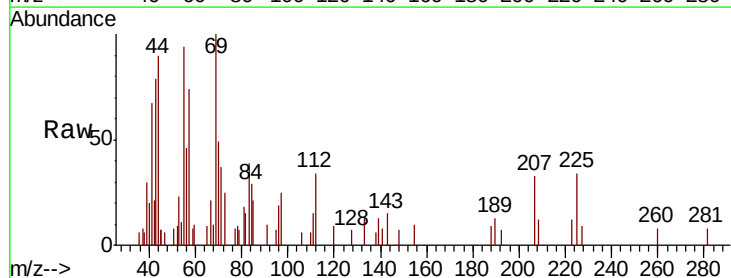

Abundance

Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

