
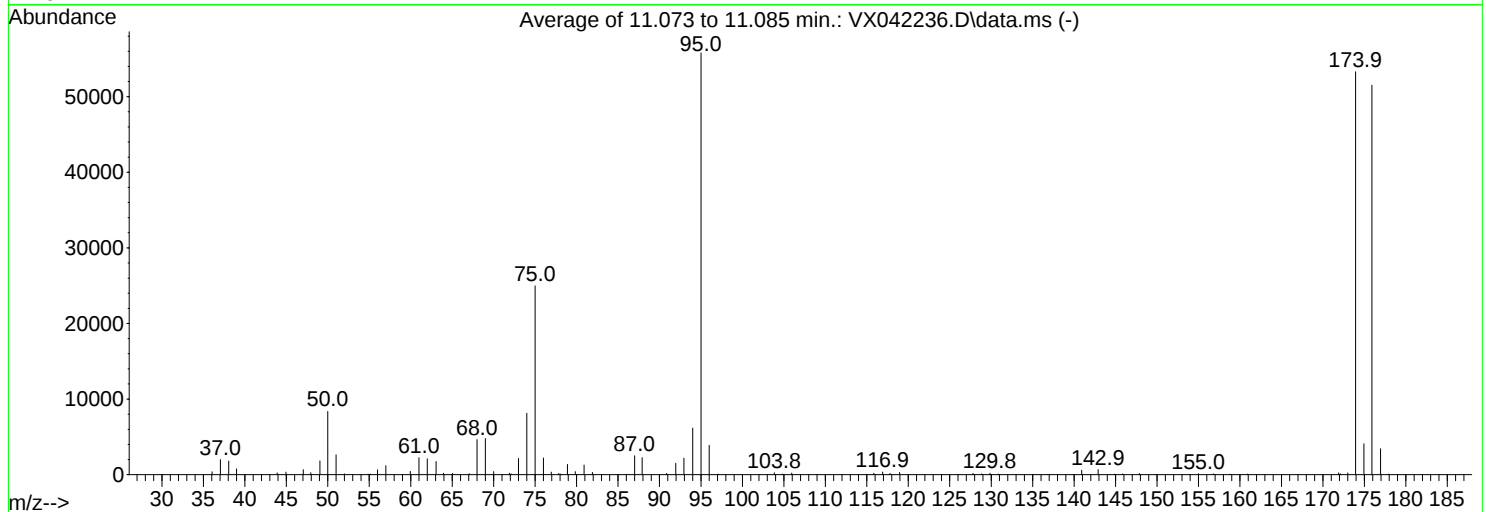


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070924\
Data File : VX042236.D
Acq On : 09 Jul 2024 09:12
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Jun 15 04:02:59 2024

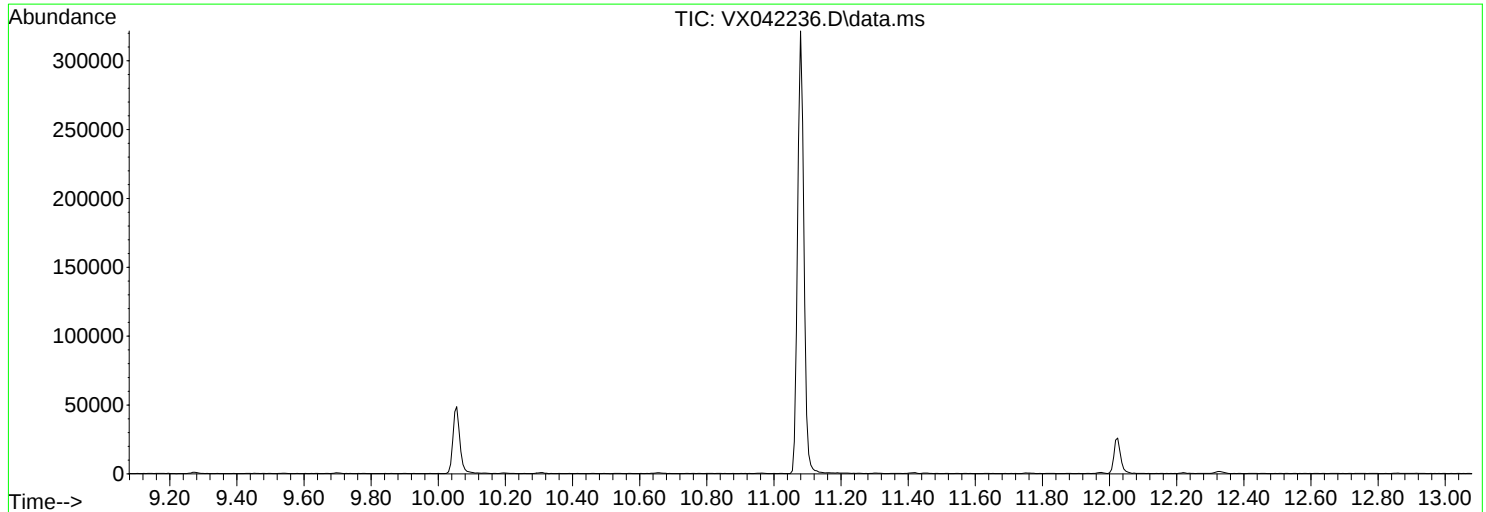

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	8369	FAIL*
75	95	30	60	44.8	24981	PASS
95	95	100	100	100.0	55795	PASS
96	95	5	9	6.9	3864	PASS
173	174	0.00	2	0.4	224	PASS
174	95	50	100	95.5	53304	PASS
175	174	5	9	7.7	4094	PASS
176	174	95	101	96.6	51515	PASS
177	176	5	9	6.7	3430	PASS