
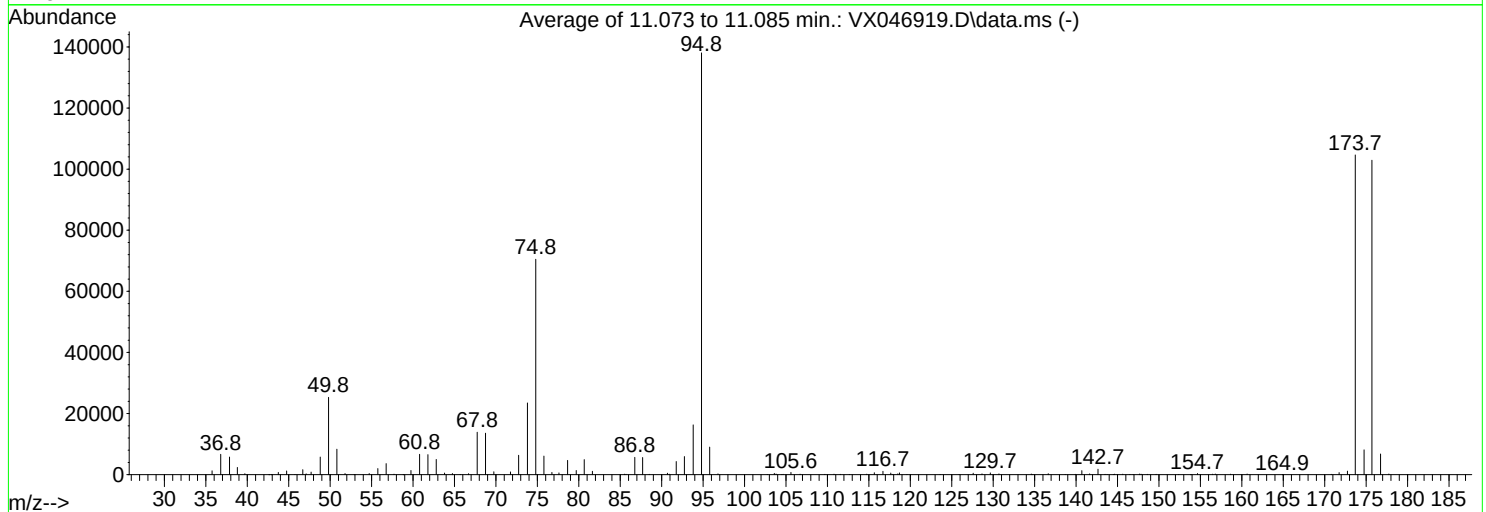


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070925\
Data File : VX046919.D
Acq On : 09 Jul 2025 08:53
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Title : SW846 8260
Last Update : Thu Jul 03 05:51:11 2025

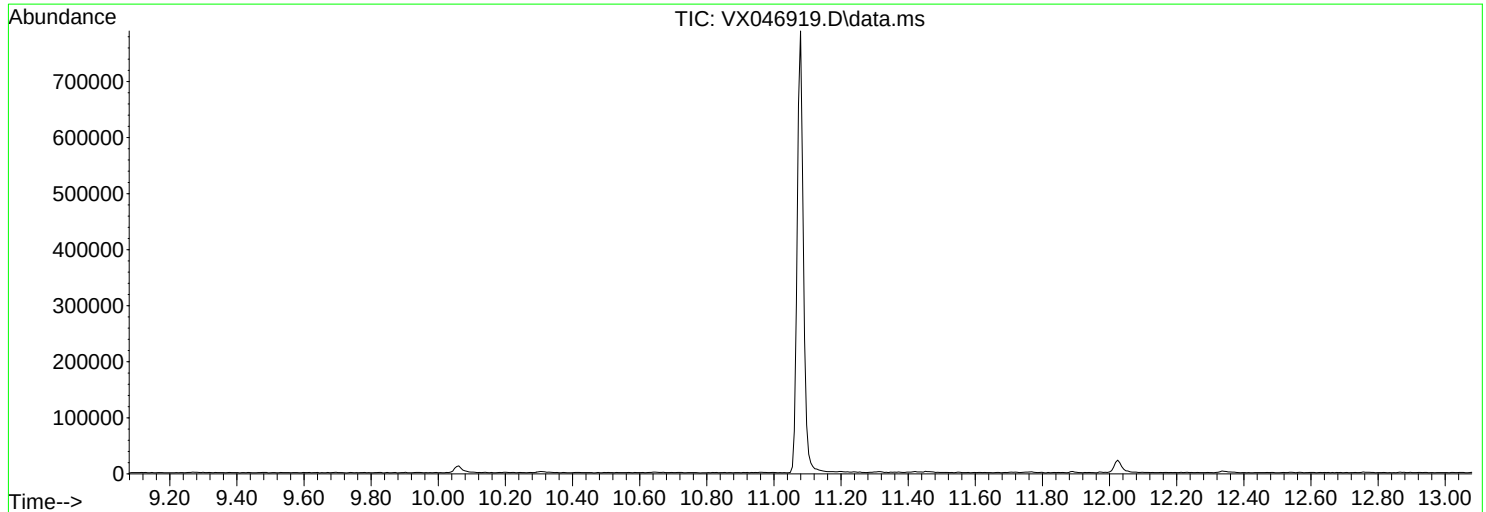

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	25299	PASS
75	95	30	60	51.1	70483	PASS
95	95	100	100	100.0	138061	PASS
96	95	5	9	6.5	9007	PASS
173	174	0.00	2	1.1	1174	PASS
174	95	50	100	75.8	104619	PASS
175	174	5	9	7.8	8124	PASS
176	174	95	101	98.4	102920	PASS
177	176	5	9	6.6	6747	PASS