


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX071018\
Data File : VX003301.D
Acq On : 10 Jul 2018 23:16
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X070918W.M
Title : SW846 8260
Last Update : Mon Jul 09 15:24:16 2018

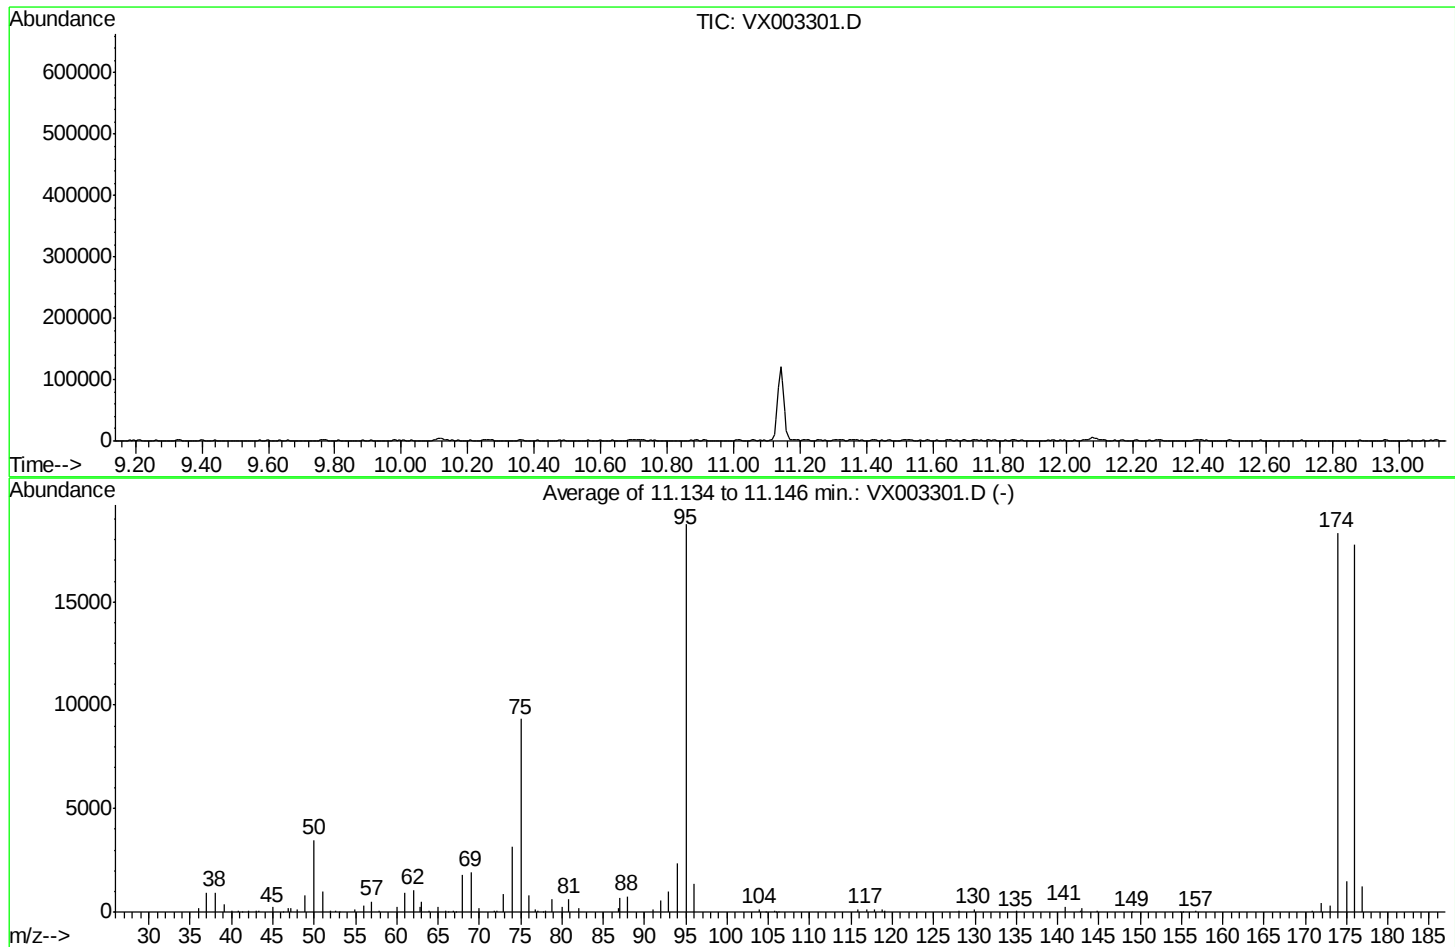

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	3491	PASS
75	95	30	60	49.7	9322	PASS
95	95	100	100	100.0	18749	PASS
96	95	5	9	7.2	1354	PASS
173	174	0.00	2	1.6	296	PASS
174	95	50	100	97.8	18345	PASS
175	174	5	9	8.1	1477	PASS
176	174	95	101	96.9	17780	PASS
177	176	5	9	7.0	1253	PASS