

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX071019\
 Data File : VX010773.D
 Acq On : 10 Jul 2019 13:39
 Operator : JC/SP
 Sample : K3636-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SP19-JMW0980

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.209	6	9	13	rVB	35461	34626	3.34%	0.497%
2	1.251	13	16	19	rVV	30774	29838	2.88%	0.428%
3	1.300	19	24	28	rVB3	18110	26797	2.58%	0.385%
4	1.392	35	39	45	rBV2	32082	39699	3.83%	0.570%
5	1.453	45	49	52	rBV	8992	11083	1.07%	0.159%
6	1.696	84	89	99	rVB	21747	34482	3.32%	0.495%
7	1.885	116	120	128	rVB	13794	19960	1.92%	0.286%
8	2.190	164	170	179	rVB	186698	279987	26.98%	4.019%
9	2.611	234	239	243	rVB	6095	10619	1.02%	0.152%
10	3.019	299	306	315	rVB2	7692	23021	2.22%	0.330%
11	3.708	412	419	425	rBV3	4378	11169	1.08%	0.160%
12	4.696	572	581	585	rBV3	4841	12326	1.19%	0.177%
13	5.501	702	713	723	rBV	127121	368610	35.52%	5.291%
14	5.665	730	740	757	rVB	211034	601509	57.96%	8.633%
15	6.061	796	805	813	rBV	121879	316733	30.52%	4.546%
16	6.141	813	818	826	rVB2	20410	53192	5.13%	0.763%
17	6.860	924	936	948	rBV	314393	750798	72.34%	10.776%
18	7.464	1028	1035	1041	rVB3	7247	16130	1.55%	0.232%
19	8.713	1234	1240	1248	rBV	670138	1037815	100.00%	14.895%
20	10.110	1461	1469	1478	rBV	673434	930439	89.65%	13.354%
21	10.359	1502	1510	1517	rVB	60564	88160	8.49%	1.265%
22	10.701	1562	1566	1572	rVB3	6595	11103	1.07%	0.159%
23	11.018	1612	1618	1625	rBV	18679	27112	2.61%	0.389%
24	11.134	1630	1637	1645	rBV	563241	722749	69.64%	10.373%
25	11.359	1667	1674	1680	rBV3	8091	11192	1.08%	0.161%
26	11.432	1680	1686	1688	rBV4	8775	14072	1.36%	0.202%
27	11.506	1695	1698	1707	rVB2	7367	11309	1.09%	0.162%
28	11.670	1719	1725	1733	rVB2	12307	18835	1.81%	0.270%
29	11.804	1742	1747	1757	rVB	22431	31494	3.03%	0.452%
30	11.945	1757	1770	1777	rVB4	12905	24025	2.31%	0.345%
31	12.079	1786	1792	1800	rBV	659200	942797	90.84%	13.532%
32	12.298	1821	1828	1835	rBV2	17606	25630	2.47%	0.368%
33	12.365	1835	1839	1848	rVB7	10845	23198	2.24%	0.333%
34	12.518	1858	1864	1869	rVB	7210	10714	1.03%	0.154%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX071019\
Data File : VX010773.D
Acq On : 10 Jul 2019 13:39
Operator : JC/SP
Sample : K3636-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP19-JMW0980

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260

35	12.957	1931	1936	1943	rBV7	6274	15504	1.49%	0.223%
36	13.078	1952	1956	1962	rVB5	9453	15002	1.45%	0.215%
37	13.194	1962	1975	1978	rBV4	11355	20430	1.97%	0.293%
38	13.304	1988	1993	1996	rBV	9676	12956	1.25%	0.186%
39	13.347	1996	2000	2004	rVV2	13870	18963	1.83%	0.272%
40	13.566	2031	2036	2038	rVV4	7560	12489	1.20%	0.179%
41	13.639	2044	2048	2052	rVV3	13722	22818	2.20%	0.327%
42	13.694	2052	2057	2058	rVV3	10917	17895	1.72%	0.257%
43	13.719	2058	2061	2066	rVB2	15214	21809	2.10%	0.313%
44	13.834	2077	2080	2087	rVB	13461	20280	1.95%	0.291%
45	13.908	2088	2092	2097	rVB4	10039	15449	1.49%	0.222%
46	13.981	2097	2104	2108	rBV4	14254	26487	2.55%	0.380%
47	14.023	2108	2111	2115	rBV3	8074	11226	1.08%	0.161%
48	14.127	2123	2128	2132	rBV2	10121	13913	1.34%	0.200%
49	14.267	2146	2151	2156	rBV3	19727	30247	2.91%	0.434%
50	14.432	2173	2178	2182	rVB	15141	21569	2.08%	0.310%
51	14.536	2191	2195	2201	rBV3	16065	27158	2.62%	0.390%
52	14.670	2213	2217	2223	rBV9	8130	15499	1.49%	0.222%
53	14.731	2223	2227	2231	rVB3	11972	17317	1.67%	0.249%
54	14.840	2239	2245	2248	rBV4	11880	18867	1.82%	0.271%
55	15.249	2306	2312	2319	rBV6	10147	20235	1.95%	0.290%


Sum of corrected areas: 6967336

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX071019\
Data File : VX010773.D
Acq On : 10 Jul 2019 13:39
Operator : JC/SP
Sample : K3636-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP19-JMW0980

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

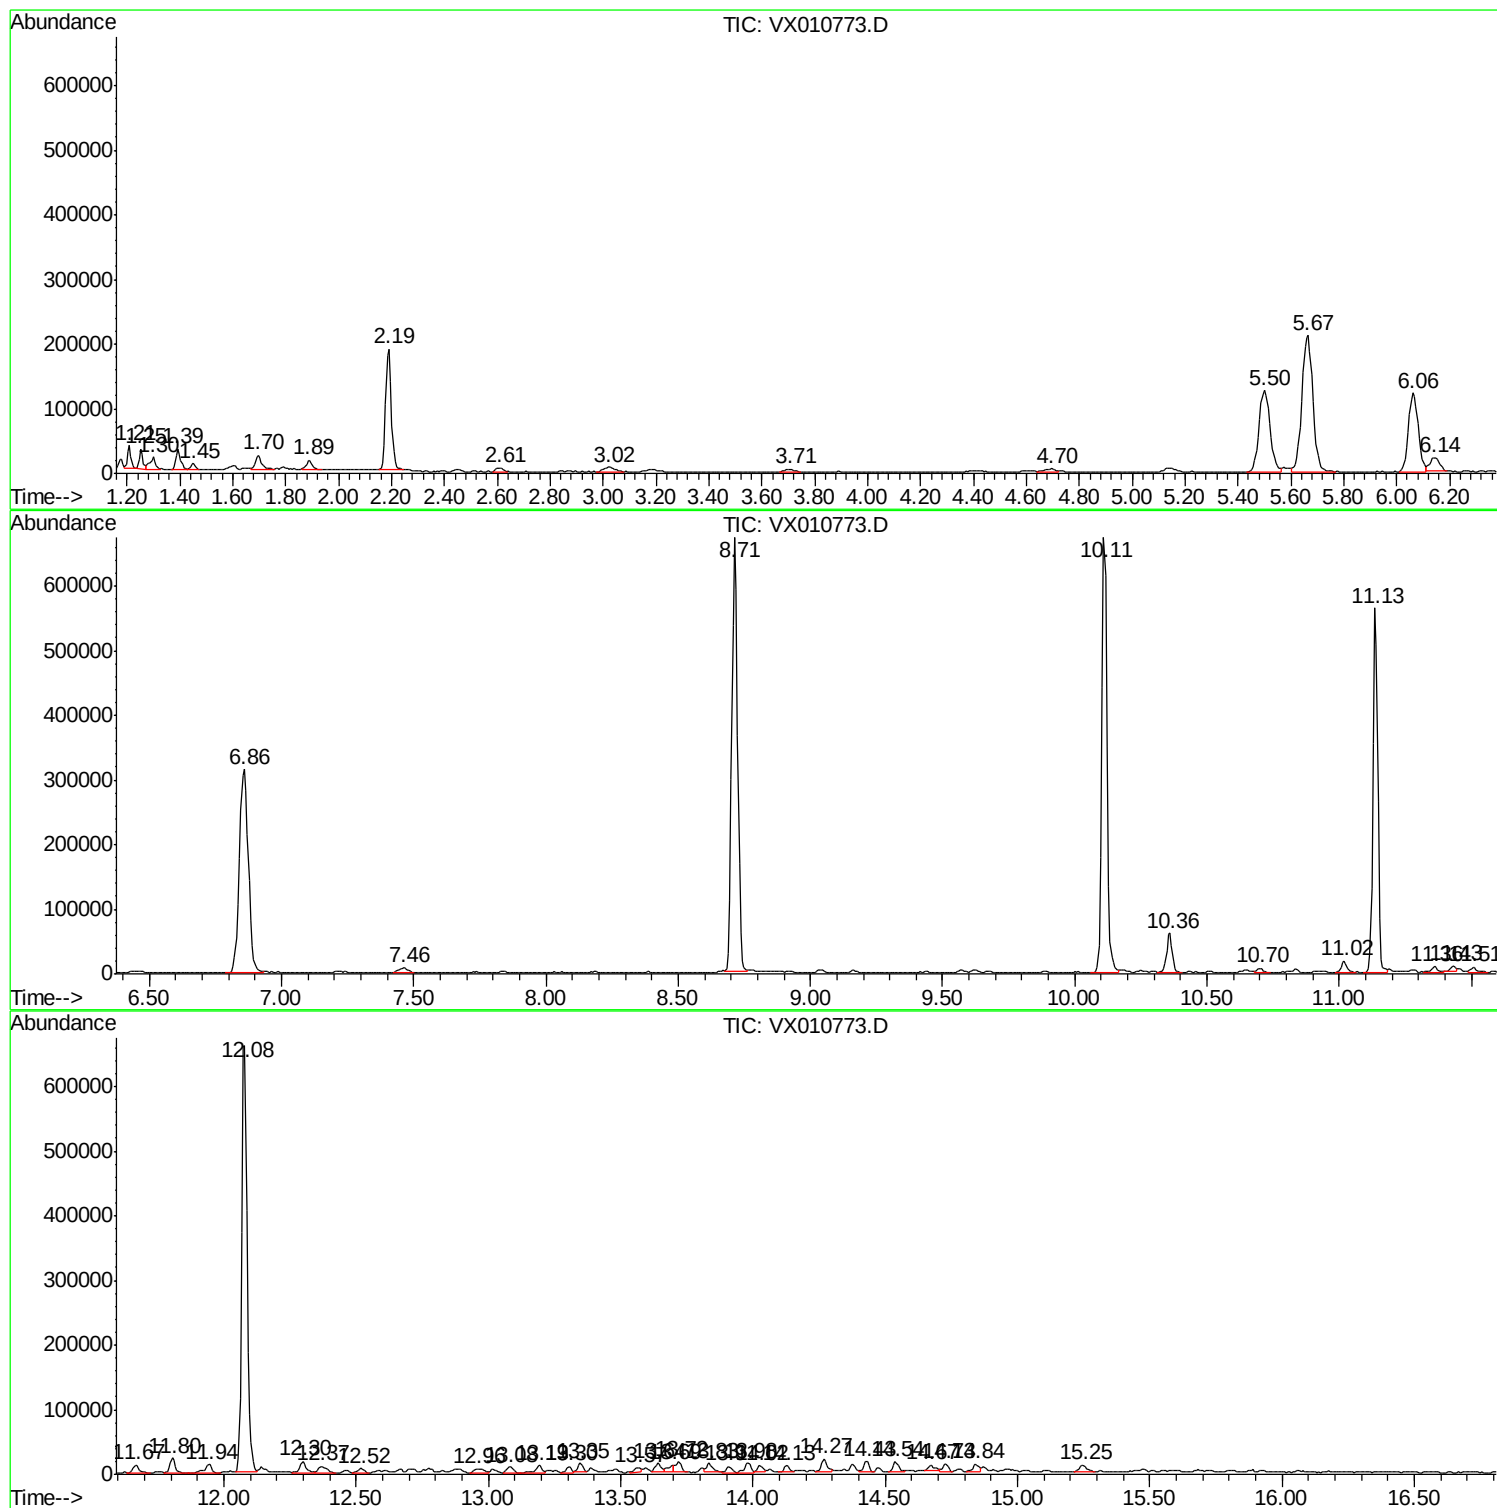

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_X\DATA\VX071019\
Data File : VX010773.D
Acq On : 10 Jul 2019 13:39
Operator : JC/SP
Sample : K3636-12
Misc : 5.0mL/MSV0A_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSV0A_X
ClientSampleId :
SP19-JMW0980

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071019\
Data File : VX010773.D
Acq On : 10 Jul 2019 13:39
Operator : JC/SP
Sample : K3636-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP19-JMW0980

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc