


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071019\
Data File : VX010765.D
Acq On : 10 Jul 2019 09:14
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260
Last Update : Thu Jun 20 03:31:56 2019

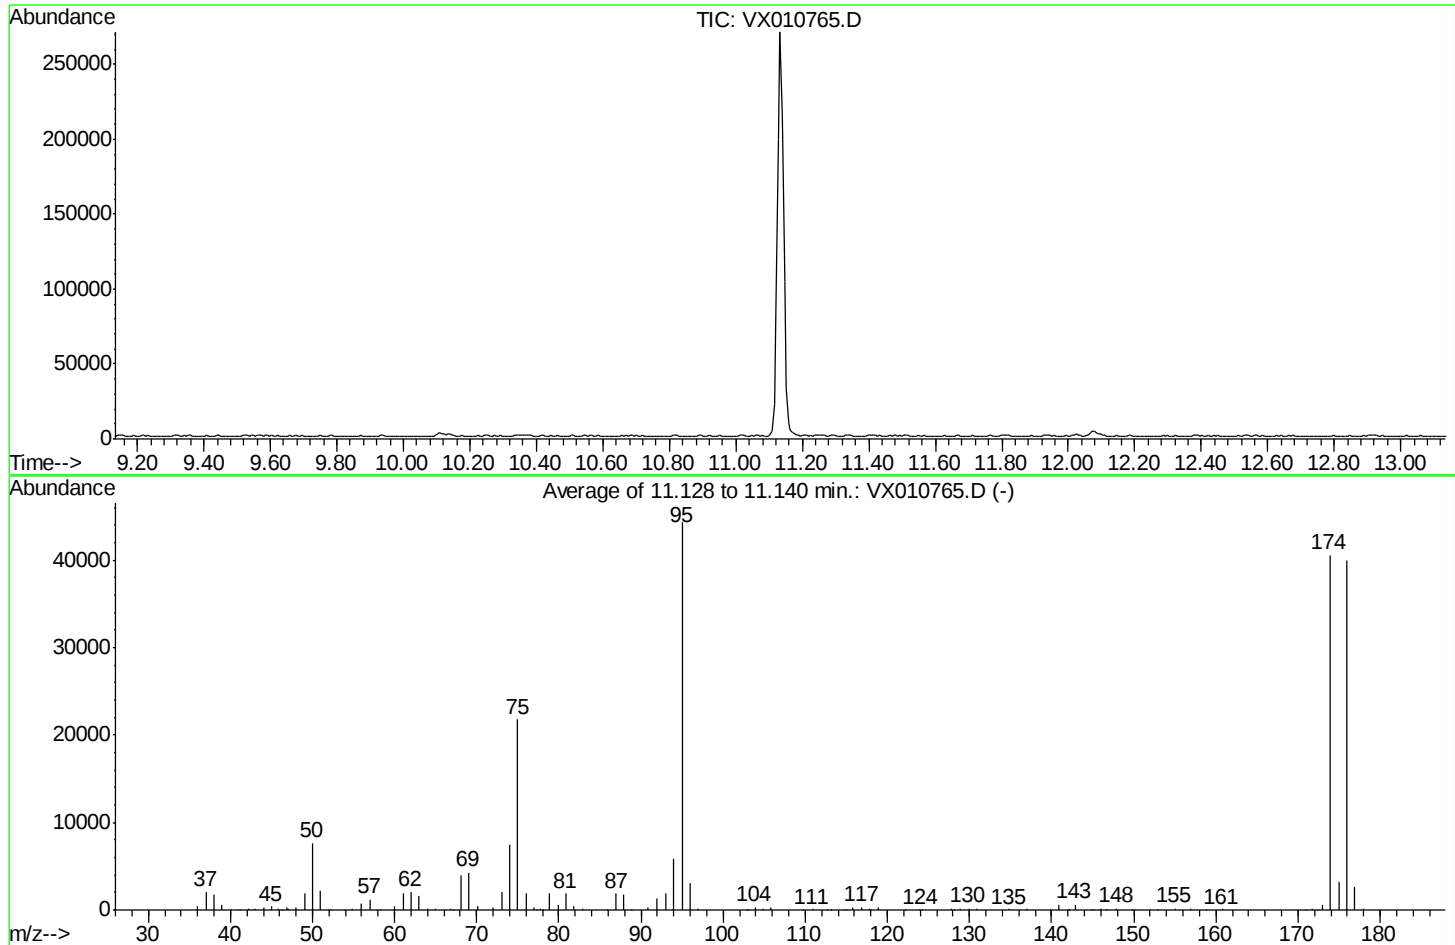

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	7657	PASS
75	95	30	60	49.2	21794	PASS
95	95	100	100	100.0	44338	PASS
96	95	5	9	6.8	3027	PASS
173	174	0.00	2	1.3	518	PASS
174	95	50	100	91.6	40626	PASS
175	174	5	9	7.9	3217	PASS
176	174	95	101	98.5	40000	PASS
177	176	5	9	6.4	2570	PASS